

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091622\
 Data File : VX031432.D
 Acq On : 17 Sep 2022 00:12
 Operator : JC/MD
 Sample : PB147603ZHE#01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB147603ZHE#01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
 Title : SW846 8260

Signal : TIC: VX031432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	42	rBV	14348	42429	3.85%	0.658%
2	1.618	76	87	100	rBV7	7142	24764	2.25%	0.384%
3	2.788	273	279	286	rBV2	8323	14691	1.33%	0.228%
4	4.727	586	597	606	rBV2	7363	21649	1.96%	0.336%
5	5.391	695	706	722	rBV2	49672	147133	13.35%	2.280%
6	5.556	722	733	745	rVV	84907	236743	21.48%	3.669%
7	5.958	790	799	814	rVB2	55079	146139	13.26%	2.265%
8	6.342	851	862	876	rBV	42847	109523	9.94%	1.697%
9	6.763	920	931	941	rBV	141652	370963	33.66%	5.749%
10	7.641	1065	1075	1080	rBV	22620	42390	3.85%	0.657%
11	7.696	1080	1084	1091	rVB	8636	14440	1.31%	0.224%
12	7.799	1094	1101	1116	rBV	656136	1101952	100.00%	17.078%
13	8.549	1218	1224	1234	rBV	146134	213164	19.34%	3.304%
14	8.653	1234	1241	1257	rVB	284308	457769	41.54%	7.094%
15	8.958	1285	1291	1300	rBV	187061	273062	24.78%	4.232%
16	9.244	1332	1338	1344	rBV	211926	286737	26.02%	4.444%
17	9.311	1344	1349	1351	rVV	15116	22420	2.03%	0.347%
18	9.342	1351	1354	1356	rVV	27060	36150	3.28%	0.560%
19	9.378	1356	1360	1366	rVB	76141	110366	10.02%	1.710%
20	9.482	1372	1377	1388	rVB	340451	440407	39.97%	6.825%
21	9.580	1388	1393	1404	rVB	245885	304698	27.65%	4.722%
22	9.915	1442	1448	1457	rBV	683870	841181	76.34%	13.036%
23	10.055	1462	1471	1477	rBV	313489	431003	39.11%	6.680%
24	10.281	1500	1508	1515	rBV2	7970	12387	1.12%	0.192%
25	10.506	1540	1545	1555	rVB2	8152	11440	1.04%	0.177%
26	10.640	1562	1567	1572	rBV	56727	69991	6.35%	1.085%
27	11.079	1634	1639	1649	rBV	235463	297373	26.99%	4.609%
28	12.024	1788	1794	1803	rBV	297949	371653	33.73%	5.760%


Sum of corrected areas: 6452617

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091622\
Data File : VX031432.D
Acq On : 17 Sep 2022 00:12
Operator : JC/MD
Sample : PB147603ZHE#01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB147603ZHE#01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

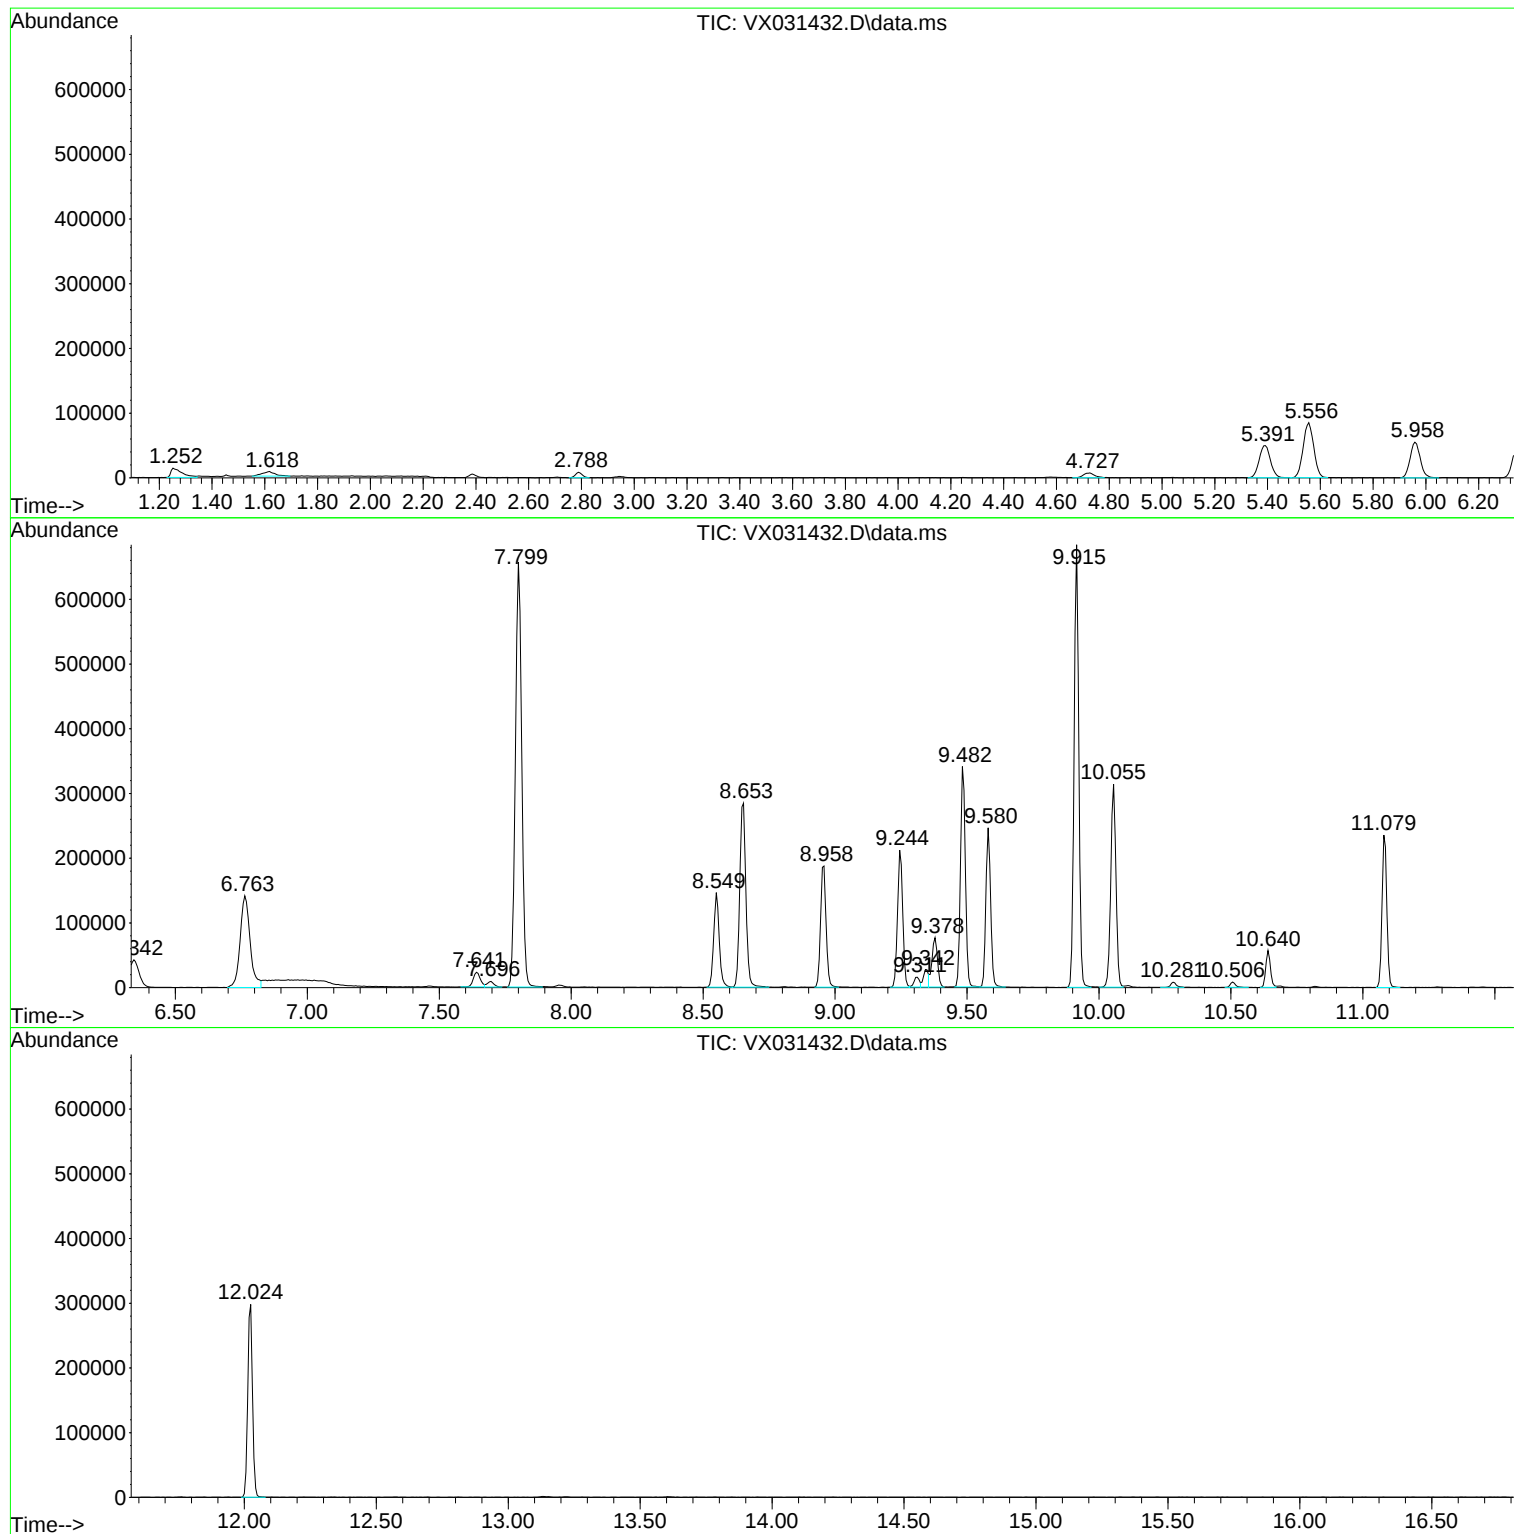

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091622\
Data File : VX031432.D
Acq On : 17 Sep 2022 00:12
Operator : JC/MD
Sample : PB147603ZHE#01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB147603ZHE#01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091622\
Data File : VX031432.D
Acq On : 17 Sep 2022 00:12
Operator : JC/MD
Sample : PB147603ZHE#01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB147603ZHE#01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------