
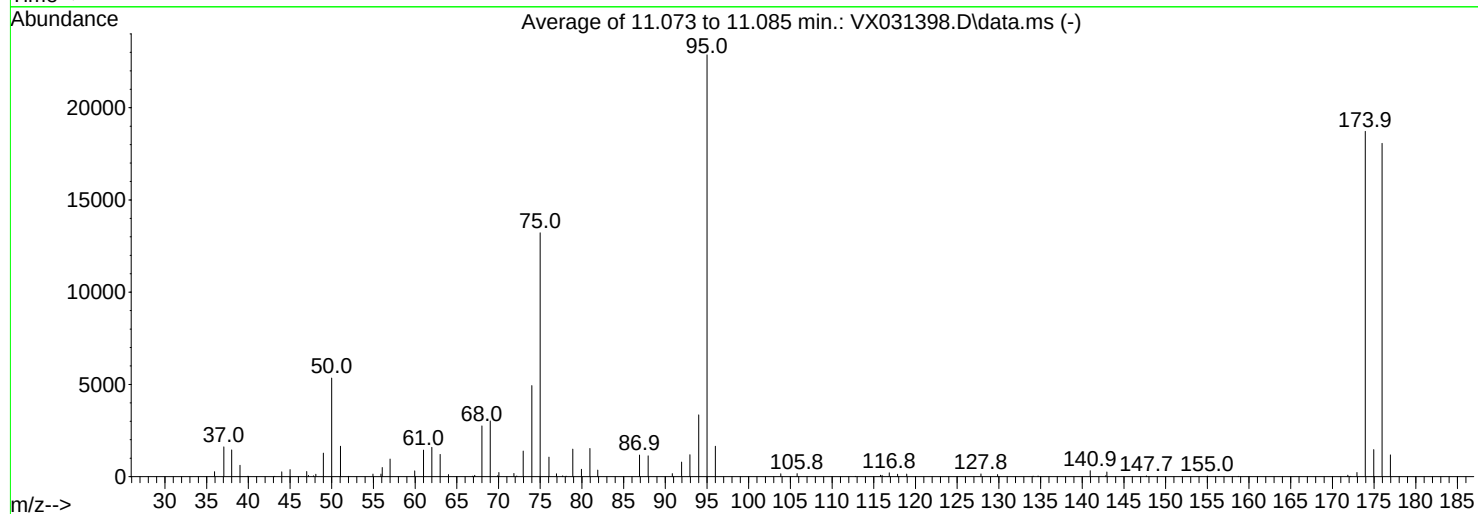


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091622\
 Data File : VX031398.D
 Acq On : 16 Sep 2022 09:43
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X091622W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Sep 16 12:41:56 2022

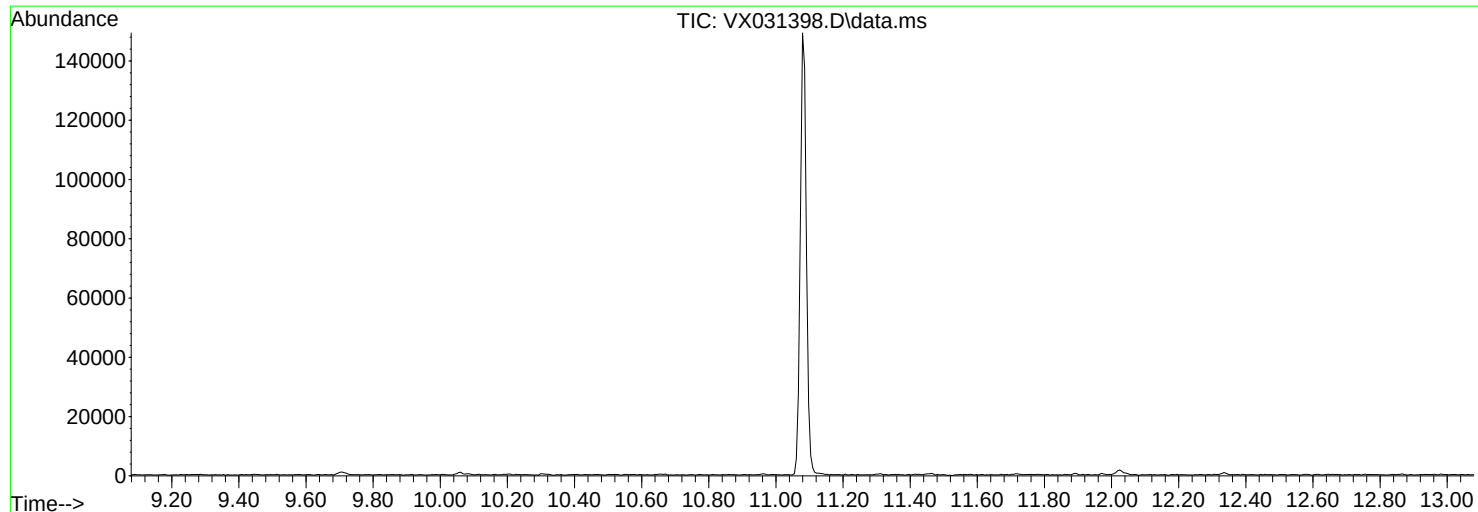

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	5341	PASS
75	95	30	60	57.8	13215	PASS
95	95	100	100	100.0	22866	PASS
96	95	5	9	7.2	1651	PASS
173	174	0.00	2	1.2	225	PASS
174	95	50	100	81.8	18715	PASS
175	174	5	9	7.8	1466	PASS
176	174	95	101	96.6	18070	PASS
177	176	5	9	6.5	1183	PASS