
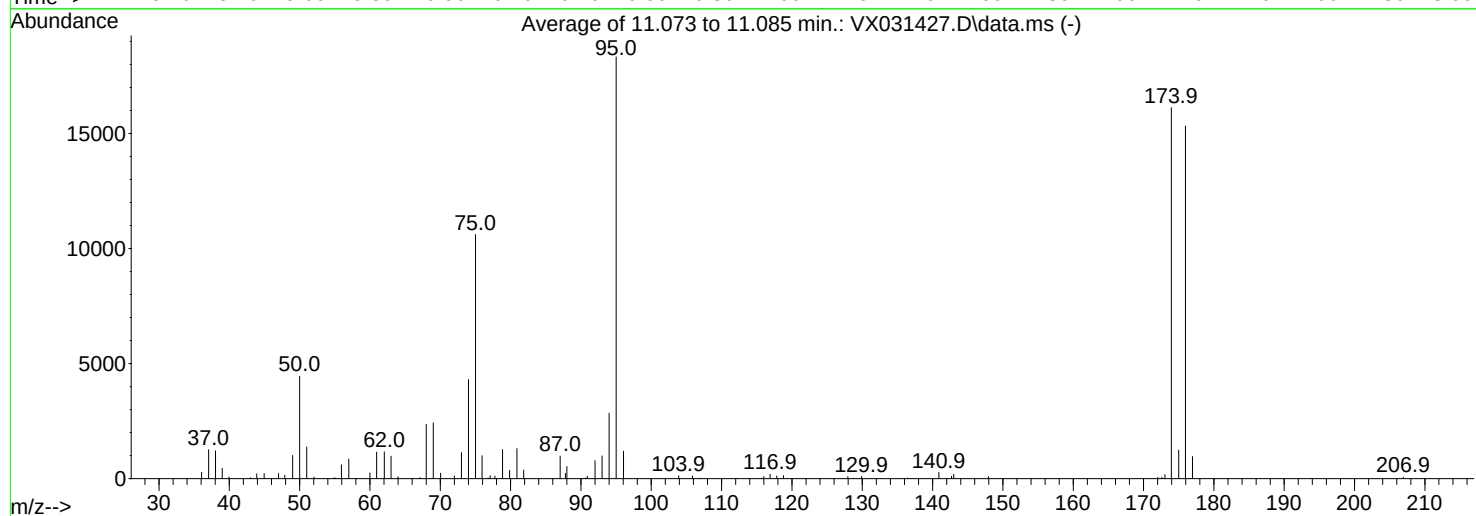


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091622\
Data File : VX031427.D
Acq On : 16 Sep 2022 22:16
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091422W.M
Title : SW846 8260
Last Update : Thu Sep 15 01:50:07 2022

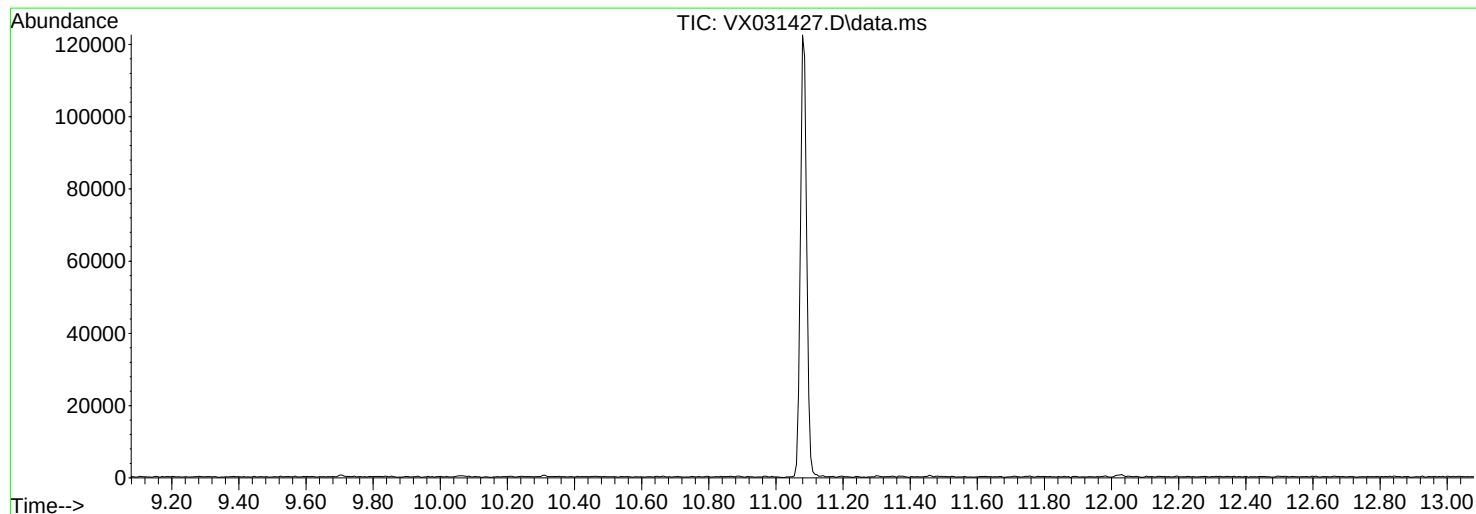

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.3	4450	PASS
75	95	30	60	57.9	10613	PASS
95	95	100	100	100.0	18329	PASS
96	95	5	9	6.5	1196	PASS
173	174	0.00	2	1.1	173	PASS
174	95	50	100	87.9	16118	PASS
175	174	5	9	7.7	1236	PASS
176	174	95	101	95.0	15314	PASS
177	176	5	9	6.3	961	PASS