

Data File : VX012459.D
Acq On : 18 Sep 2019 02:07
Operator : JC/SP
Sample : K4858-16 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D2-20190909

Quant Time: Sep 18 03:33:19 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091719W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 17 15:27:10 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	158350	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	252305	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	220035	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	94771	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	109831	48.39	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.78%	
35) Dibromofluoromethane	5.49	113	77765	50.92	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.84%	
50) Toluene-d8	8.71	98	299204	52.93	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.86%	
62) 4-Bromofluorobenzene	11.14	95	112492	47.93	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.86%	


Target Compounds			Qvalue			
2) Dichlorodifluoromethane	1.20	85	53	0.441	ug/l #	43
5) Bromomethane	1.64	94	252	0.682	ug/l #	48
6) Chloroethane	1.72	64	421	0.572	ug/l #	59
8) Diethyl Ether	2.16	74	159	0.204	ug/l	51
9) 1,1,2-Trichlorotrifluoroet	2.37	101	2699	2.163	ug/l	90
10) Methyl Iodide	2.50	142	21	4.460	ug/l #	35
11) Tert butyl alcohol	3.00	59	5272	3.367	ug/l #	84
12) 1,1-Dichloroethene	2.36	96	756	0.759	ug/l	92
13) Acrolein	2.29	56	141	Below Cal	#	1
16) Acetone	2.44	43	968	Below Cal		90
17) Carbon Disulfide	2.55	76	163	1.918	ug/l #	75
20) Methylene Chloride	2.86	84	531	0.387	ug/l #	57
26) 2,2-Dichloropropane	4.67	77	666	0.261	ug/l	82
27) cis-1,2-Dichloroethene	4.59	96	350	0.227	ug/l #	1
30) Chloroform	5.20	83	1252	0.420	ug/l #	64
31) Cyclohexane	5.65	56	4088	2.608	ug/l #	3
36) 1,1-Dichloropropene	5.65	75	13597	8.867	ug/l #	54
38) Carbon Tetrachloride	5.78	117	513	0.269	ug/l #	67
39) Methylcyclohexane	7.21	83	6732	4.516	ug/l #	1
44) Trichloroethene	7.21	130	518541	404.265	ug/l	99
49) 1,4-Dioxane	7.56	88	39	0.805	ug/l #	73
55) 1,1,2-Trichloroethane	9.21	97	350	0.216	ug/l #	89
64) Tetrachloroethene	9.33	164	290	0.288	ug/l #	80
76) 1,2,3-Trichloropropane	11.14	75	57896	26.595	ug/l #	38
81) trans-1,4-Dichloro-2-buten	11.14	75	57896	71.588	ug/l #	8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VX012459.D
Acq On : 18 Sep 2019 02:07
Operator : JC/SP
Sample : K4858-16 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D2-20190909

Quant Time: Sep 18 03:33:19 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091719W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 17 15:27:10 2019
Response via : Initial Calibration

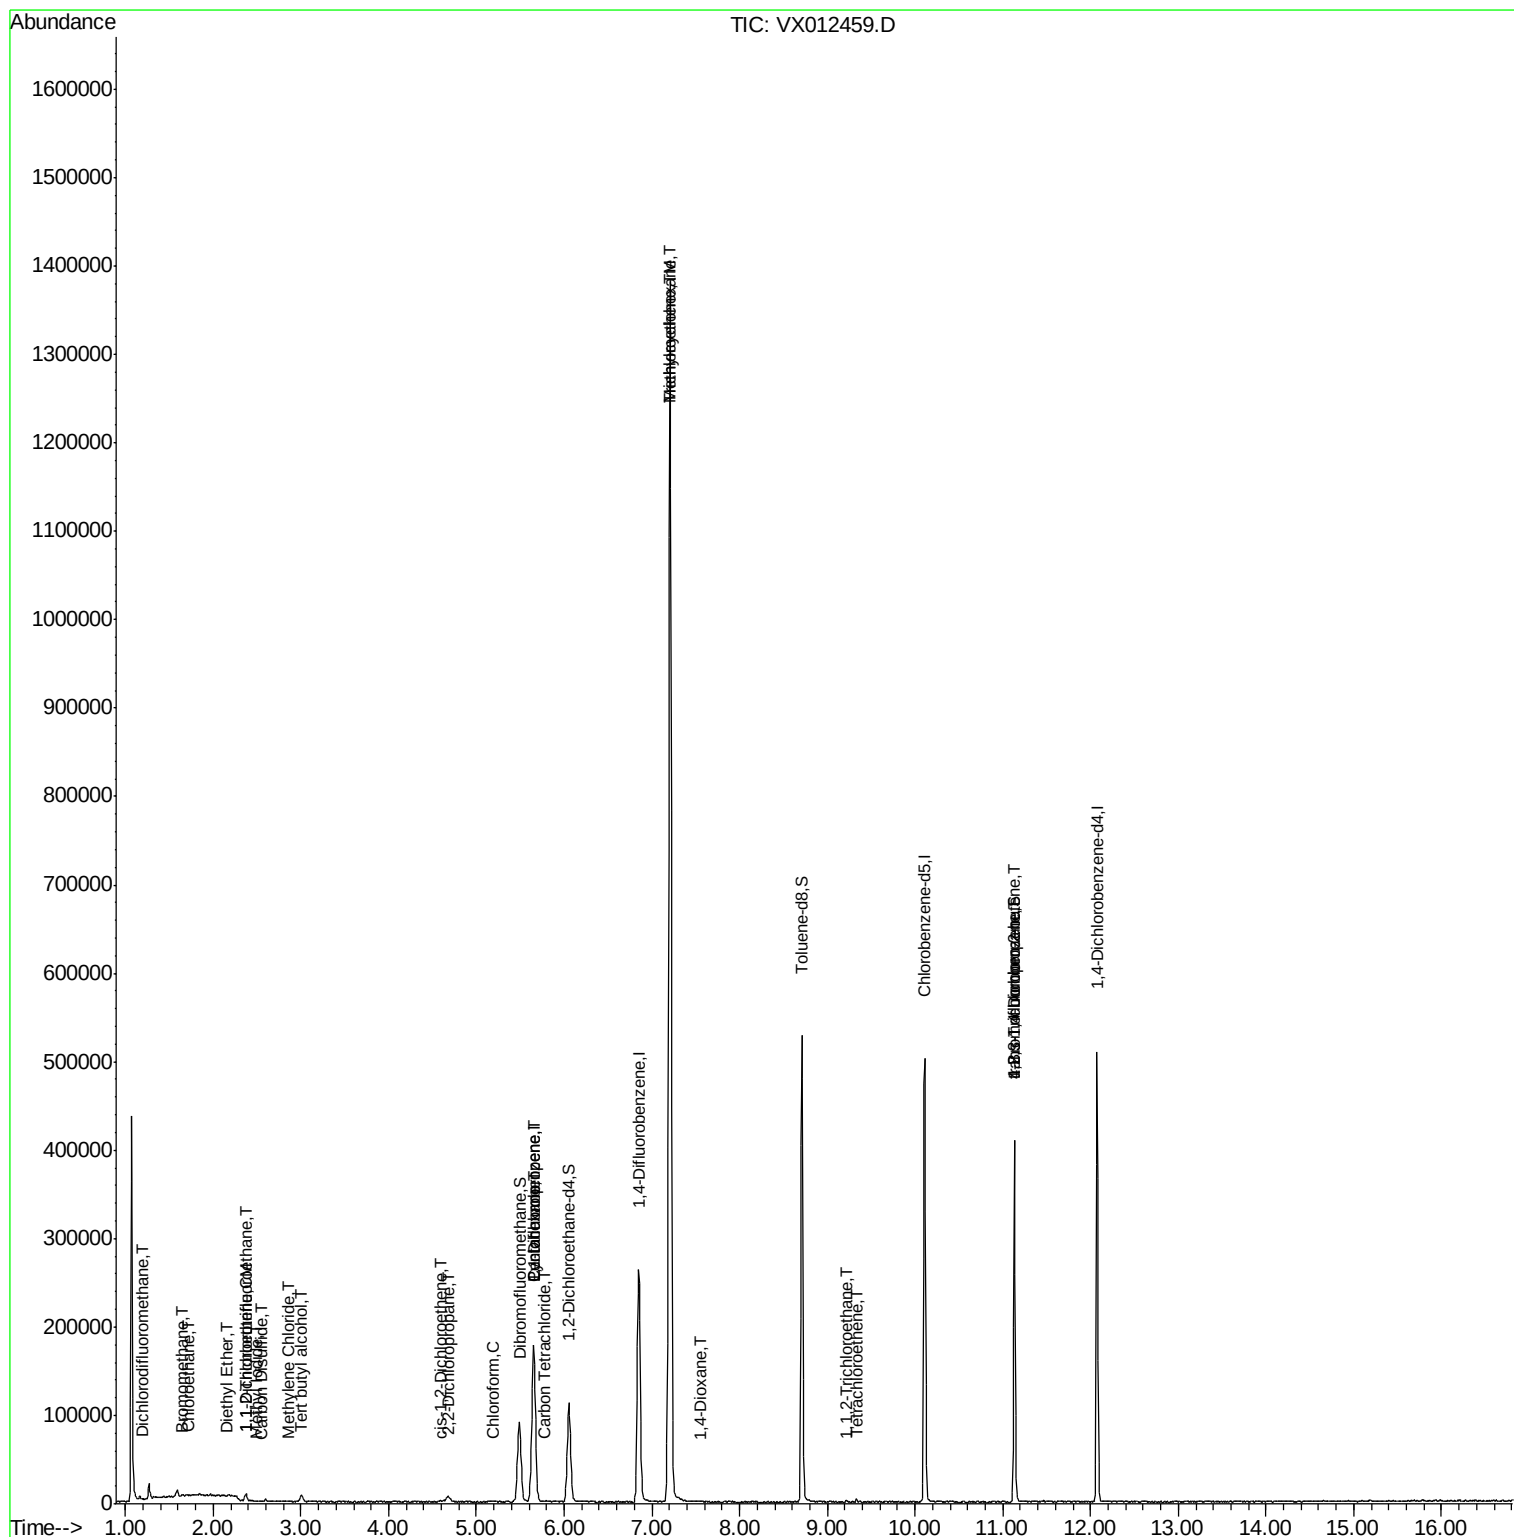



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 782

Delta R.T. 0.01 min

Lab File: VX012459.D

Acq: 18 Sep 2019 02:07

Instrument :

MSVOA_X

ClientSampleId :


RE122D2-20190909

Tgt Ion:168 Resp: 158350

Ion Ratio Lower Upper




168 100

99 64.1 51.4 77.2



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

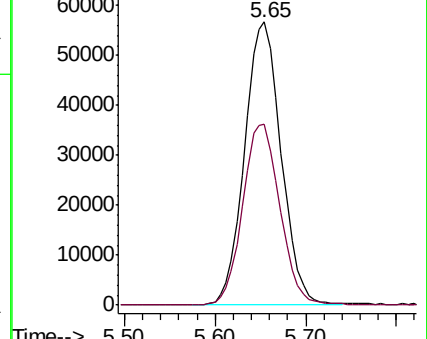

#2

Dichlorodifluoromethane

Concen: 0.441 ug/l

RT: 1.20 min Scan# 51

Delta R.T. 0.01 min

Lab File: VX012459.D


Acq: 18 Sep 2019 02:07

Tgt Ion: 85 Resp: 53

Ion Ratio Lower Upper



85 100


87 0.0 15.6 46.8#



Abundance Ion 84.90 (84.60 to 85.60): VX0

Ion 86.90 (86.60 to 87.60): VX0

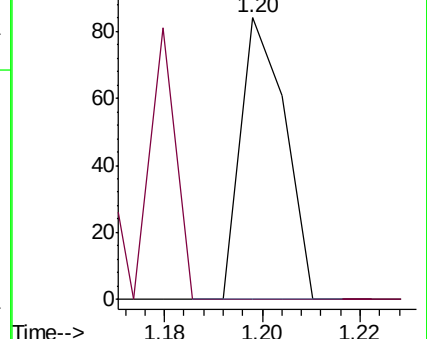



#5

Bromomethane

Concen: 0.682 ug/l

RT: 1.64 min Scan# 123

Delta R.T. 0.01 min

Lab File: VX012459.D

Acq: 18 Sep 2019 02:07

Instrument :

MSVOA_X

ClientSampleId :


RE122D2-20190909

Tgt Ion: 94 Resp: 252

Ion Ratio Lower Upper




94 100

96 140.0 72.8 109.2#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

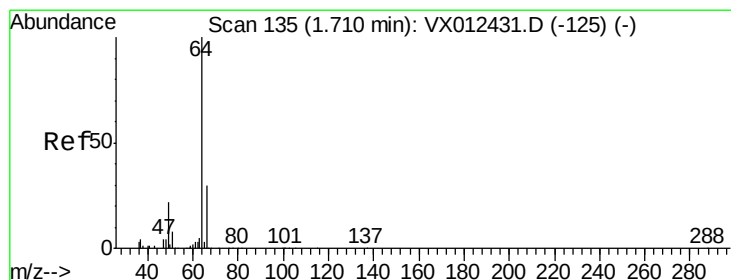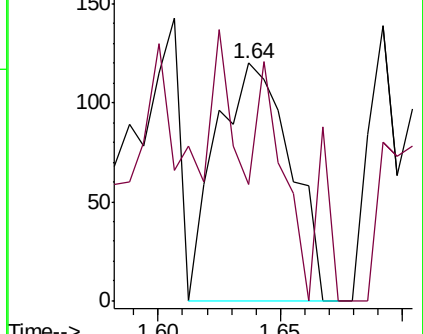

#6

Chloroethane

Concen: 0.572 ug/l

RT: 1.72 min Scan# 136

Delta R.T. 0.01 min

Lab File: VX012459.D


Acq: 18 Sep 2019 02:07

Tgt Ion: 64 Resp: 421

Ion Ratio Lower Upper



64 100


66 7.9 24.0 36.0#



Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0

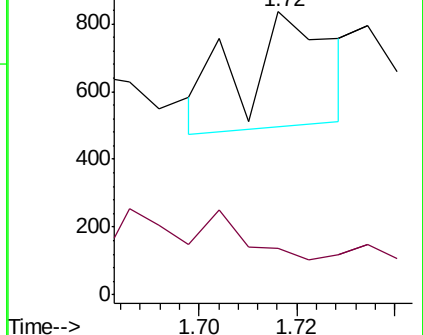

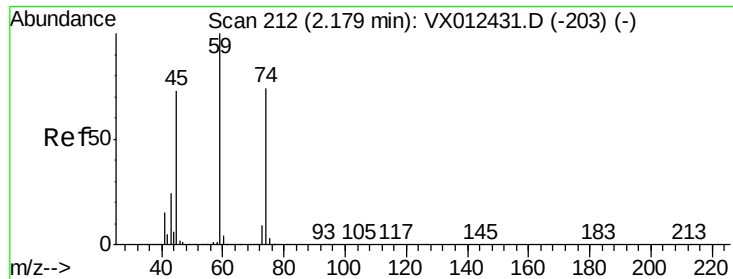

#8

Diethyl Ether

Concen: 0.204 ug/l

RT: 2.16 min Scan# 208

Delta R.T. -0.02 min

Lab File: VX012459.D

Acq: 18 Sep 2019 02:07

Instrument :

MSVOA_X

ClientSampleId :


RE122D2-20190909

Tgt Ion: 74 Resp: 159

Ion Ratio Lower Upper




74 100

45 148.4 49.9 149.7

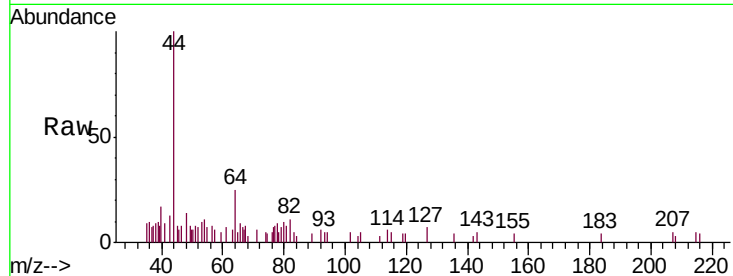

Abundance Ion 74.00 (73.70 to 74.70): VX0

Ion 45.00 (44.70 to 45.70): VX0

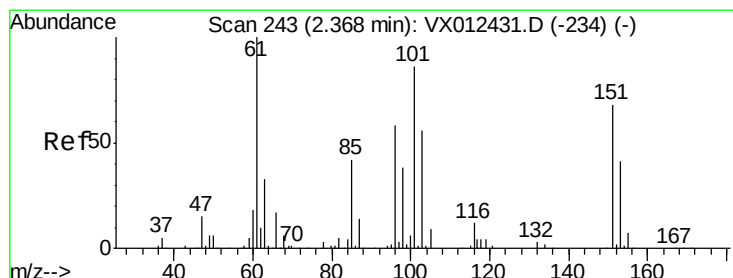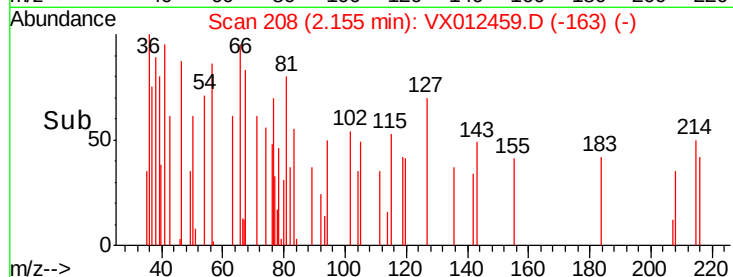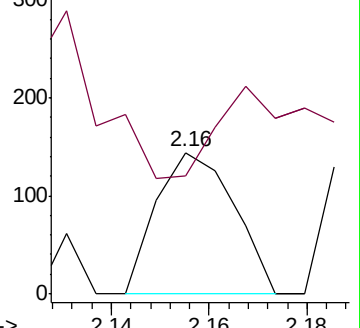

#9

1,1,2-Trichlorotrifluoroethane

Concen: 2.163 ug/l

RT: 2.37 min Scan# 244

Delta R.T. 0.01 min

Lab File: VX012459.D

Acq: 18 Sep 2019 02:07


Tgt Ion: 101 Resp: 2699

Ion Ratio Lower Upper

101 100

85 53.4 37.3 55.9



151 84.9 61.0 91.4

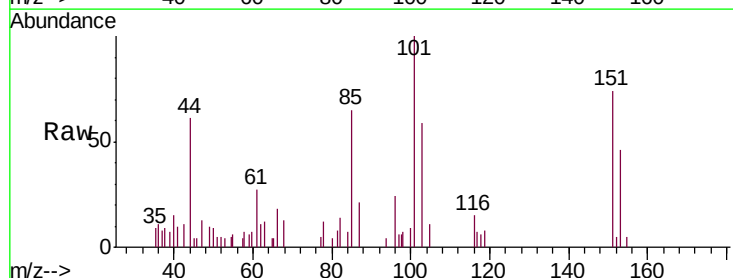


Abundance Ion 100.90 (100.60 to 101.60): V

Ion 84.90 (84.60 to 85.60): VX0

Ion 150.80 (150.50 to 151.50): V

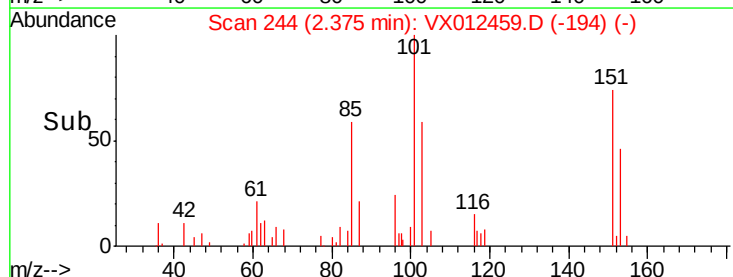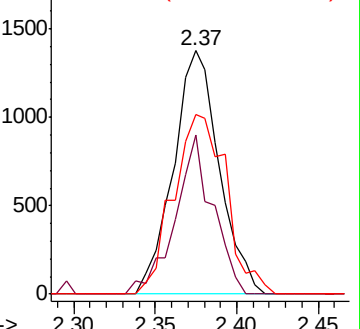


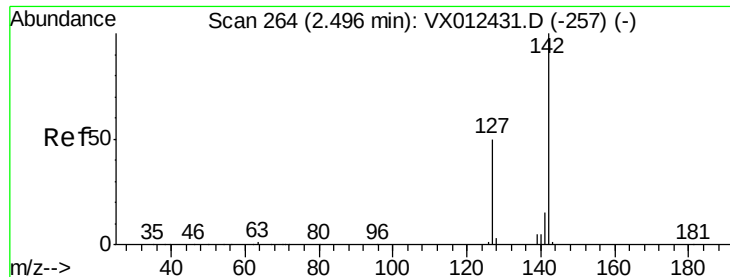




#10
Methyl Iodide
Concen: 4.460 ug/l
RT: 2.50 min Scan# 265
Delta R.T. 0.01 min
Lab File: VX012459.D
Acq: 18 Sep 2019 02:07

Instrument :
MSVOA_X
ClientSampleId :
RE122D2-20190909

Tgt Ion: 142 Resp: 21
Ion Ratio Lower Upper
142 100
127 0.0 40.8 61.2#
141 0.0 12.1 18.1#

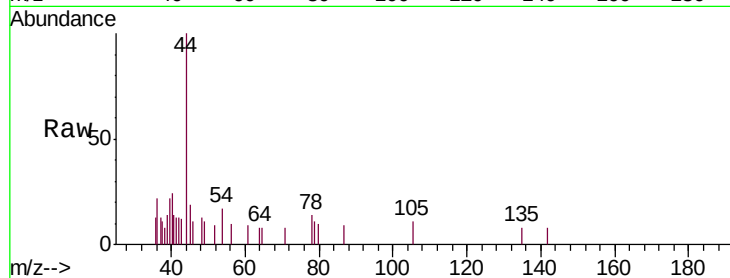


Abundance Ion 141.80 (141.50 to 142.50): V
Ion 126.80 (126.50 to 127.50): V
Ion 140.80 (140.50 to 141.50): V

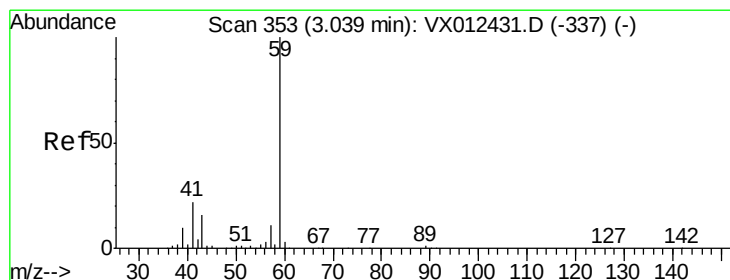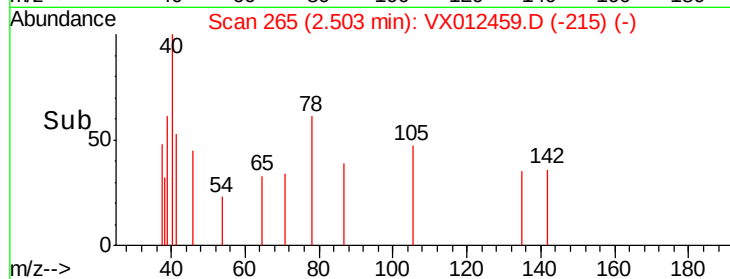
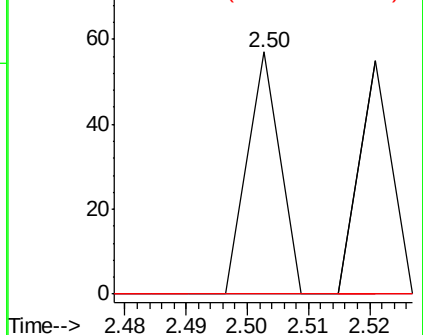



#11
Tert butyl alcohol
Concen: 3.367 ug/l
RT: 3.00 min Scan# 347
Delta R.T. -0.04 min
Lab File: VX012459.D
Acq: 18 Sep 2019 02:07

Tgt Ion: 59 Resp: 5272
Ion Ratio Lower Upper
59 100
57 4.5 8.3 12.5#

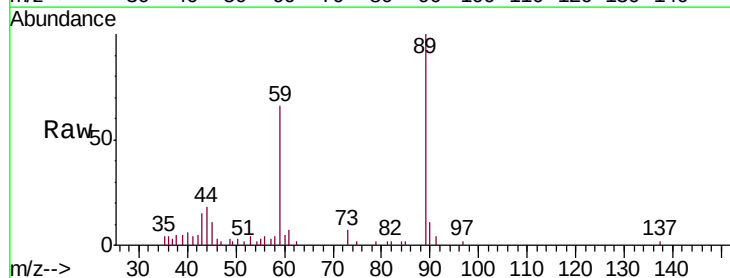

Abundance Ion 59.00 (58.70 to 59.70): VX0
Ion 57.00 (56.70 to 57.70): VX0



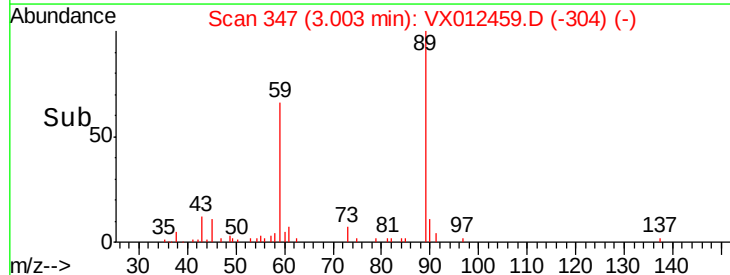
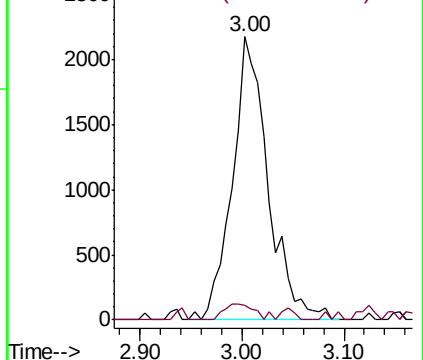




#12
 1,1-Dichloroethene
 Concen: 0.759 ug/l
 RT: 2.36 min Scan# 242
 Delta R.T. 0.00 min
 Lab File: VX012459.D
 Acq: 18 Sep 2019 02:07




Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D2-20190909


Tgt Ion: 96 Resp: 756
 Ion Ratio Lower Upper
 96 100
 61 177.3 133.8 200.6
 98 69.2 49.9 74.9

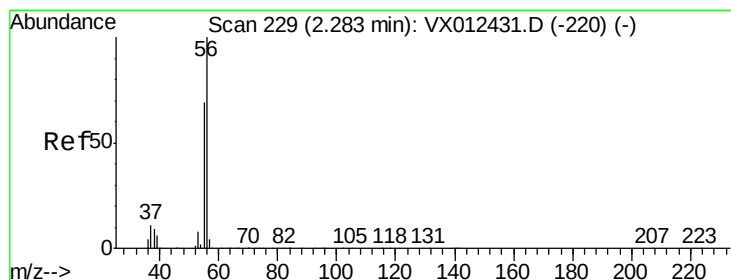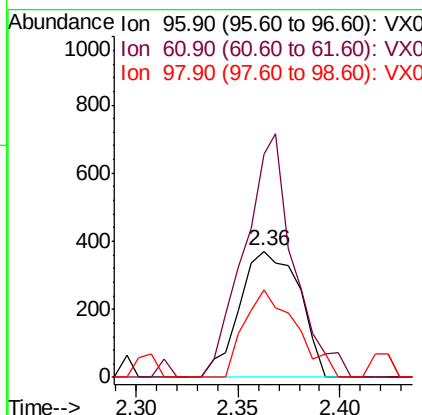

#13
 Acrolein
 Concen: Below Cal
 RT: 2.29 min Scan# 230
 Delta R.T. 0.01 min
 Lab File: VX012459.D
 Acq: 18 Sep 2019 02:07

Tgt Ion: 56 Resp: 141
 Ion Ratio Lower Upper
 56 100
 55 209.2 55.8 83.8#

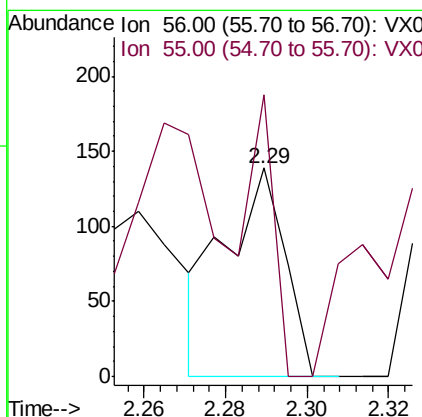



#16

Acetone

Concen: Below Cal

RT: 2.44 min Scan# 254

Delta R.T. 0.00 min

Lab File: VX012459.D

Acq: 18 Sep 2019 02:07

Instrument :

MSVOA_X

ClientSampleId :


RE122D2-20190909

Tgt Ion: 43 Resp: 968




Ion Ratio Lower Upper

43 100

58 34.2 23.3 34.9



Abundance Ion 43.00 (42.70 to 43.70): VX0

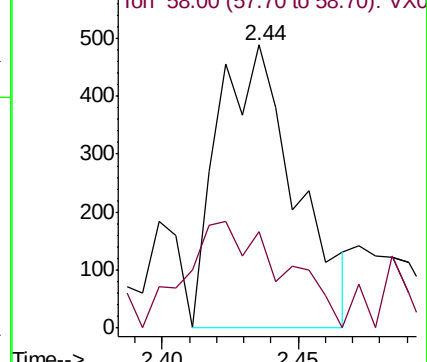

#17

Carbon Disulfide

Concen: 1.918 ug/l

RT: 2.55 min Scan# 273

Delta R.T. -0.01 min

Lab File: VX012459.D


Acq: 18 Sep 2019 02:07

Tgt Ion: 76 Resp: 163



Ion Ratio Lower Upper


76 100

78 0.0 7.3 10.9#



Abundance Ion 75.90 (75.60 to 76.60): VX0




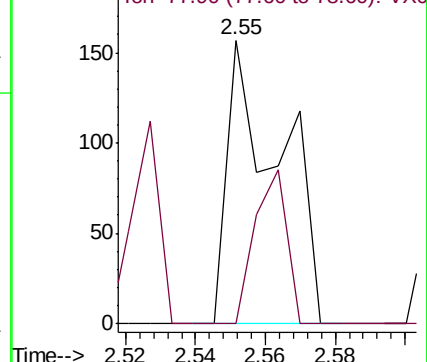




#20
Methylene Chloride
Concen: 0.387 ug/l
RT: 2.86 min Scan# 323
Delta R.T. 0.01 min
Lab File: VX012459.D
Acq: 18 Sep 2019 02:07




Instrument :
MSVOA_X
ClientSampleId :
RE122D2-20190909


Tgt Ion: 84 Resp: 531
Ion Ratio Lower Upper
84 100
49 66.5 106.8 160.2#
51 31.5 32.3 48.5#
86 39.0 51.3 76.9#

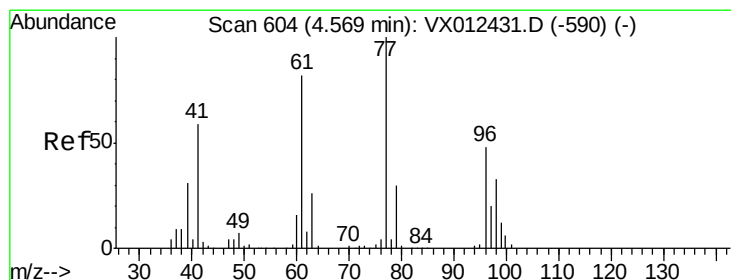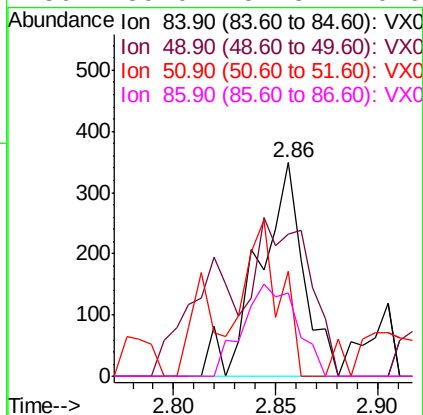

#26
2,2-Dichloropropane
Concen: 0.261 ug/l
RT: 4.67 min Scan# 620
Delta R.T. 0.10 min
Lab File: VX012459.D
Acq: 18 Sep 2019 02:07

Tgt Ion: 77 Resp: 666
Ion Ratio Lower Upper
77 100
97 12.8 10.5 31.6

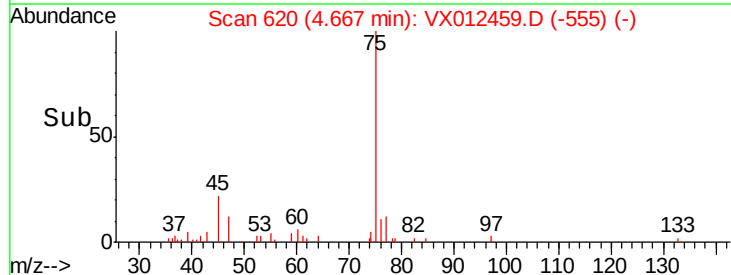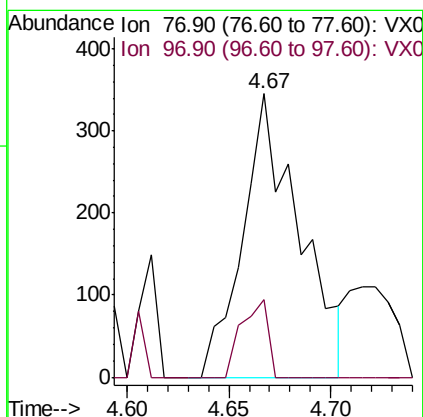







#27

cis-1,2-Dichloroethene
 Concen: 0.227 ug/l
 RT: 4.59 min Scan# 607
 Delta R.T. 0.01 min
 Lab File: VX012459.D
 Acq: 18 Sep 2019 02:07

Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D2-20190909




Tgt Ion: 96 Resp: 350
 Ion Ratio Lower Upper
 96 100
 61 324.6 0.0 319.4#
 98 135.4 0.0 130.6#

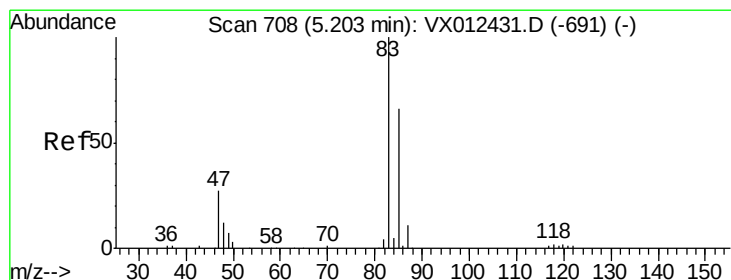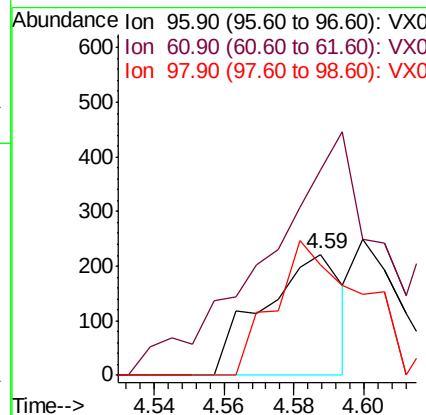


#30

Chloroform
 Concen: 0.420 ug/l
 RT: 5.20 min Scan# 707
 Delta R.T. -0.01 min
 Lab File: VX012459.D
 Acq: 18 Sep 2019 02:07

Tgt Ion: 83 Resp: 1252
 Ion Ratio Lower Upper
 83 100
 85 37.6 53.0 79.4#

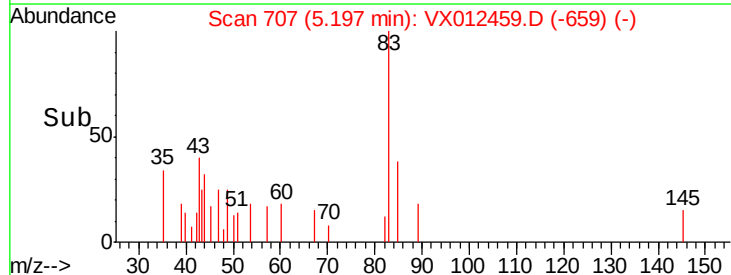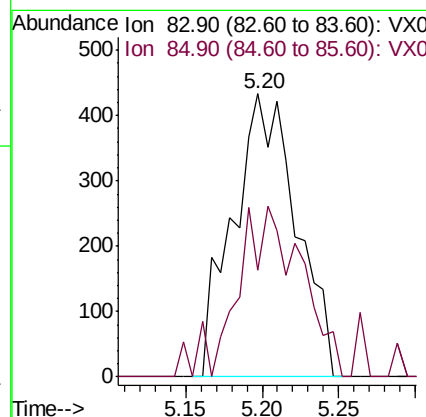

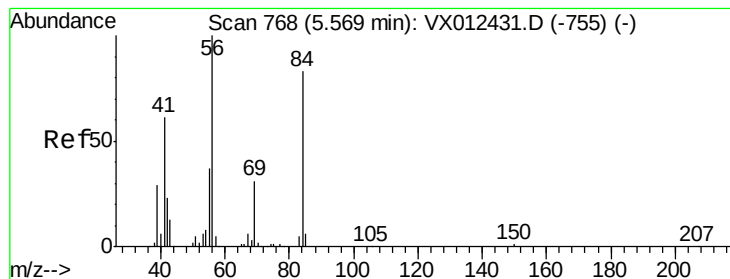

#31

Cyclohexane

Concen: 2.608 ug/l

RT: 5.65 min Scan# 781

Delta R.T. 0.08 min

Lab File: VX012459.D

Acq: 18 Sep 2019 02:07

Instrument :

MSVOA_X

ClientSampleId :

RE122D2-20190909


Tgt Ion: 56 Resp: 4088

Ion Ratio Lower Upper

56 100

69 167.5 25.0 37.6#




84 119.4 66.4 99.6#

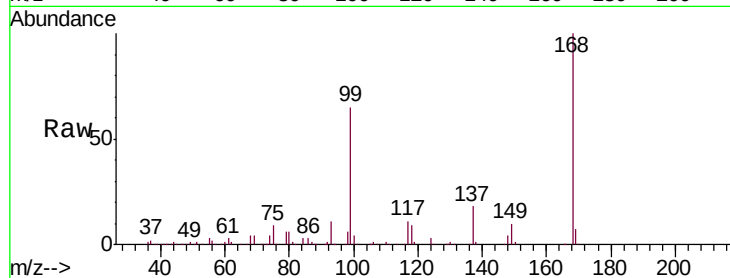

Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0

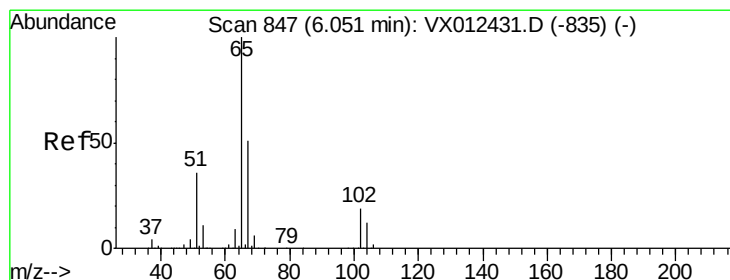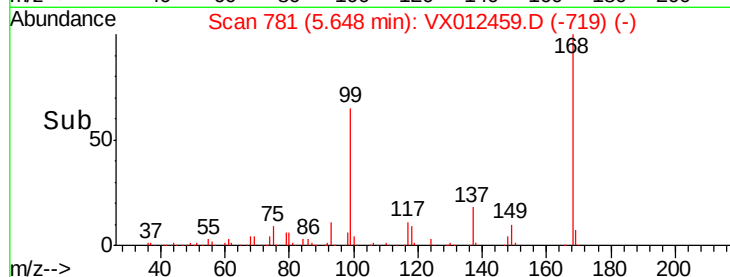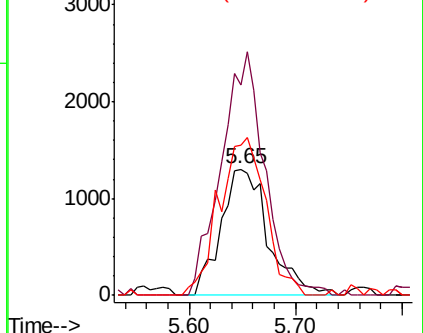

#33

1,2-Dichloroethane-d4

Concen: 48.395 ug/l

RT: 6.05 min Scan# 847

Delta R.T. 0.00 min

Lab File: VX012459.D


Acq: 18 Sep 2019 02:07

Tgt Ion: 65 Resp: 109831

Ion Ratio Lower Upper



65 100


67 51.0 0.0 101.2

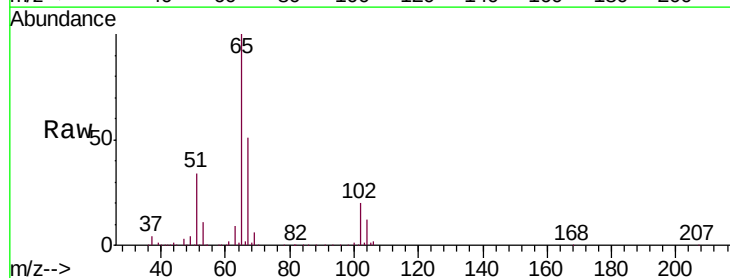

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

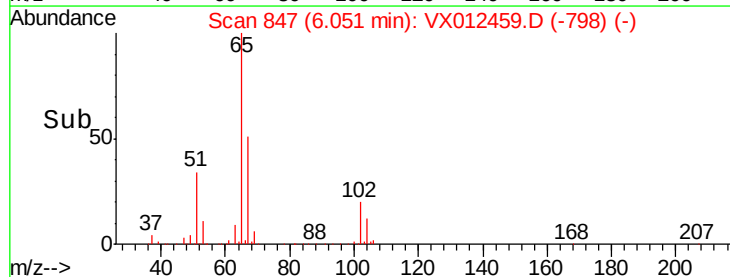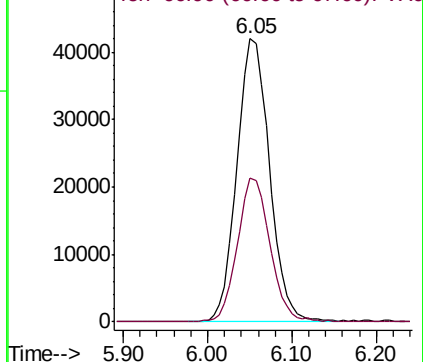







#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.85 min Scan# 978
 Delta R.T. 0.00 min
 Lab File: VX012459.D
 Acq: 18 Sep 2019 02:07

Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D2-20190909

Tgt Ion:114 Resp: 252305
 Ion Ratio Lower Upper
 114 100
 63 22.1 0.0 43.2
 88 16.7 0.0 33.2




Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VX0
 Ion 87.90 (87.60 to 88.60): VX0


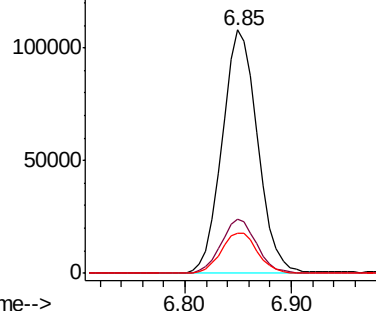



#35
 Dibromofluoromethane
 Concen: 50.923 ug/l
 RT: 5.49 min Scan# 755
 Delta R.T. 0.00 min
 Lab File: VX012459.D
 Acq: 18 Sep 2019 02:07

Tgt Ion:113 Resp: 77765
 Ion Ratio Lower Upper
 113 100
 111 102.9 83.4 125.2
 192 18.5 14.4 21.6



Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



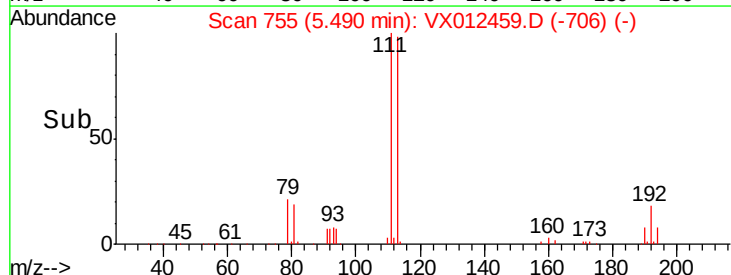
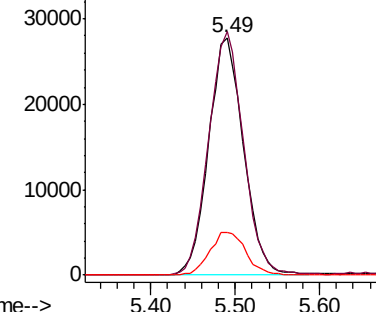


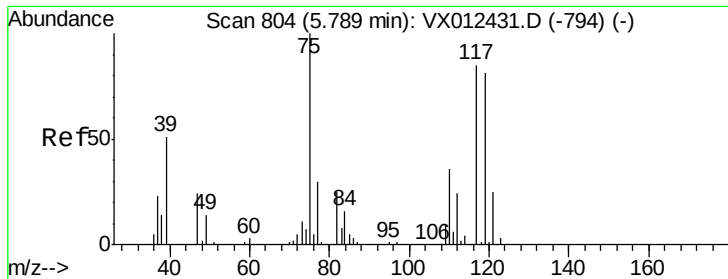

#36
 1,1-Dichloropropene
 Concen: 8.867 ug/l
 RT: 5.65 min Scan# 781
 Delta R.T. -0.14 min
 Lab File: VX012459.D
 Acq: 18 Sep 2019 02:07




Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D2-20190909


Tgt Ion: 75 Resp: 13597
 Ion Ratio Lower Upper
 75 100
 110 12.1 16.7 50.0#
 77 0.0 24.2 36.2#

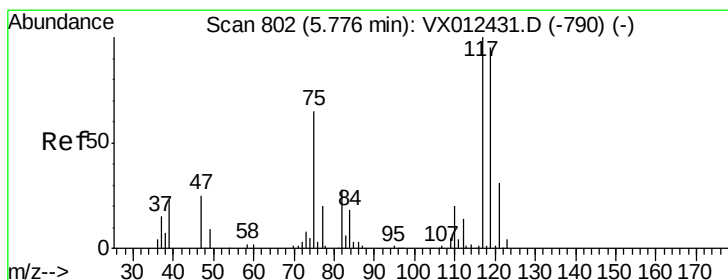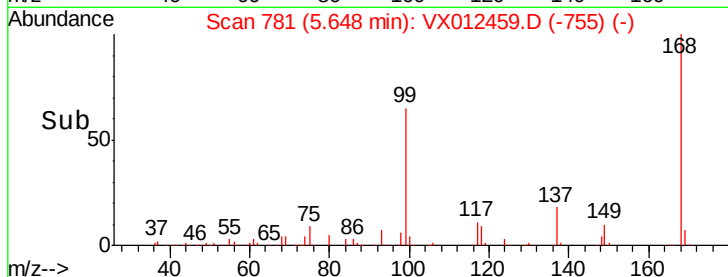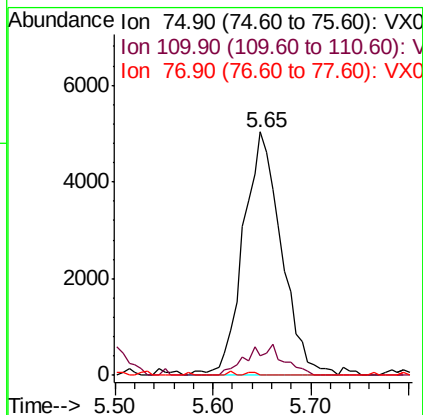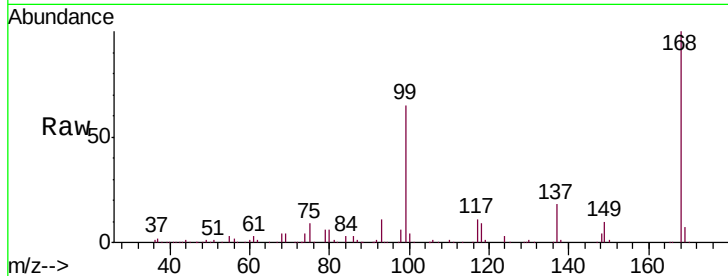

#38
 Carbon Tetrachloride
 Concen: 0.269 ug/l
 RT: 5.78 min Scan# 802
 Delta R.T. 0.00 min
 Lab File: VX012459.D
 Acq: 18 Sep 2019 02:07

Tgt Ion: 117 Resp: 513
 Ion Ratio Lower Upper
 117 100
 119 62.1 75.7 113.5#
 121 48.3 24.2 36.4#


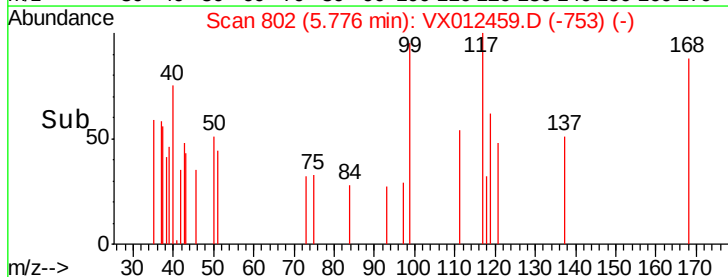
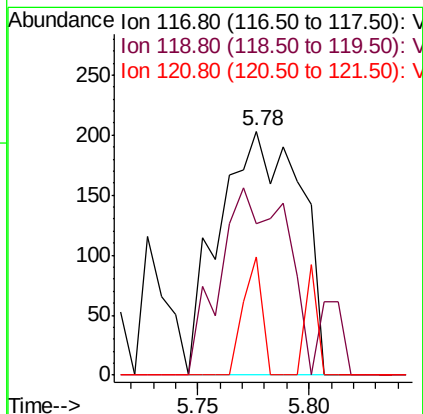
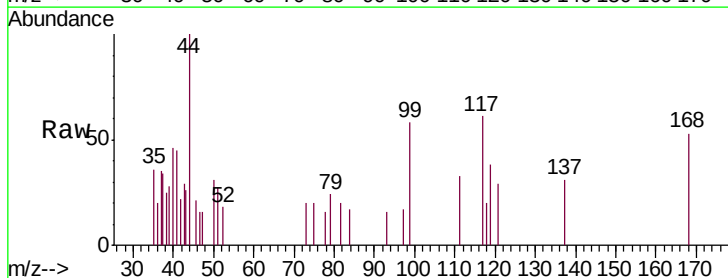


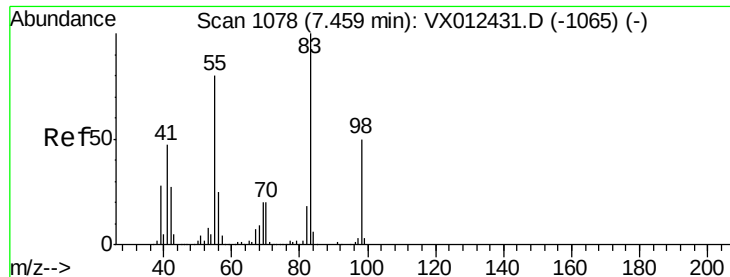

#39
Methylcyclohexane
Concen: 4.516 ug/l
RT: 7.21 min Scan# 1037
Delta R.T. -0.25 min
Lab File: VX012459.D
Acq: 18 Sep 2019 02:07




Instrument :
MSVOA_X
ClientSampleId :
RE122D2-20190909


Tgt Ion: 83 Resp: 6732
Ion Ratio Lower Upper
83 100
55 0.0 64.4 96.6#
98 202.4 40.1 60.1#

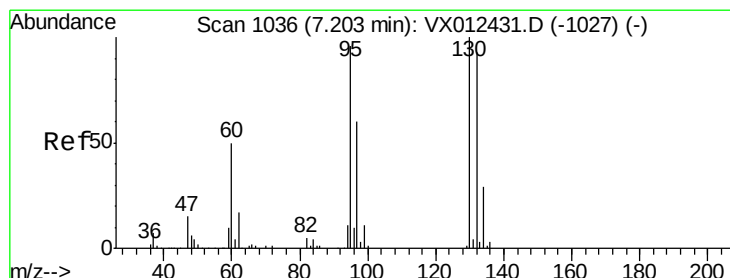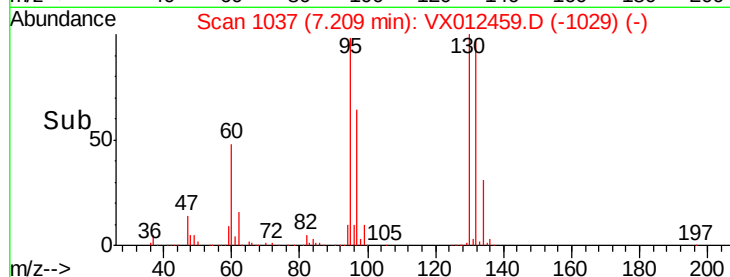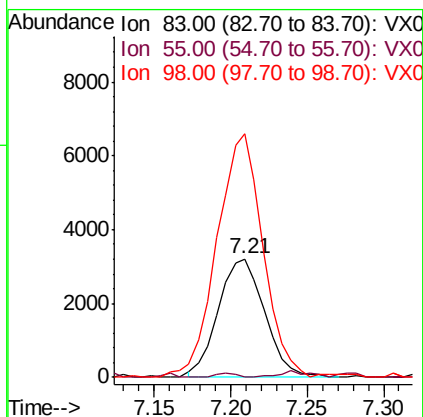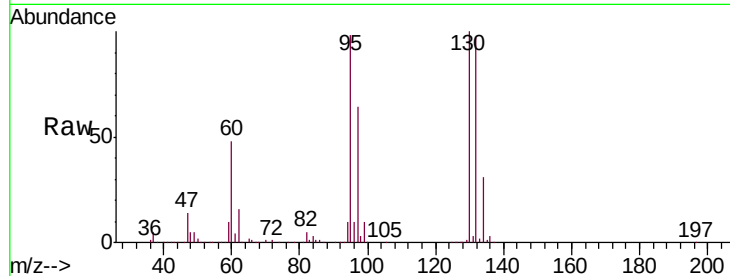

#44
Trichloroethene
Concen: 404.265 ug/l
RT: 7.21 min Scan# 1037
Delta R.T. 0.01 min
Lab File: VX012459.D
Acq: 18 Sep 2019 02:07

Tgt Ion:130 Resp: 518541
Ion Ratio Lower Upper
130 100
95 97.7 0.0 193.0

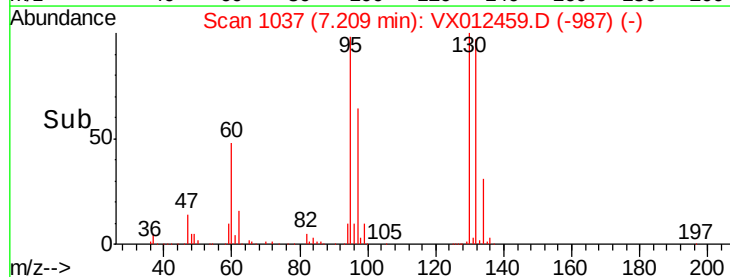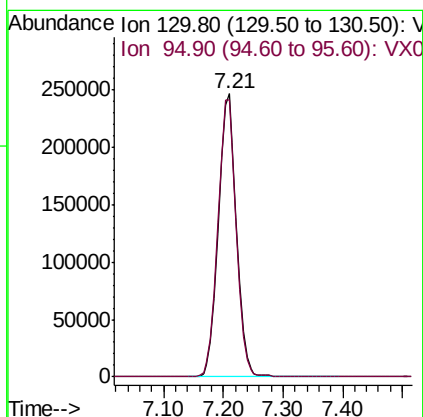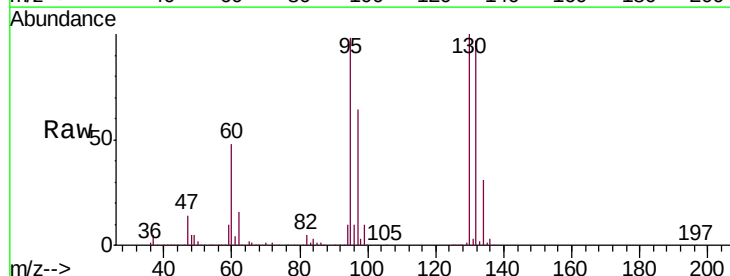







#49
1,4-Dioxane
Concen: 0.805 ug/l
RT: 7.56 min Scan# 1095
Delta R.T. -0.17 min
Lab File: VX012459.D
Acq: 18 Sep 2019 02:07

Instrument :
MSVOA_X
ClientSampleId :
RE122D2-20190909

Tgt Ion: 88 Resp: 39
Ion Ratio Lower Upper
88 100
43 0.0 29.4 44.0#
58 64.1 57.5 86.3




Abundance Ion 88.00 (87.70 to 88.70): VX0
Ion 43.00 (42.70 to 43.70): VX0
Ion 58.00 (57.70 to 58.70): VX0


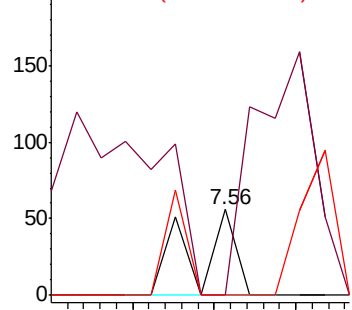



#50
Toluene-d8
Concen: 52.933 ug/l
RT: 8.71 min Scan# 1283
Delta R.T. 0.00 min
Lab File: VX012459.D
Acq: 18 Sep 2019 02:07

Tgt Ion: 98 Resp: 299204
Ion Ratio Lower Upper
98 100
100 66.3 53.4 80.2



Abundance Ion 98.00 (97.70 to 98.70): VX0
Ion 100.00 (99.70 to 100.70): VX0

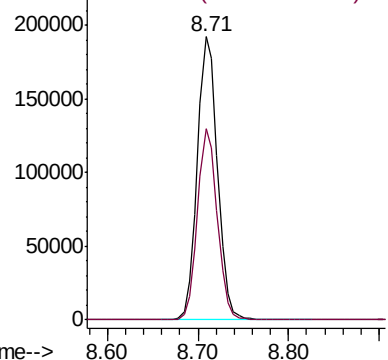


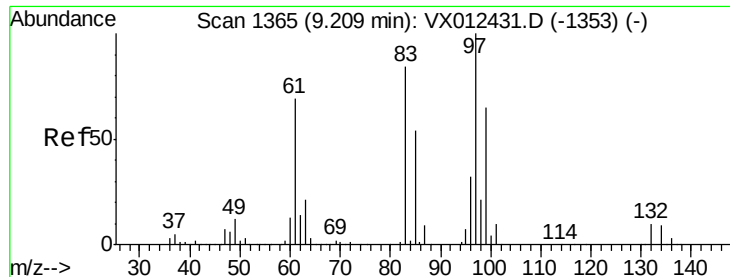




#55
 1,1,2-Trichloroethane
 Concen: 0.216 ug/l
 RT: 9.21 min Scan# 1365
 Delta R.T. 0.00 min
 Lab File: VX012459.D
 Acq: 18 Sep 2019 02:07

Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D2-20190909

Tgt Ion: 97 Resp: 350
 Ion Ratio Lower Upper
 97 100
 83 71.3 67.4 101.2
 85 42.1 43.5 65.3#
 99 64.4 51.8 77.8

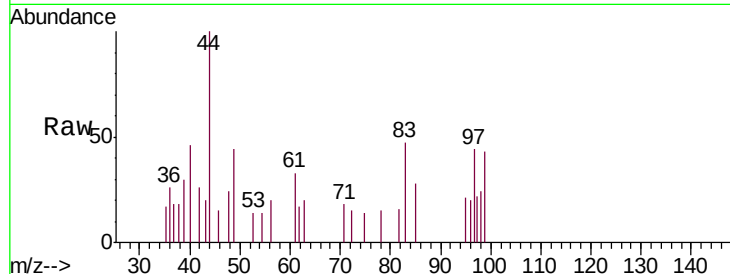


Abundance Ion 96.90 (96.60 to 97.60): VX0
 Ion 82.90 (82.60 to 83.60): VX0
 Ion 84.90 (84.60 to 85.60): VX0
 Ion 98.90 (98.60 to 99.60): VX0

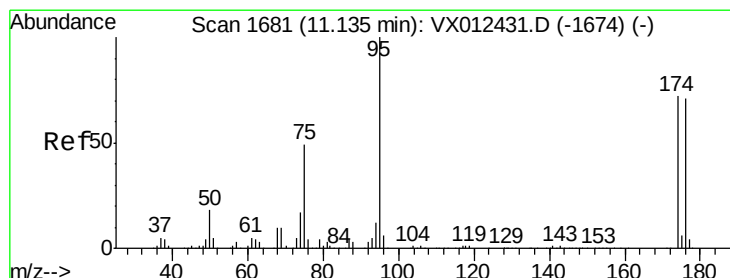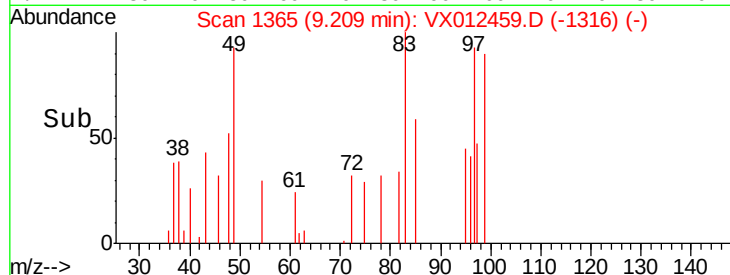
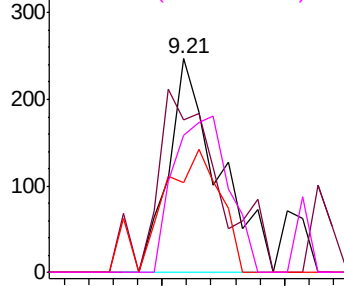



#62
 4-Bromofluorobenzene
 Concen: 47.931 ug/l
 RT: 11.14 min Scan# 1681
 Delta R.T. 0.00 min
 Lab File: VX012459.D
 Acq: 18 Sep 2019 02:07

Tgt Ion: 95 Resp: 112492
 Ion Ratio Lower Upper
 95 100
 174 70.0 0.0 140.0
 176 67.8 0.0 135.4

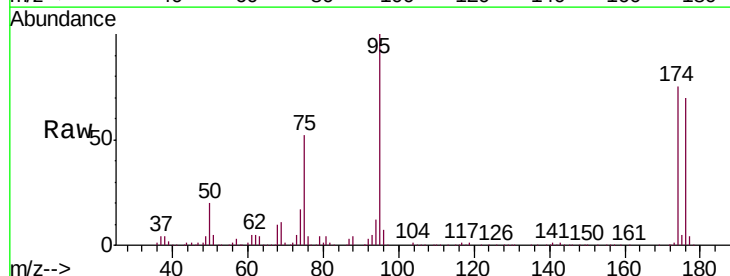

Abundance Ion 94.90 (94.60 to 95.60): VX0
 Ion 173.80 (173.50 to 174.50): V
 Ion 175.80 (175.50 to 176.50): V



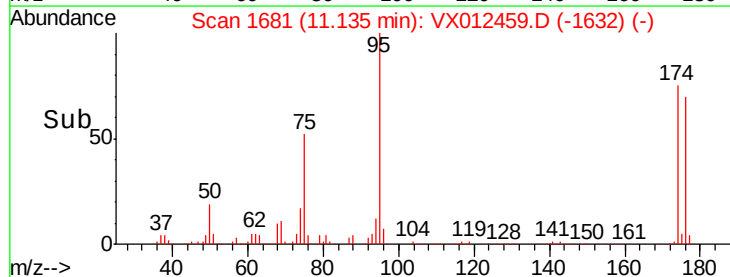
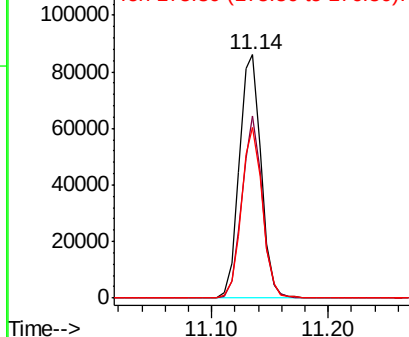




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1513
Delta R.T. 0.00 min
Lab File: VX012459.D
Acq: 18 Sep 2019 02:07




Instrument :
MSVOA_X
ClientSampleId :
RE122D2-20190909


Tgt Ion:117 Resp: 220035
Ion Ratio Lower Upper
117 100
82 58.7 45.9 68.9
119 32.8 25.3 37.9

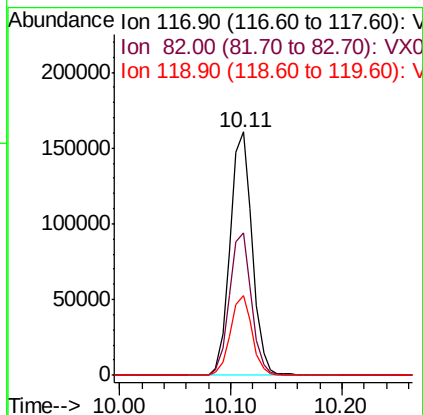

#64
Tetrachloroethene
Concen: 0.288 ug/l
RT: 9.33 min Scan# 1385
Delta R.T. 0.00 min
Lab File: VX012459.D
Acq: 18 Sep 2019 02:07

Tgt Ion:164 Resp: 290
Ion Ratio Lower Upper
164 100
166 152.5 107.8 161.6
129 112.3 86.2 129.2
131 58.3 80.4 120.6#



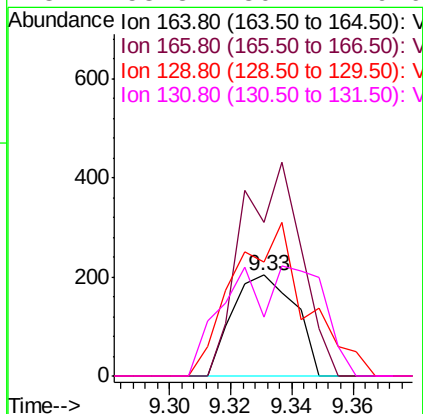





#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.07 min Scan# 1835
 Delta R.T. 0.00 min
 Lab File: VX012459.D
 Acq: 18 Sep 2019 02:07




Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D2-20190909


Tgt Ion: 152 Resp: 94771
 Ion Ratio Lower Upper
 152 100
 115 63.1 44.1 132.3
 150 157.8 0.0 343.8

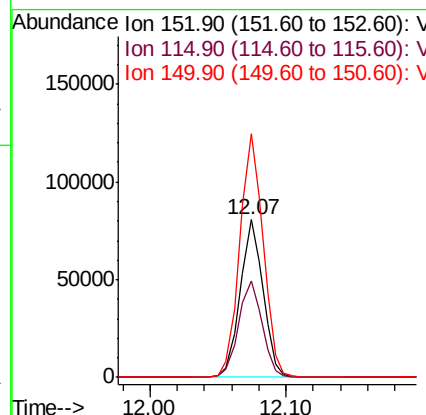

#76
 1,2,3-Trichloropropane
 Concen: 26.595 ug/l
 RT: 11.14 min Scan# 1681
 Delta R.T. -0.16 min
 Lab File: VX012459.D
 Acq: 18 Sep 2019 02:07

Tgt Ion: 75 Resp: 57896
 Ion Ratio Lower Upper
 75 100
 77 1.3 19.7 59.0#

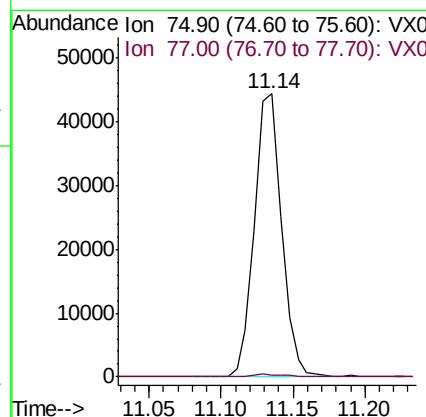

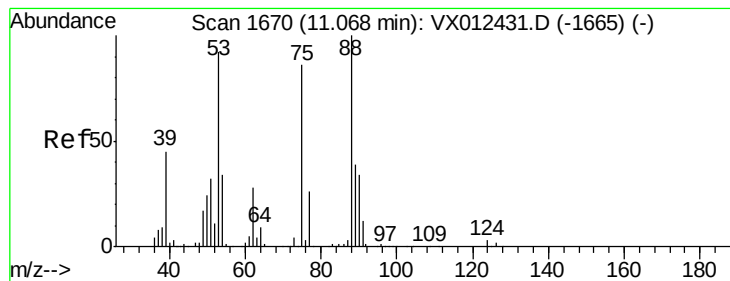

#81

trans-1,4-Dichloro-2-butene

Concen: 71.588 ug/l

RT: 11.14 min Scan# 1681

Delta R.T. 0.07 min

Lab File: VX012459.D

Acq: 18 Sep 2019 02:07

Instrument :

MSVOA_X

ClientSampleId :

RE122D2-20190909


Tgt Ion: 75 Resp: 57896

Ion Ratio Lower Upper

75 100

53 0.2 83.6 125.4#

89 0.1 36.3 54.5#

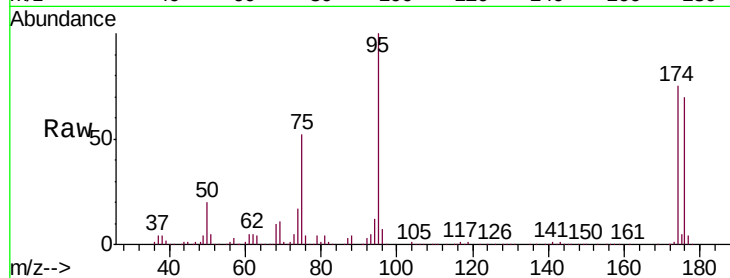

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

