



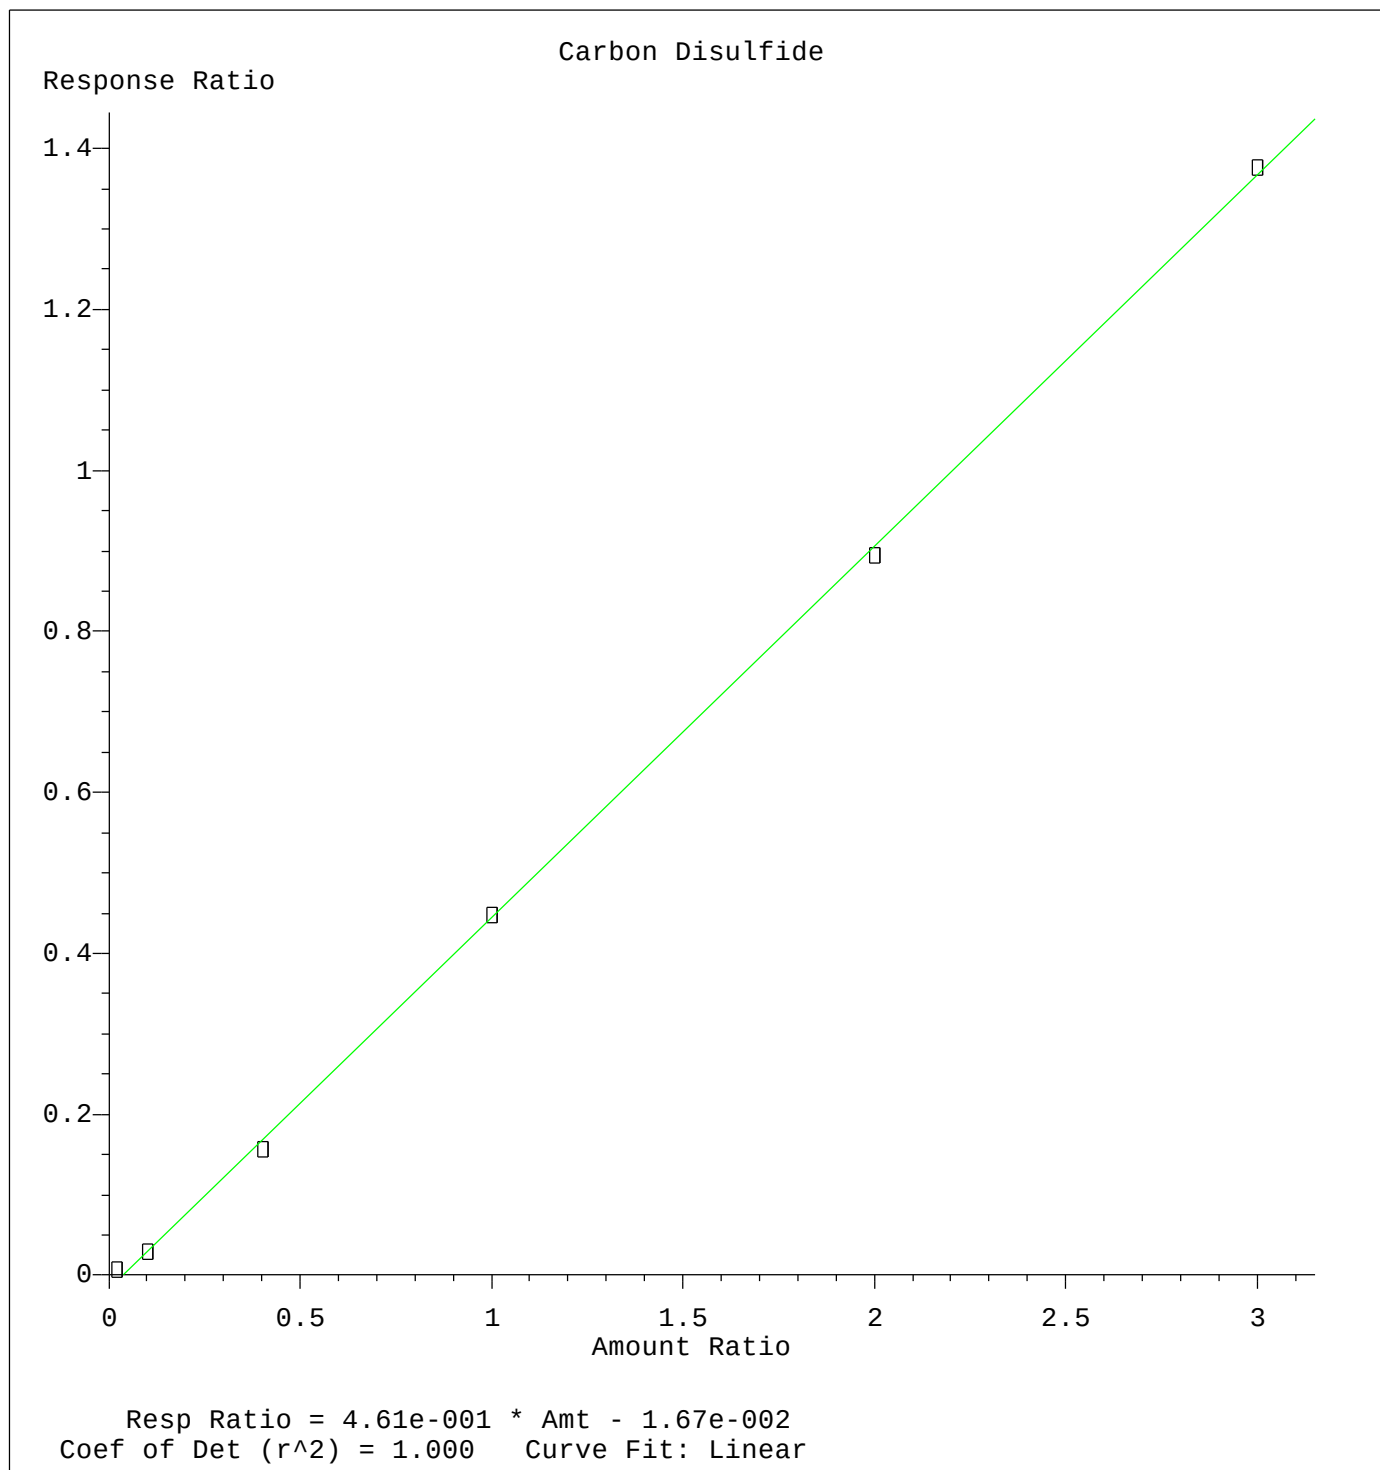


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091719W.M
Calibration Table Last Updated: Tue Sep 17 15:27:10 2019

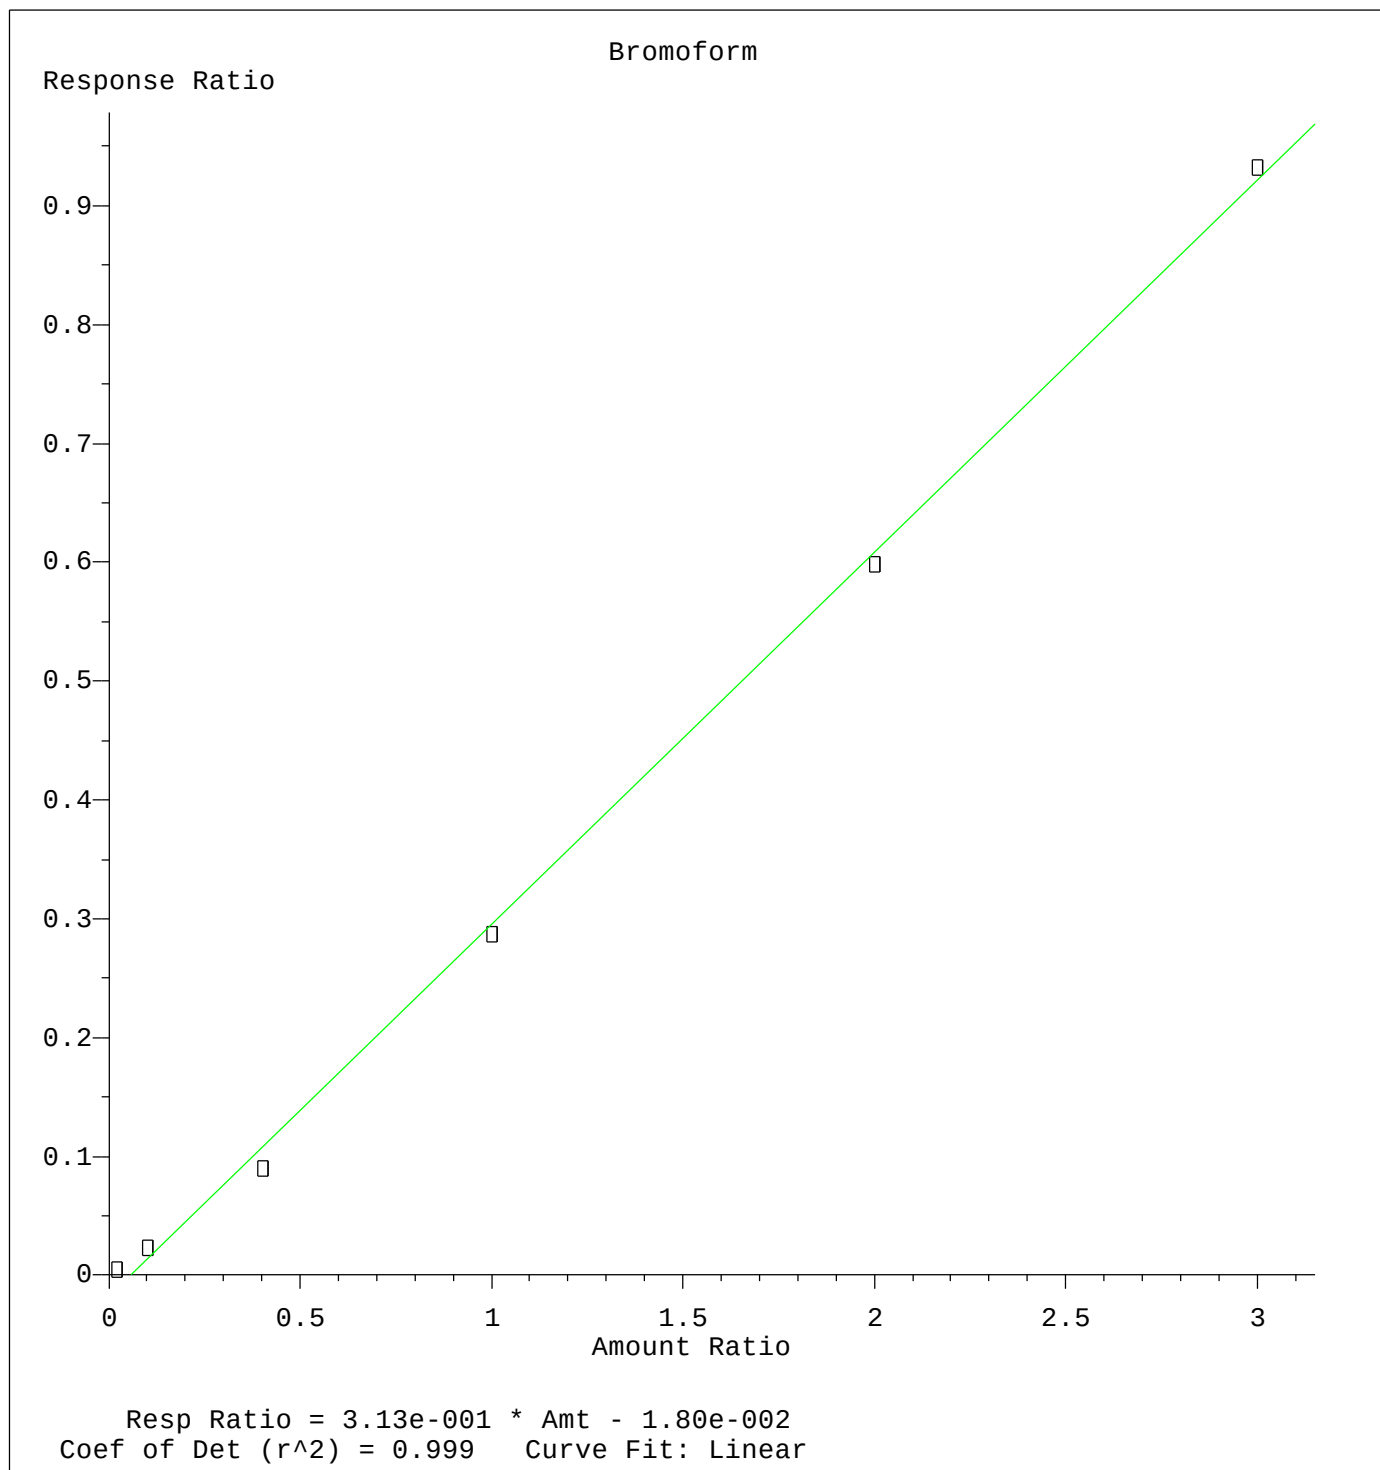

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091719W.M
Calibration Table Last Updated: Tue Sep 17 15:27:10 2019

trans-1,4-Dichloro-2-butene

Response Ratio

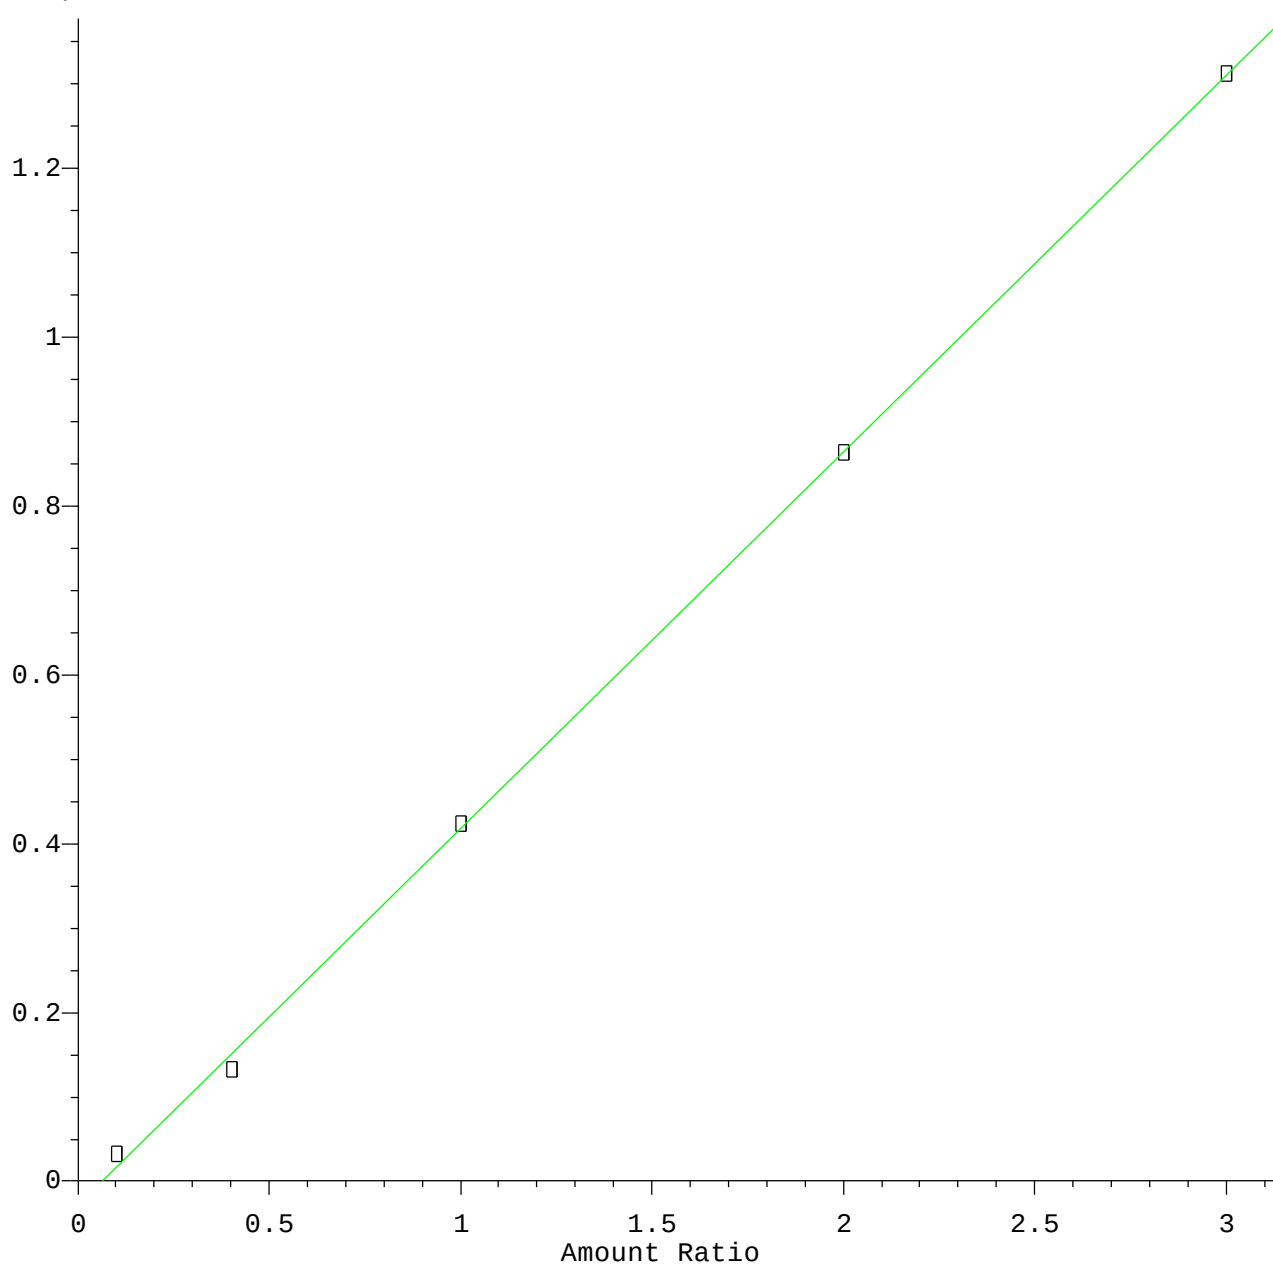


Resp Ratio = $4.46 \times 10^{-1} \times \text{Amt} - 2.76 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091719W.M
Calibration Table Last Updated: Tue Sep 17 15:27:10 2019


Dichlorodifluoromethane

Response Ratio

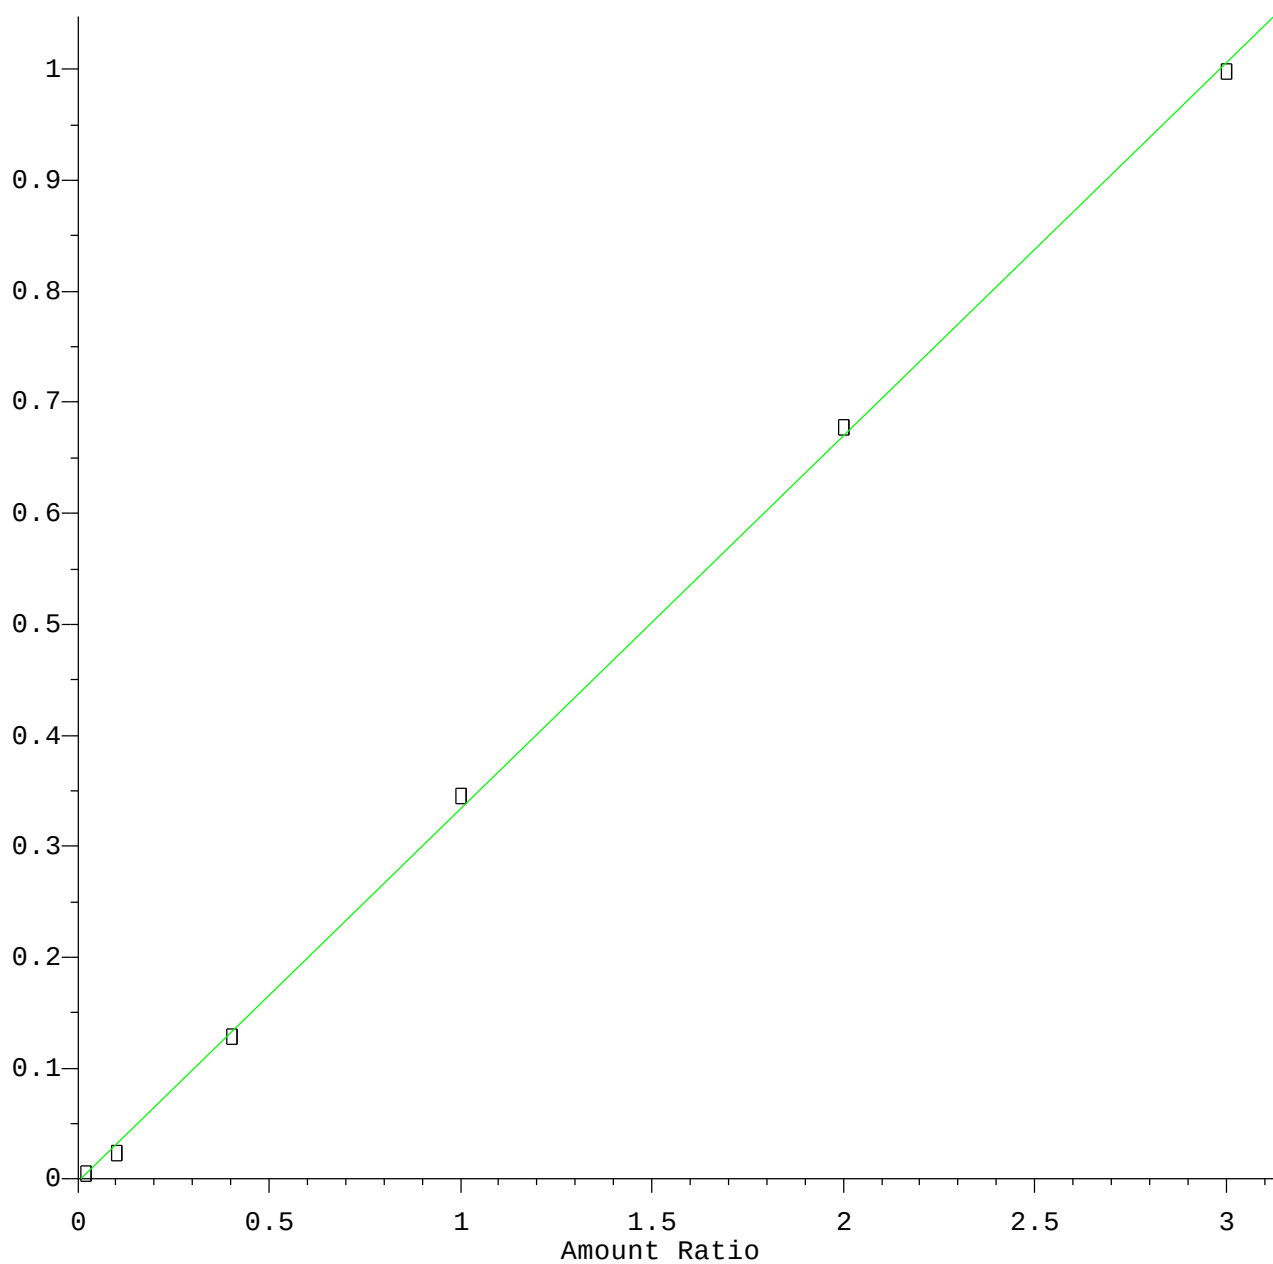


Resp Ratio = $3.36 \times 10^{-1} \times \text{Amt} - 2.63 \times 10^{-3}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091719W.M
Calibration Table Last Updated: Tue Sep 17 15:27:10 2019

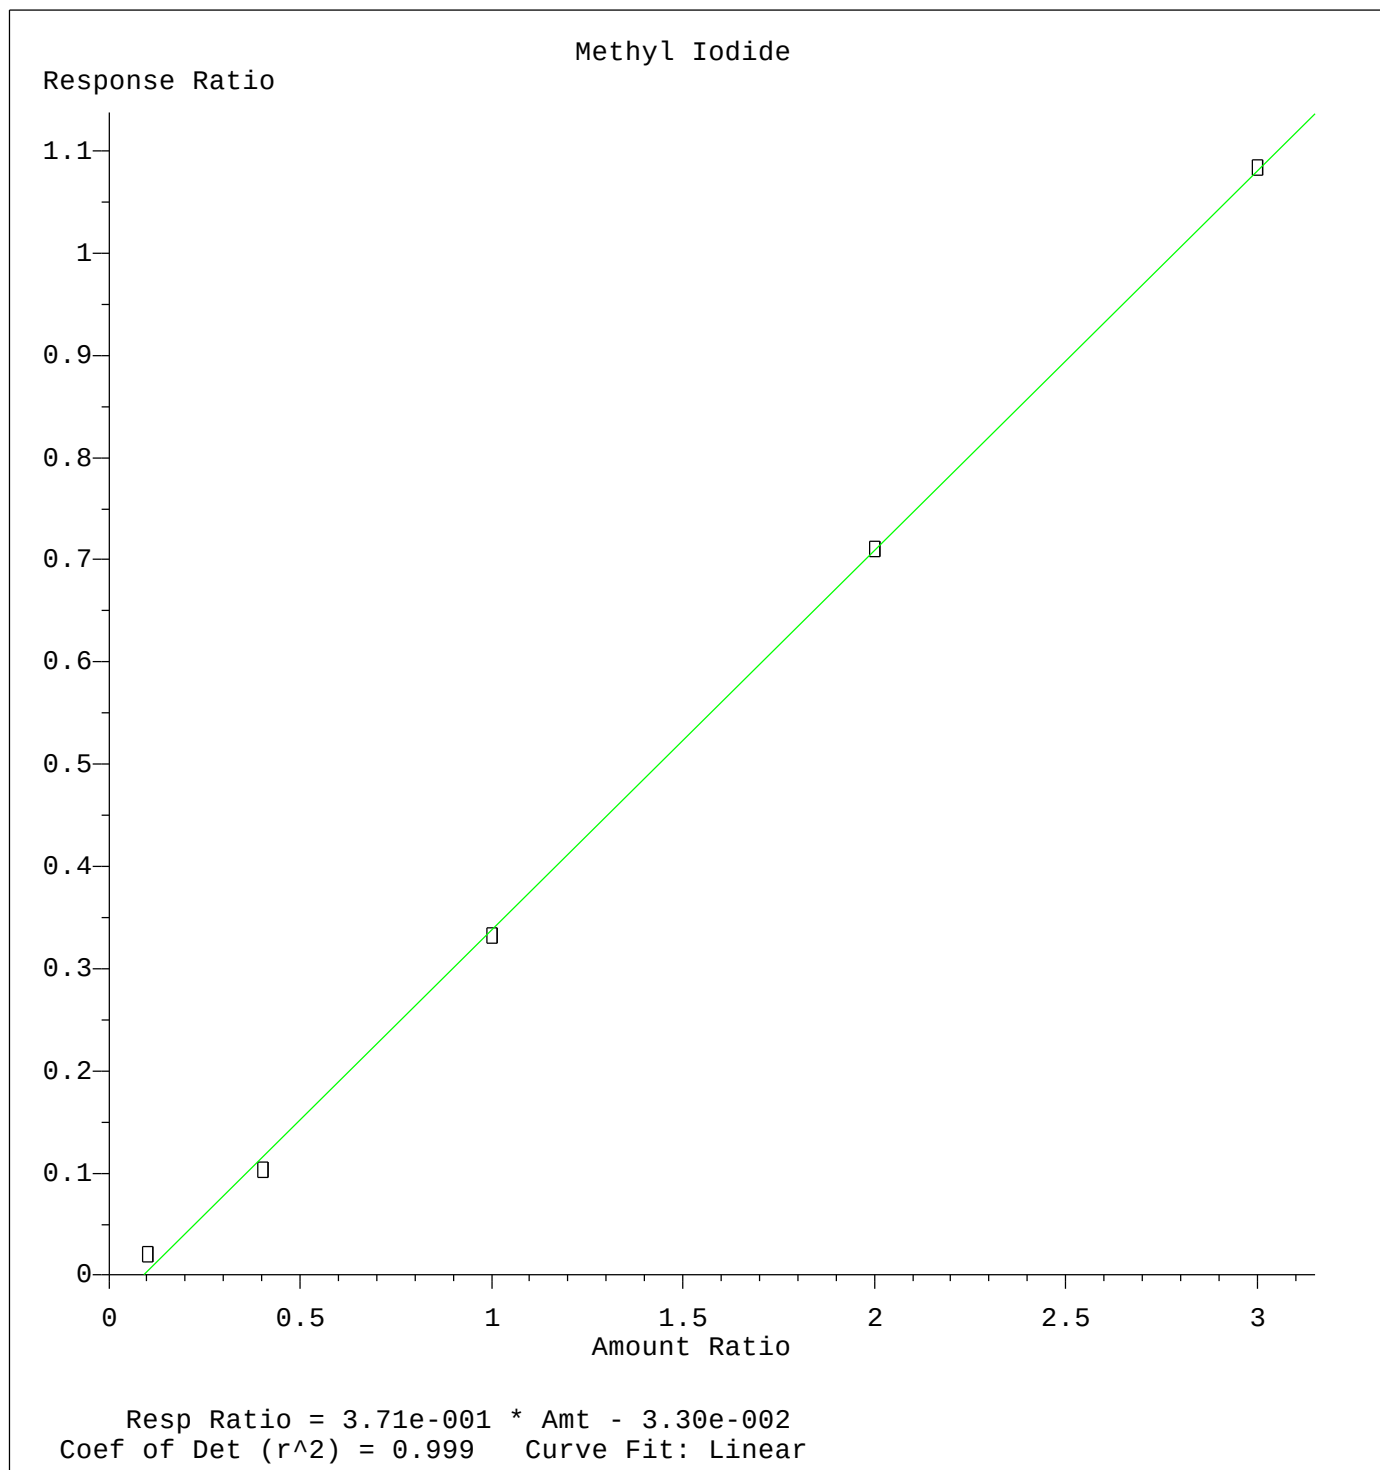


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091719W.M
Calibration Table Last Updated: Tue Sep 17 15:27:10 2019

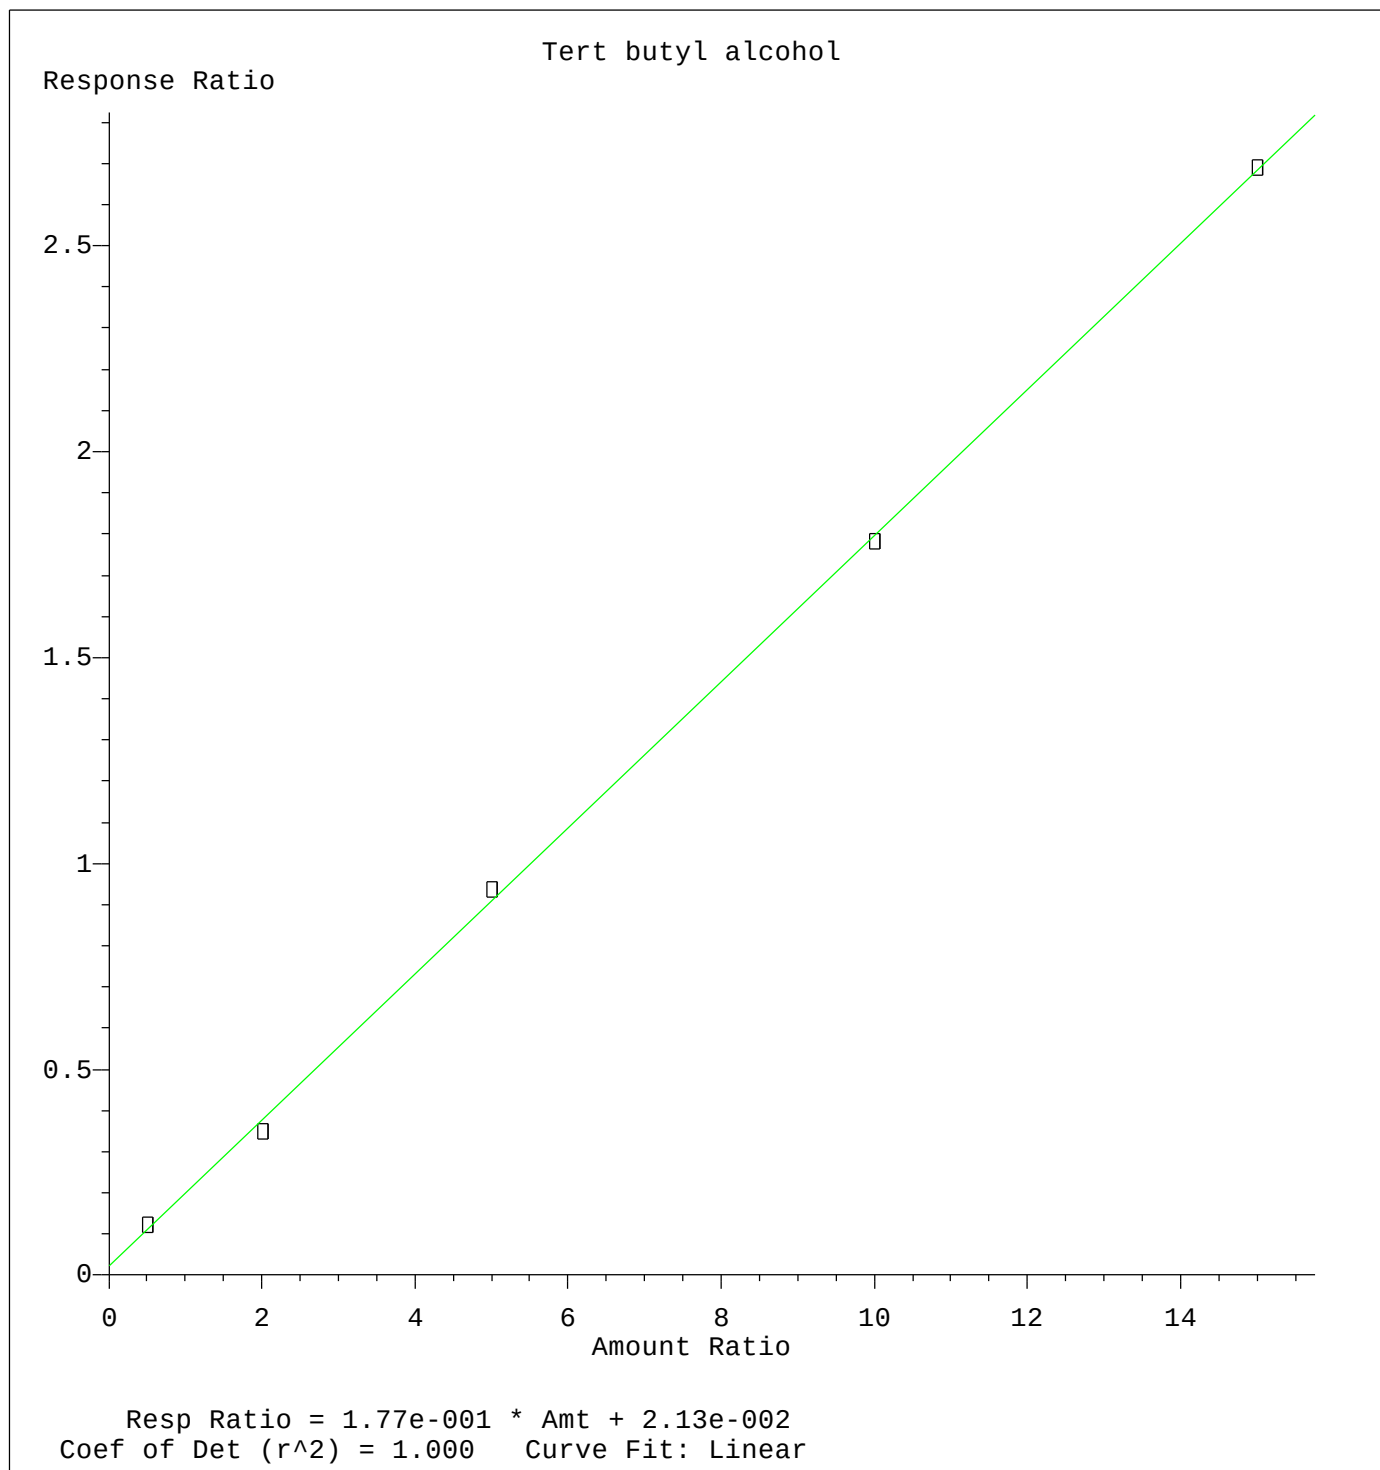

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091719W.M
Calibration Table Last Updated: Tue Sep 17 15:27:10 2019

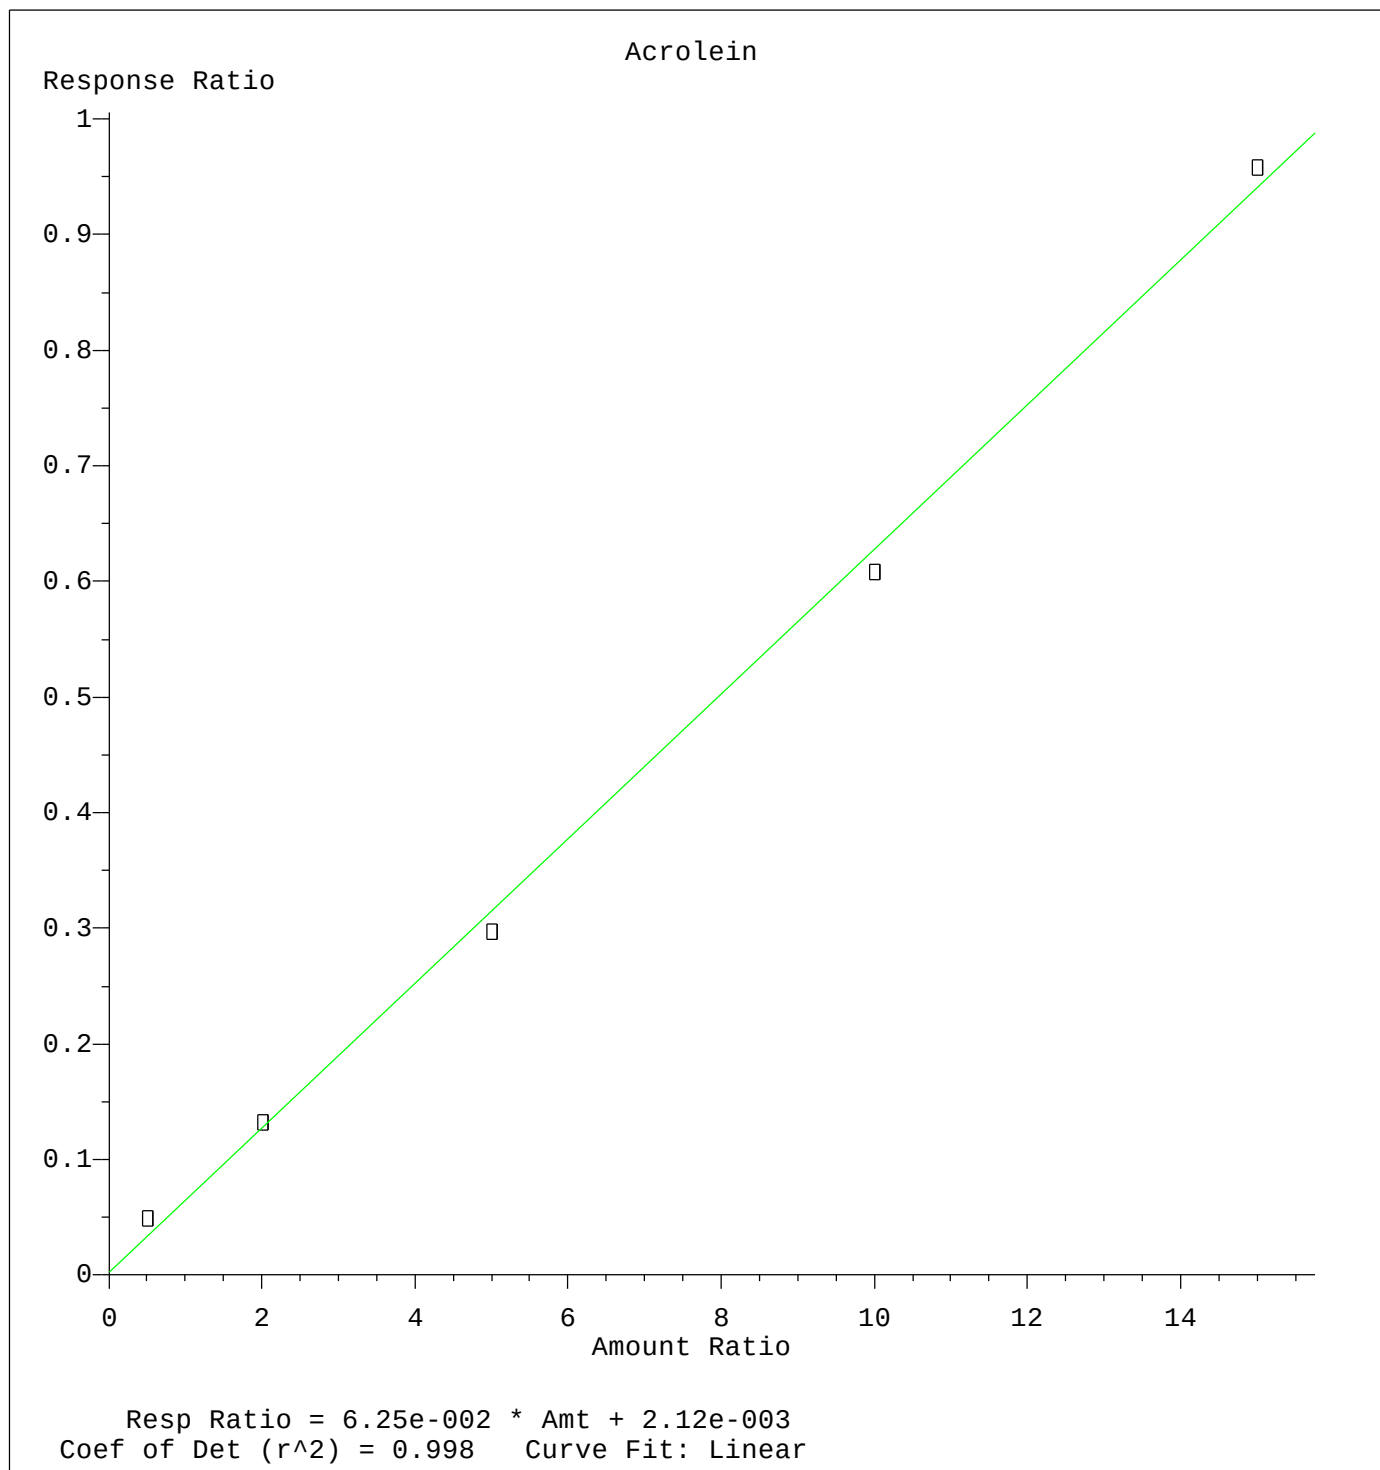

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091719W.M
Calibration Table Last Updated: Tue Sep 17 15:27:10 2019

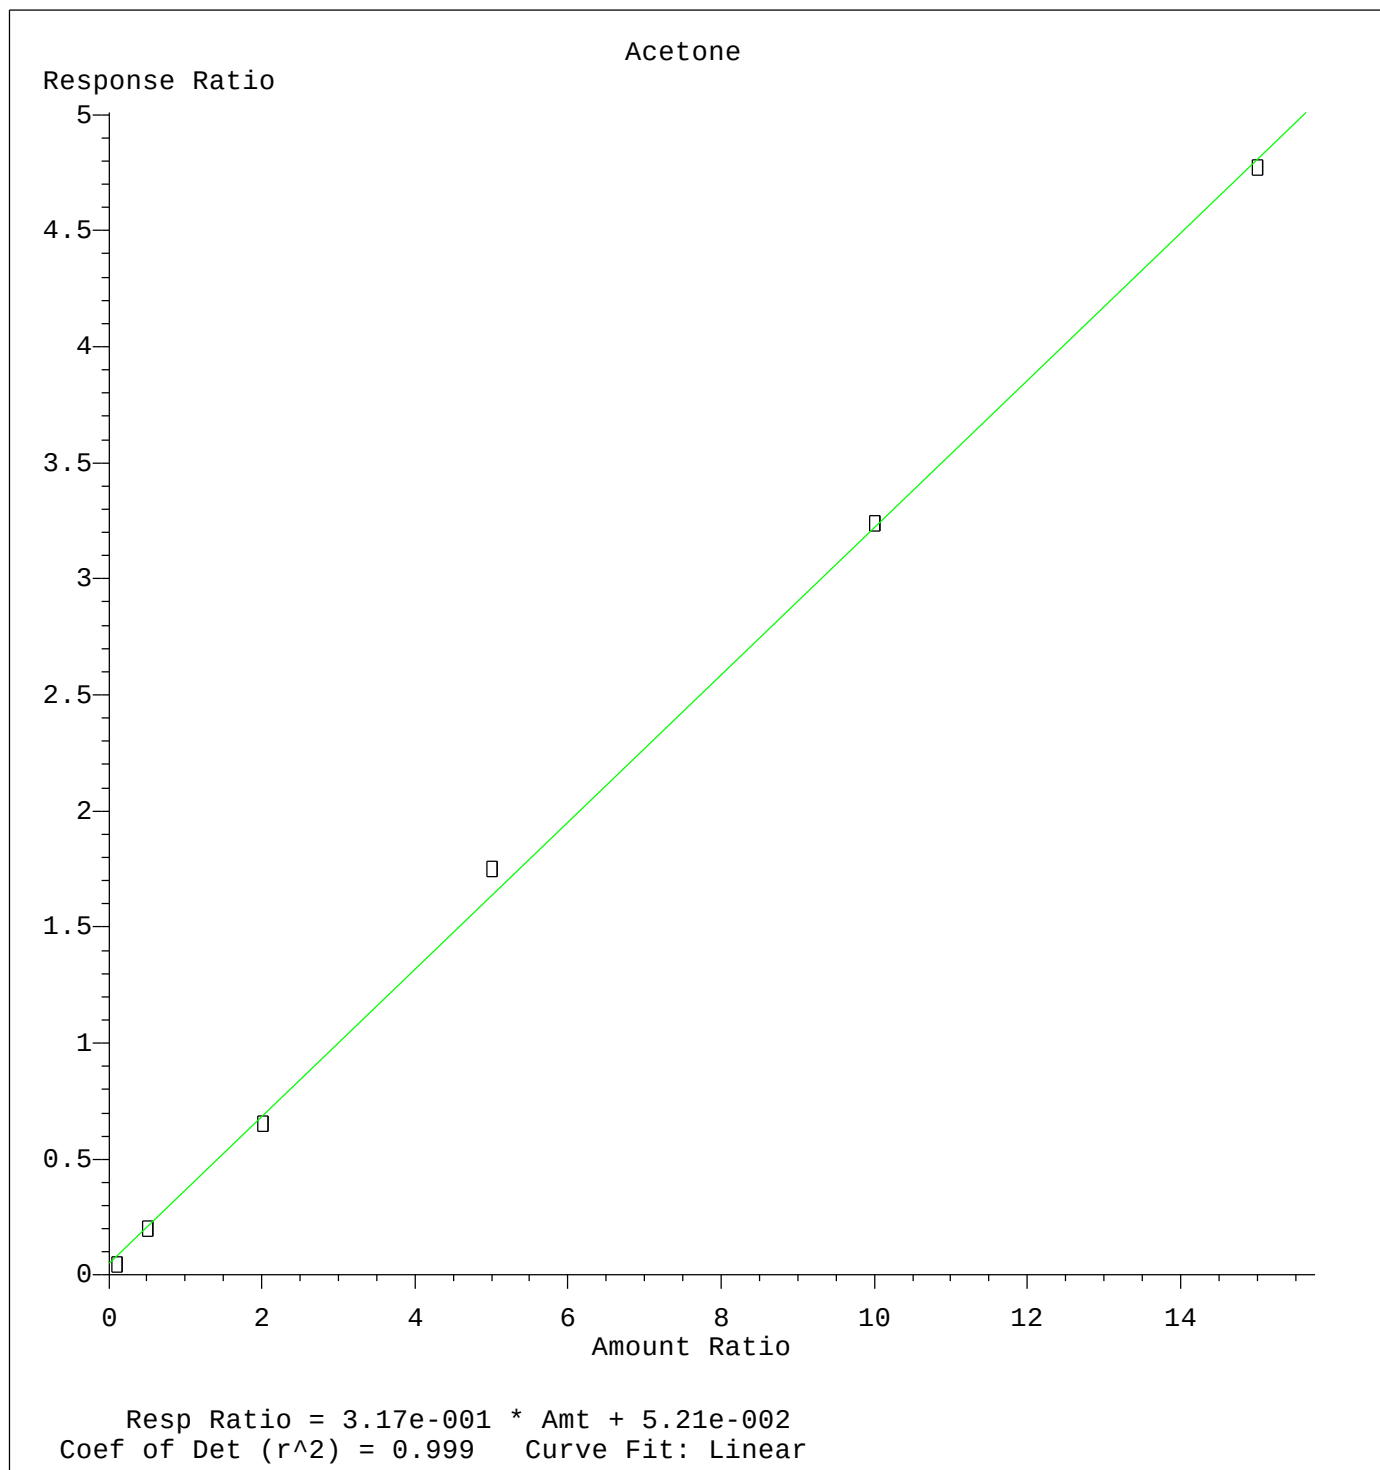

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091719W.M
Calibration Table Last Updated: Tue Sep 17 15:27:10 2019