


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX091719\
Data File : VX012435.D
Acq On : 17 Sep 2019 15:50
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091719W.M
Title : SW846 8260
Last Update : Tue Sep 17 15:27:10 2019

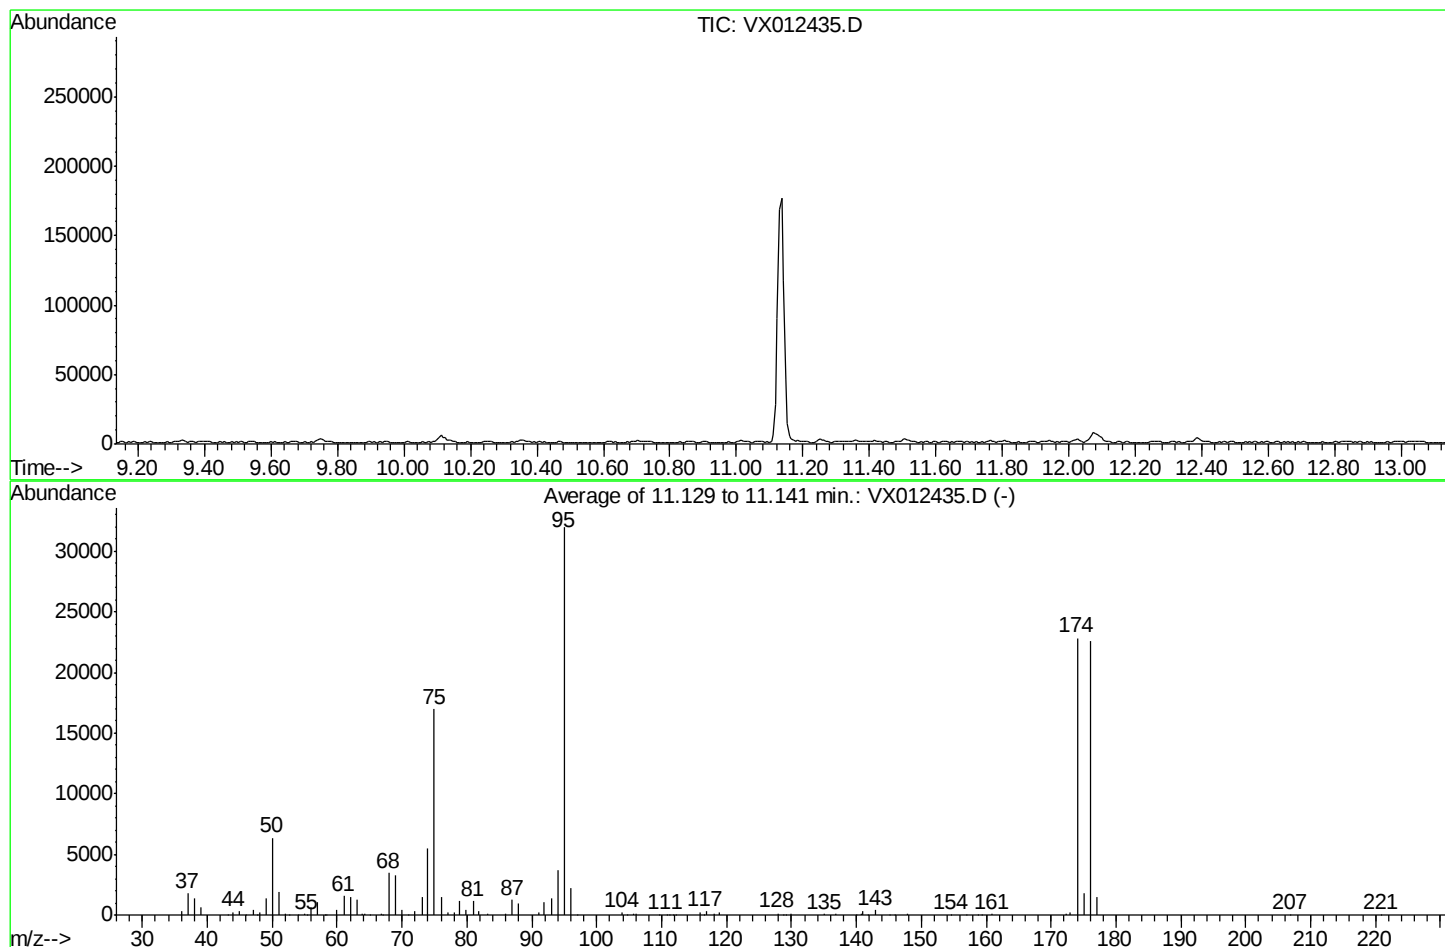

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1674

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	6391	PASS
75	95	30	60	53.0	16953	PASS
95	95	100	100	100.0	31978	PASS
96	95	5	9	7.1	2265	PASS
173	174	0.00	2	0.9	205	PASS
174	95	50	100	71.4	22834	PASS
175	174	5	9	7.9	1794	PASS
176	174	95	101	98.9	22589	PASS
177	176	5	9	6.7	1519	PASS