


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX091720\
 Data File : VX018456.D
 Acq On : 17 Sep 2020 09:20
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091720W.M
 Title : SW846 8260
 Last Update : Thu Sep 17 12:17:36 2020

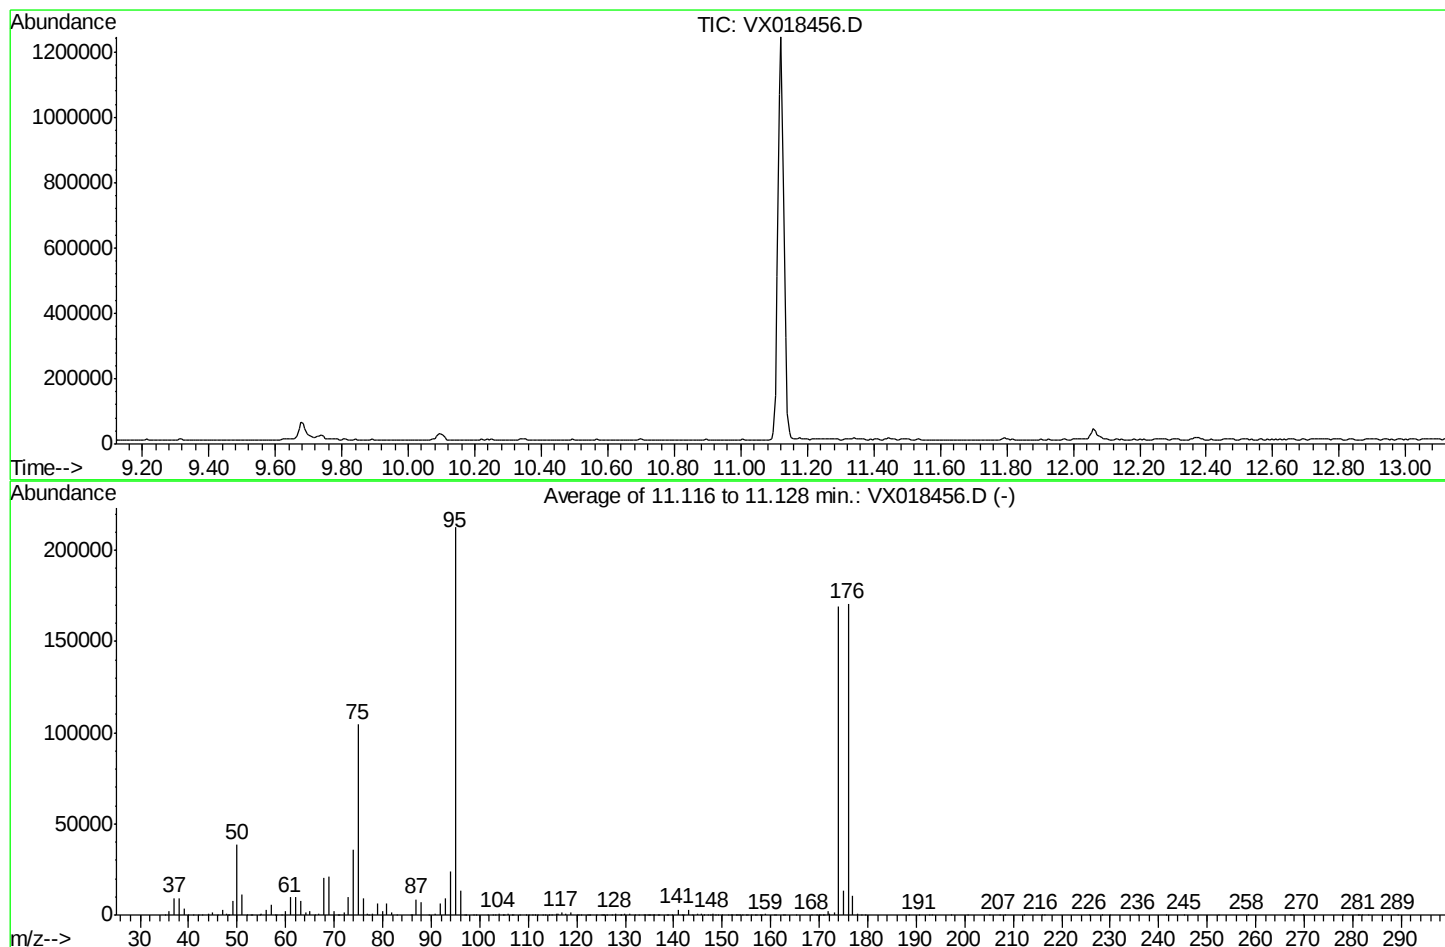

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	38343	PASS
75	95	30	60	49.1	104326	PASS
95	95	100	100	100.0	212586	PASS
96	95	5	9	6.3	13379	PASS
173	174	0.00	2	1.0	1613	PASS
174	95	50	100	79.6	169280	PASS
175	174	5	9	7.9	13402	PASS
176	174	95	101	101.0	170922	PASS
177	176	5	9	6.2	10638	PASS