

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091721\
 Data File : VX024329.D
 Acq On : 18 Sep 2021 00:12
 Operator : JC/MD
 Sample : M3782-01 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE132D7-20210914DL

Quant Time: Sep 20 02:43:00 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 14 12:18:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	132513	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	229368	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	191717	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	74385	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	97454	51.574	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	103.140%
35) Dibromofluoromethane	5.397	113	76813	49.936	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.880%
50) Toluene-d8	8.653	98	232979	41.576	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	83.160%#
62) 4-Bromofluorobenzene	11.079	95	86386	39.612	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	79.220%#
Target Compounds						
						Qvalue
3) Chloromethane	1.295	50	463	0.348	ug/l	98
6) Chloroethane	1.685	64	155	2.140	ug/l	94
9) 1,1,2-Trichlorotrifluo...	2.331	101	3857	2.957	ug/l	92
10) Methyl Iodide	2.465	142	1667	0.924	ug/l #	89
11) Tert butyl alcohol	2.953	59	10032	4.416	ug/l #	73
12) 1,1-Dichloroethene	2.325	96	1248	1.021	ug/l	82
15) Acrylonitrile	3.081	53	243	0.314	ug/l #	82
16) Acetone	2.386	43	1616	2.006	ug/l	89
17) Carbon Disulfide	2.514	76	1444	0.472	ug/l #	92
20) Methylene Chloride	2.794	84	3535	2.285	ug/l #	83
21) trans-1,2-Dichloroethene	3.087	96	287	0.215	ug/l #	61
24) 1,1-Dichloroethane	3.623	63	540	0.211	ug/l #	81
25) 2-Butanone	4.593	43	700	0.590	ug/l #	45
26) 2,2-Dichloropropane	4.593	77	957	0.427	ug/l #	52
27) cis-1,2-Dichloroethene	4.507	96	655	0.424	ug/l	69
30) Chloroform	5.111	83	657	0.241	ug/l #	49
31) Cyclohexane	5.562	56	3057	1.383	ug/l #	24
38) Carbon Tetrachloride	5.690	117	520	0.219	ug/l #	72
44) Trichloroethene	7.135	130	252934	148.838	ug/l	100
60) Dibromochloromethane	9.531	129	20	1.736	ug/l #	11
64) Tetrachloroethene	9.281	164	571	0.384	ug/l #	75
76) 1,2,3-Trichloropropane	11.079	75	47128	27.554	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	47128	81.035	ug/l #	12
87) 1,3-Dichlorobenzene	11.976	146	525	0.211	ug/l	88
88) 1,4-Dichlorobenzene	11.976	146	525	0.206	ug/l	89
89) n-Butylbenzene	12.335	91	914	0.223	ug/l	94
93) 1,2,4-Trichlorobenzene	13.597	180	392	0.272	ug/l	92
94) Hexachlorobutadiene	13.725	225	265	0.368	ug/l #	60
95) Naphthalene	13.780	128	779	1.430	ug/l #	80
96) 1,2,3-Trichlorobenzene	13.969	180	346	0.238	ug/l	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091721\
 Data File : VX024329.D
 Acq On : 18 Sep 2021 00:12
 Operator : JC/MD
 Sample : M3782-01 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE132D7-20210914DL

Quant Time: Sep 20 02:43:00 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 14 12:18:04 2021
 Response via : Initial Calibration




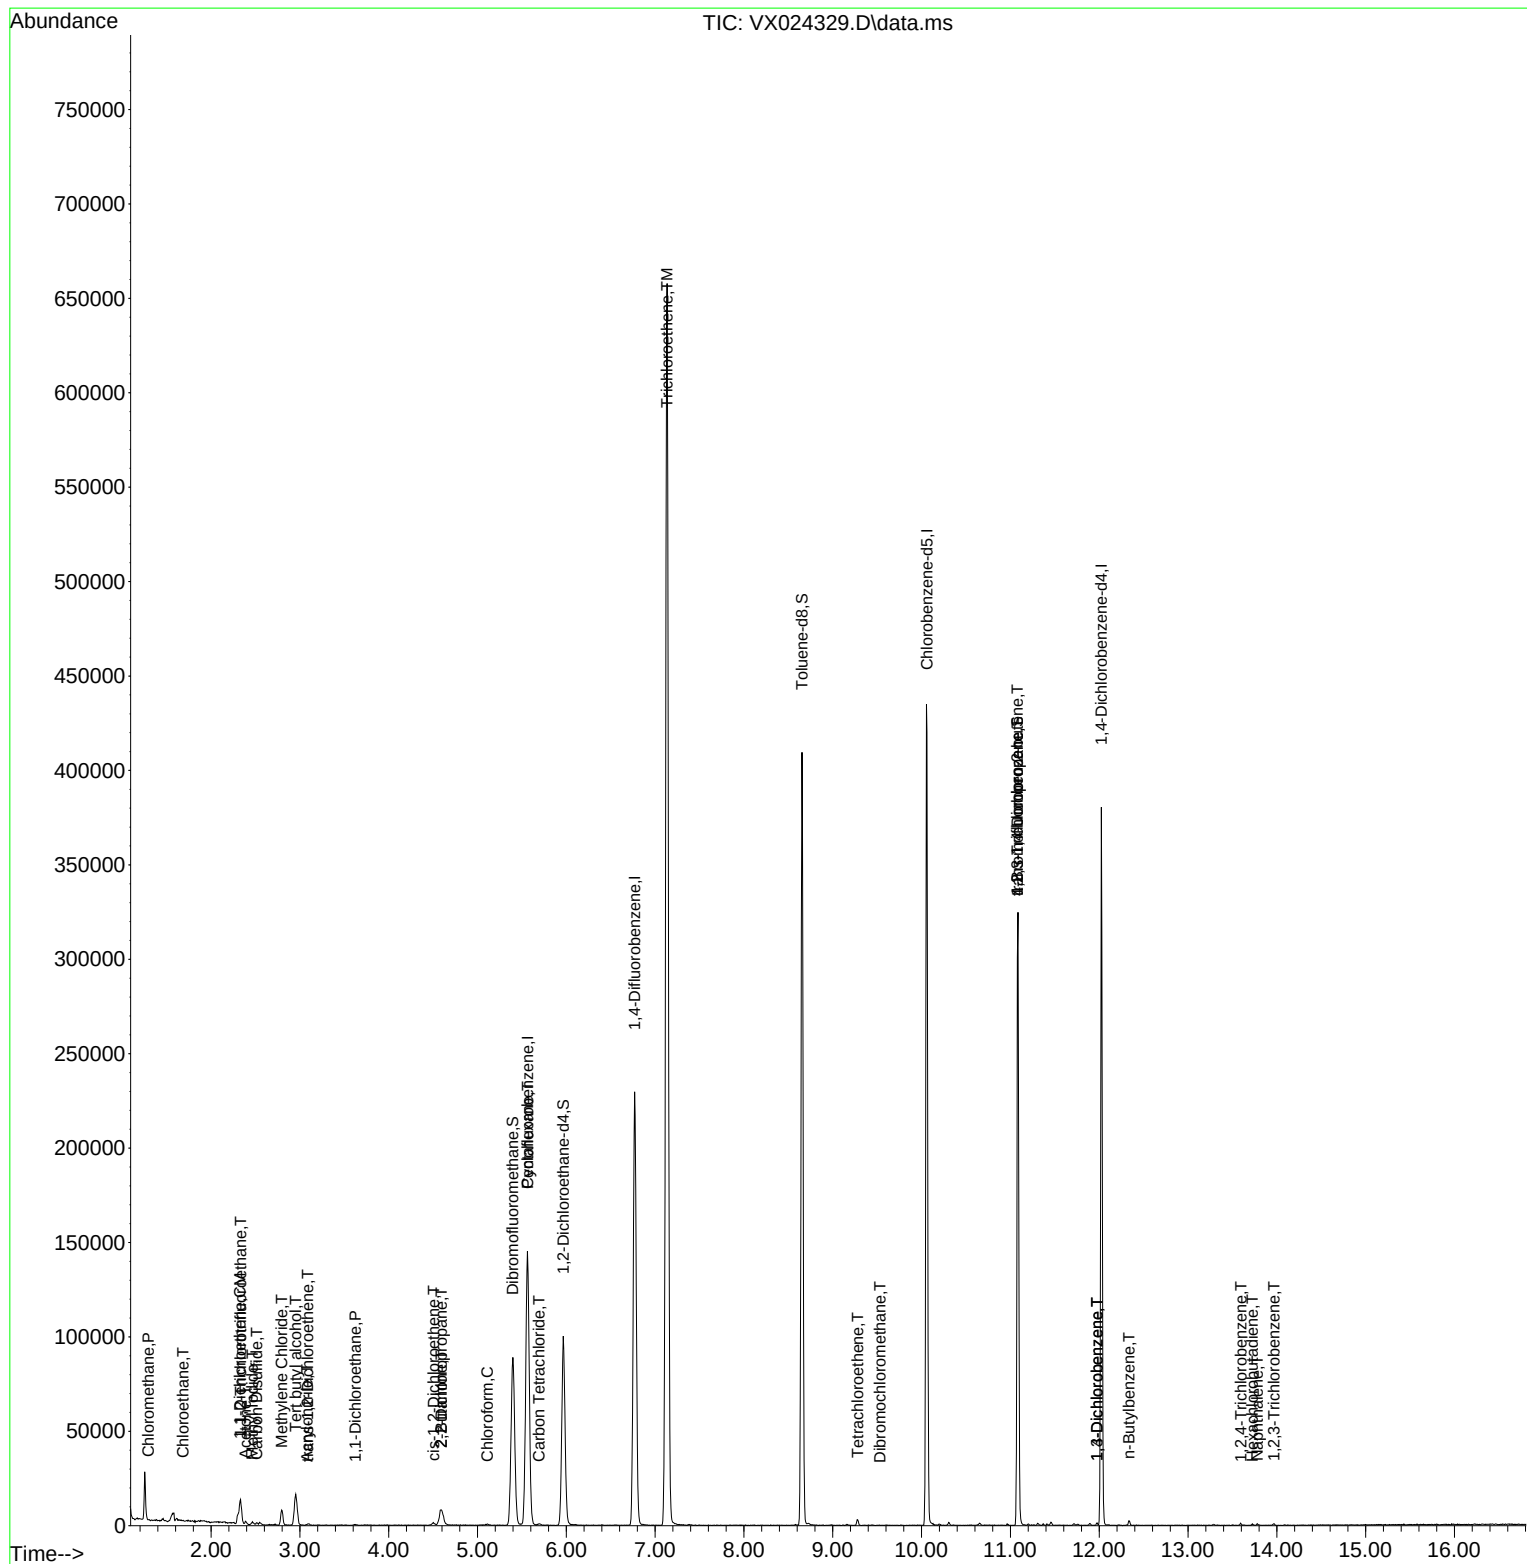


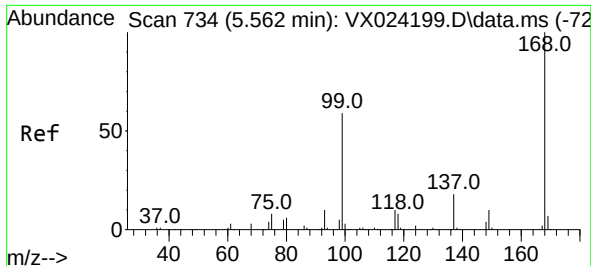

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.000 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914DL


Tgt Ion:168 Resp: 132513
Ion Ratio Lower Upper
168 100
99 62.3 45.8 68.6

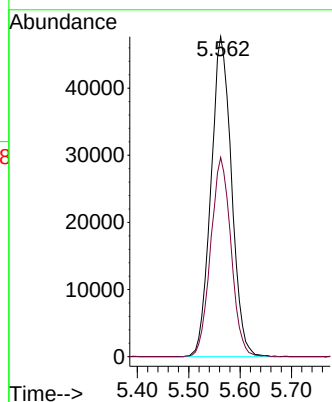

#3
Chloromethane
Concen: 0.348 ug/l
RT: 1.295 min Scan# 34
Delta R.T. -0.000 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Tgt Ion: 50 Resp: 463
Ion Ratio Lower Upper
50 100
52 31.9 26.4 39.6


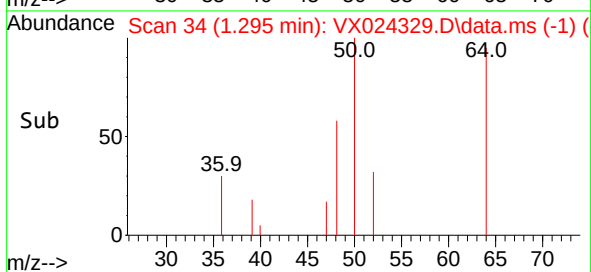
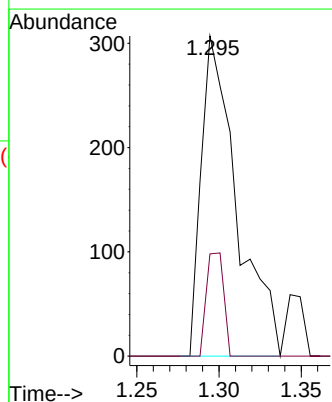
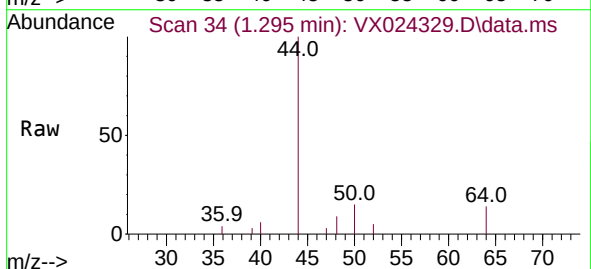


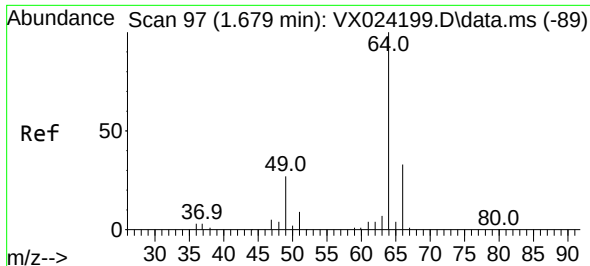

#6
Chloroethane
Concen: 2.140 ug/l
RT: 1.685 min Scan# 98
Delta R.T. 0.006 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914DL


Tgt Ion: 64 Resp: 155
Ion Ratio Lower Upper
64 100
66 28.5 25.4 38.0

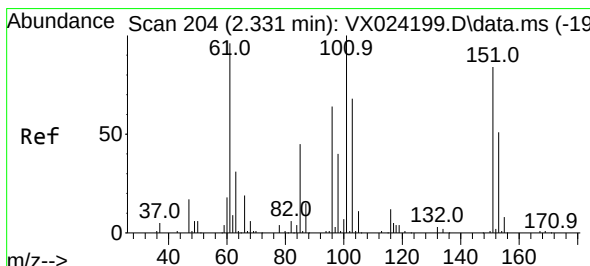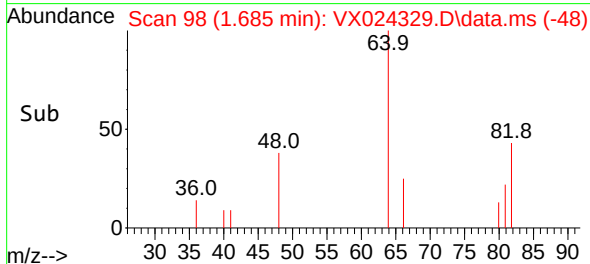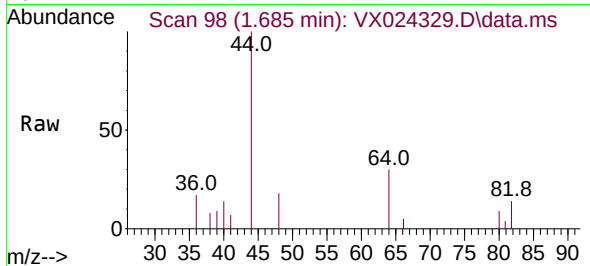

#9
1,1,2-Trichlorotrifluoroethane
Concen: 2.957 ug/l
RT: 2.331 min Scan# 204
Delta R.T. -0.000 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Tgt Ion: 101 Resp: 3857
Ion Ratio Lower Upper
101 100
85 47.2 34.9 52.3
151 84.7 61.4 92.2


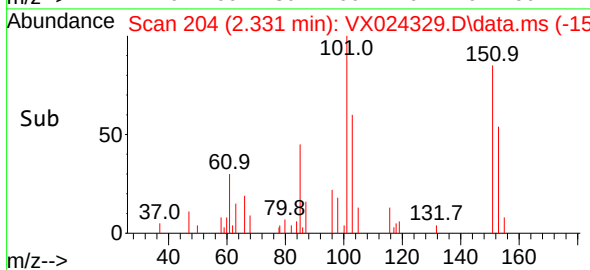

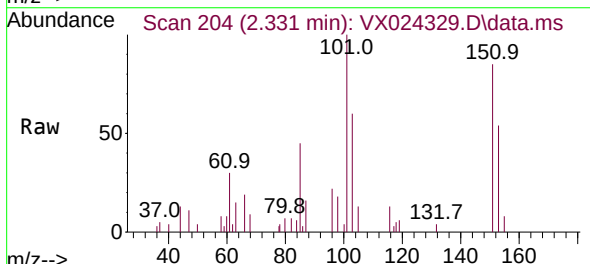


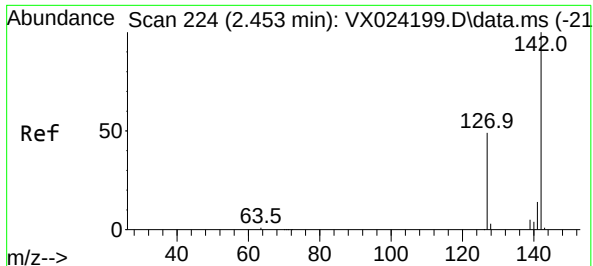

#10
Methyl Iodide
Concen: 0.924 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.012 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914DL


Tgt Ion:142 Resp: 1667
Ion Ratio Lower Upper
142 100
127 50.4 33.3 49.9#
141 15.5 11.4 17.0

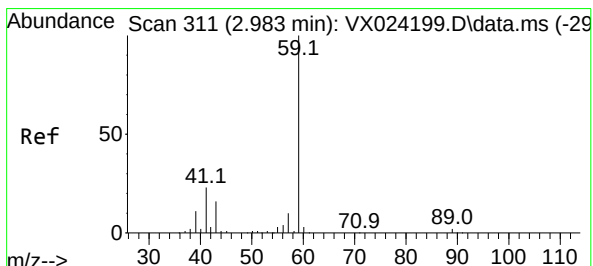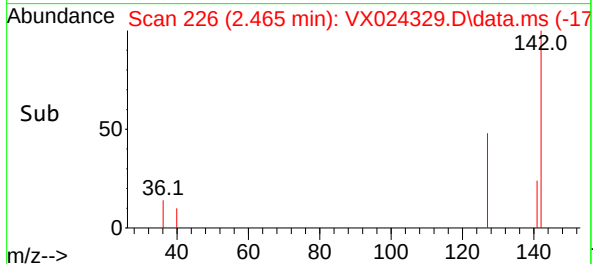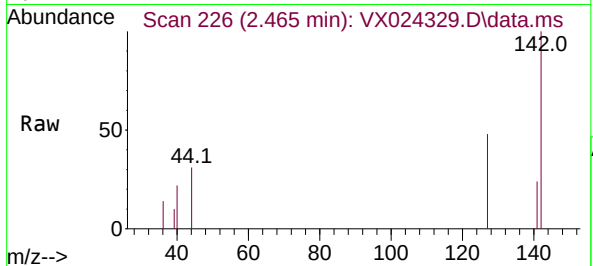

#11
Tert butyl alcohol
Concen: 4.416 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.030 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Tgt Ion: 59 Resp: 10032
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#




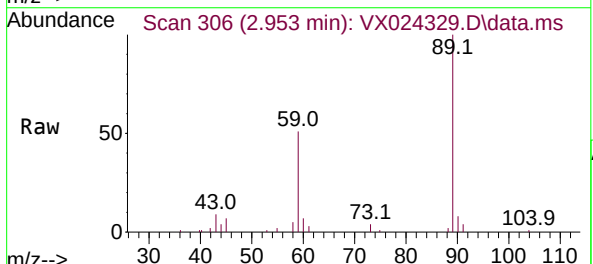




#12
1,1-Dichloroethene
Concen: 1.021 ug/l
RT: 2.325 min Scan# 203
Delta R.T. 0.006 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914DL


Tgt Ion:	96	Resp:	1248
Ion	Ratio	Lower	Upper
96	100		
61	182.1	124.6	187.0
98	73.1	50.6	76.0

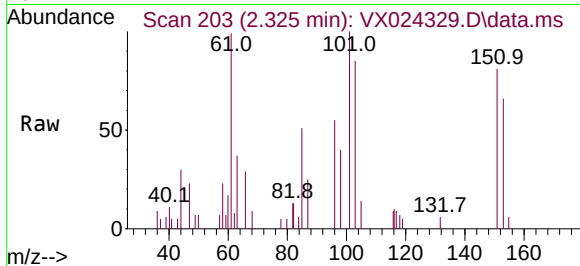

#15
Acrylonitrile
Concen: 0.314 ug/l
RT: 3.081 min Scan# 327
Delta R.T. 0.006 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Tgt Ion:	53	Resp:	243
Ion	Ratio	Lower	Upper
53	100		
52	81.9	65.3	97.9
51	0.0	28.2	42.2#


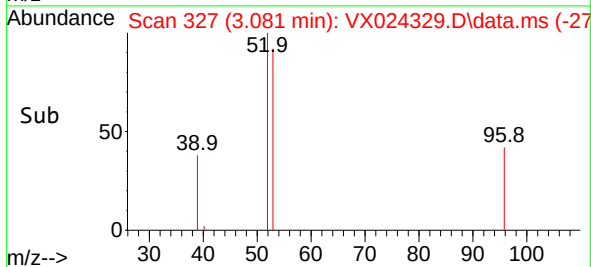

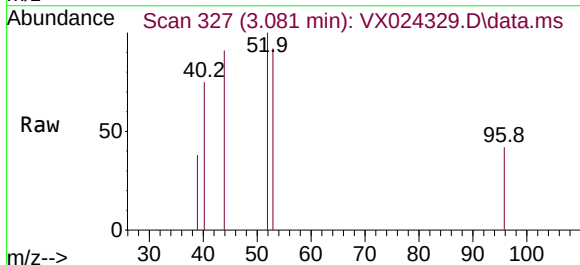




#16
Acetone
Concen: 2.006 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914DL


Tgt Ion: 43 Resp: 1616
Ion Ratio Lower Upper
43 100
58 28.2 27.8 41.8

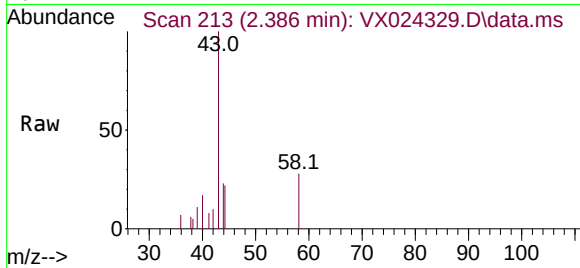

#17
Carbon Disulfide
Concen: 0.472 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Tgt Ion: 76 Resp: 1444
Ion Ratio Lower Upper
76 100
78 11.9 7.2 10.8#

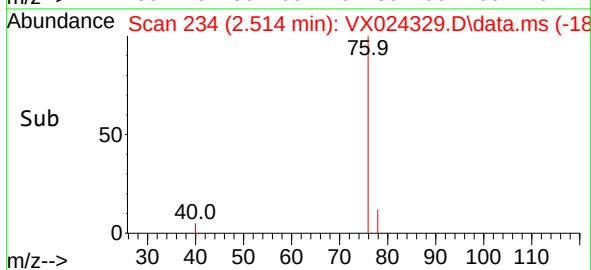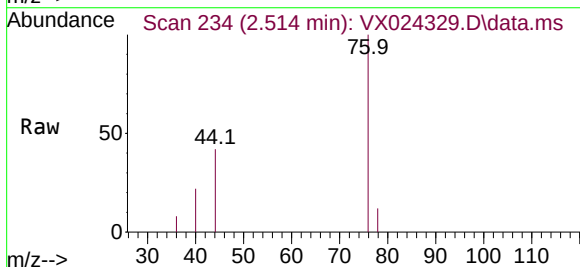

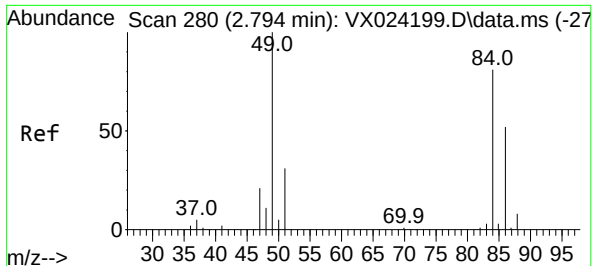

#20

Methylene Chloride

Concen: 2.285 ug/l

RT: 2.794 min Scan# 280

Delta R.T. 0.000 min

Lab File: VX024329.D

Acq: 18 Sep 2021 00:12

Instrument :

MSVOA_X

ClientSampleId :

RE132D7-20210914DL

Tgt Ion: 84 Resp: 3535





Ion Ratio Lower Upper

84 100

49 139.8 88.6 132.8#

51 37.8 27.0 40.6

86 60.8 50.3 75.5

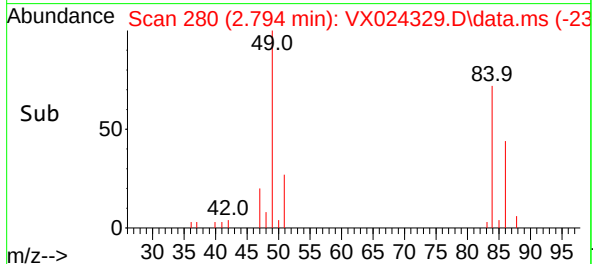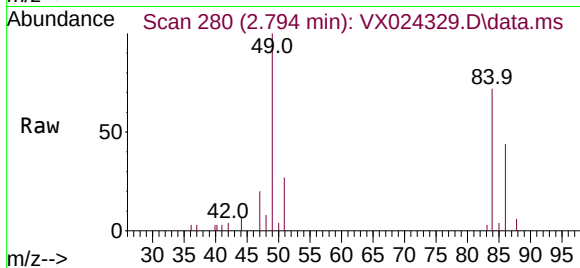

#21

trans-1,2-Dichloroethene

Concen: 0.215 ug/l

RT: 3.087 min Scan# 328

Delta R.T. -0.012 min

Lab File: VX024329.D

Acq: 18 Sep 2021 00:12




Tgt Ion: 96 Resp: 287


Ion Ratio Lower Upper

96 100

61 83.2 107.7 161.5#

98 39.4 50.4 75.6#




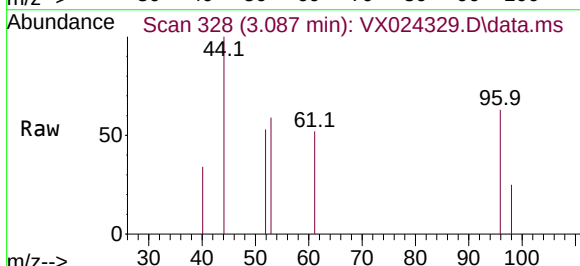


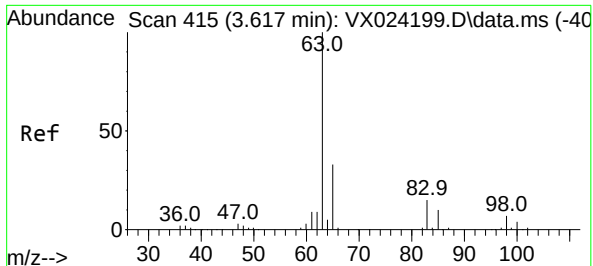

#24
1,1-Dichloroethane
Concen: 0.211 ug/l
RT: 3.623 min Scan# 416
Delta R.T. 0.006 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914DL


Tgt Ion: 63 Resp: 540
Ion Ratio Lower Upper
63 100
98 0.0 3.8 11.2#
100 0.0 2.5 7.5#

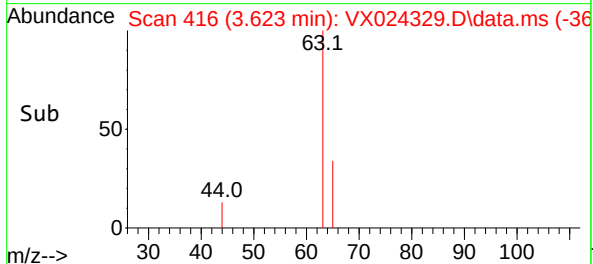

#25
2-Butanone
Concen: 0.590 ug/l
RT: 4.593 min Scan# 575
Delta R.T. 0.025 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Tgt Ion: 43 Resp: 700
Ion Ratio Lower Upper
43 100
72 0.0 23.7 35.5#

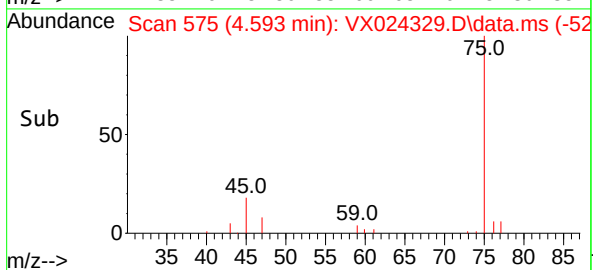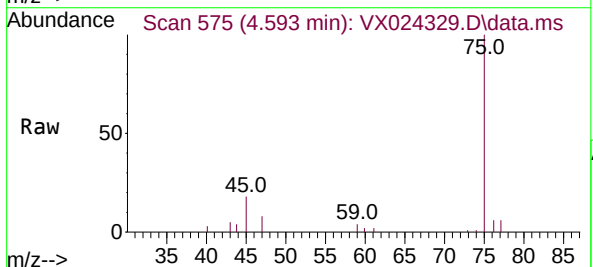



#26

2,2-Dichloropropane

Concen: 0.427 ug/l

RT: 4.593 min Scan# 575

Delta R.T. 0.104 min





Lab File: VX024329.D

Acq: 18 Sep 2021 00:12

Tgt Ion: 77 Resp: 957

Ion Ratio Lower Upper

77 100
97 0.0 11.7 35.1#

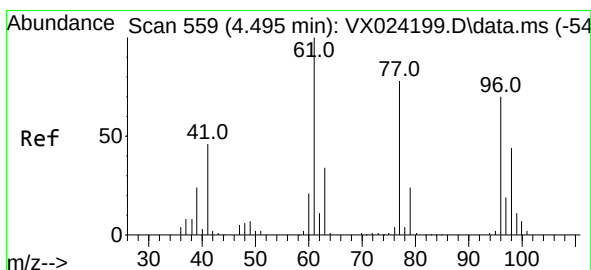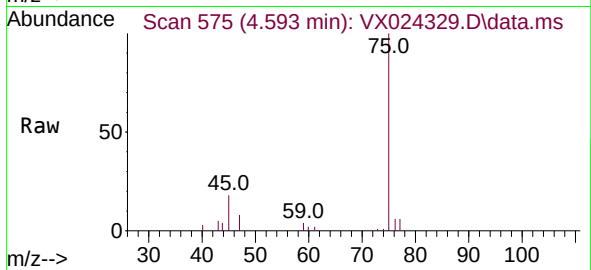

#27

cis-1,2-Dichloroethene

Concen: 0.424 ug/l

RT: 4.507 min Scan# 561

Delta R.T. 0.012 min




Lab File: VX024329.D


Acq: 18 Sep 2021 00:12

Tgt Ion: 96 Resp: 655

Ion Ratio Lower Upper

96 100
61 193.9 0.0 285.6
98 58.6 0.0 129.6

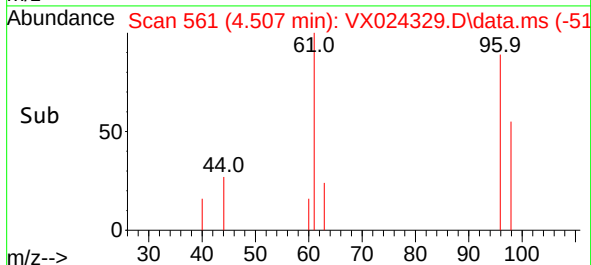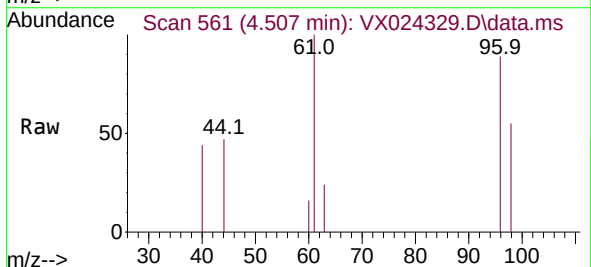

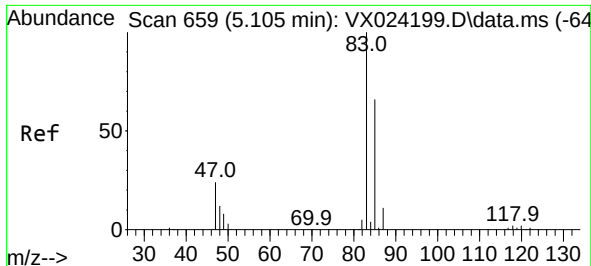

#30

Chloroform

Concen: 0.241 ug/l

RT: 5.111 min Scan# 660

Delta R.T. 0.006 min

Lab File: VX024329.D

Acq: 18 Sep 2021 00:12

Tgt Ion: 83 Resp: 657

Ion Ratio Lower Upper

83 100





85 24.5 52.0 78.0#

Instrument :

MSVOA_X

ClientSampleId :

RE132D7-20210914DL

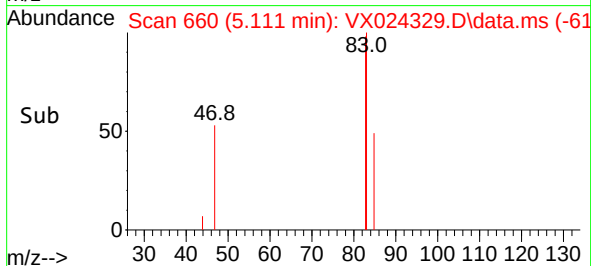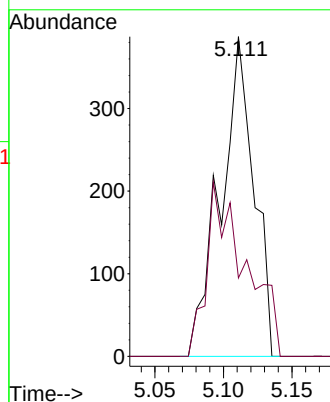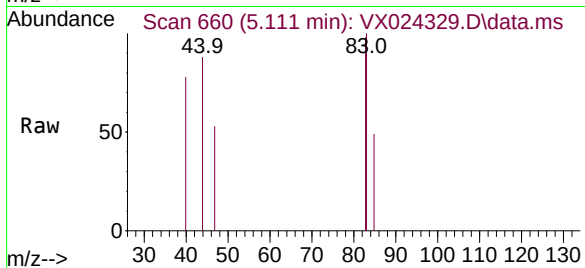

#31

Cyclohexane

Concen: 1.383 ug/l

RT: 5.562 min Scan# 734

Delta R.T. 0.085 min

Lab File: VX024329.D

Acq: 18 Sep 2021 00:12




Tgt Ion: 56 Resp: 3057


Ion Ratio Lower Upper

56 100

69 165.0 25.3 37.9#

84 106.1 71.4 107.0

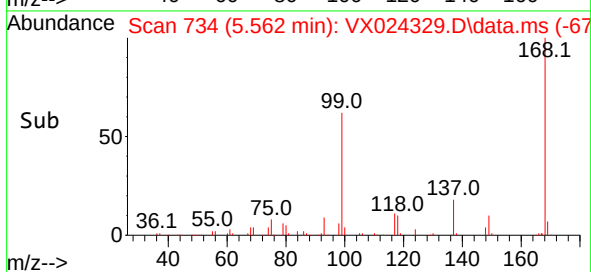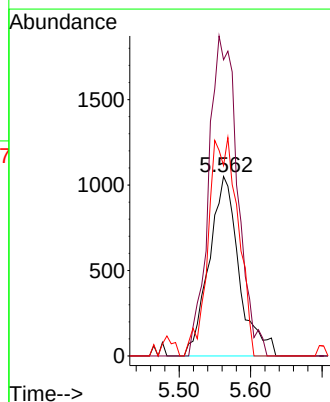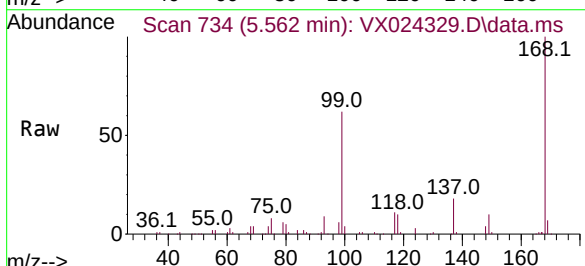




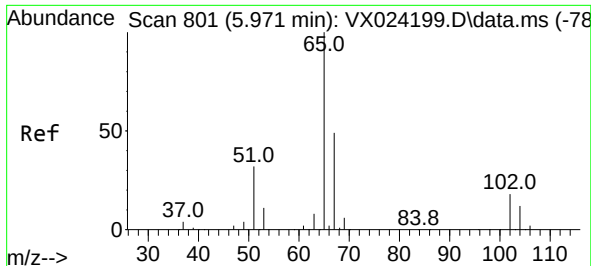


#33

1,2-Dichloroethane-d4
Concen: 51.574 ug/l
RT: 5.964 min Scan# 800
Delta R.T. -0.007 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914DL




Tgt Ion: 65 Resp: 97454
Ion Ratio Lower Upper
65 100
67 51.2 0.0 105.4




#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Tgt Ion: 114 Resp: 229368
Ion Ratio Lower Upper
114 100
63 20.9 0.0 40.8
88 16.5 0.0 32.8

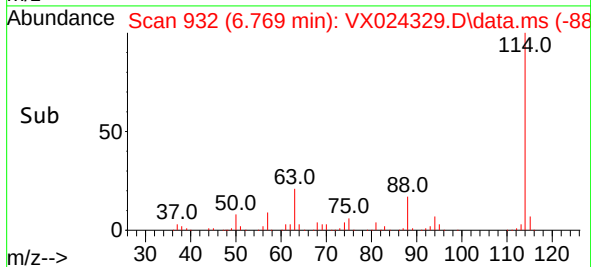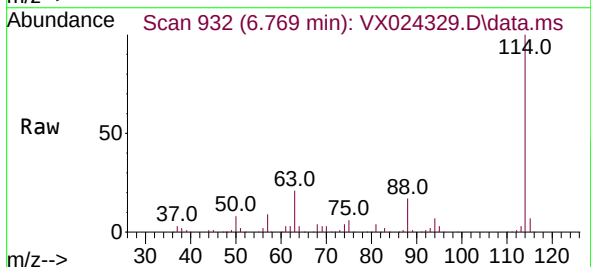

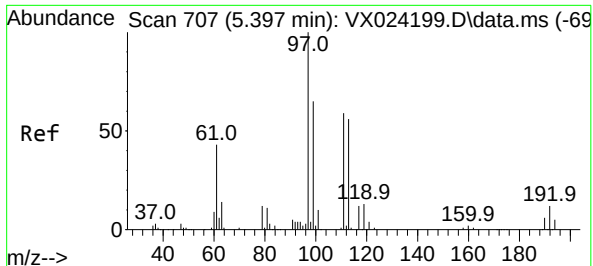

#35

Dibromofluoromethane

Concen: 49.936 ug/l

RT: 5.397 min Scan# 707

Delta R.T. 0.000 min

Lab File: VX024329.D

Acq: 18 Sep 2021 00:12

Tgt Ion:113 Resp: 76813

Ion Ratio Lower Upper

113 100

111 103.1 81.9 122.9





192 19.1 16.7 25.1

Instrument :

MSVOA_X

ClientSampleId :

RE132D7-20210914DL

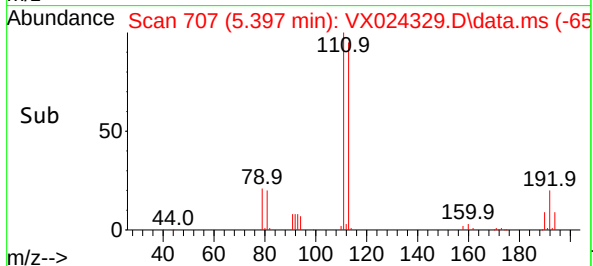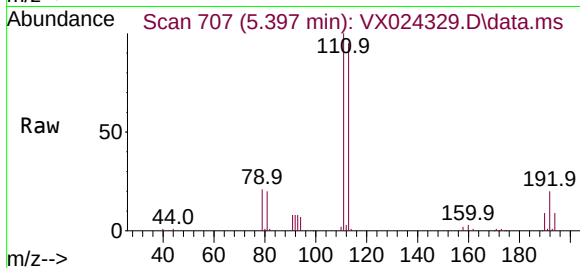

#38

Carbon Tetrachloride

Concen: 0.219 ug/l

RT: 5.690 min Scan# 755

Delta R.T. 0.006 min

Lab File: VX024329.D

Acq: 18 Sep 2021 00:12




Tgt Ion:117 Resp: 520


Ion Ratio Lower Upper

117 100

119 77.2 76.2 114.2

121 0.0 24.8 37.2#


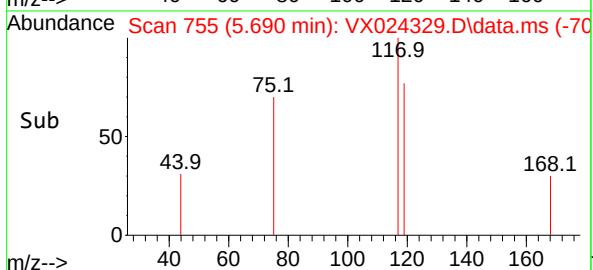

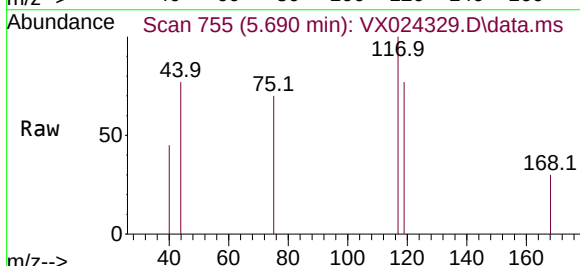


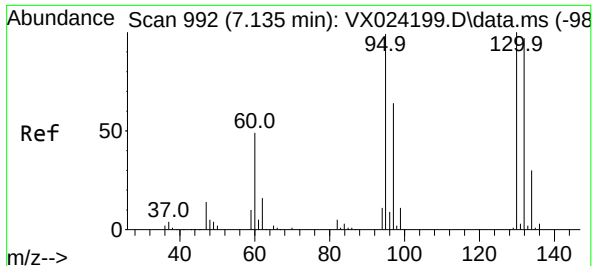

#44
Trichloroethene
Concen: 148.838 ug/l
RT: 7.135 min Scan# 992
Delta R.T. -0.000 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914DL


Tgt Ion:130 Resp: 252934
Ion Ratio Lower Upper
130 100
95 99.1 0.0 198.0

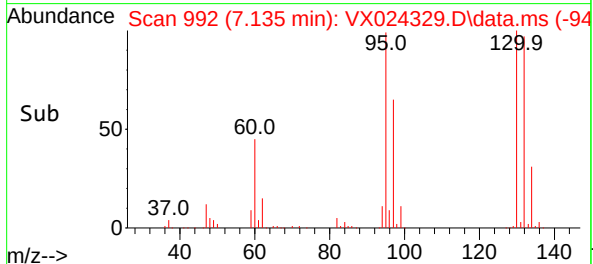

#50
Toluene-d8
Concen: 41.576 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Tgt Ion: 98 Resp: 232979
Ion Ratio Lower Upper
98 100
100 64.4 51.9 77.9


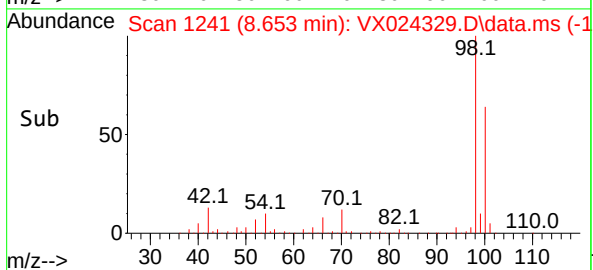

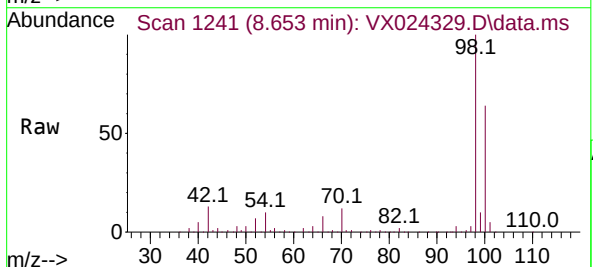


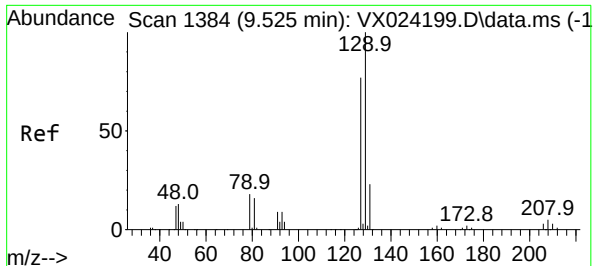

#60
Dibromochloromethane
Concen: 1.736 ug/l
RT: 9.531 min Scan# 1385
Delta R.T. 0.006 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914DL


Tgt Ion:129 Resp: 20
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#

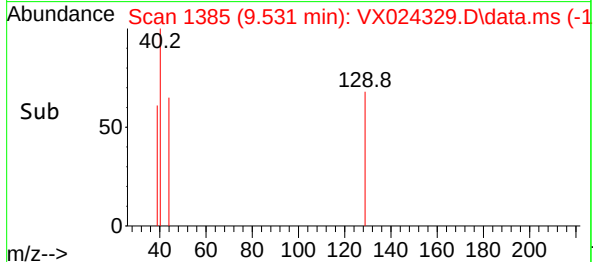

#62
4-Bromofluorobenzene
Concen: 39.612 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Tgt Ion: 95 Resp: 86386
Ion Ratio Lower Upper
95 100
174 79.7 0.0 154.6
176 78.3 0.0 155.8


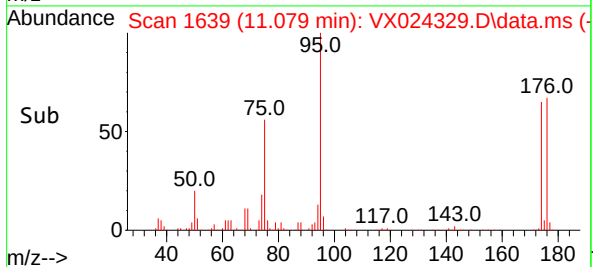

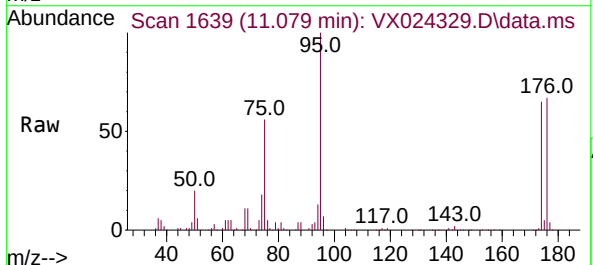




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.000 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914DL


Tgt Ion:117 Resp: 191717
Ion Ratio Lower Upper
117 100
82 53.7 47.4 71.2
119 32.1 26.6 39.8

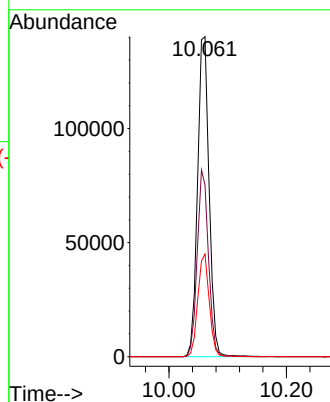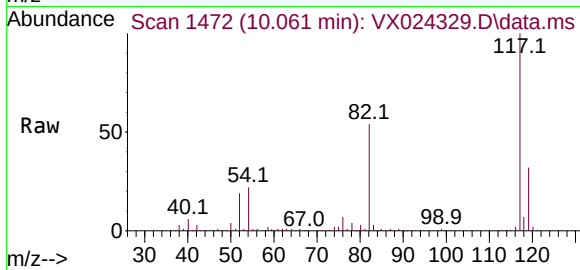

#64
Tetrachloroethene
Concen: 0.384 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. -0.000 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Tgt Ion:164 Resp: 571
Ion Ratio Lower Upper
164 100
166 79.5 103.4 155.2#
129 76.2 70.8 106.2
131 79.1 72.5 108.7


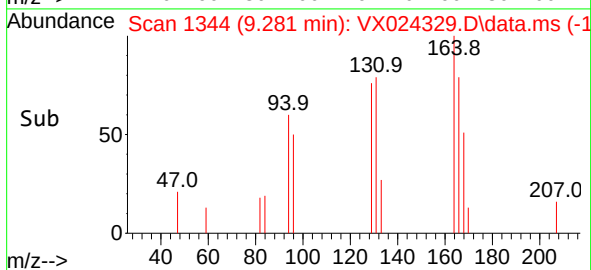

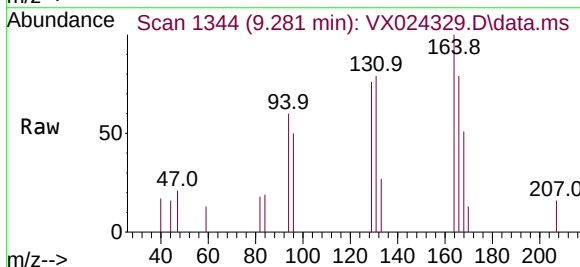




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 1794
 Delta R.T. 0.000 min
 Lab File: VX024329.D
 Acq: 18 Sep 2021 00:12




Instrument :
 MSVOA_X
 ClientSampleId :
 RE132D7-20210914DL


Tgt Ion:152 Resp: 74385
 Ion Ratio Lower Upper
 152 100
 115 59.7 41.1 123.3
 150 157.0 0.0 349.0

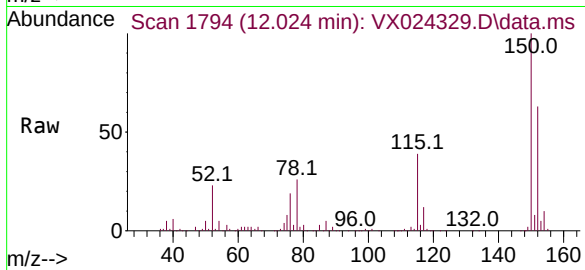

#76
 1,2,3-Trichloropropane
 Concen: 27.554 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.165 min
 Lab File: VX024329.D
 Acq: 18 Sep 2021 00:12

Tgt Ion: 75 Resp: 47128
 Ion Ratio Lower Upper
 75 100
 77 1.0 19.1 57.5#




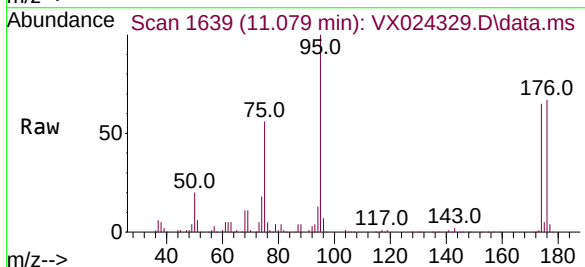




#81
trans-1,4-Dichloro-2-butene
Concen: 81.035 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.054 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914DL


Tgt Ion: 75 Resp: 47128
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

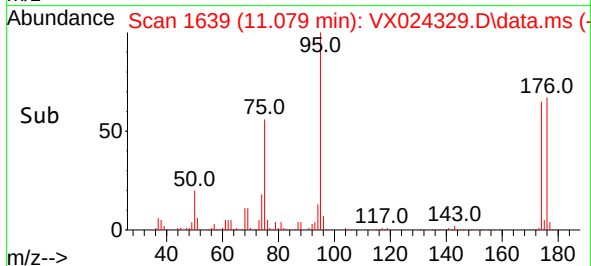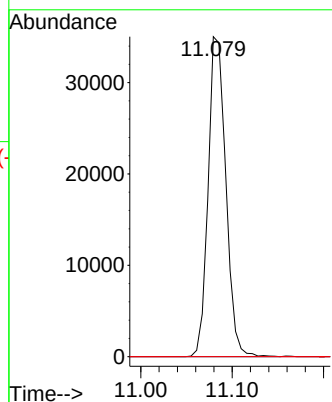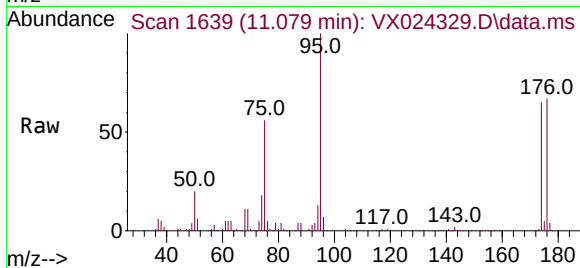

#87
1,3-Dichlorobenzene
Concen: 0.211 ug/l
RT: 11.976 min Scan# 1786
Delta R.T. -0.001 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Tgt Ion:146 Resp: 525
Ion Ratio Lower Upper
146 100
111 29.0 20.2 60.5
148 57.3 31.9 95.7


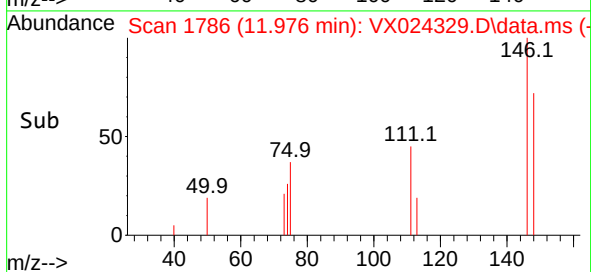
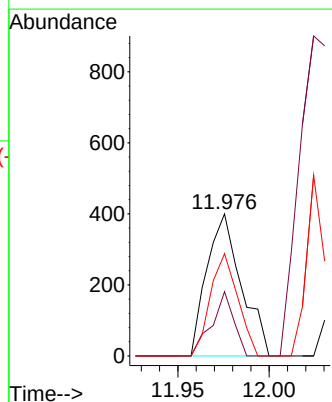
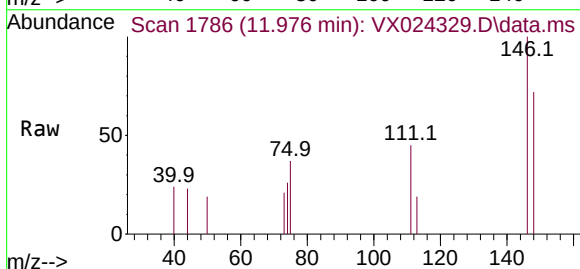


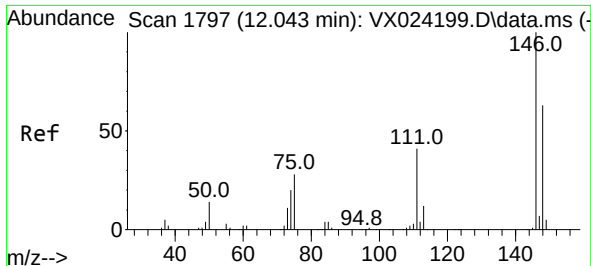

#88
1,4-Dichlorobenzene
Concen: 0.206 ug/l
RT: 11.976 min Scan# 1786
Delta R.T. -0.067 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914DL


Tgt Ion:146 Resp: 525
Ion Ratio Lower Upper
146 100
111 29.0 19.6 58.8
148 57.3 31.6 95.0

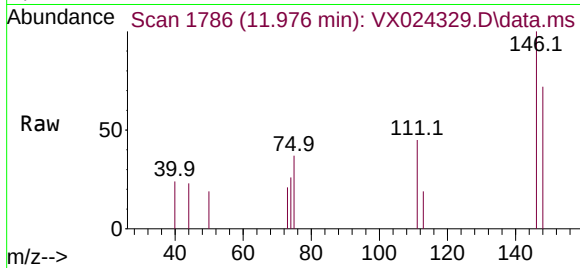

#89
n-Butylbenzene
Concen: 0.223 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Tgt Ion: 91 Resp: 914
Ion Ratio Lower Upper
91 100
92 53.6 27.4 82.0
134 17.9 13.2 39.5




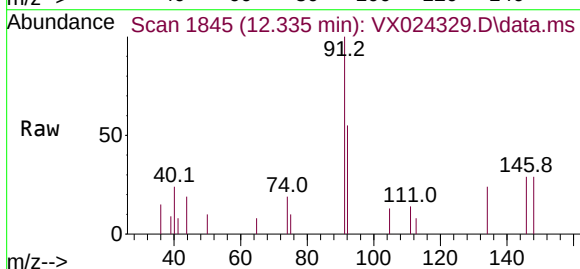


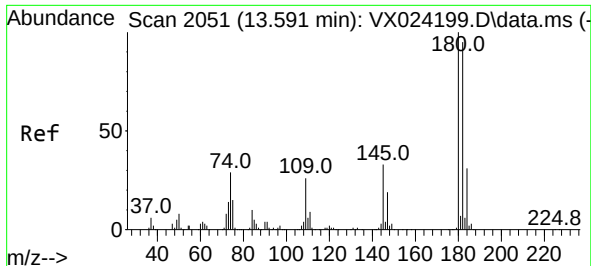

#93
1,2,4-Trichlorobenzene
Concen: 0.272 ug/l
RT: 13.597 min Scan# 2052
Delta R.T. 0.006 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914DL


Tgt Ion:180 Resp: 392
Ion Ratio Lower Upper
180 100
182 90.3 47.7 143.1
145 19.9 15.0 45.0

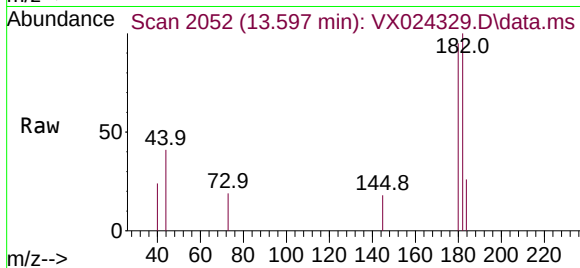

#94
Hexachlorobutadiene
Concen: 0.368 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. 0.000 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Tgt Ion:225 Resp: 265
Ion Ratio Lower Upper
225 100
223 34.3 31.1 93.2
227 29.1 31.6 95.0#


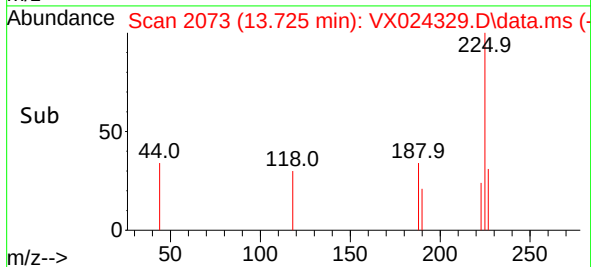

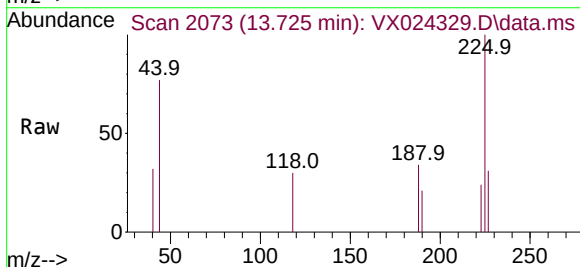




#95
Naphthalene
Concen: 1.430 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914DL

Tgt Ion:128 Resp: 779
Ion Ratio Lower Upper
128 100
127 5.5 10.3 15.5#
129 2.6 8.8 13.2#

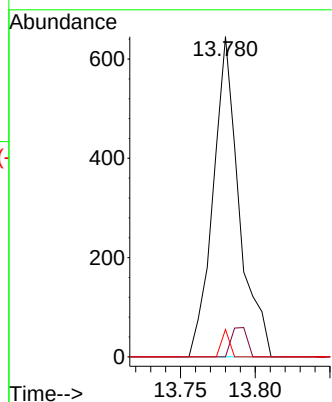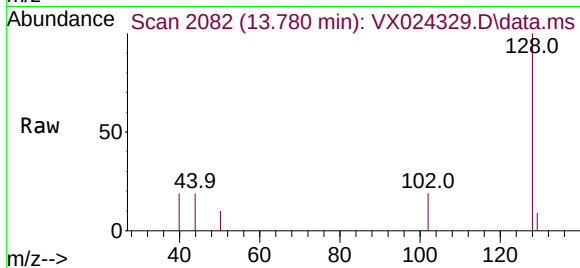

#96
1,2,3-Trichlorobenzene
Concen: 0.238 ug/l
RT: 13.969 min Scan# 2113
Delta R.T. 0.006 min
Lab File: VX024329.D
Acq: 18 Sep 2021 00:12

Tgt Ion:180 Resp: 346
Ion Ratio Lower Upper
180 100
182 88.2 47.6 142.9
145 19.4 16.1 48.3

