

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091721\
 Data File : VX024337.D
 Acq On : 18 Sep 2021 03:21
 Operator : JC/MD
 Sample : M3782-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE131D2-20210915

Quant Time: Sep 20 02:45:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 14 12:18:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	114686	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	197111	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	189505	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	80392	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	86244	52.736	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 105.480%	
35) Dibromofluoromethane	5.397	113	66469	50.283	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.560%	
50) Toluene-d8	8.653	98	244720	50.817	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 101.640%	
62) 4-Bromofluorobenzene	11.085	95	89196	47.594	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 95.180%	


Target Compounds			Qvalue			
2) Dichlorodifluoromethane	1.172	85	645	0.585	ug/l	95
3) Chloromethane	1.301	50	350	0.304	ug/l	90
5) Bromomethane	1.630	94	526	0.771	ug/l #	68
6) Chloroethane	1.660	64	155	2.162	ug/l #	43
7) Trichlorofluoromethane	1.892	101	390	0.203	ug/l	96
8) Diethyl Ether	2.331	74	301	0.453	ug/l #	5
9) 1,1,2-Trichlorotrifluo...	2.331	101	294710	261.019	ug/l	95
11) Tert butyl alcohol	2.953	59	334	Below Cal	#	73
12) 1,1-Dichloroethene	2.325	96	3511	3.320	ug/l #	76
14) Allyl chloride	2.550	41	675	0.351	ug/l #	39
16) Acetone	2.386	43	2001	2.870	ug/l #	65
20) Methylene Chloride	2.800	84	423	0.316	ug/l #	72
22) Diisopropyl ether	3.757	45	1323	0.351	ug/l #	61
23) Vinyl Acetate	3.770	43	824	0.269	ug/l #	68
24) 1,1-Dichloroethane	3.611	63	943	0.426	ug/l #	81
27) cis-1,2-Dichloroethene	4.495	96	8122	6.075	ug/l	96
29) Tetrahydrofuran	5.038	42	334	0.520	ug/l #	27
30) Chloroform	5.111	83	1093	0.464	ug/l	84
31) Cyclohexane	5.568	56	2562	1.339	ug/l #	20
32) 1,1,1-Trichloroethane	5.397	97	601	0.285	ug/l #	37
36) 1,1-Dichloropropene	5.568	75	8726	4.815	ug/l #	51
38) Carbon Tetrachloride	5.568	117	11593	5.684	ug/l #	18
39) Methylcyclohexane	7.135	83	2578	1.191	ug/l #	1
42) 1,2-Dichloroethane	6.117	62	976	0.450	ug/l #	73
44) Trichloroethene	7.135	130	204736	140.192	ug/l	99
49) 1,4-Dioxane	7.671	88	1143	32.547	ug/l #	76
51) 4-Methyl-2-Pentanone	8.653	43	1219	0.569	ug/l #	1
60) Dibromochloromethane	9.281	129	19437	13.132	ug/l #	11
64) Tetrachloroethene	9.281	164	20372	13.877	ug/l	94
76) 1,2,3-Trichloropropane	11.085	75	47913	25.919	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	47913	76.229	ug/l #	12
95) Naphthalene	13.786	128	28	1.292	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091721\
Data File : VX024337.D
Acq On : 18 Sep 2021 03:21
Operator : JC/MD
Sample : M3782-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE131D2-20210915

Quant Time: Sep 20 02:45:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 14 12:18:04 2021
Response via : Initial Calibration




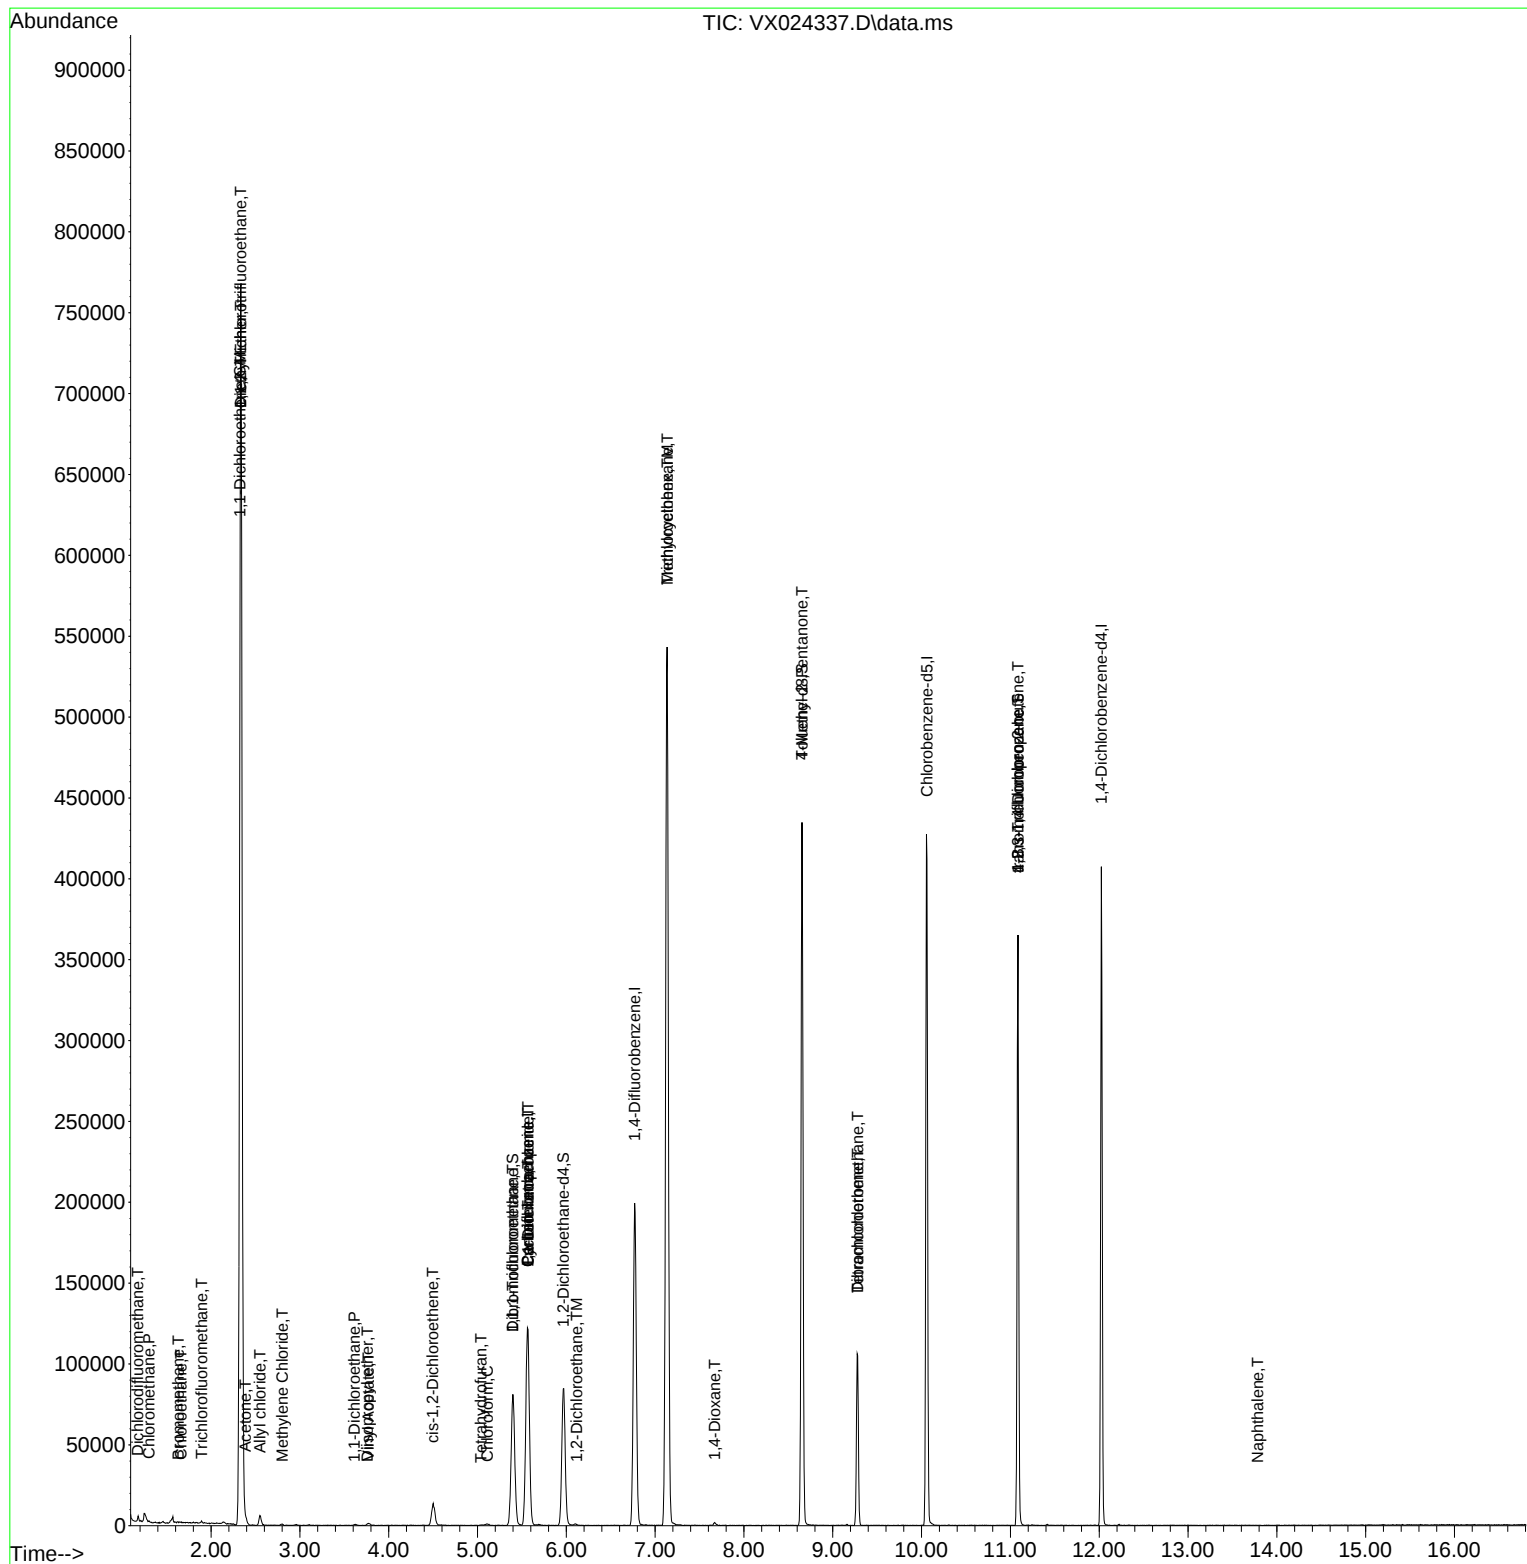


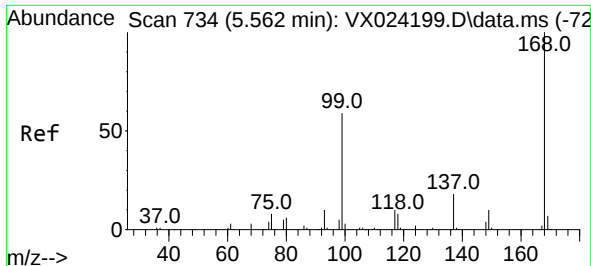

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21




Instrument :
MSVOA_X
ClientSampleId :
RE131D2-20210915


Tgt Ion:168 Resp: 114686
Ion Ratio Lower Upper
168 100
99 59.4 45.8 68.6

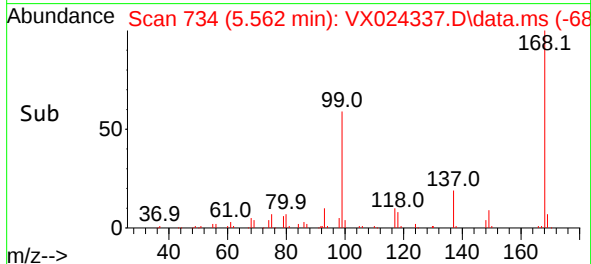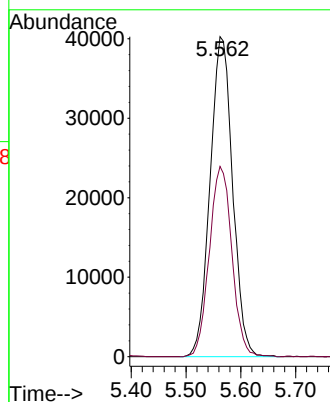

#2
Dichlorodifluoromethane
Concen: 0.585 ug/l
RT: 1.172 min Scan# 14
Delta R.T. -0.001 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Tgt Ion: 85 Resp: 645
Ion Ratio Lower Upper
85 100
87 35.9 16.4 49.2


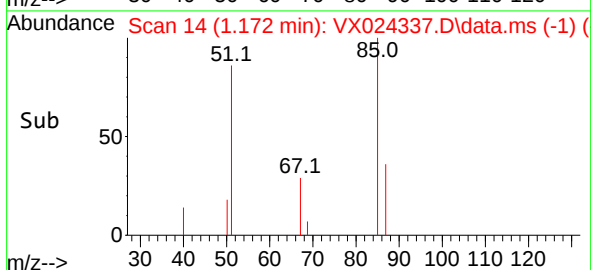

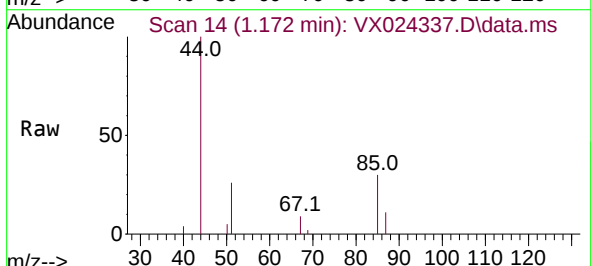


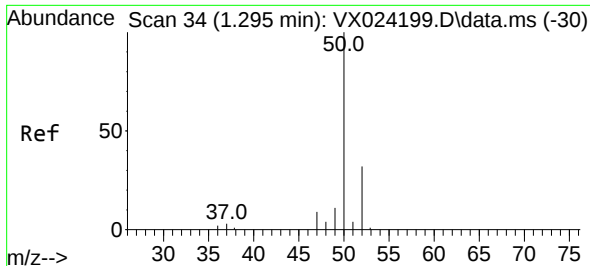

#3
Chloromethane
Concen: 0.304 ug/l
RT: 1.301 min Scan# 35
Delta R.T. 0.006 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21




Instrument :
MSVOA_X
ClientSampleId :
RE131D2-20210915


Tgt Ion: 50 Resp: 350
Ion Ratio Lower Upper
50 100
52 27.5 26.4 39.6

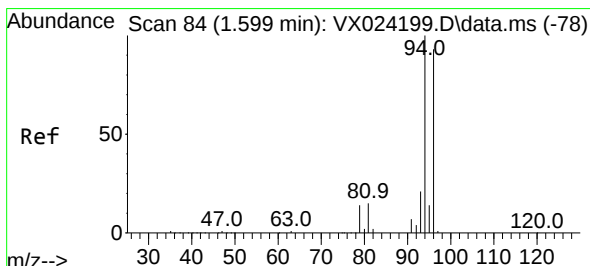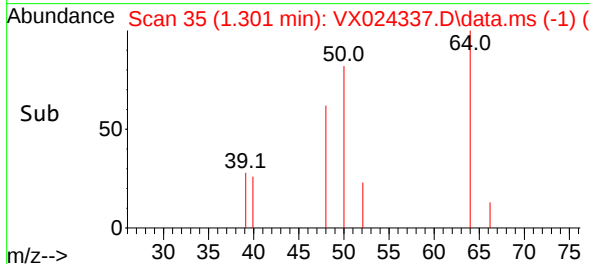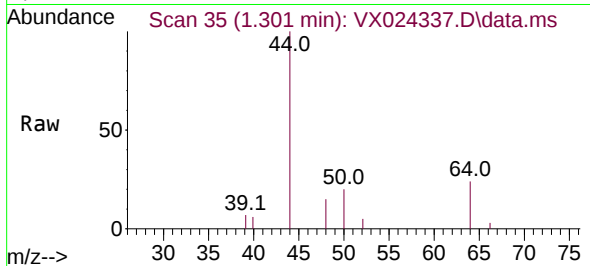

#5
Bromomethane
Concen: 0.771 ug/l
RT: 1.630 min Scan# 89
Delta R.T. 0.031 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Tgt Ion: 94 Resp: 526
Ion Ratio Lower Upper
94 100
96 64.8 76.4 114.6#


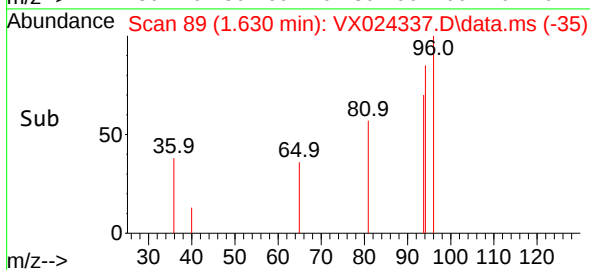

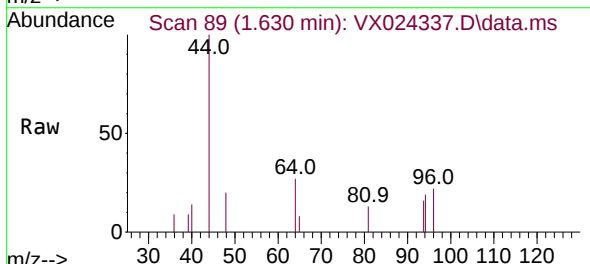


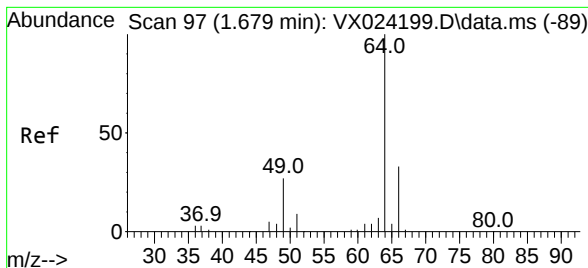

#6
Chloroethane
Concen: 2.162 ug/l
RT: 1.660 min Scan# 94
Delta R.T. -0.019 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21




Instrument :
MSVOA_X
ClientSampleId :
RE131D2-20210915


Tgt Ion: 64 Resp: 155
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.0#

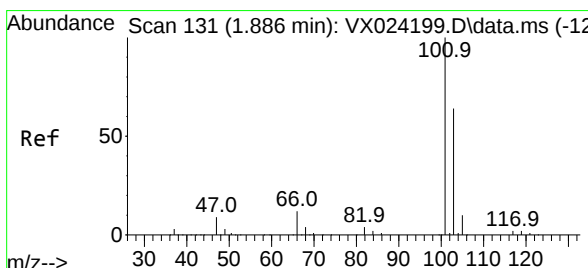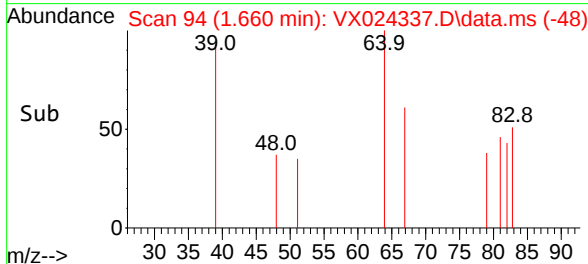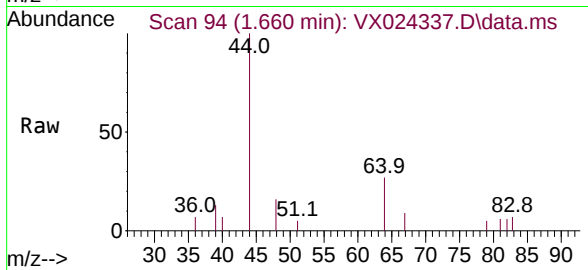

#7
Trichlorofluoromethane
Concen: 0.203 ug/l
RT: 1.892 min Scan# 132
Delta R.T. 0.006 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Tgt Ion: 101 Resp: 390
Ion Ratio Lower Upper
101 100
103 69.7 53.2 79.8


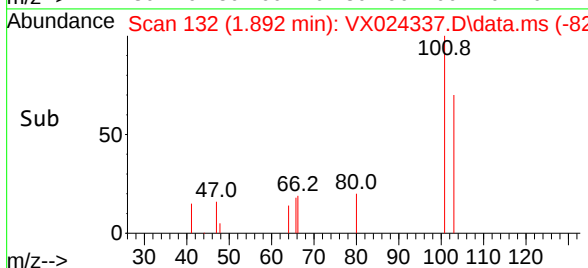

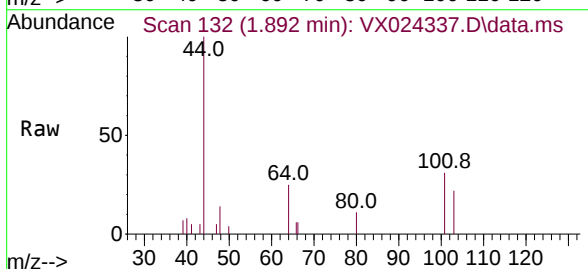




#8
Diethyl Ether
Concen: 0.453 ug/l
RT: 2.331 min Scan# 204
Delta R.T. 0.189 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21




Instrument :
MSVOA_X
ClientSampleId :
RE131D2-20210915


Tgt Ion: 74 Resp: 301
Ion Ratio Lower Upper
74 100
45 0.0 44.5 133.5#

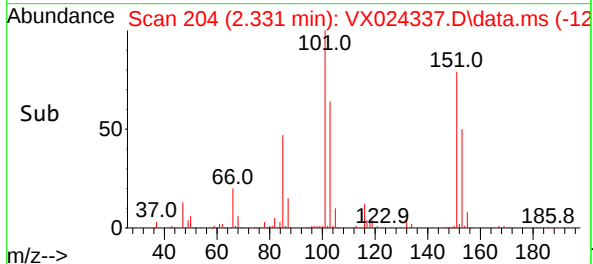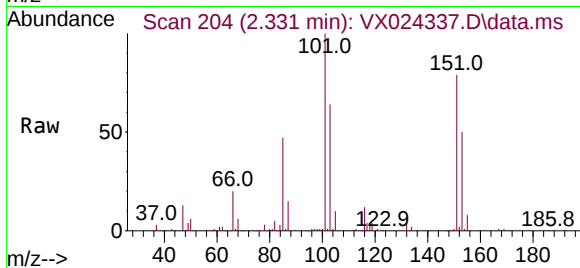

#9
1,1,2-Trichlorotrifluoroethane
Concen: 261.019 ug/l
RT: 2.331 min Scan# 204
Delta R.T. -0.000 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Tgt Ion:101 Resp: 294710
Ion Ratio Lower Upper
101 100
85 46.3 34.9 52.3
151 81.6 61.4 92.2

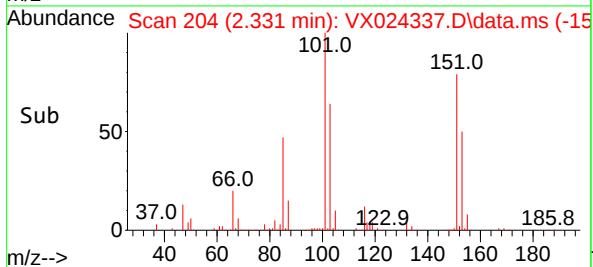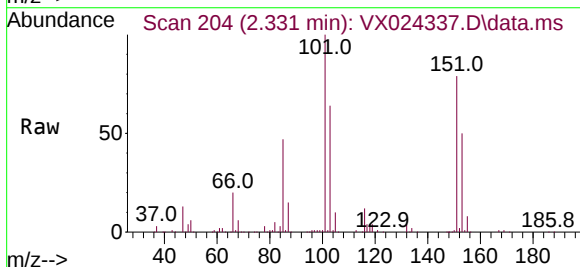







#11

Tert butyl alcohol
Concen: Below Cal
RT: 2.953 min Scan# 306
Delta R.T. -0.030 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Instrument :
MSVOA_X
ClientSampleId :
RE131D2-20210915




Tgt Ion: 59 Resp: 334
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#




#12

1,1-Dichloroethene
Concen: 3.320 ug/l
RT: 2.325 min Scan# 203
Delta R.T. 0.006 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Tgt Ion: 96 Resp: 3511
Ion Ratio Lower Upper
96 100
61 127.2 124.6 187.0
98 42.0 50.6 76.0#




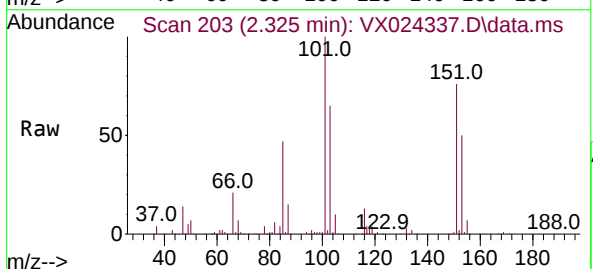


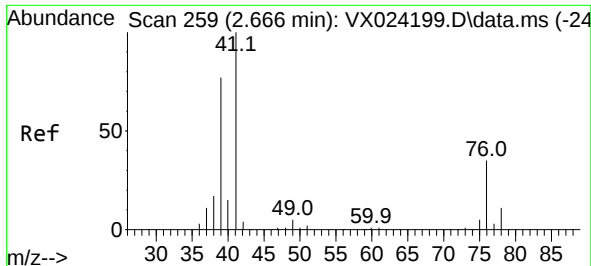

#14
Allyl chloride
Concen: 0.351 ug/l
RT: 2.550 min Scan# 240
Delta R.T. -0.116 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21




Instrument :
MSVOA_X
ClientSampleId :
RE131D2-20210915


Tgt Ion:	41	Resp:	675
Ion	Ratio	Lower	Upper
41	100		
39	112.0	51.6	77.4#
76	0.0	30.5	45.7#

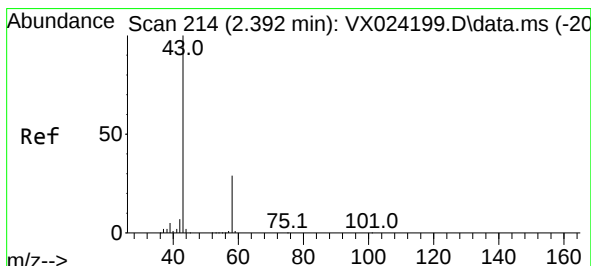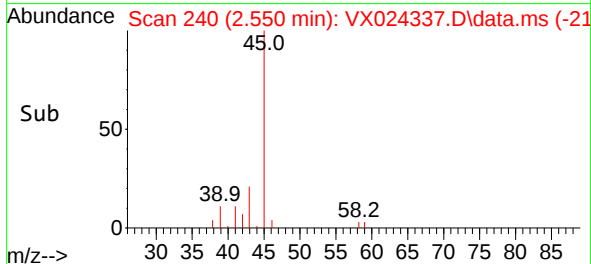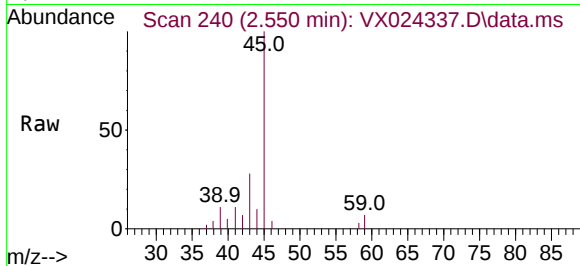

#16
Acetone
Concen: 2.870 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Tgt Ion:	43	Resp:	2001
Ion	Ratio	Lower	Upper
43	100		
58	14.6	27.8	41.8#

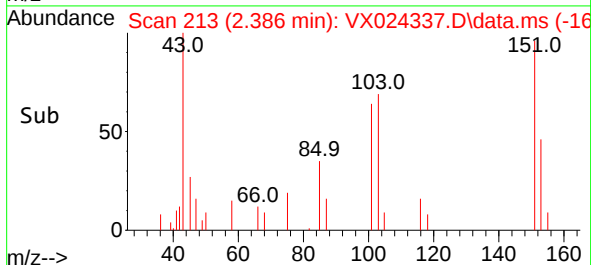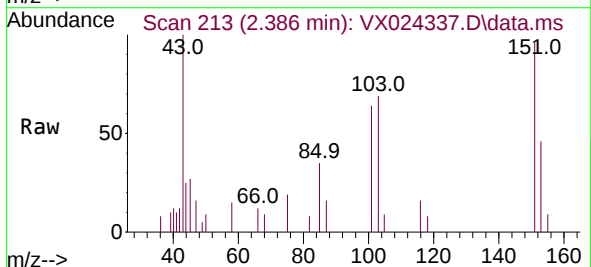



#20

Methylene Chloride

Concen: 0.316 ug/l

RT: 2.800 min Scan# 281

Delta R.T. 0.006 min

Lab File: VX024337.D

Acq: 18 Sep 2021 03:21

Instrument :

MSVOA_X

ClientSampleId :

RE131D2-20210915

Tgt Ion: 84 Resp: 423





Ion Ratio Lower Upper

84 100

49 93.2 88.6 132.8

51 0.0 27.0 40.6#

86 38.7 50.3 75.5#



#22

Diisopropyl ether

Concen: 0.351 ug/l

RT: 3.757 min Scan# 438

Delta R.T. -0.019 min

Lab File: VX024337.D

Acq: 18 Sep 2021 03:21

Tgt Ion: 45 Resp: 1323




Ion Ratio Lower Upper


45 100

43 38.6 58.0 87.0#

87 10.9 25.4 38.0#

59 0.0 10.2 15.2#


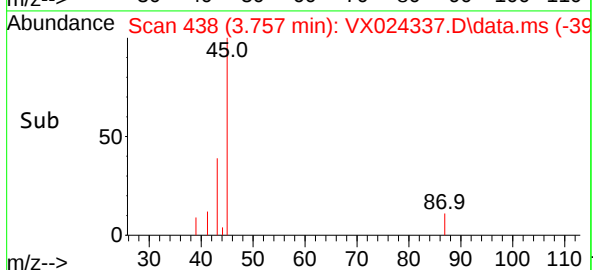
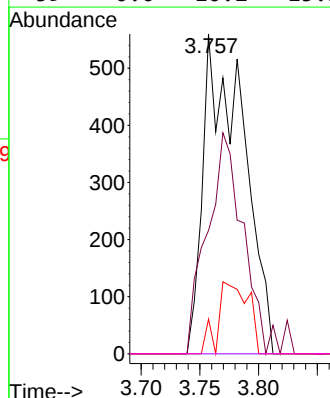





#23
 Vinyl Acetate
 Concen: 0.269 ug/l
 RT: 3.770 min Scan# 440
 Delta R.T. 0.037 min
 Lab File: VX024337.D
 Acq: 18 Sep 2021 03:21




Instrument :
 MSVOA_X
 ClientSampleId :
 RE131D2-20210915


Tgt Ion: 43 Resp: 824
 Ion Ratio Lower Upper
 43 100
 86 0.0 9.9 14.9#



#24
 1,1-Dichloroethane
 Concen: 0.426 ug/l
 RT: 3.611 min Scan# 414
 Delta R.T. -0.006 min
 Lab File: VX024337.D
 Acq: 18 Sep 2021 03:21

Tgt Ion: 63 Resp: 943
 Ion Ratio Lower Upper
 63 100
 98 0.0 3.8 11.2#
 100 0.0 2.5 7.5#

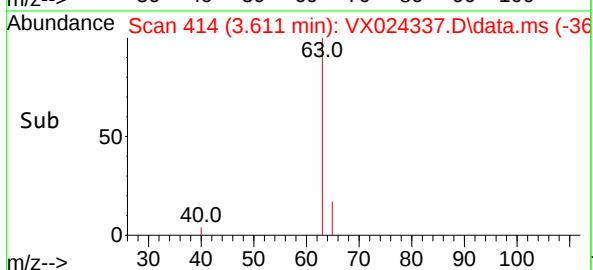



#27

cis-1,2-Dichloroethene

Concen: 6.075 ug/l

RT: 4.495 min Scan# 559

Delta R.T. 0.000 min

Lab File: VX024337.D

Acq: 18 Sep 2021 03:21

Tgt Ion: 96 Resp: 8122





Ion	Ratio	Lower	Upper
96	100		
61	136.1	0.0	285.6
98	65.3	0.0	129.6

Instrument :

MSVOA_X

ClientSampleId :

RE131D2-20210915

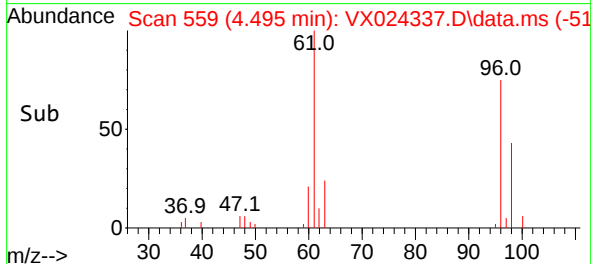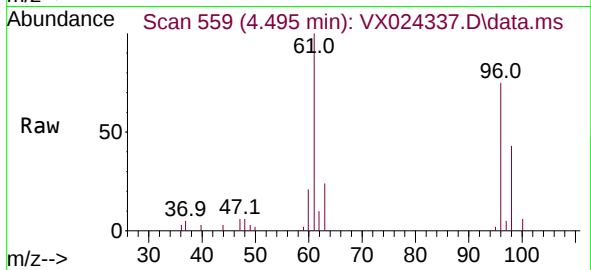

#29

Tetrahydrofuran

Concen: 0.520 ug/l

RT: 5.038 min Scan# 648




Delta R.T. 0.019 min


Lab File: VX024337.D

Acq: 18 Sep 2021 03:21

Tgt Ion: 42 Resp: 334

Ion	Ratio	Lower	Upper
42	100		
72	0.0	41.7	62.5#
71	0.0	38.4	57.6#

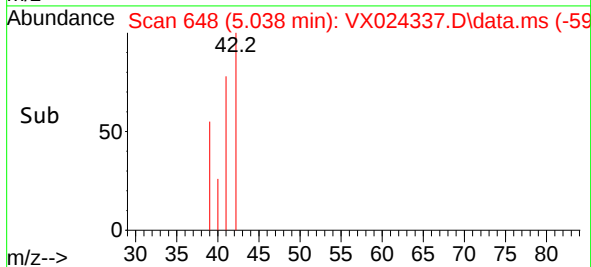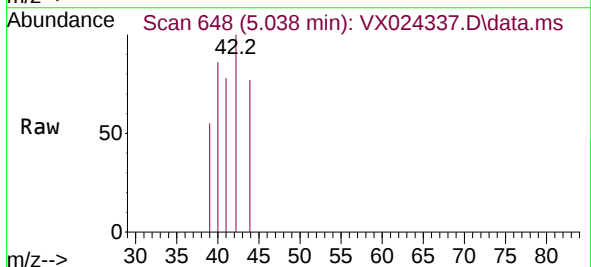

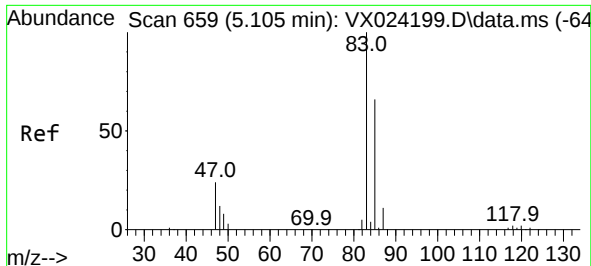

#30

Chloroform

Concen: 0.464 ug/l

RT: 5.111 min Scan# 660

Delta R.T. 0.006 min

Lab File: VX024337.D





Acq: 18 Sep 2021 03:21

Tgt Ion: 83 Resp: 1093

Ion Ratio Lower Upper

83 100

85 52.6 52.0 78.0

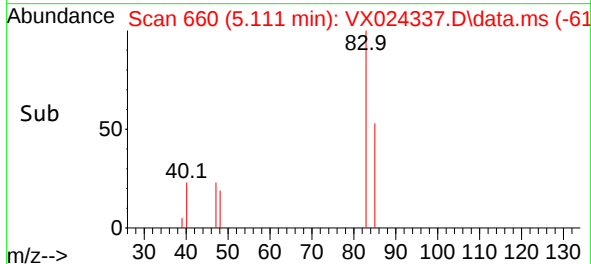

#31

Cyclohexane

Concen: 1.339 ug/l

RT: 5.568 min Scan# 735

Delta R.T. 0.091 min

Lab File: VX024337.D

Acq: 18 Sep 2021 03:21




Tgt Ion: 56 Resp: 2562


Ion Ratio Lower Upper

56 100

69 144.5 25.3 37.9#

84 123.4 71.4 107.0#

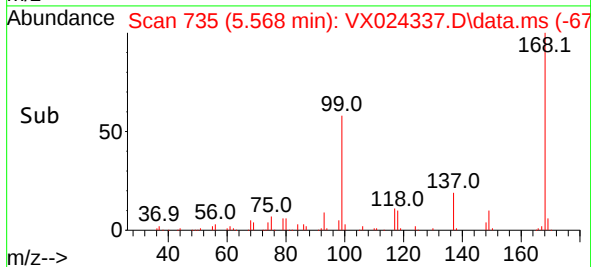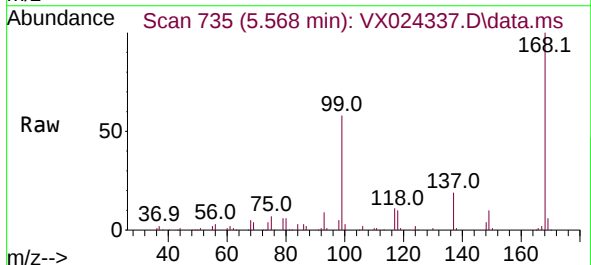







#32

1,1,1-Trichloroethane
Concen: 0.285 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Instrument :
MSVOA_X
ClientSampleId :
RE131D2-20210915




Tgt Ion: 97 Resp: 601
Ion Ratio Lower Upper
97 100
99 0.0 51.5 77.3#
61 21.6 34.2 51.4#

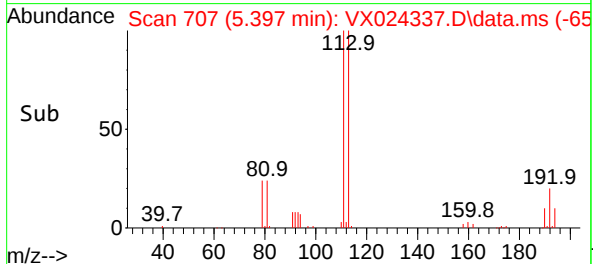


#33

1,2-Dichloroethane-d4
Concen: 52.736 ug/l
RT: 5.964 min Scan# 800
Delta R.T. -0.007 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Tgt Ion: 65 Resp: 86244
Ion Ratio Lower Upper
65 100
67 49.0 0.0 105.4


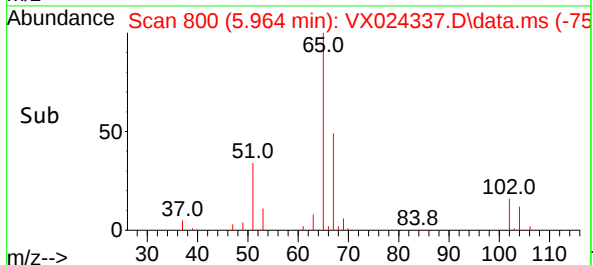

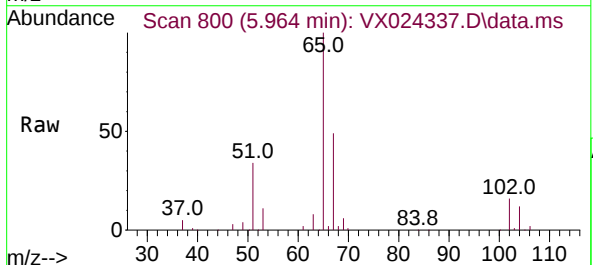




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21




Instrument :
MSVOA_X
ClientSampleId :
RE131D2-20210915


Tgt Ion:114 Resp: 197111
Ion Ratio Lower Upper
114 100
63 20.9 0.0 40.8
88 16.4 0.0 32.8

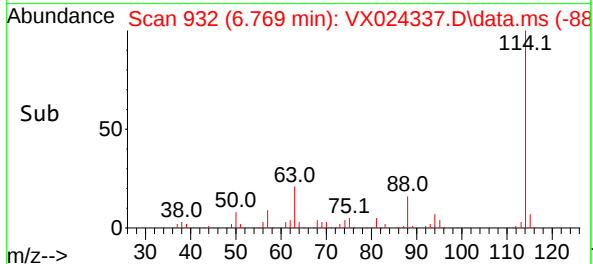

#35
Dibromofluoromethane
Concen: 50.283 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Tgt Ion:113 Resp: 66469
Ion Ratio Lower Upper
113 100
111 103.9 81.9 122.9
192 20.4 16.7 25.1


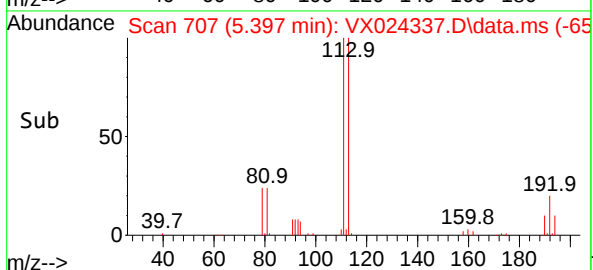




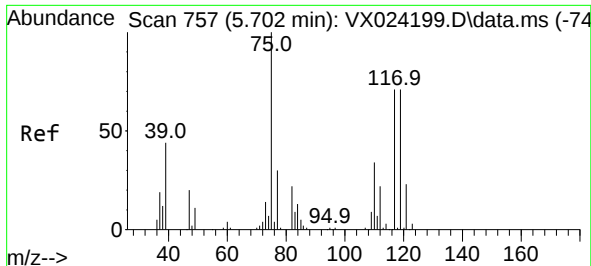

#36
1,1-Dichloropropene
Concen: 4.815 ug/l
RT: 5.568 min Scan# 735
Delta R.T. -0.134 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21




Instrument :
MSVOA_X
ClientSampleId :
RE131D2-20210915


Tgt Ion: 75 Resp: 8726
Ion Ratio Lower Upper
75 100
110 12.0 18.1 54.4#
77 0.0 25.3 37.9#

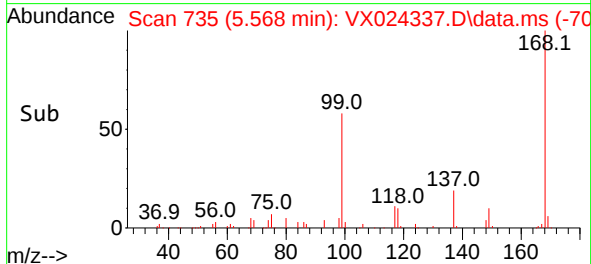

#38
Carbon Tetrachloride
Concen: 5.684 ug/l
RT: 5.568 min Scan# 735
Delta R.T. -0.116 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Tgt Ion: 117 Resp: 11593
Ion Ratio Lower Upper
117 100
119 6.8 76.2 114.2#
121 0.0 24.8 37.2#

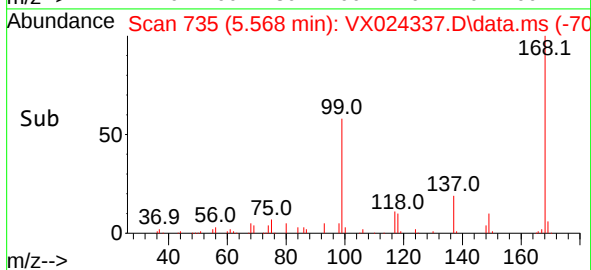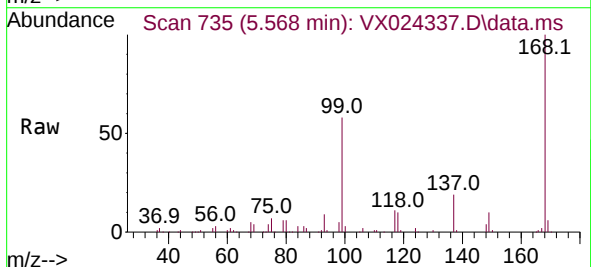



#39

Methylcyclohexane

Concen: 1.191 ug/l

RT: 7.135 min Scan# 992

Delta R.T. -0.250 min

Lab File: VX024337.D

Acq: 18 Sep 2021 03:21

Tgt Ion: 83 Resp: 2578

Ion Ratio Lower Upper

83 100

55 0.0 58.9 88.3#





98 196.5 38.1 57.1#

Instrument :

MSVOA_X

ClientSampleId :

RE131D2-20210915

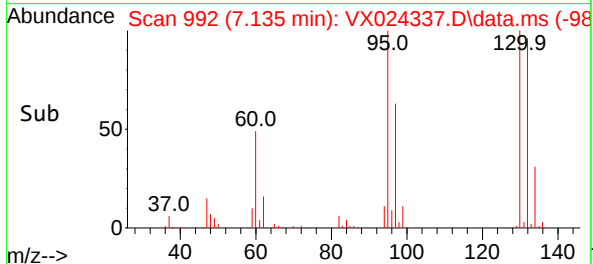

#42

1,2-Dichloroethane

Concen: 0.450 ug/l

RT: 6.117 min Scan# 825

Delta R.T. 0.018 min

Lab File: VX024337.D




Acq: 18 Sep 2021 03:21


Tgt Ion: 62 Resp: 976

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.2


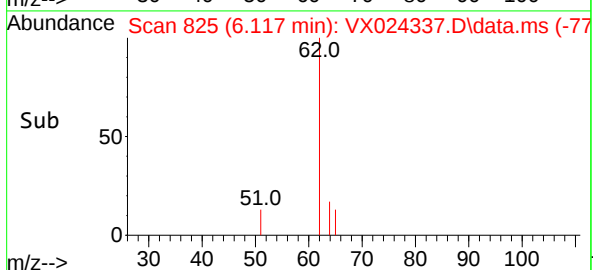






#44
Trichloroethene
Concen: 140.192 ug/l
RT: 7.135 min Scan# 992
Delta R.T. -0.000 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21




Instrument :
MSVOA_X
ClientSampleId :
RE131D2-20210915


Tgt Ion:130 Resp: 204736
Ion Ratio Lower Upper
130 100
95 99.8 0.0 198.0

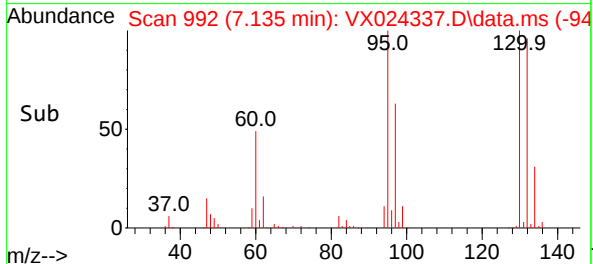

#49
1,4-Dioxane
Concen: 32.547 ug/l
RT: 7.671 min Scan# 1080
Delta R.T. 0.006 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Tgt Ion: 88 Resp: 1143
Ion Ratio Lower Upper
88 100
43 37.3 23.2 34.8#
58 91.0 55.0 82.4#


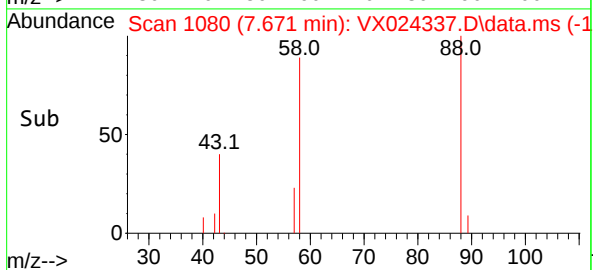

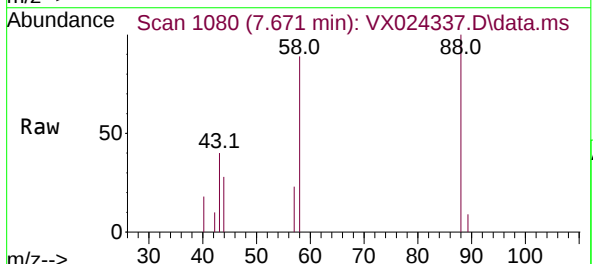


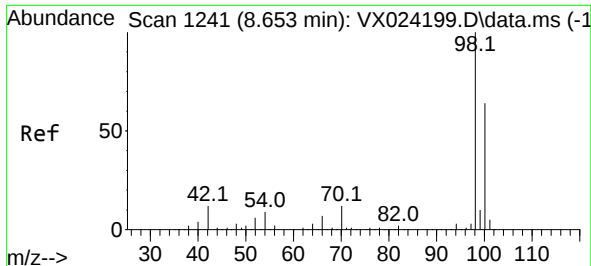

#50
Toluene-d8
Concen: 50.817 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21




Instrument :
MSVOA_X
ClientSampleId :
RE131D2-20210915


Tgt Ion: 98 Resp: 244720
Ion Ratio Lower Upper
98 100
100 63.7 51.9 77.9

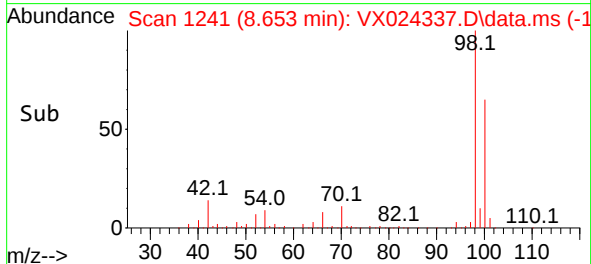

#51
4-Methyl-2-Pentanone
Concen: 0.569 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.073 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Tgt Ion: 43 Resp: 1219
Ion Ratio Lower Upper
43 100
58 194.0 35.4 53.0#


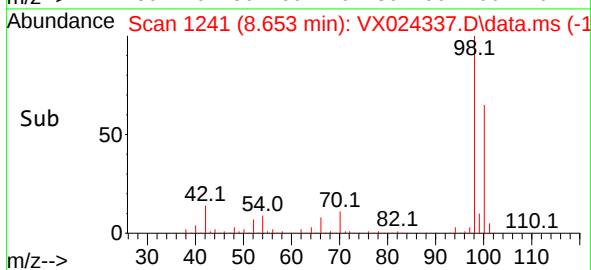

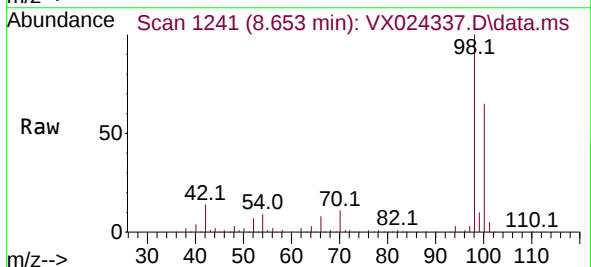




#60
Dibromochloromethane
Concen: 13.132 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. -0.244 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21




Instrument :
MSVOA_X
ClientSampleId :
RE131D2-20210915


Tgt Ion:129 Resp: 19437
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#

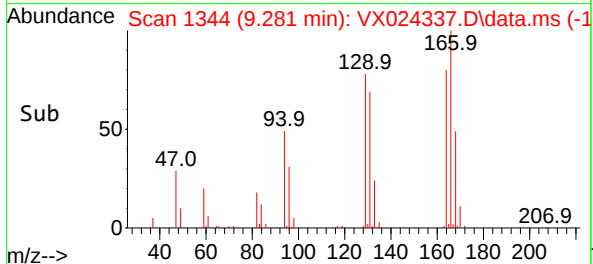

#62
4-Bromofluorobenzene
Concen: 47.594 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Tgt Ion: 95 Resp: 89196
Ion Ratio Lower Upper
95 100
174 79.5 0.0 154.6
176 77.6 0.0 155.8


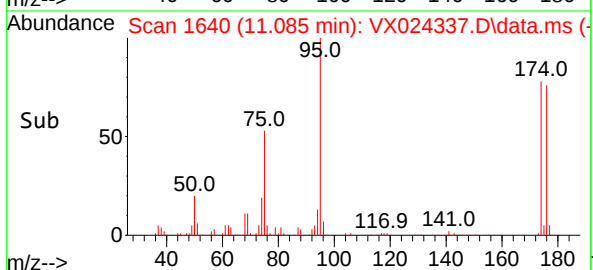

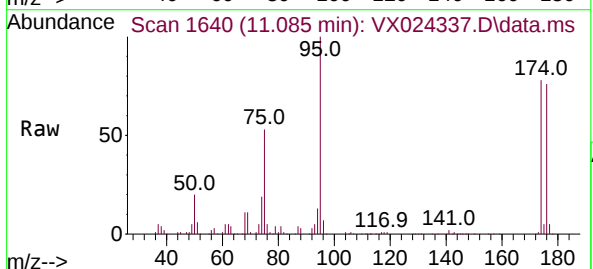




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.000 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21




Instrument :
MSVOA_X
ClientSampleId :
RE131D2-20210915


Tgt Ion:117 Resp: 189505
Ion Ratio Lower Upper
117 100
82 55.1 47.4 71.2
119 32.5 26.6 39.8

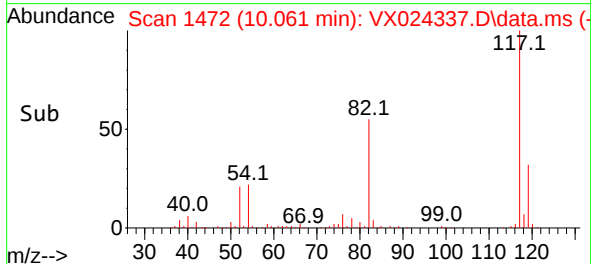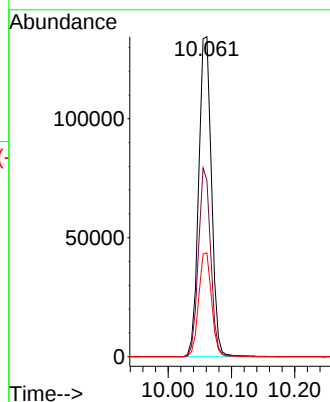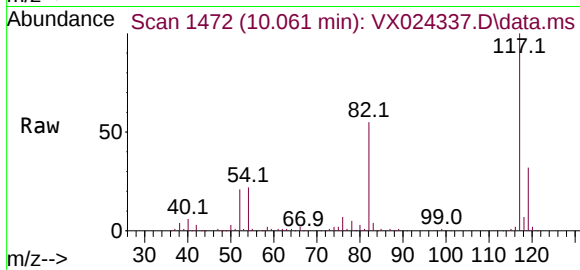

#64
Tetrachloroethene
Concen: 13.877 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. -0.000 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Tgt Ion:164 Resp: 20372
Ion Ratio Lower Upper
164 100
166 125.5 103.4 155.2
129 98.1 70.8 106.2
131 86.0 72.5 108.7


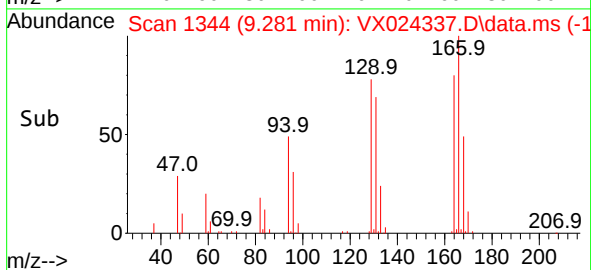

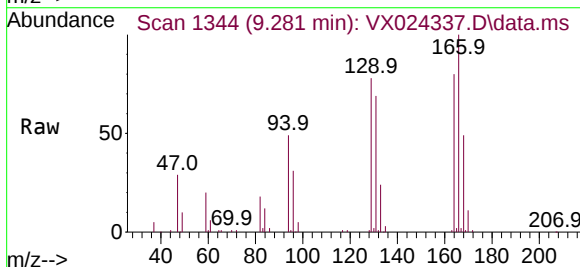




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 1794
 Delta R.T. 0.000 min
 Lab File: VX024337.D
 Acq: 18 Sep 2021 03:21




Instrument :
 MSVOA_X
 ClientSampleId :
 RE131D2-20210915


Tgt Ion:152 Resp: 80392
 Ion Ratio Lower Upper
 152 100
 115 58.0 41.1 123.3
 150 157.6 0.0 349.0

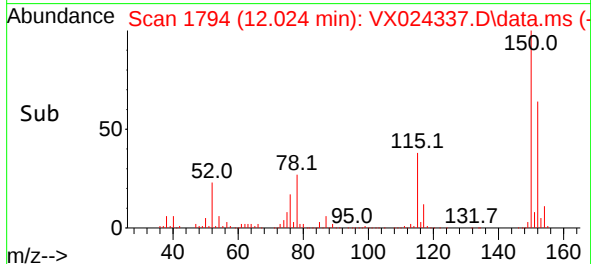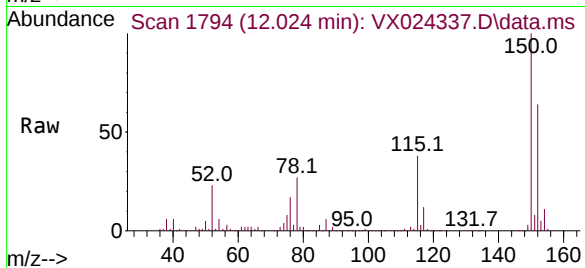

#76
 1,2,3-Trichloropropane
 Concen: 25.919 ug/l
 RT: 11.085 min Scan# 1640
 Delta R.T. -0.159 min
 Lab File: VX024337.D
 Acq: 18 Sep 2021 03:21

Tgt Ion: 75 Resp: 47913
 Ion Ratio Lower Upper
 75 100
 77 0.9 19.1 57.5#


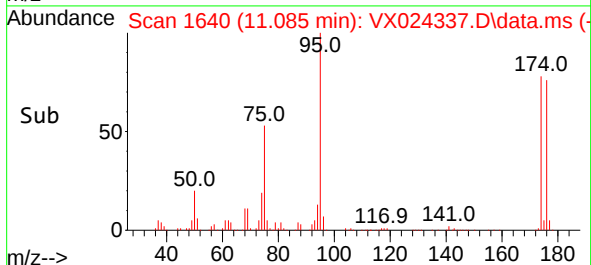

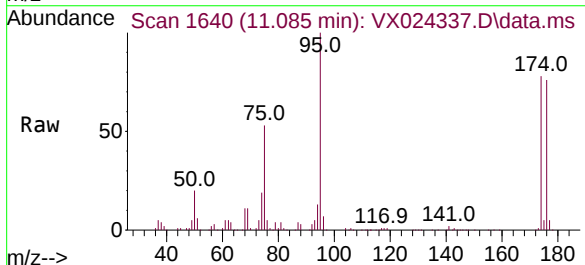




#81
trans-1,4-Dichloro-2-butene
Concen: 76.229 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.060 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Instrument :
MSVOA_X
ClientSampleId :
RE131D2-20210915

Tgt Ion: 75 Resp: 47913
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

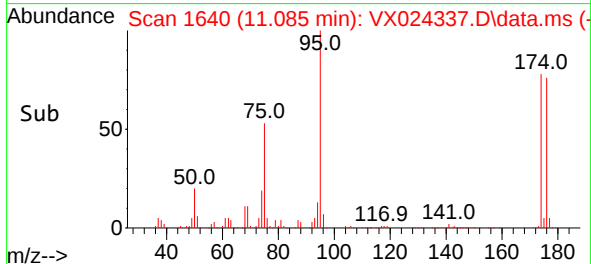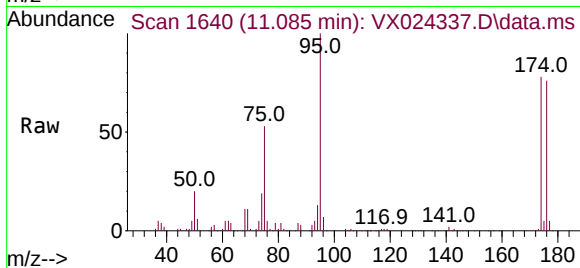

#95
Naphthalene
Concen: 1.292 ug/l
RT: 13.786 min Scan# 2083
Delta R.T. 0.006 min
Lab File: VX024337.D
Acq: 18 Sep 2021 03:21

Tgt Ion: 128 Resp: 28
Ion Ratio Lower Upper
128 100
127 0.0 10.3 15.5#
129 0.0 8.8 13.2#

