

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091721\
 Data File : VX024326.D
 Acq On : 17 Sep 2021 23:01
 Operator : JC/MD
 Sample : VX0917WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0917WBL02

Quant Time: Sep 20 02:28:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 14 12:18:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	142501	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	240715	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	236097	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	79802	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	110777	54.516	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 109.040%	
35) Dibromofluoromethane	5.397	113	82999	51.414	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 102.820%	
50) Toluene-d8	8.653	98	283747	48.248	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 96.500%	
62) 4-Bromofluorobenzene	11.085	95	109667	47.917	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 95.840%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091721\
Data File : VX024326.D
Acq On : 17 Sep 2021 23:01
Operator : JC/MD
Sample : VX0917WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0917WBL02

Quant Time: Sep 20 02:28:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 14 12:18:04 2021
Response via : Initial Calibration




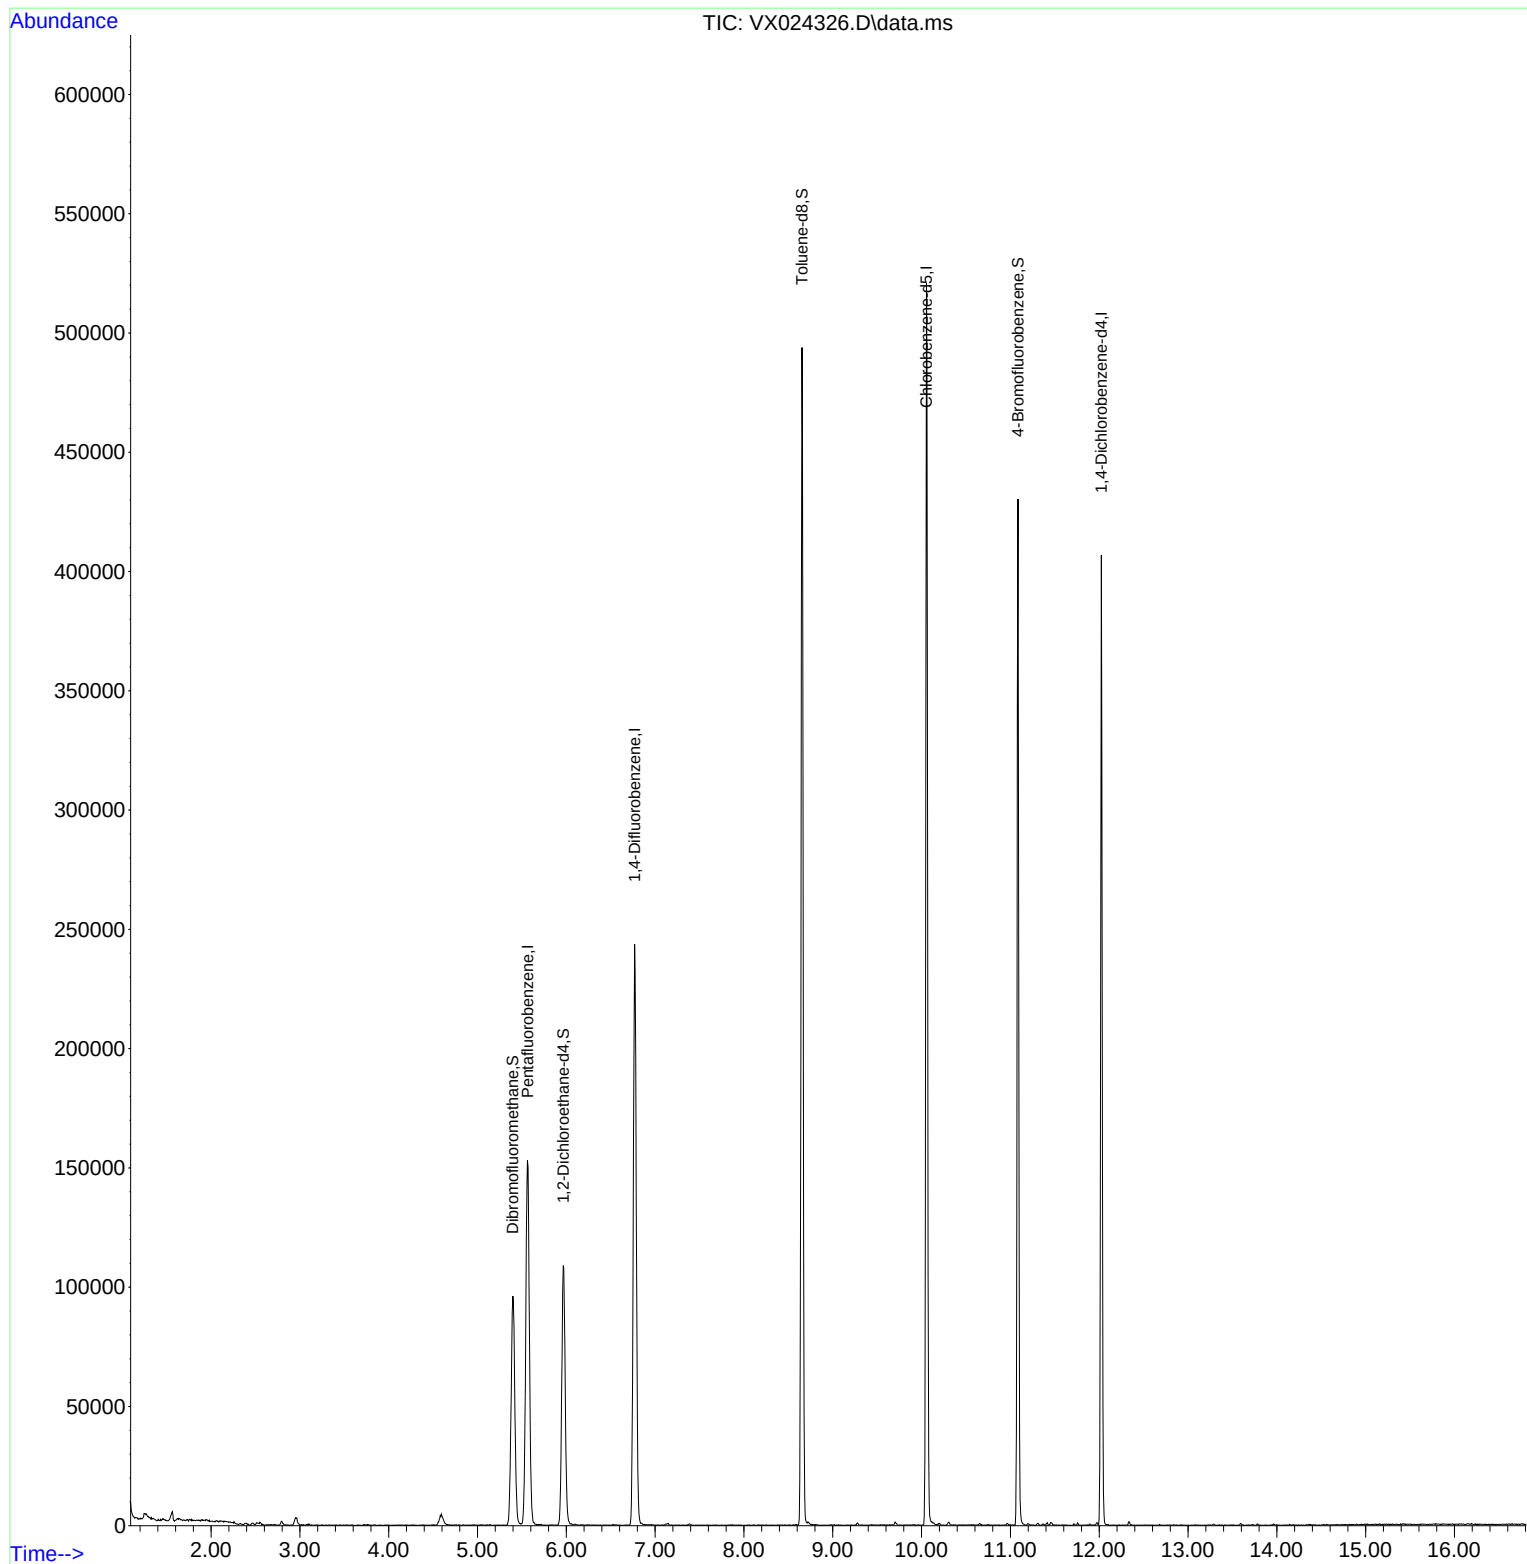


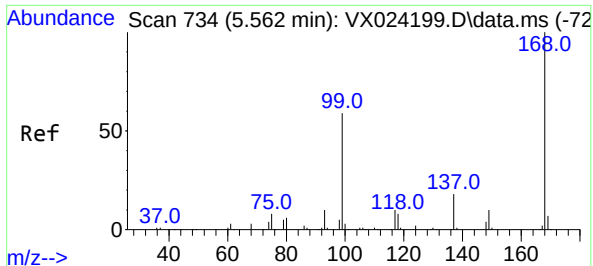

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX024326.D
Acq: 17 Sep 2021 23:01




Instrument :
MSVOA_X
ClientSampleId :
VX0917WBL02


Tgt Ion:168 Resp: 142501
Ion Ratio Lower Upper
168 100
99 61.7 45.8 68.6

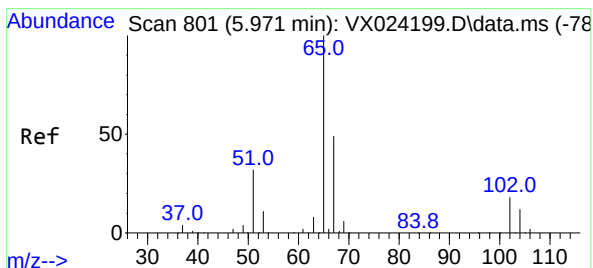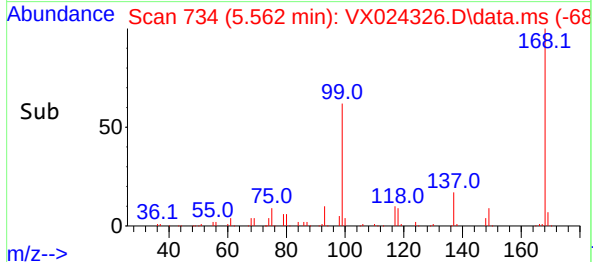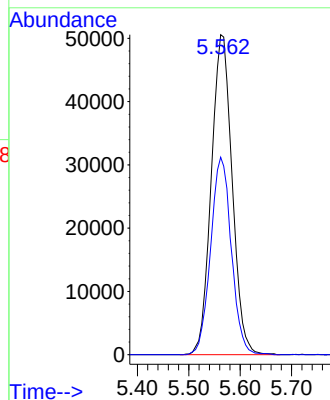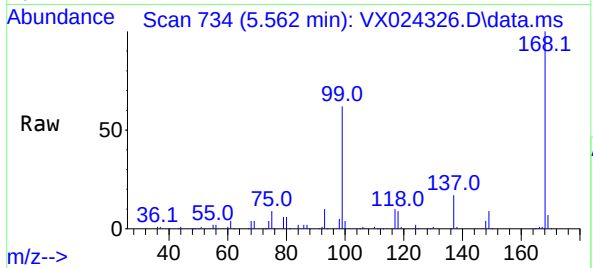

#33
1,2-Dichloroethane-d4
Concen: 54.516 ug/l
RT: 5.964 min Scan# 800
Delta R.T. -0.007 min
Lab File: VX024326.D
Acq: 17 Sep 2021 23:01

Tgt Ion: 65 Resp: 110777
Ion Ratio Lower Upper
65 100
67 51.3 0.0 105.4


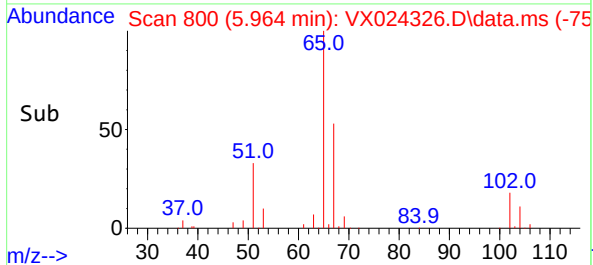
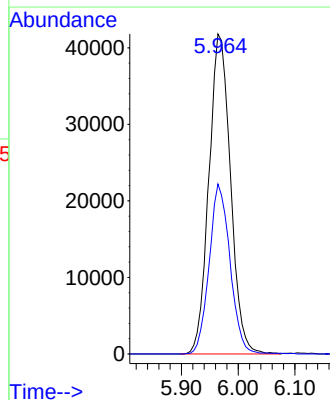
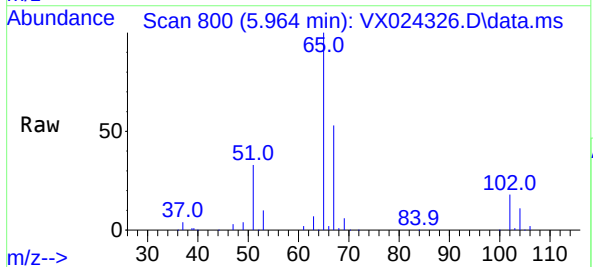


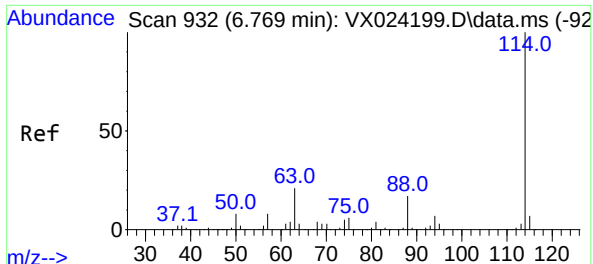

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX024326.D
Acq: 17 Sep 2021 23:01




Instrument :
MSVOA_X
ClientSampleId :
VX0917WBL02


Tgt Ion:114 Resp: 240715
Ion Ratio Lower Upper
114 100
63 20.5 0.0 40.8
88 16.1 0.0 32.8

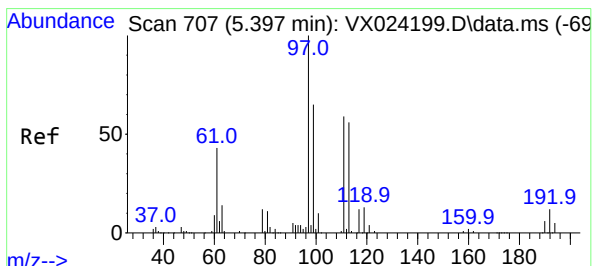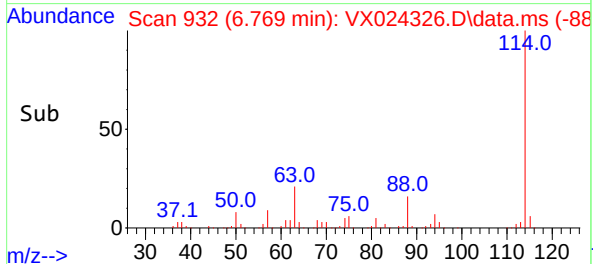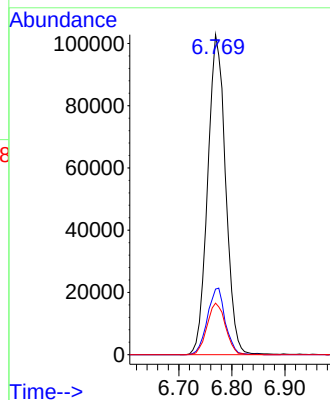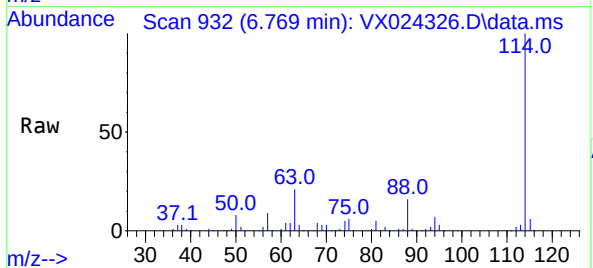

#35
Dibromofluoromethane
Concen: 51.414 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX024326.D
Acq: 17 Sep 2021 23:01

Tgt Ion:113 Resp: 82999
Ion Ratio Lower Upper
113 100
111 101.6 81.9 122.9
192 19.6 16.7 25.1


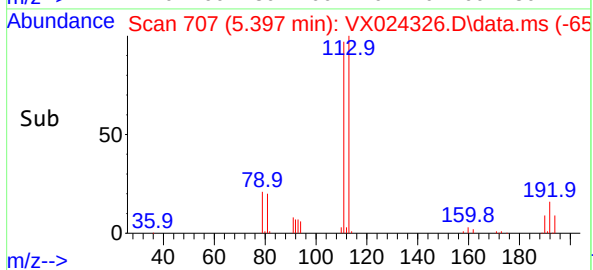
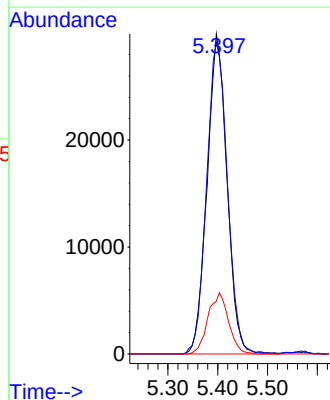
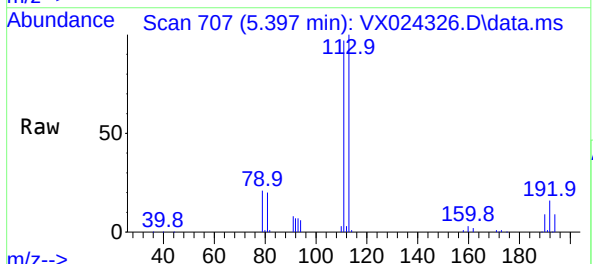


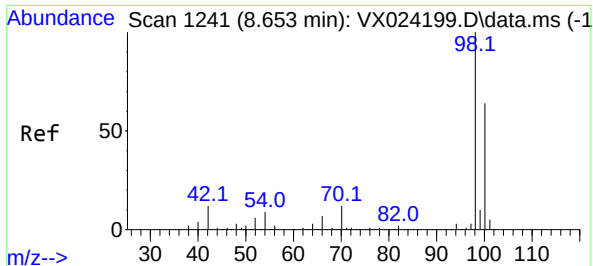

#50
Toluene-d8
Concen: 48.248 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX024326.D
Acq: 17 Sep 2021 23:01




Instrument :
MSVOA_X
ClientSampleId :
VX0917WBL02


Tgt Ion: 98 Resp: 283747
Ion Ratio Lower Upper
98 100
100 63.8 51.9 77.9

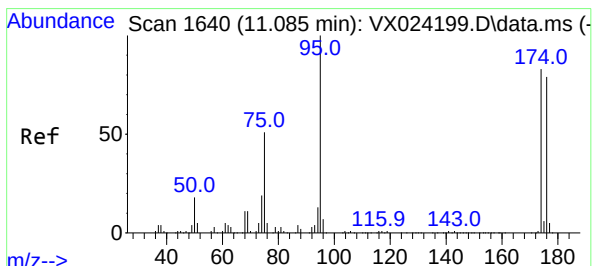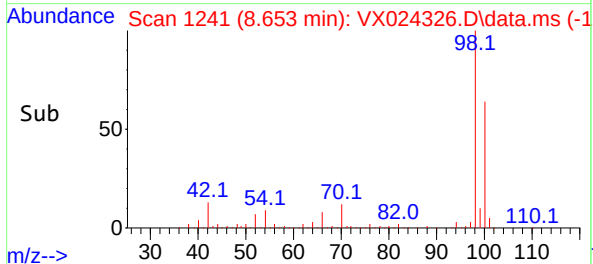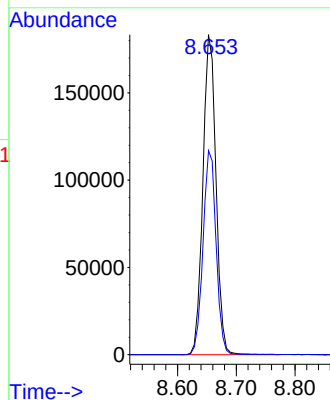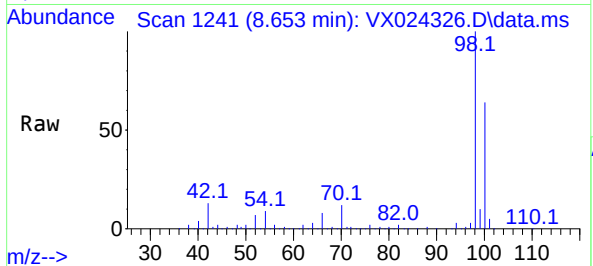

#62
4-Bromofluorobenzene
Concen: 47.917 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX024326.D
Acq: 17 Sep 2021 23:01

Tgt Ion: 95 Resp: 109667
Ion Ratio Lower Upper
95 100
174 80.4 0.0 154.6
176 76.2 0.0 155.8


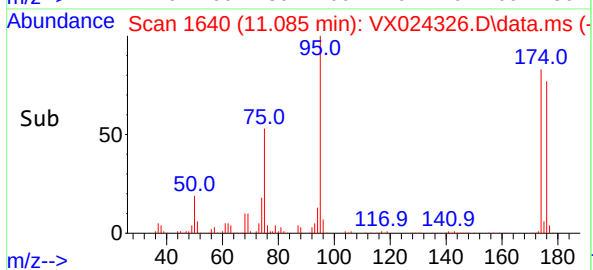
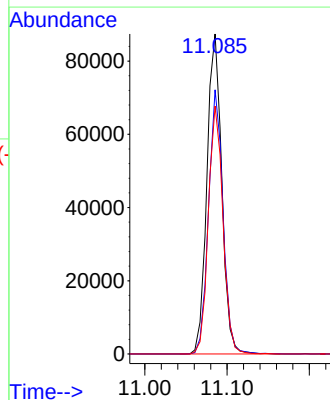
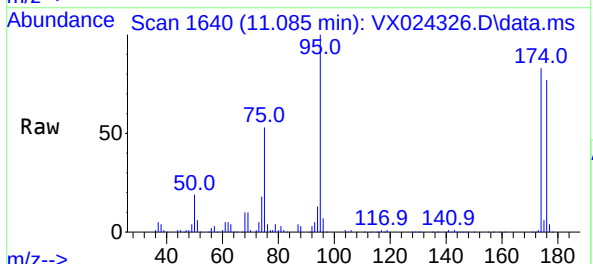


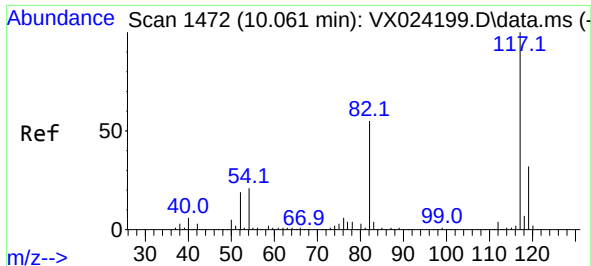

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX024326.D
Acq: 17 Sep 2021 23:01

Instrument :
MSVOA_X
ClientSampleId :
VX0917WBL02

Tgt Ion:117 Resp: 236097
Ion Ratio Lower Upper
117 100
82 58.8 47.4 71.2
119 31.8 26.6 39.8

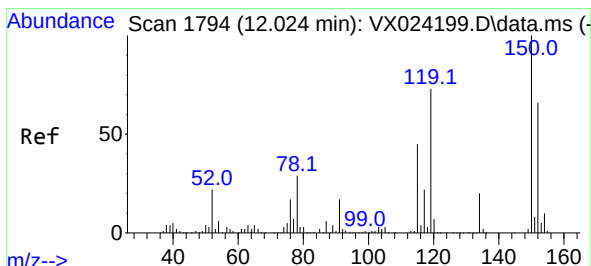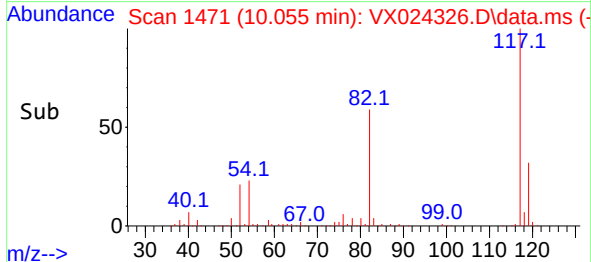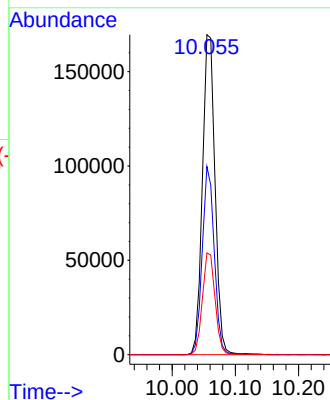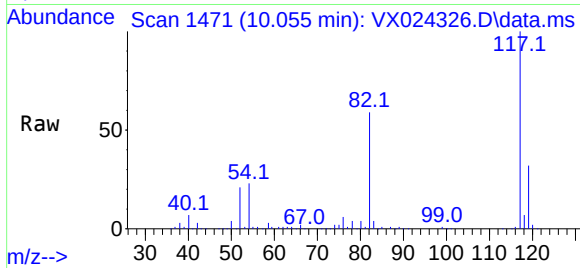

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX024326.D
Acq: 17 Sep 2021 23:01

Tgt Ion:152 Resp: 79802
Ion Ratio Lower Upper
152 100
115 59.8 41.1 123.3
150 157.7 0.0 349.0

