

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091721\
 Data File : VX024336.D
 Acq On : 18 Sep 2021 02:57
 Operator : JC/MD
 Sample : M3782-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE117D2-20210914

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M

Title : SW846 8260

Signal : TIC: VX024336.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	21	27	33	rBV3	5183	9234	1.44%	0.269%
2	2.392	207	214	223	rVB	3429	6411	1.00%	0.187%
3	2.550	233	240	247	rBV	9189	15695	2.45%	0.458%
4	5.397	695	707	723	rBV	76817	221695	34.64%	6.469%
5	5.562	723	734	748	rVB	120445	339636	53.07%	9.910%
6	5.964	788	800	817	rBV	81220	217590	34.00%	6.349%
7	6.769	922	932	942	rBV	194245	461582	72.12%	13.468%
8	8.653	1234	1241	1252	rBV	416767	640025	100.00%	18.675%
9	10.055	1466	1471	1487	rVB	426605	573551	89.61%	16.735%
10	11.085	1634	1640	1653	rVB	350905	440033	68.75%	12.839%
11	12.024	1789	1794	1807	rVB	412805	501810	78.40%	14.642%




Sum of corrected areas: 3427262

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091721\
Data File : VX024336.D
Acq On : 18 Sep 2021 02:57
Operator : JC/MD
Sample : M3782-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D2-20210914

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

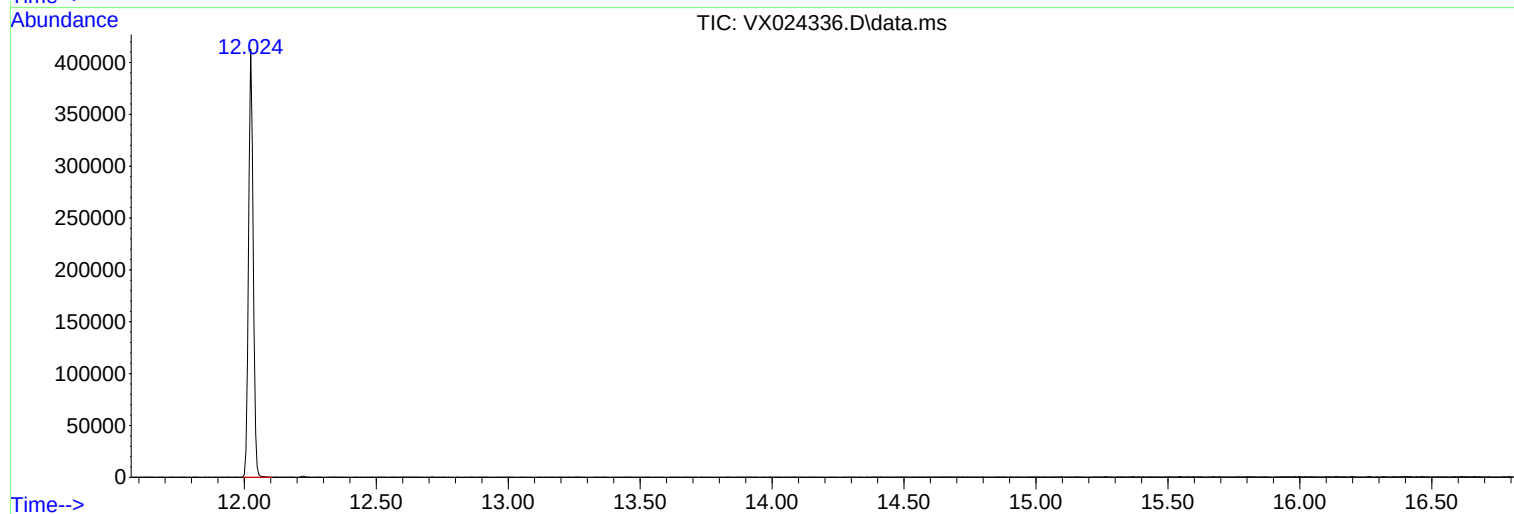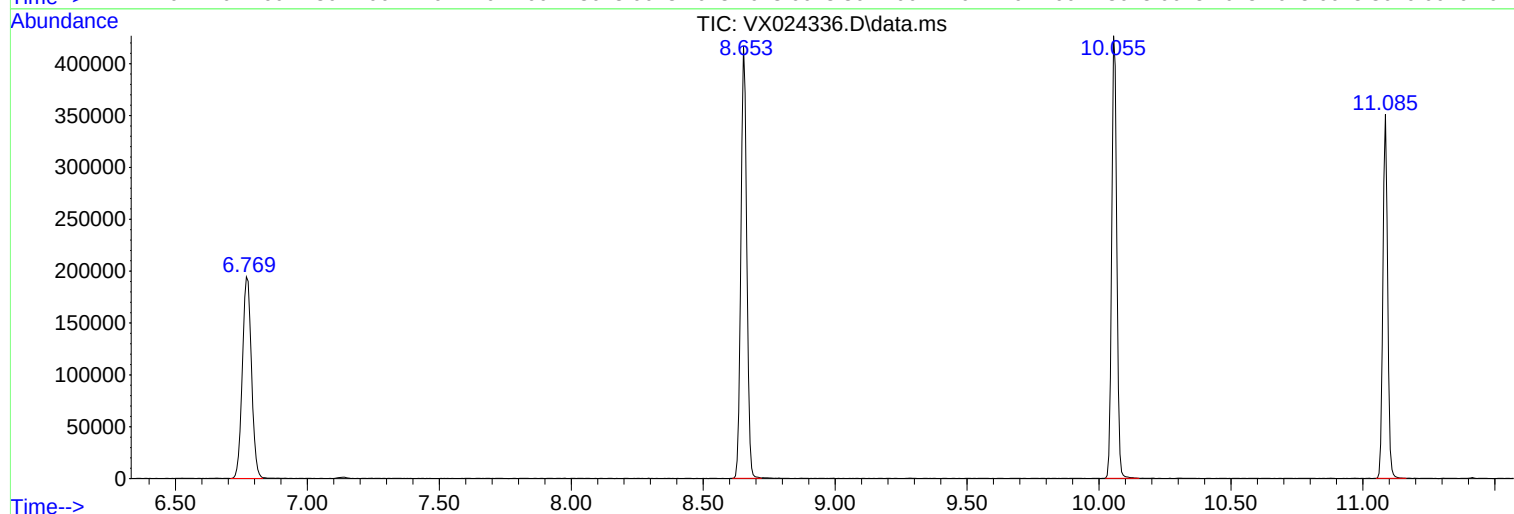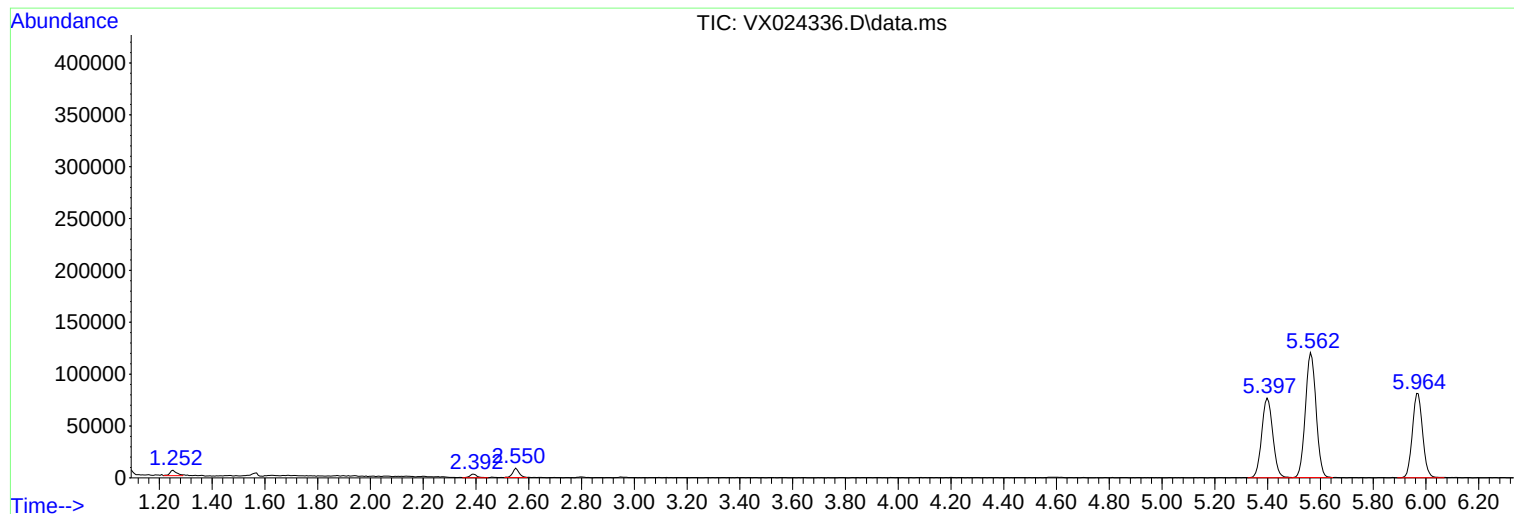

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091721\
Data File : VX024336.D
Acq On : 18 Sep 2021 02:57
Operator : JC/MD
Sample : M3782-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D2-20210914

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091721\
Data File : VX024336.D
Acq On : 18 Sep 2021 02:57
Operator : JC/MD
Sample : M3782-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D2-20210914

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
