
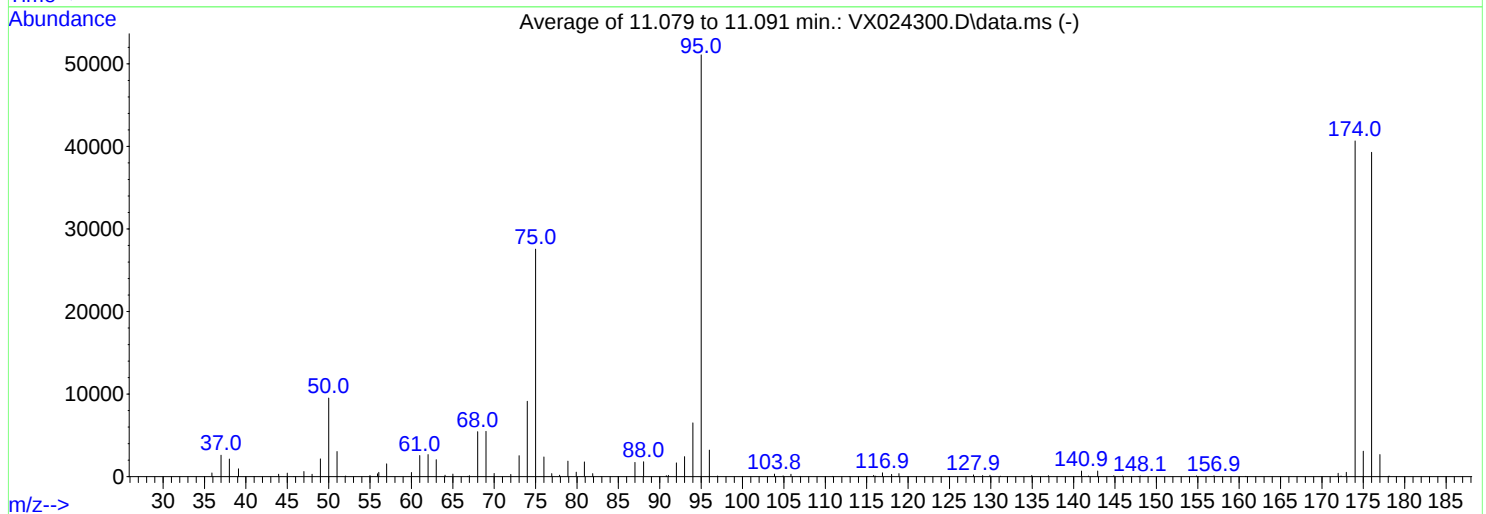


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX091721\  
 Data File : VX024300.D  
 Acq On : 17 Sep 2021 09:16  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091421W.M  
 Title : SW846 8260  
 Last Update : Tue Sep 21 10:52:48 2021

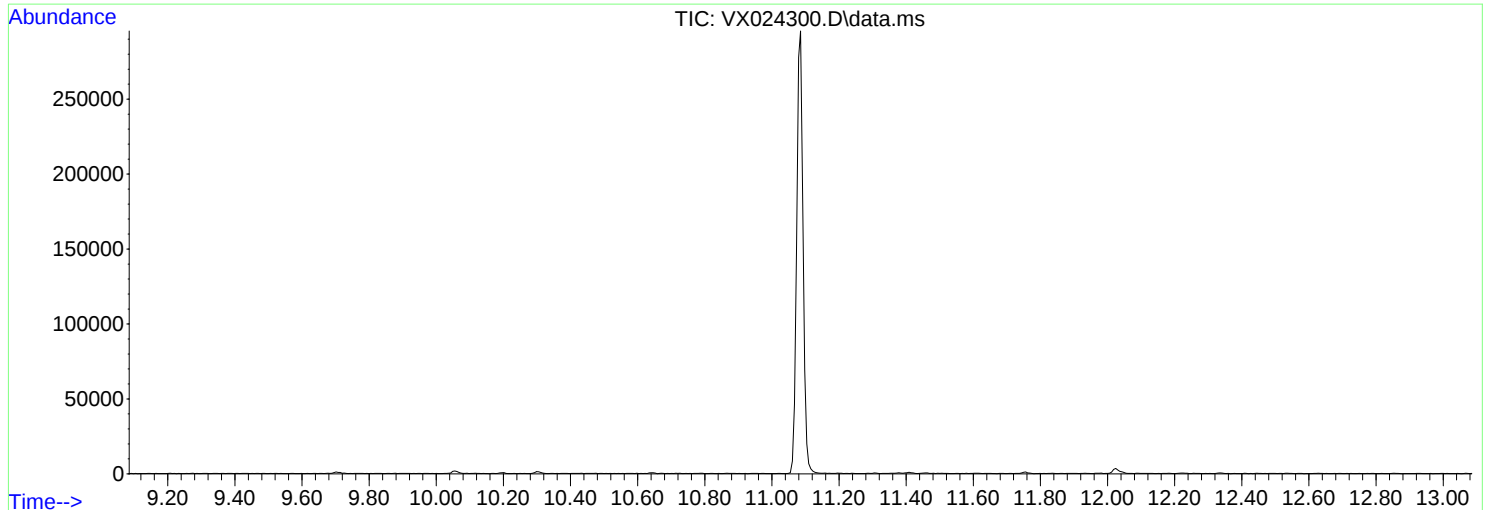

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 18.6         | 9519       | PASS                |
| 75             | 95              | 30              | 60              | 54.0         | 27571      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 51096      | PASS                |
| 96             | 95              | 5               | 9               | 6.3          | 3212       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.3          | 530        | PASS                |
| 174            | 95              | 50              | 100             | 79.6         | 40659      | PASS                |
| 175            | 174             | 5               | 9               | 7.6          | 3085       | PASS                |
| 176            | 174             | 95              | 101             | 96.6         | 39296      | PASS                |
| 177            | 176             | 5               | 9               | 6.8          | 2677       | PASS                |