
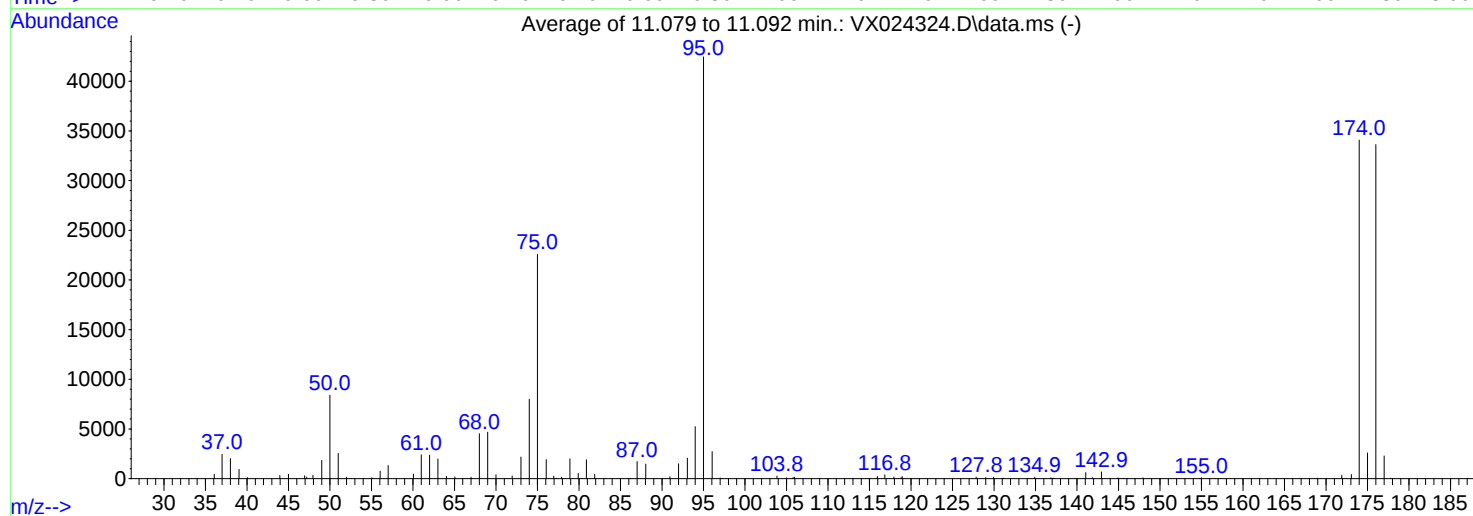


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091721\
 Data File : VX024324.D
 Acq On : 17 Sep 2021 21:27
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
 Title : SW846 8260
 Last Update : Tue Sep 21 10:52:48 2021

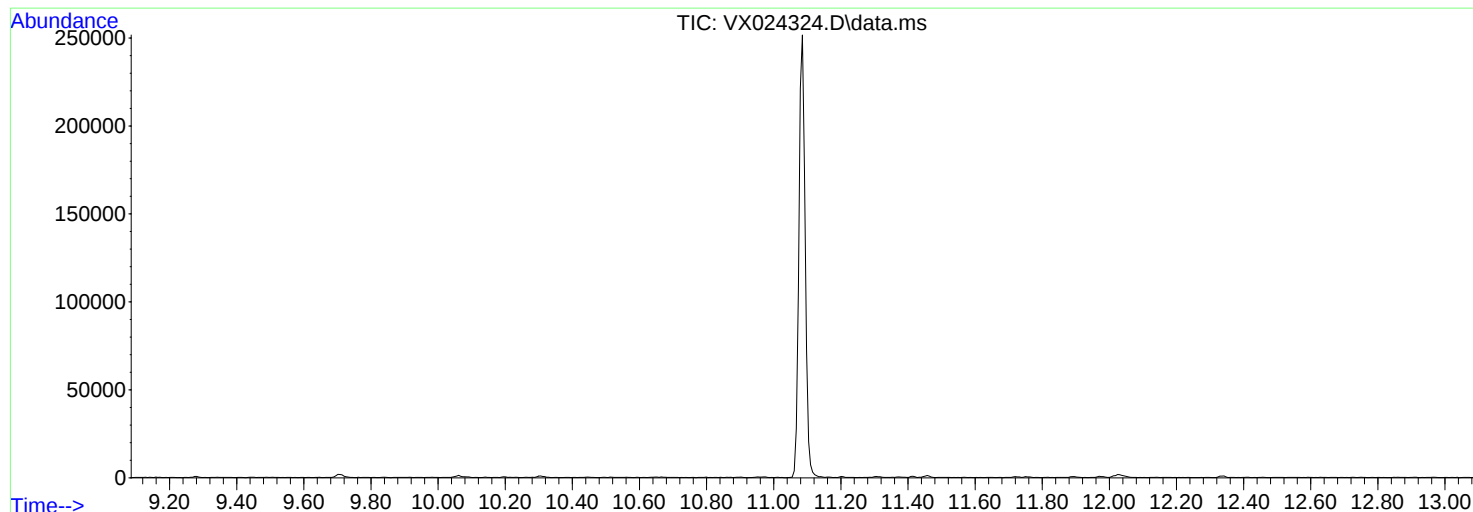

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	8404	PASS
75	95	30	60	53.2	22581	PASS
95	95	100	100	100.0	42456	PASS
96	95	5	9	6.4	2727	PASS
173	174	0.00	2	1.2	414	PASS
174	95	50	100	80.3	34083	PASS
175	174	5	9	7.6	2598	PASS
176	174	95	101	98.7	33632	PASS
177	176	5	9	6.8	2281	PASS