

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091725\
 Data File : VX047609.D
 Acq On : 17 Sep 2025 12:00
 Operator : JC/MD
 Sample : Q3095-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW201D-20250908

Quant Time: Sep 22 03:04:31 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.543	168	164440	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	329692	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	318034	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	152611	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	120762	46.137	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	92.280%
35) Dibromofluoromethane	5.373	113	99168	44.850	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	89.700%
50) Toluene-d8	8.634	98	346603	45.303	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	90.600%#
62) 4-Bromofluorobenzene	11.067	95	145287	50.036	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	100.080%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.178	85	18261	10.724	ug/l	95
7) Trichlorofluoromethane	1.898	101	463624	142.533	ug/l	100
9) 1,1,2-Trichlorotrifluo...	2.337	101	4819	2.534	ug/l	97
11) Tert butyl alcohol	2.934	59	399	1.369	ug/l #	72
12) 1,1-Dichloroethene	2.325	96	88304	45.198	ug/l	94
13) Acrolein	2.251	56	58	0.216	ug/l #	1
16) Acetone	2.373	43	3298	2.898	ug/l	92
19) Methyl tert-butyl Ether	3.111	73	5994	0.840	ug/l	98
20) Methylene Chloride	2.788	84	618	0.257	ug/l #	41
21) trans-1,2-Dichloroethene	3.093	96	807	0.384	ug/l #	75
24) 1,1-Dichloroethane	3.611	63	18699	4.503	ug/l	96
27) cis-1,2-Dichloroethene	4.489	96	5493	2.132	ug/l	92
28) Bromochloromethane	5.098	49	2602	1.435	ug/l #	15
29) Tetrahydrofuran	5.013	42	855	1.001	ug/l #	57
30) Chloroform	5.086	83	31914	7.605	ug/l	94
31) Cyclohexane	5.537	56	3894	1.126	ug/l #	1
32) 1,1,1-Trichloroethane	5.373	97	15234	4.280	ug/l	98
36) 1,1-Dichloropropene	5.537	75	14579	4.512	ug/l #	50
38) Carbon Tetrachloride	5.537	117	18163	5.174	ug/l #	18
42) 1,2-Dichloroethane	6.080	62	1005	0.269	ug/l #	76
44) Trichloroethene	7.110	130	197550	83.268	ug/l	96
49) 1,4-Dioxane	7.653	88	757	26.505	ug/l #	87
51) 4-Methyl-2-Pentanone	8.628	43	1604	0.510	ug/l #	1
55) 1,1,2-Trichloroethane	9.140	97	907	0.389	ug/l #	85
58) 2-Chloroethyl Vinyl ether	8.159	63	20	7.904	ug/l #	47
60) Dibromochloromethane	9.256	129	178560	66.475	ug/l #	11
64) Tetrachloroethene	9.256	164	179402	86.532	ug/l	99
76) 1,2,3-Trichloropropane	11.061	75	75679	24.492	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.061	75	75679	62.459	ug/l #	8
94) Hexachlorobutadiene	13.713	225	314	0.281	ug/l	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091725\
Data File : VX047609.D
Acq On : 17 Sep 2025 12:00
Operator : JC/MD
Sample : Q3095-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW201D-20250908

Quant Time: Sep 22 03:04:31 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:39:58 2025
Response via : Initial Calibration




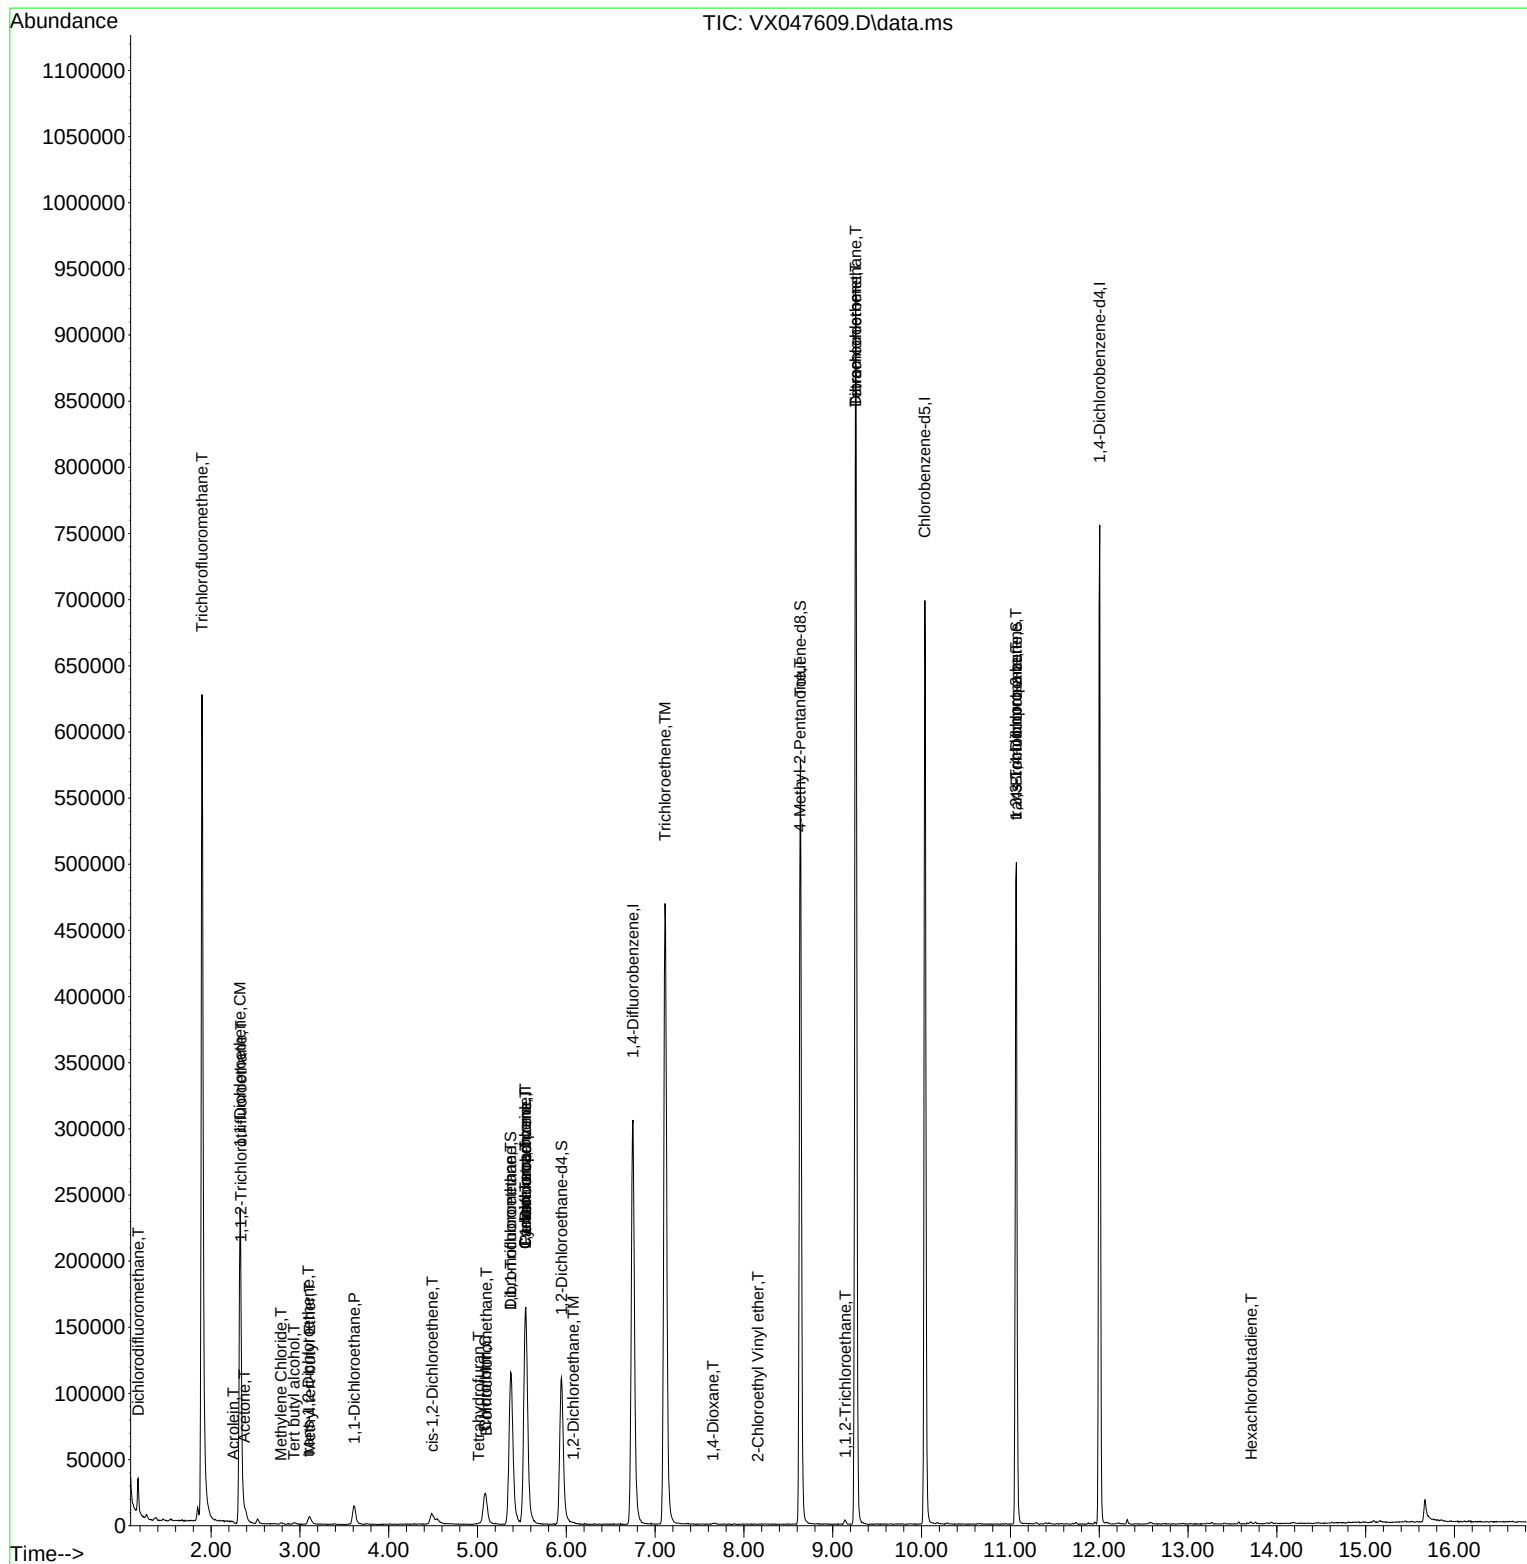




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.543 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00




Instrument :
MSVOA_X
ClientSampleId :
MW201D-20250908


Tgt Ion:168 Resp: 164440
Ion Ratio Lower Upper
168 100
99 63.1 48.8 73.2

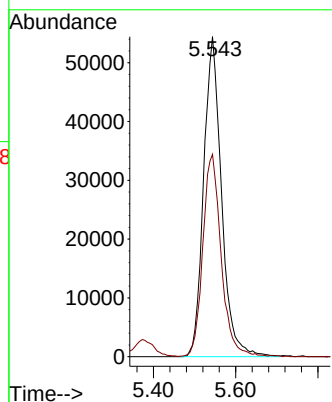

#2
Dichlorodifluoromethane
Concen: 10.724 ug/l
RT: 1.178 min Scan# 15
Delta R.T. 0.006 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00

Tgt Ion: 85 Resp: 18261
Ion Ratio Lower Upper
85 100
87 34.1 15.8 47.3


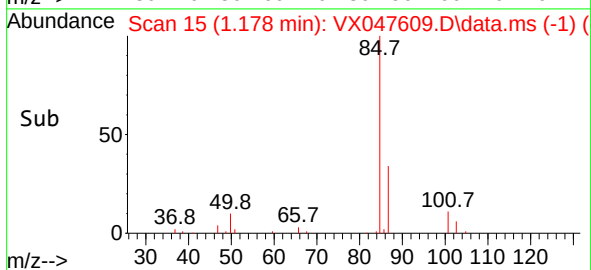
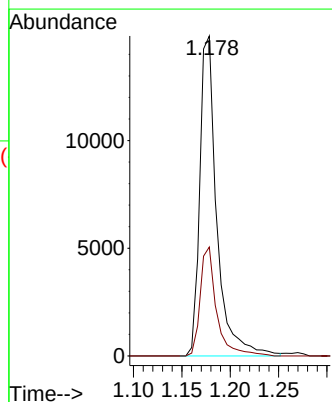





#7
 Trichlorofluoromethane
 Concen: 142.533 ug/l
 RT: 1.898 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX047609.D
 Acq: 17 Sep 2025 12:00




Instrument :
 MSVOA_X
 ClientSampleId :
 MW201D-20250908


Tgt Ion:101 Resp: 463624
 Ion Ratio Lower Upper
 101 100
 103 64.4 51.4 77.2

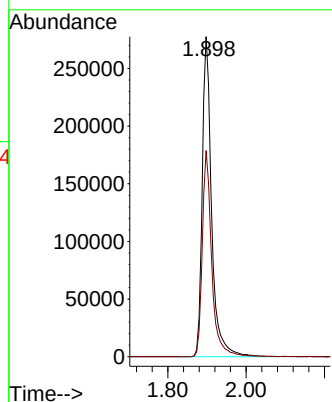

#9
 1,1,2-Trichlorotrifluoroethane
 Concen: 2.534 ug/l
 RT: 2.337 min Scan# 205
 Delta R.T. -0.000 min
 Lab File: VX047609.D
 Acq: 17 Sep 2025 12:00

Tgt Ion:101 Resp: 4819
 Ion Ratio Lower Upper
 101 100
 85 43.7 35.5 53.3
 151 70.6 59.4 89.0

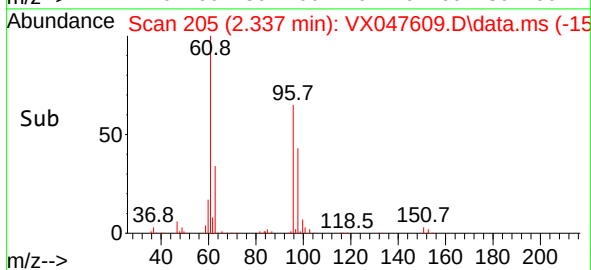

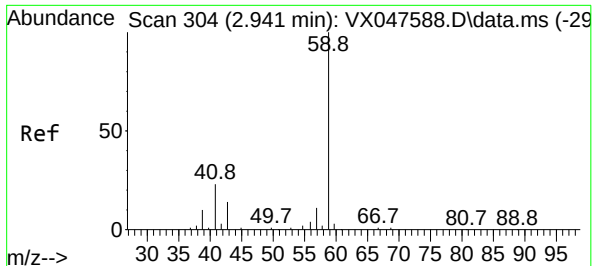

#11

Tert butyl alcohol

Concen: 1.369 ug/l

RT: 2.934 min Scan# 30

Delta R.T. -0.006 min

Lab File: VX047609.D

Acq: 17 Sep 2025 12:00

Instrument :

MSVOA_X

ClientSampleId :





MW201D-20250908

Tgt Ion: 59 Resp: 399

Ion Ratio Lower Upper

59 100

57 0.0 8.3 12.5#

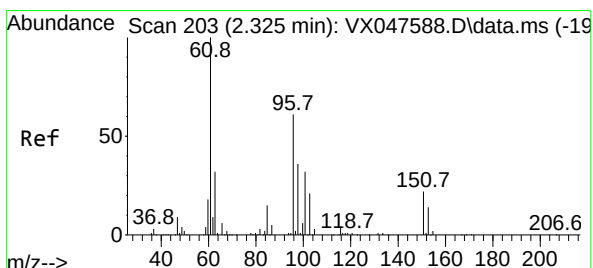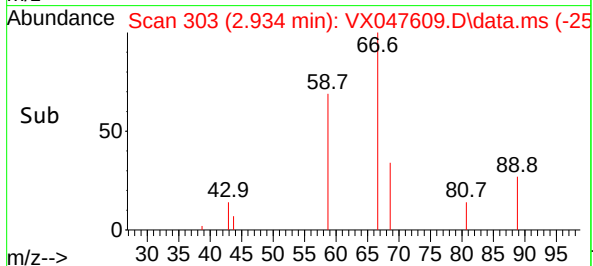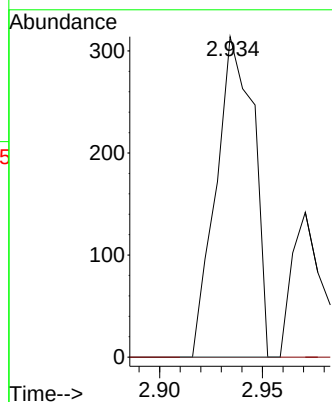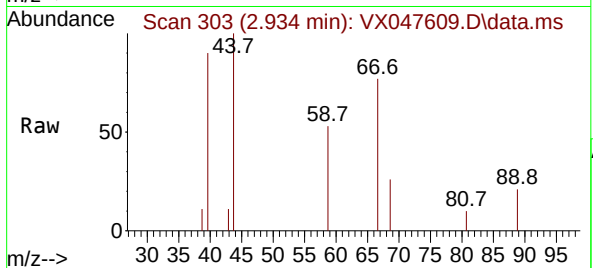

#12

1,1-Dichloroethene

Concen: 45.198 ug/l

RT: 2.325 min Scan# 203

Delta R.T. -0.000 min

Lab File: VX047609.D

Acq: 17 Sep 2025 12:00




Tgt Ion: 96 Resp: 88304


Ion Ratio Lower Upper

96 100

61 171.0 131.0 196.6

98 65.5 47.7 71.5


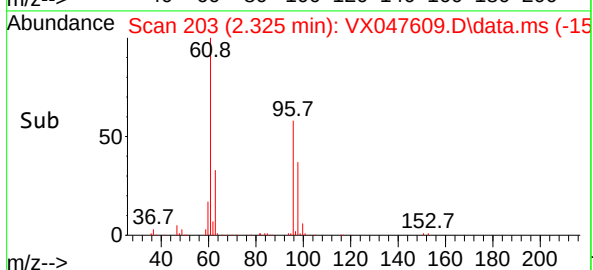

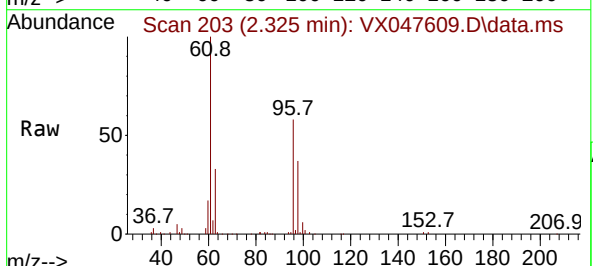




#13
Acrolein
Concen: 0.216 ug/l
RT: 2.251 min Scan# 191
Delta R.T. 0.012 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00




Instrument :
MSVOA_X
ClientSampleId :
MW201D-20250908


Tgt Ion: 56 Resp: 58
Ion Ratio Lower Upper
56 100
55 375.9 57.2 85.8#

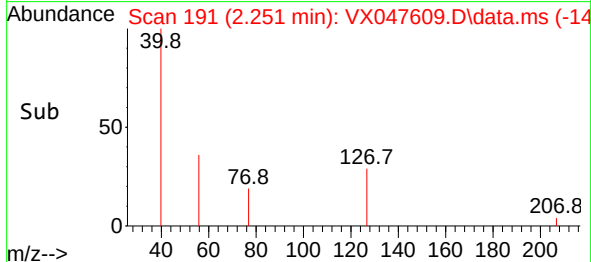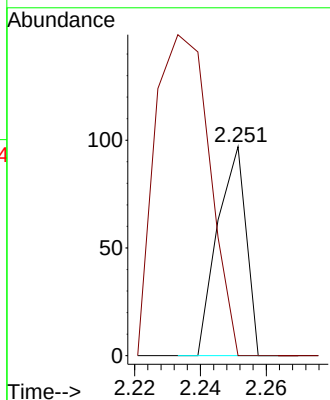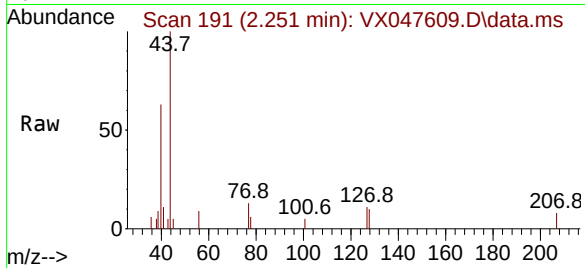

#16
Acetone
Concen: 2.898 ug/l
RT: 2.373 min Scan# 211
Delta R.T. -0.000 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00

Tgt Ion: 43 Resp: 3298
Ion Ratio Lower Upper
43 100
58 24.7 23.4 35.0


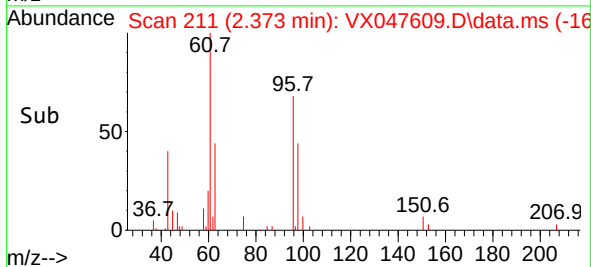
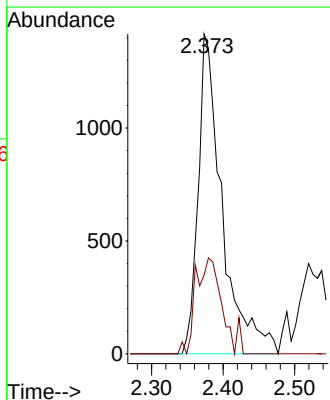
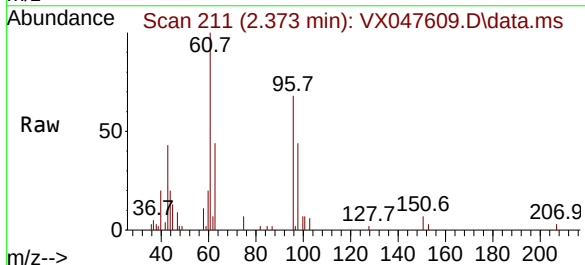




#19
Methyl tert-butyl Ether
Concen: 0.840 ug/l
RT: 3.111 min Scan# 311
Delta R.T. -0.000 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00




Instrument :
MSVOA_X
ClientSampleId :
MW201D-20250908


Tgt Ion: 73 Resp: 5994
Ion Ratio Lower Upper
73 100
57 21.0 17.4 26.2

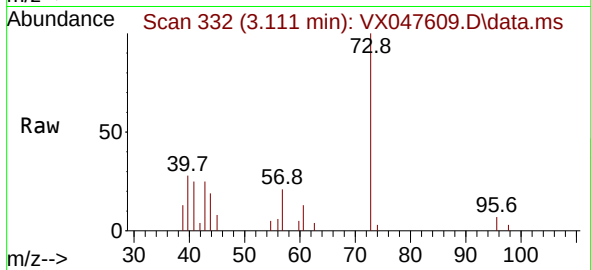

#20
Methylene Chloride
Concen: 0.257 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00

Tgt Ion: 84 Resp: 618
Ion Ratio Lower Upper
84 100
49 53.9 108.6 162.8#
51 22.8 32.6 48.8#
86 18.8 52.0 78.0#


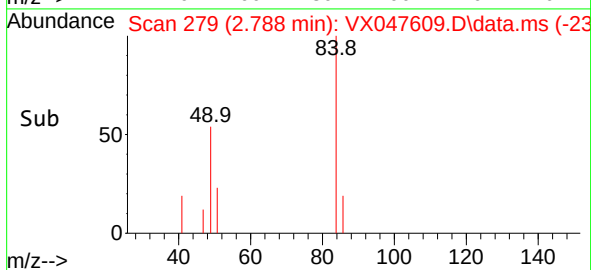

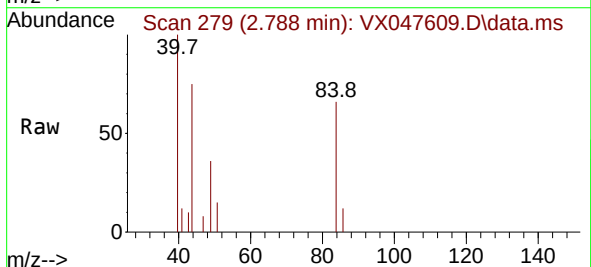




#21
trans-1,2-Dichloroethene
Concen: 0.384 ug/l
RT: 3.093 min Scan# 31
Delta R.T. -0.000 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00




Instrument :
MSVOA_X
ClientSampleId :
MW201D-20250908


Tgt Ion: 96 Resp: 807
Ion Ratio Lower Upper
96 100
61 115.9 116.2 174.2#
98 39.6 49.3 73.9#

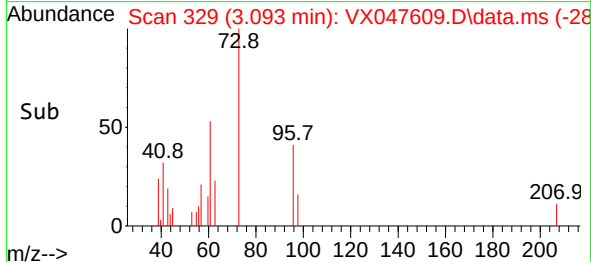

#24
1,1-Dichloroethane
Concen: 4.503 ug/l
RT: 3.611 min Scan# 414
Delta R.T. 0.006 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00

Tgt Ion: 63 Resp: 18699
Ion Ratio Lower Upper
63 100
98 5.7 3.8 11.2
100 4.3 2.3 6.9


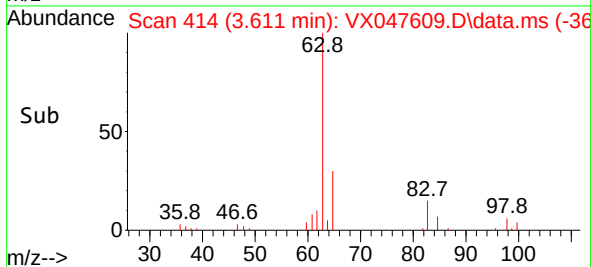

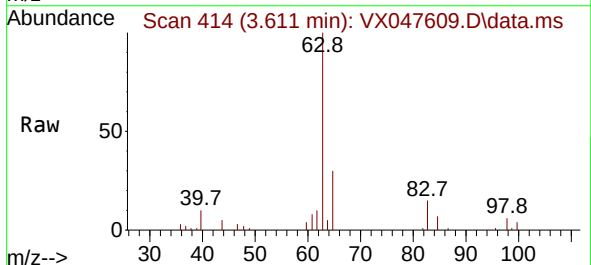




#27
 cis-1,2-Dichloroethene
 Concen: 2.132 ug/l
 RT: 4.489 min Scan# 51
 Delta R.T. 0.006 min
 Lab File: VX047609.D
 Acq: 17 Sep 2025 12:00




Instrument :
 MSVOA_X
 ClientSampleId :
 MW201D-20250908


Tgt Ion: 96 Resp: 5493
 Ion Ratio Lower Upper
 96 100
 61 138.6 0.0 303.2
 98 65.1 0.0 127.8

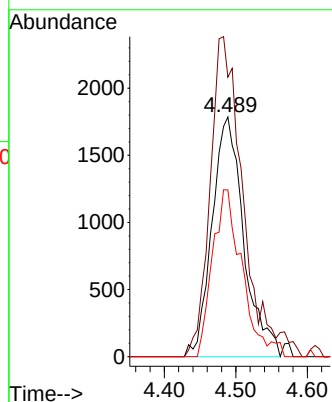

#28
 Bromochloromethane
 Concen: 1.435 ug/l
 RT: 5.098 min Scan# 658
 Delta R.T. 0.207 min
 Lab File: VX047609.D
 Acq: 17 Sep 2025 12:00

Tgt Ion: 49 Resp: 2602
 Ion Ratio Lower Upper
 49 100
 129 0.0 0.0 3.2
 130 0.0 57.8 86.8#

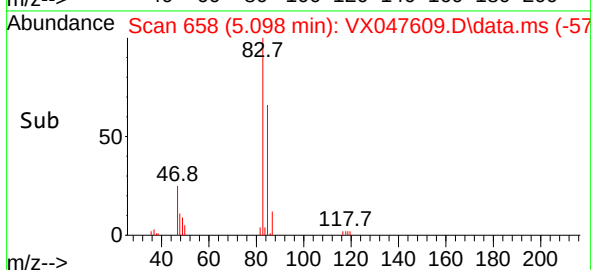



#29

Tetrahydrofuran

Concen: 1.001 ug/l

RT: 5.013 min Scan# 64

Delta R.T. 0.024 min

Lab File: VX047609.D


Acq: 17 Sep 2025 12:00

Instrument :




MSVOA_X

ClientSampleId :

MW201D-20250908



Tgt Ion:	42	Resp:	855
Ion	Ratio	Lower	Upper
42	100		
72	27.7	34.2	51.2#
71	0.0	31.9	47.9#

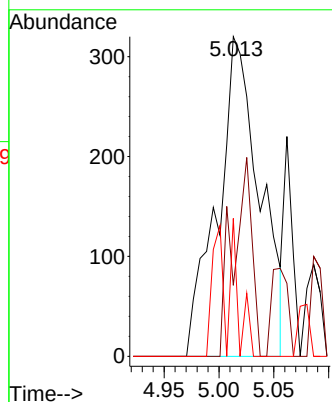

#30

Chloroform

Concen: 7.605 ug/l




RT: 5.086 min Scan# 656


Delta R.T. 0.006 min

Lab File: VX047609.D

Acq: 17 Sep 2025 12:00

Tgt Ion:	83	Resp:	31914
Ion	Ratio	Lower	Upper
83	100		
85	60.0	51.8	77.6


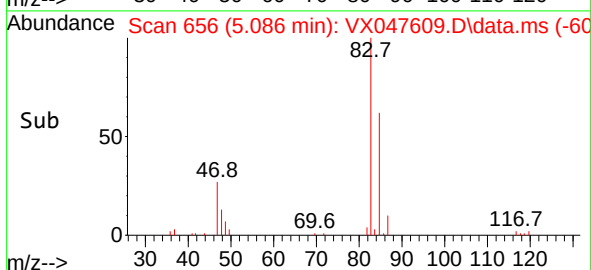






#31
Cyclohexane
Concen: 1.126 ug/l
RT: 5.537 min Scan# 717
Delta R.T. 0.079 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00




Instrument :
MSVOA_X
ClientSampleId :
MW201D-20250908


Tgt Ion: 56 Resp: 3894
Ion Ratio Lower Upper
56 100
69 191.7 23.8 35.8#
84 125.2 64.6 97.0#

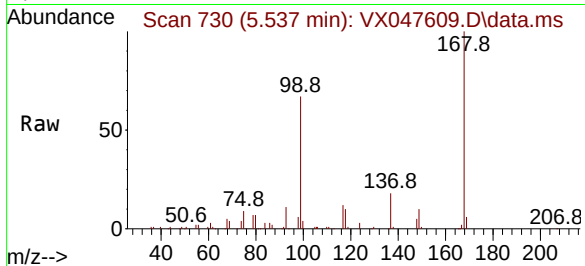

#32
1,1,1-Trichloroethane
Concen: 4.280 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.000 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00

Tgt Ion: 97 Resp: 15234
Ion Ratio Lower Upper
97 100
99 64.2 50.6 76.0
61 46.1 35.8 53.8

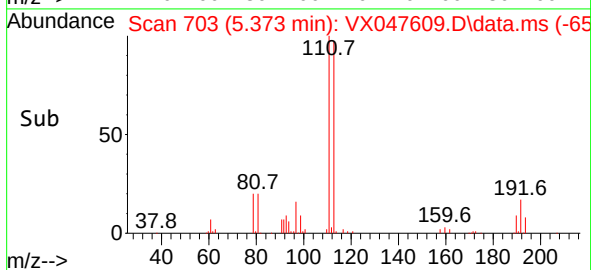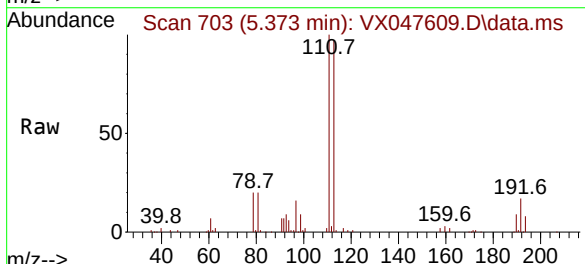



#33

1,2-Dichloroethane-d4

Concen: 46.137 ug/l

RT: 5.946 min Scan# 796

Delta R.T. 0.006 min

Lab File: VX047609.D

Acq: 17 Sep 2025 12:00

Instrument :

MSVOA_X

ClientSampleId :





MW201D-20250908

Tgt Ion: 65 Resp: 120762

Ion Ratio Lower Upper

65 100

67 51.9 0.0 103.0

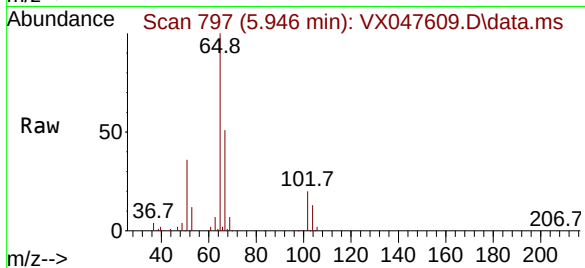

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.751 min Scan# 929

Delta R.T. 0.006 min

Lab File: VX047609.D

Acq: 17 Sep 2025 12:00




Tgt Ion: 114 Resp: 329692


Ion Ratio Lower Upper

114 100

63 21.9 0.0 44.0

88 16.4 0.0 34.2


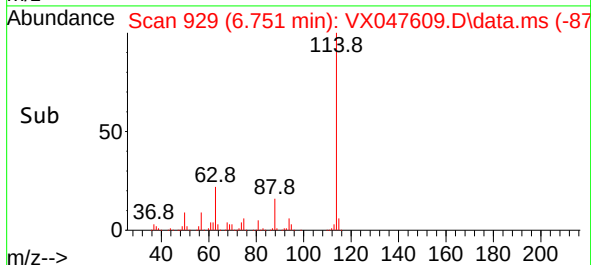
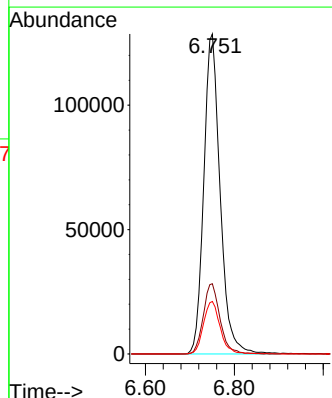
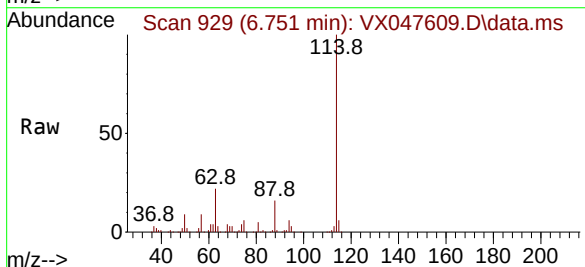


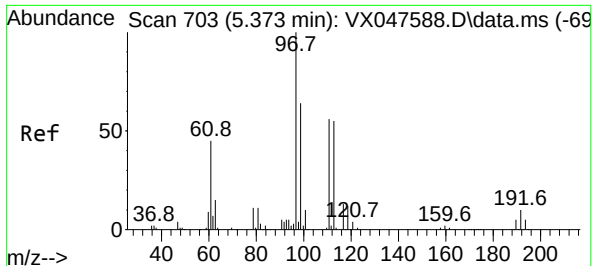

#35
Dibromofluoromethane
Concen: 44.850 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.000 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00




Instrument :
MSVOA_X
ClientSampleId :
MW201D-20250908


Tgt Ion:113 Resp: 99168
Ion Ratio Lower Upper
113 100
111 101.6 80.9 121.3
192 18.0 14.2 21.4

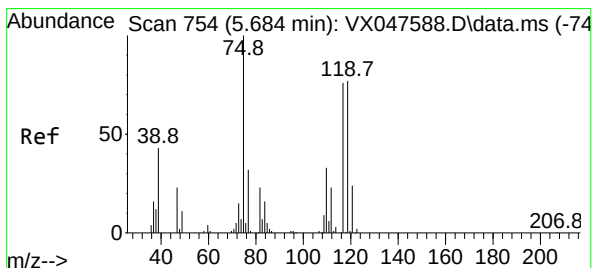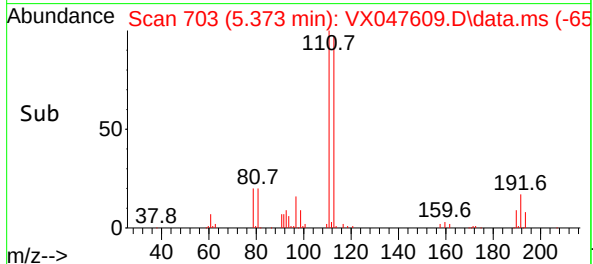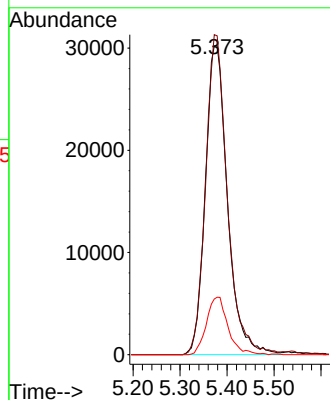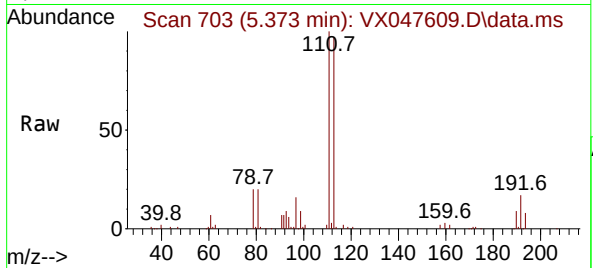

#36
1,1-Dichloropropene
Concen: 4.512 ug/l
RT: 5.537 min Scan# 730
Delta R.T. -0.147 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00

Tgt Ion: 75 Resp: 14579
Ion Ratio Lower Upper
75 100
110 8.3 16.7 50.1#
77 0.0 24.3 36.5#


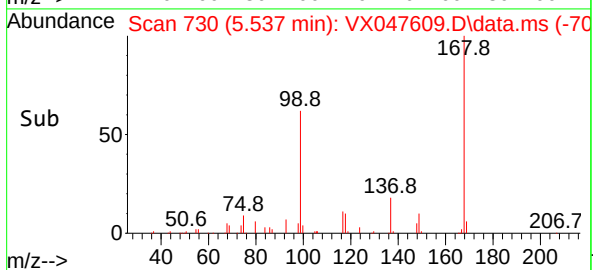
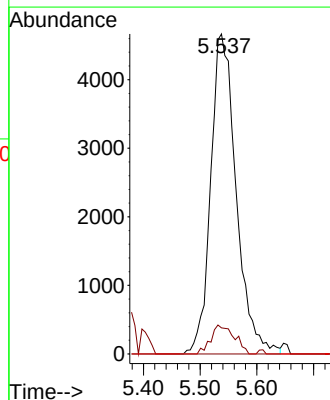
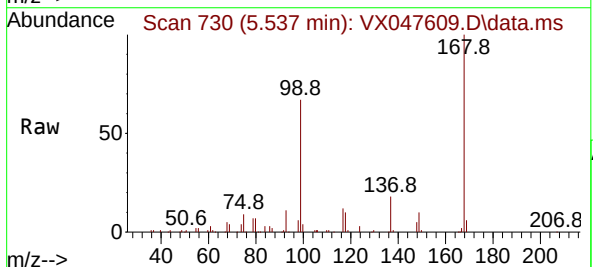




#38
Carbon Tetrachloride
Concen: 5.174 ug/l
RT: 5.537 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00




Instrument :
MSVOA_X
ClientSampleId :
MW201D-20250908


Tgt Ion:117 Resp: 18163
Ion Ratio Lower Upper
117 100
119 5.6 73.4 110.2#
121 0.0 23.8 35.6#

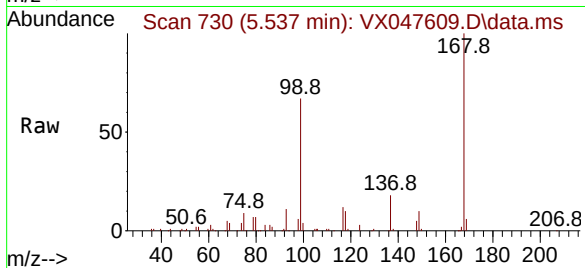

#42
1,2-Dichloroethane
Concen: 0.269 ug/l
RT: 6.080 min Scan# 819
Delta R.T. 0.006 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00

Tgt Ion: 62 Resp: 1005
Ion Ratio Lower Upper
62 100
98 0.0 0.0 17.0


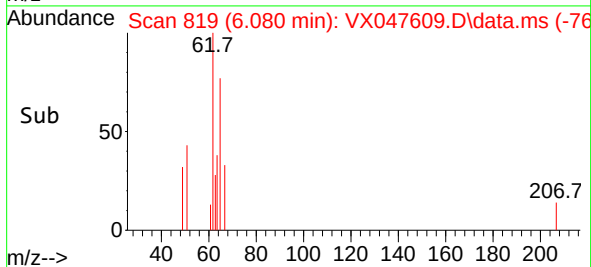

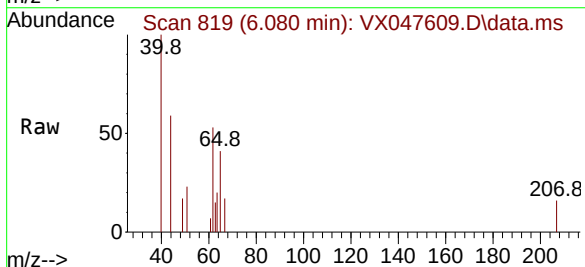




#44
Trichloroethene
Concen: 83.268 ug/l
RT: 7.110 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00




Instrument :
MSVOA_X
ClientSampleId :
MW201D-20250908


Tgt Ion:130 Resp: 197550
Ion Ratio Lower Upper
130 100
95 101.4 0.0 210.8

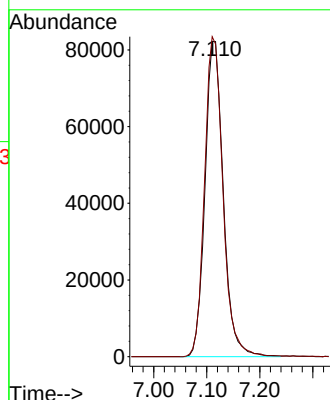

#49
1,4-Dioxane
Concen: 26.505 ug/l
RT: 7.653 min Scan# 1077
Delta R.T. 0.006 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00

Tgt Ion: 88 Resp: 757
Ion Ratio Lower Upper
88 100
43 15.3 30.2 45.2#
58 74.9 59.5 89.3


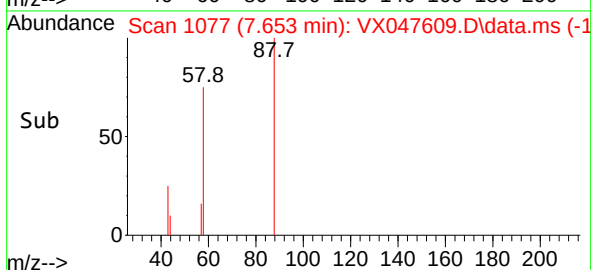
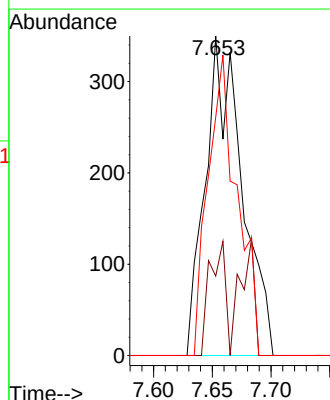
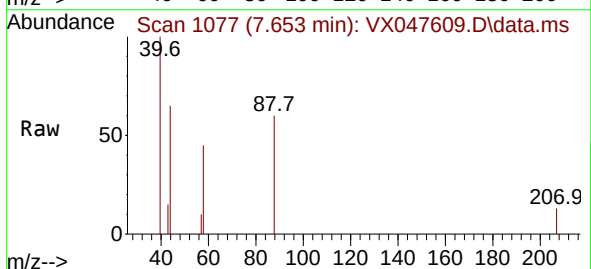




#50
Toluene-d8
Concen: 45.303 ug/l
RT: 8.634 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00




Instrument :
MSVOA_X
ClientSampleId :
MW201D-20250908


Tgt Ion: 98 Resp: 346603
Ion Ratio Lower Upper
98 100
100 67.4 53.0 79.4

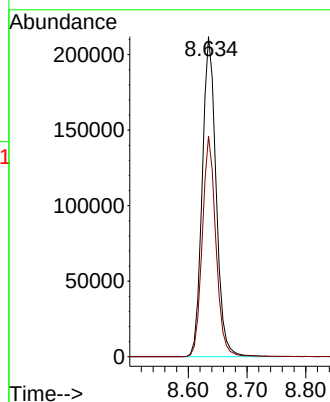

#51
4-Methyl-2-Pentanone
Concen: 0.510 ug/l
RT: 8.628 min Scan# 1237
Delta R.T. 0.067 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00

Tgt Ion: 43 Resp: 1604
Ion Ratio Lower Upper
43 100
58 184.8 30.3 45.5#



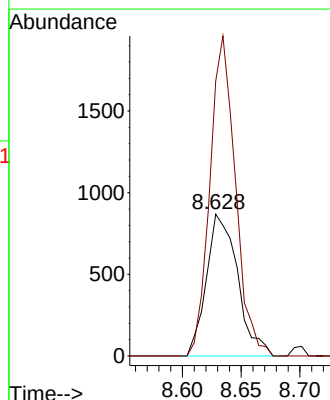
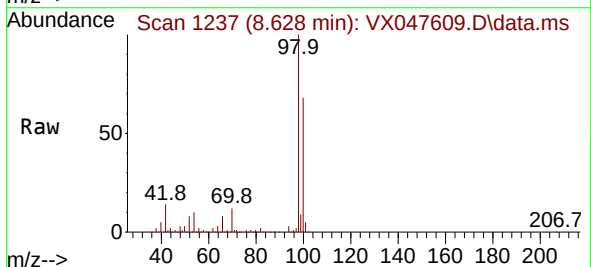


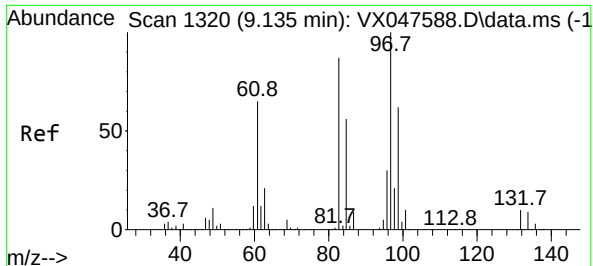

#55
 1,1,2-Trichloroethane
 Concen: 0.389 ug/l
 RT: 9.140 min Scan# 1160
 Delta R.T. 0.006 min
 Lab File: VX047609.D
 Acq: 17 Sep 2025 12:00




Instrument :
 MSVOA_X
 ClientSampleId :
 MW201D-20250908


Tgt Ion: 97	Resp: 907
Ion Ratio	Lower Upper
97 100	
83 61.5	69.6 104.4#
85 50.7	45.0 67.6
99 64.3	49.6 74.4

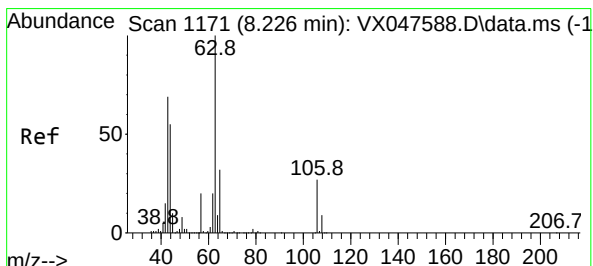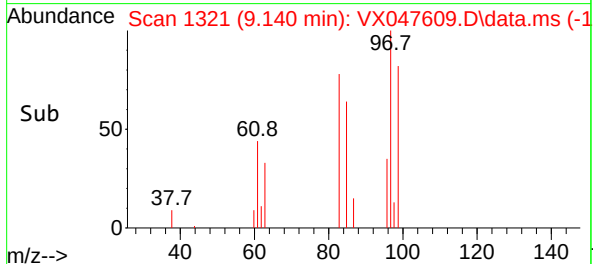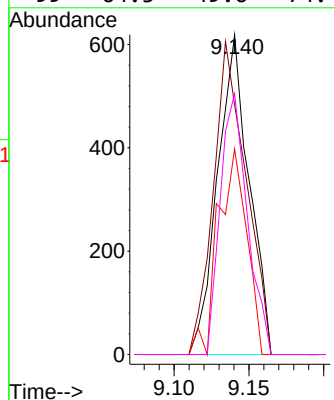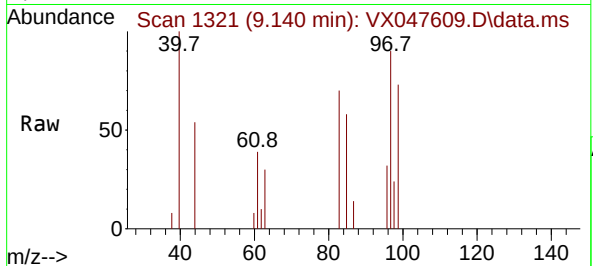

#58
 2-Chloroethyl Vinyl ether
 Concen: 7.904 ug/l
 RT: 8.159 min Scan# 1160
 Delta R.T. -0.067 min
 Lab File: VX047609.D
 Acq: 17 Sep 2025 12:00

Tgt Ion: 63	Resp:	20	
Ion	Ratio	Lower	Upper
63	100		
106	0.0	21.9	32.9#


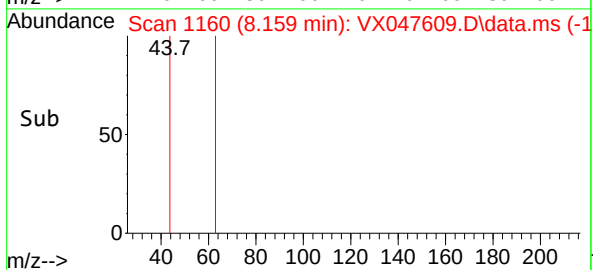
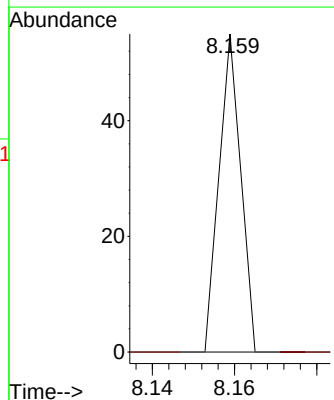
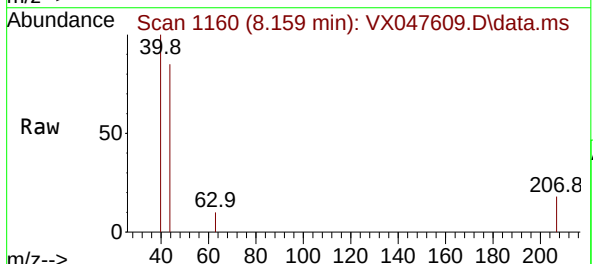




#60
Dibromochloromethane
Concen: 66.475 ug/l
RT: 9.256 min Scan# 11
Delta R.T. -0.250 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00




Instrument :
MSVOA_X
ClientSampleId :
MW201D-20250908


Tgt Ion:129 Resp: 178560
Ion Ratio Lower Upper
129 100
127 0.1 38.4 115.2#

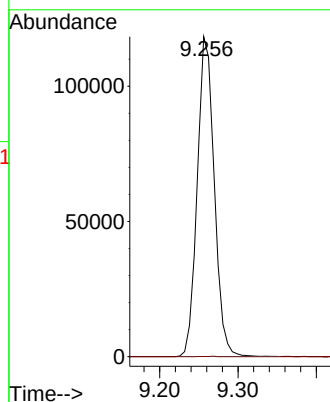

#62
4-Bromofluorobenzene
Concen: 50.036 ug/l
RT: 11.067 min Scan# 1637
Delta R.T. 0.006 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00

Tgt Ion: 95 Resp: 145287
Ion Ratio Lower Upper
95 100
174 71.3 0.0 141.6
176 68.4 0.0 138.4


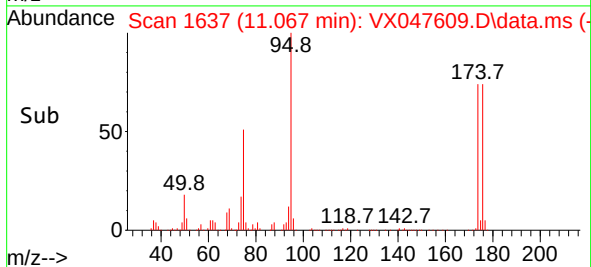
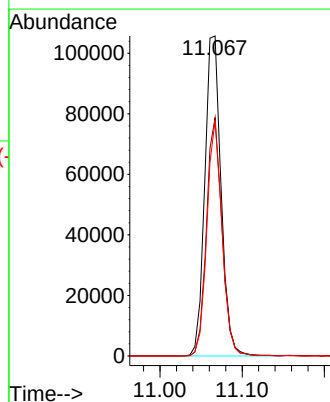
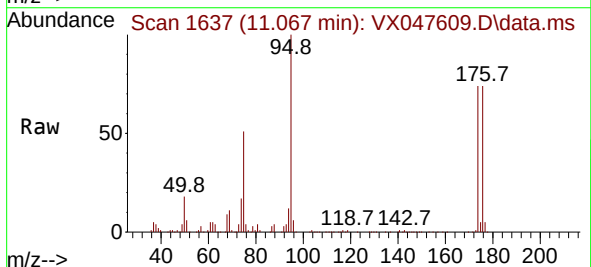




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00




Instrument :
MSVOA_X
ClientSampleId :
MW201D-20250908


Tgt Ion:117 Resp: 318034
Ion Ratio Lower Upper
117 100
82 58.5 47.8 71.6
119 32.0 25.2 37.8

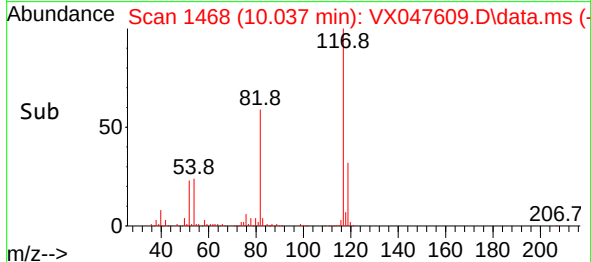

#64
Tetrachloroethene
Concen: 86.532 ug/l
RT: 9.256 min Scan# 1340
Delta R.T. -0.000 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00

Tgt Ion:164 Resp: 179402
Ion Ratio Lower Upper
164 100
166 122.9 100.2 150.2
129 101.7 81.8 122.6
131 97.8 78.6 118.0


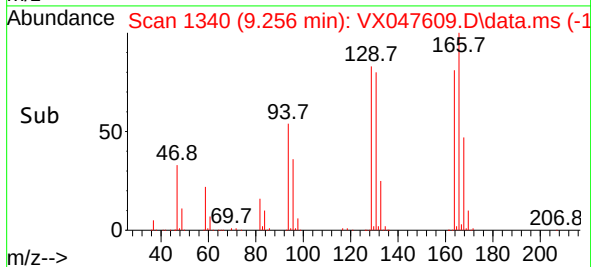

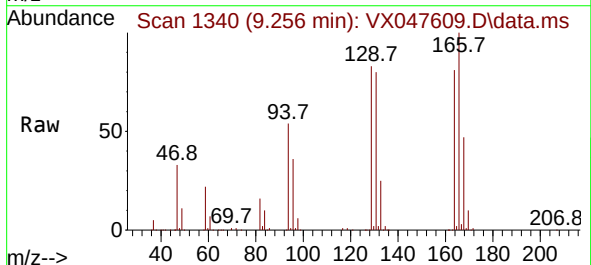




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00




Instrument :
MSVOA_X
ClientSampleId :
MW201D-20250908


Tgt Ion:152 Resp: 152611
Ion Ratio Lower Upper
152 100
115 63.1 44.9 134.5
150 155.5 0.0 352.0

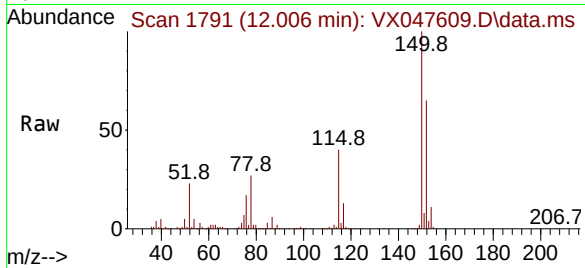

#76
1,2,3-Trichloropropane
Concen: 24.492 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.159 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00

Tgt Ion: 75 Resp: 75679
Ion Ratio Lower Upper
75 100
77 1.2 18.8 56.4#


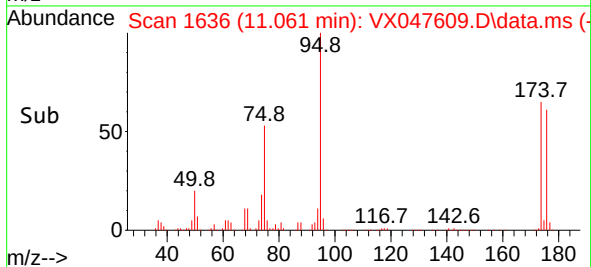

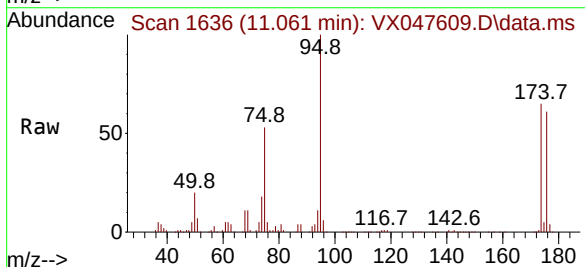




#81
trans-1,4-Dichloro-2-butene
Concen: 62.459 ug/l
RT: 11.061 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00

Instrument :
MSVOA_X
ClientSampleId :
MW201D-20250908

Tgt Ion: 75 Resp: 75679
Ion Ratio Lower Upper
75 100
53 0.0 83.4 125.2#
89 0.0 36.3 54.5#

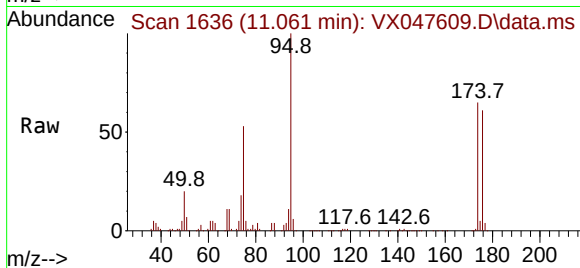

#94
Hexachlorobutadiene
Concen: 0.281 ug/l
RT: 13.713 min Scan# 2071
Delta R.T. 0.006 min
Lab File: VX047609.D
Acq: 17 Sep 2025 12:00

Tgt Ion: 225 Resp: 314
Ion Ratio Lower Upper
225 100
223 72.0 31.7 95.1
227 37.6 32.0 96.0

