

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091725\
 Data File : VX047603.D
 Acq On : 17 Sep 2025 09:41
 Operator : JC/MD
 Sample : VX0917WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0917WBL01

Quant Time: Sep 18 01:59:12 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.538	168	235094	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.745	114	478397	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	460978	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	224854	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	187947	50.225	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	100.440%
35) Dibromofluoromethane	5.373	113	150745	46.985	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.960%
50) Toluene-d8	8.635	98	526623	47.436	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	94.880%
62) 4-Bromofluorobenzene	11.061	95	222687	52.854	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	105.700%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091725\
Data File : VX047603.D
Acq On : 17 Sep 2025 09:41
Operator : JC/MD
Sample : VX0917WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0917WBL01

Quant Time: Sep 18 01:59:12 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:39:58 2025
Response via : Initial Calibration




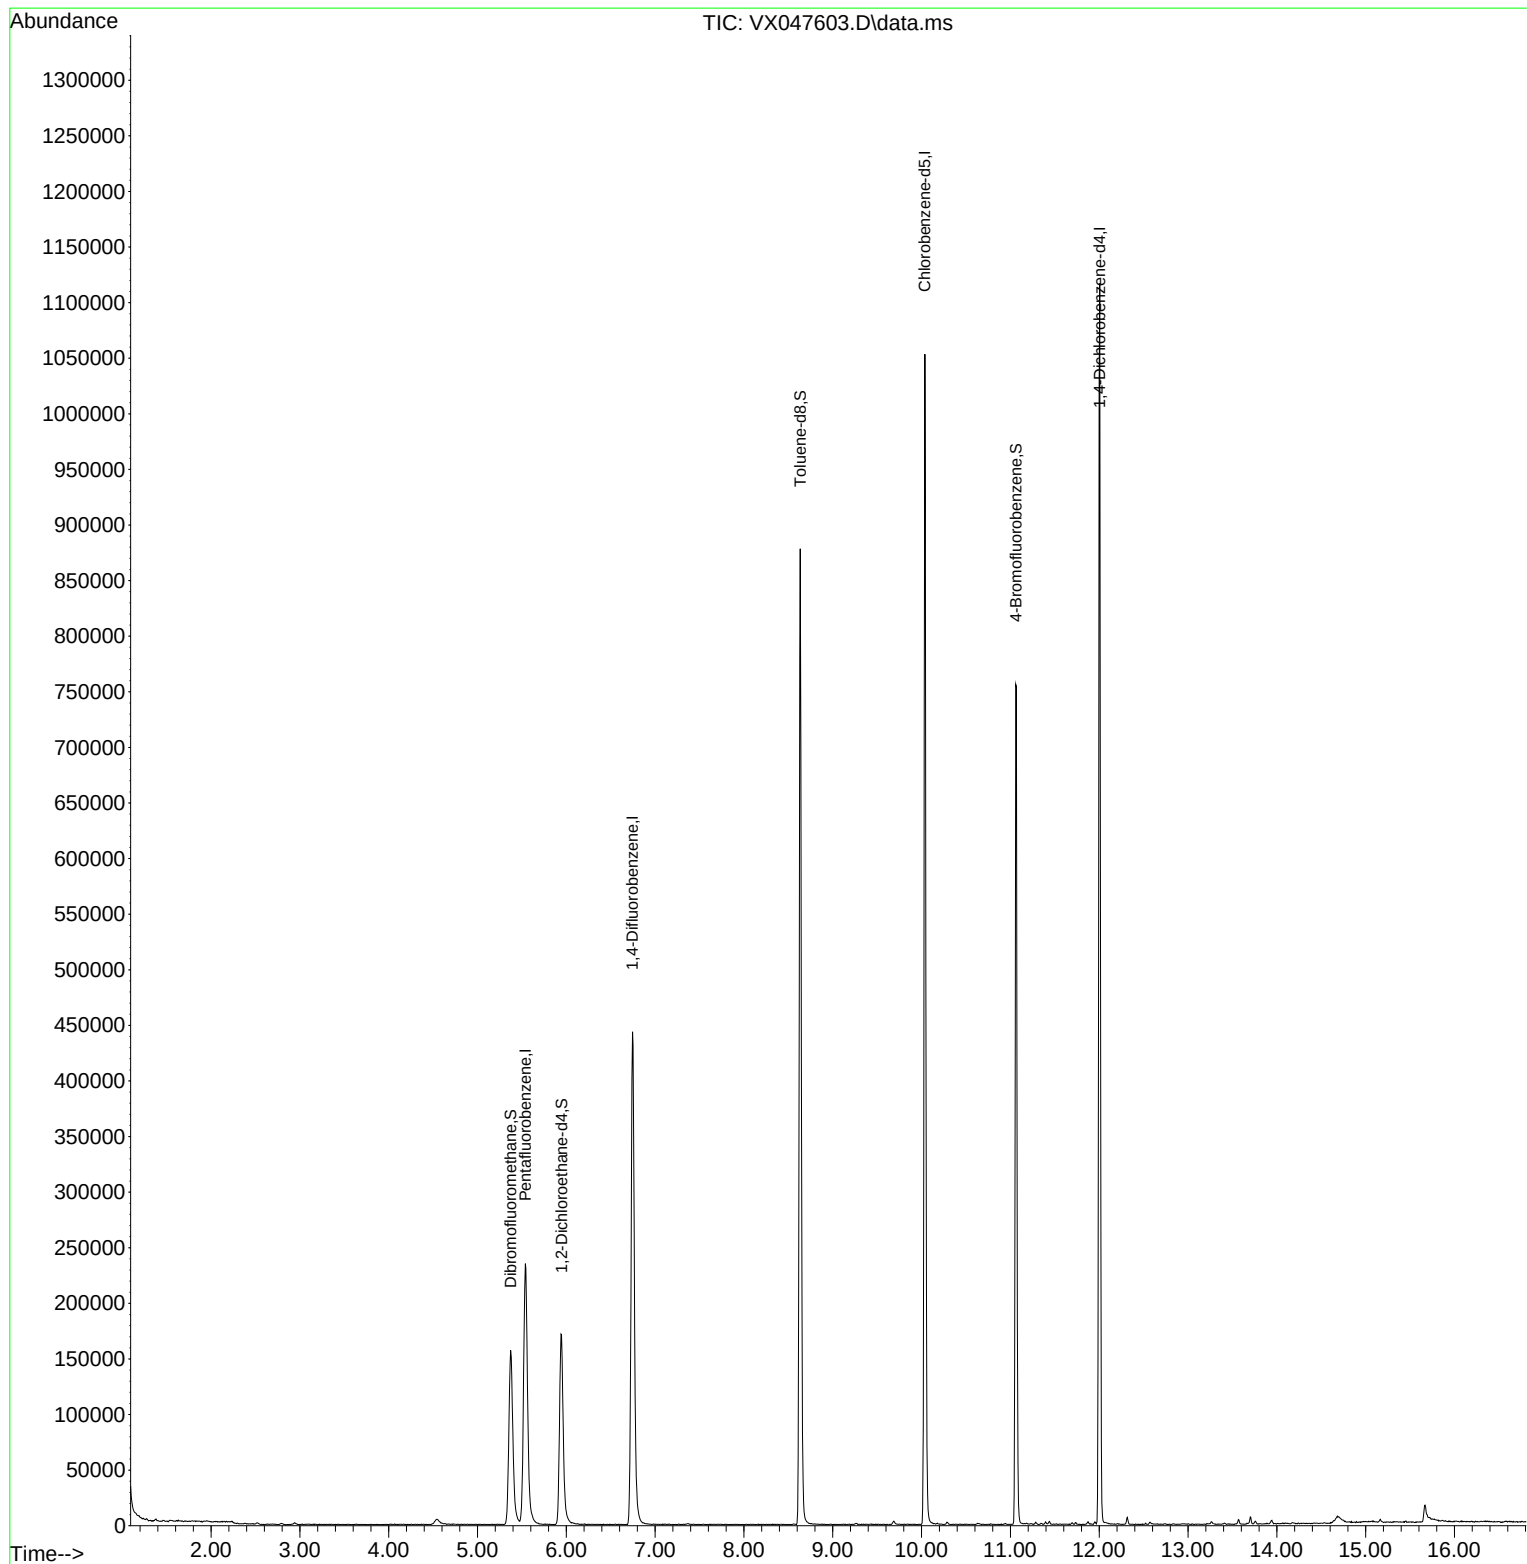


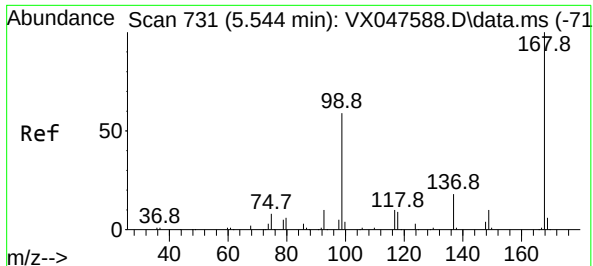

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.538 min Scan# 713
Delta R.T. -0.006 min
Lab File: VX047603.D
Acq: 17 Sep 2025 09:41




Instrument :
MSVOA_X
ClientSampleId :
VX0917WBL01


Tgt Ion:168 Resp: 235094
Ion Ratio Lower Upper
168 100
99 66.3 48.8 73.2

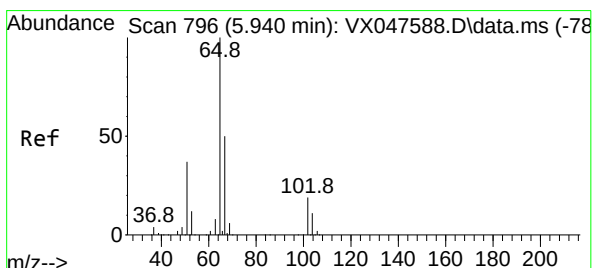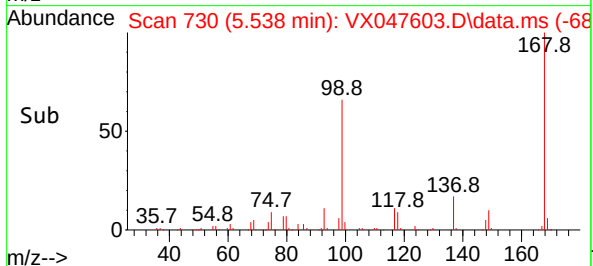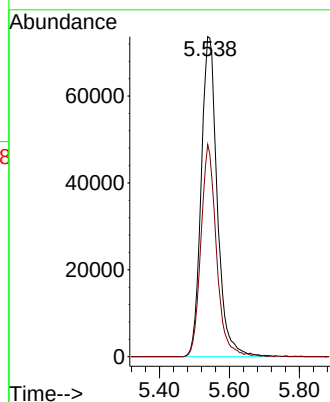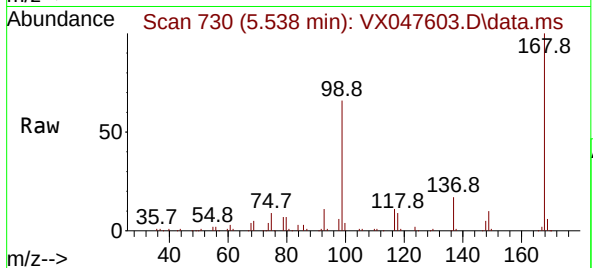

#33
1,2-Dichloroethane-d4
Concen: 50.225 ug/l
RT: 5.946 min Scan# 797
Delta R.T. 0.006 min
Lab File: VX047603.D
Acq: 17 Sep 2025 09:41

Tgt Ion: 65 Resp: 187947
Ion Ratio Lower Upper
65 100
67 50.3 0.0 103.0


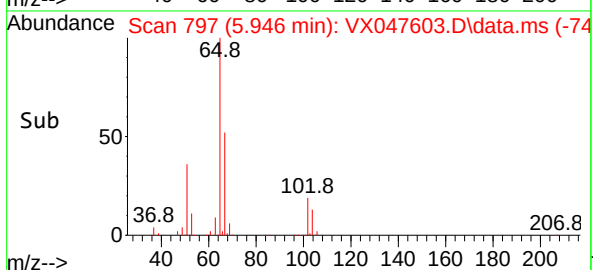
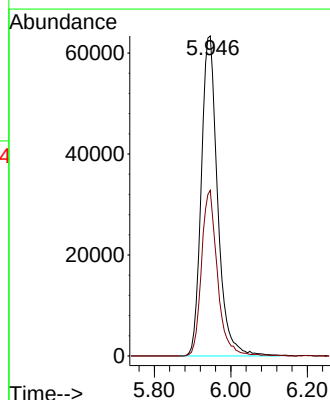
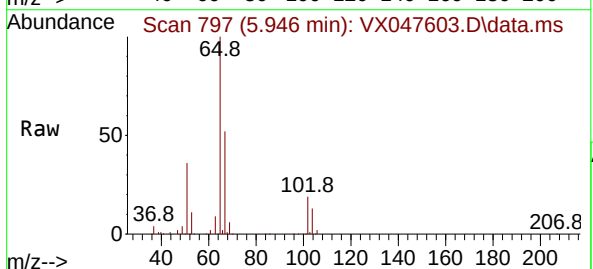


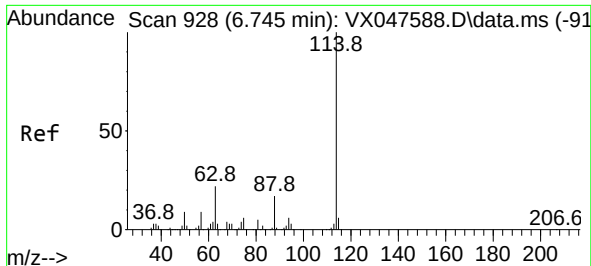

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.745 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: VX047603.D
 Acq: 17 Sep 2025 09:41




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0917WBL01


Tgt Ion:114 Resp: 478397
 Ion Ratio Lower Upper
 114 100
 63 21.8 0.0 44.0
 88 16.8 0.0 34.2

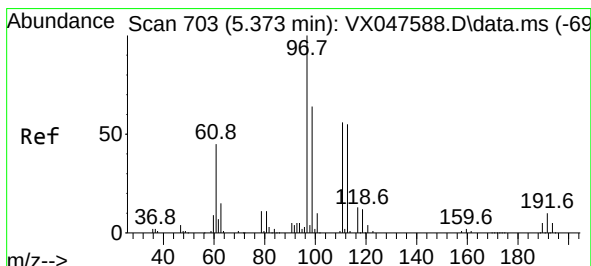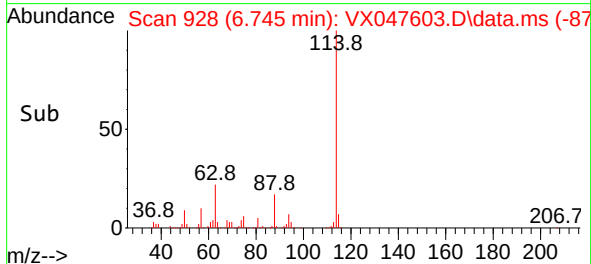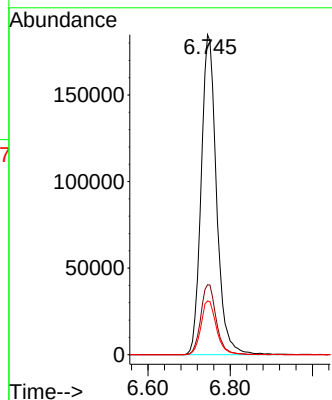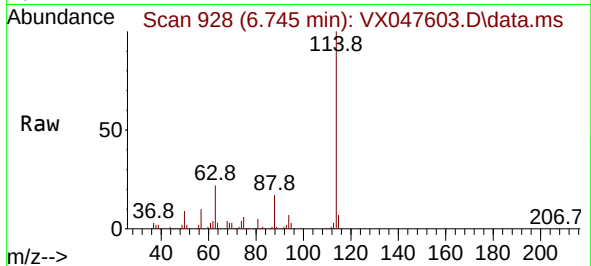

#35
 Dibromofluoromethane
 Concen: 46.985 ug/l
 RT: 5.373 min Scan# 703
 Delta R.T. -0.000 min
 Lab File: VX047603.D
 Acq: 17 Sep 2025 09:41

Tgt Ion:113 Resp: 150745
 Ion Ratio Lower Upper
 113 100
 111 103.5 80.9 121.3
 192 18.2 14.2 21.4


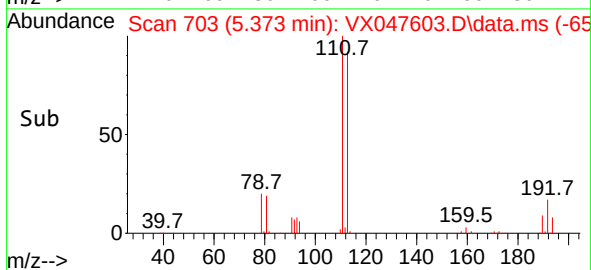
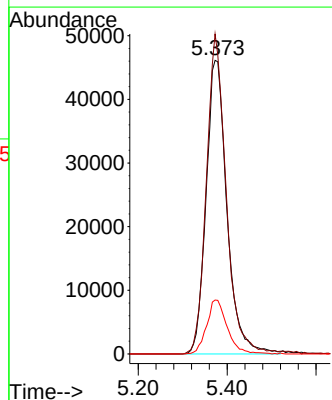
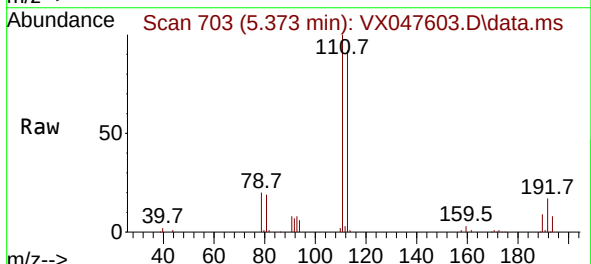


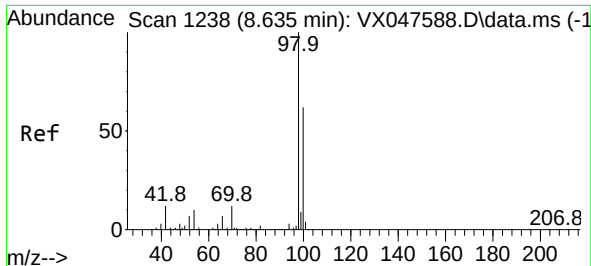

#50
Toluene-d8
Concen: 47.436 ug/l
RT: 8.635 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX047603.D
Acq: 17 Sep 2025 09:41




Instrument :
MSVOA_X
ClientSampleId :
VX0917WBL01


Tgt Ion: 98 Resp: 526623
Ion Ratio Lower Upper
98 100
100 67.1 53.0 79.4

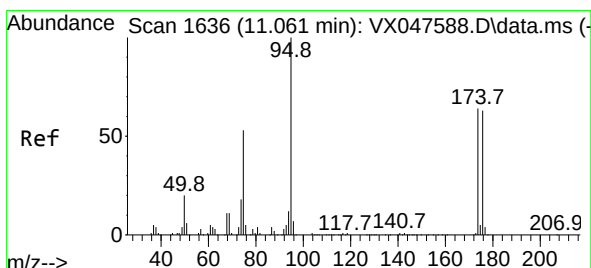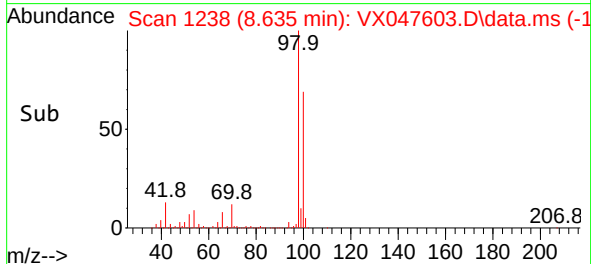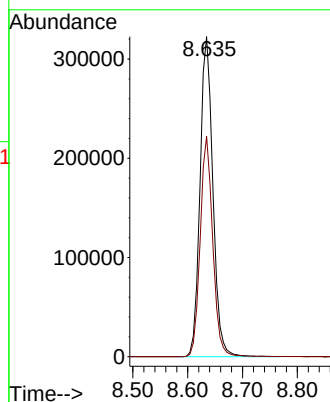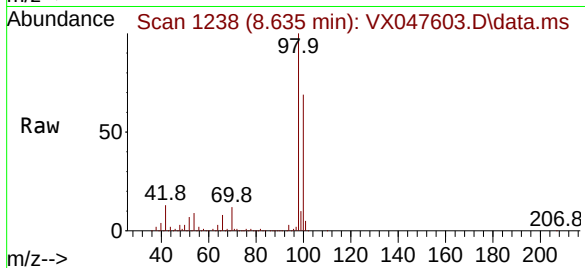

#62
4-Bromofluorobenzene
Concen: 52.854 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.000 min
Lab File: VX047603.D
Acq: 17 Sep 2025 09:41

Tgt Ion: 95 Resp: 222687
Ion Ratio Lower Upper
95 100
174 69.8 0.0 141.6
176 68.4 0.0 138.4


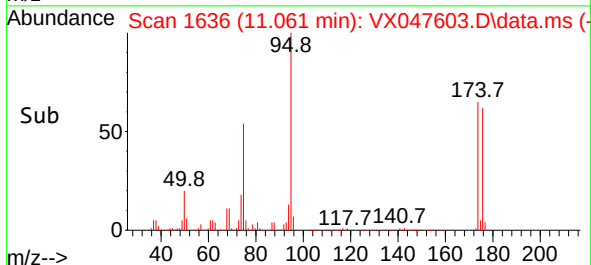
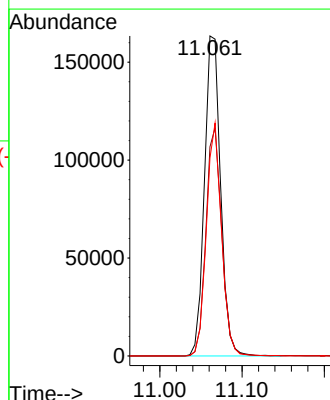
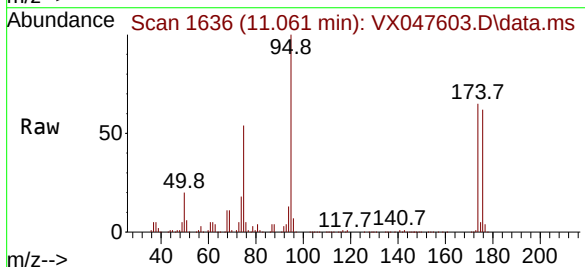


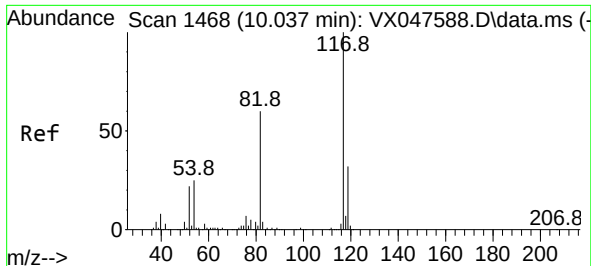

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VX047603.D
Acq: 17 Sep 2025 09:41

Instrument :
MSVOA_X
ClientSampleId :
VX0917WBL01

Tgt Ion:117 Resp: 460978
Ion Ratio Lower Upper
117 100
82 58.6 47.8 71.6
119 32.1 25.2 37.8

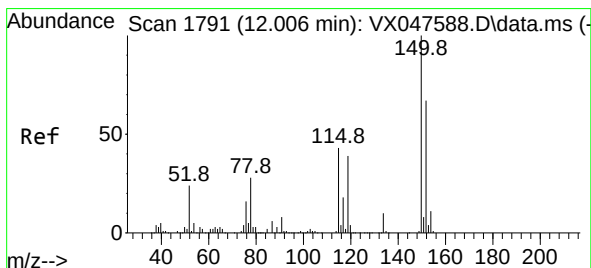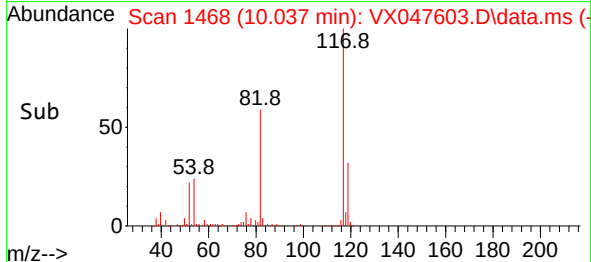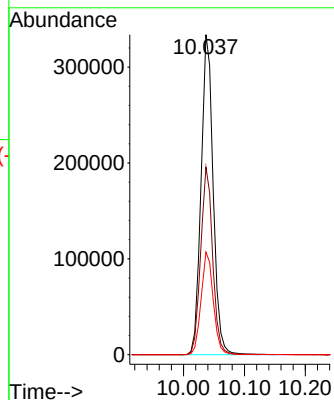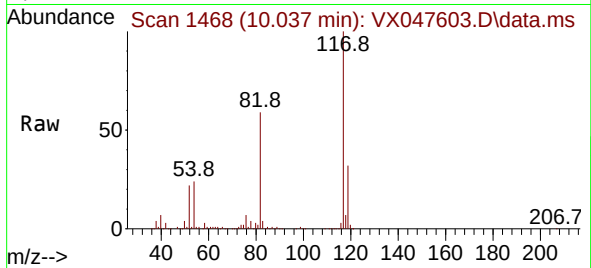

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX047603.D
Acq: 17 Sep 2025 09:41

Tgt Ion:152 Resp: 224854
Ion Ratio Lower Upper
152 100
115 63.7 44.9 134.5
150 159.6 0.0 352.0

