


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX091818\
Data File : VX004644.D
Acq On : 18 Sep 2018 08:33
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091118W.M
Title : SW846 8260
Last Update : Wed Sep 12 02:17:23 2018

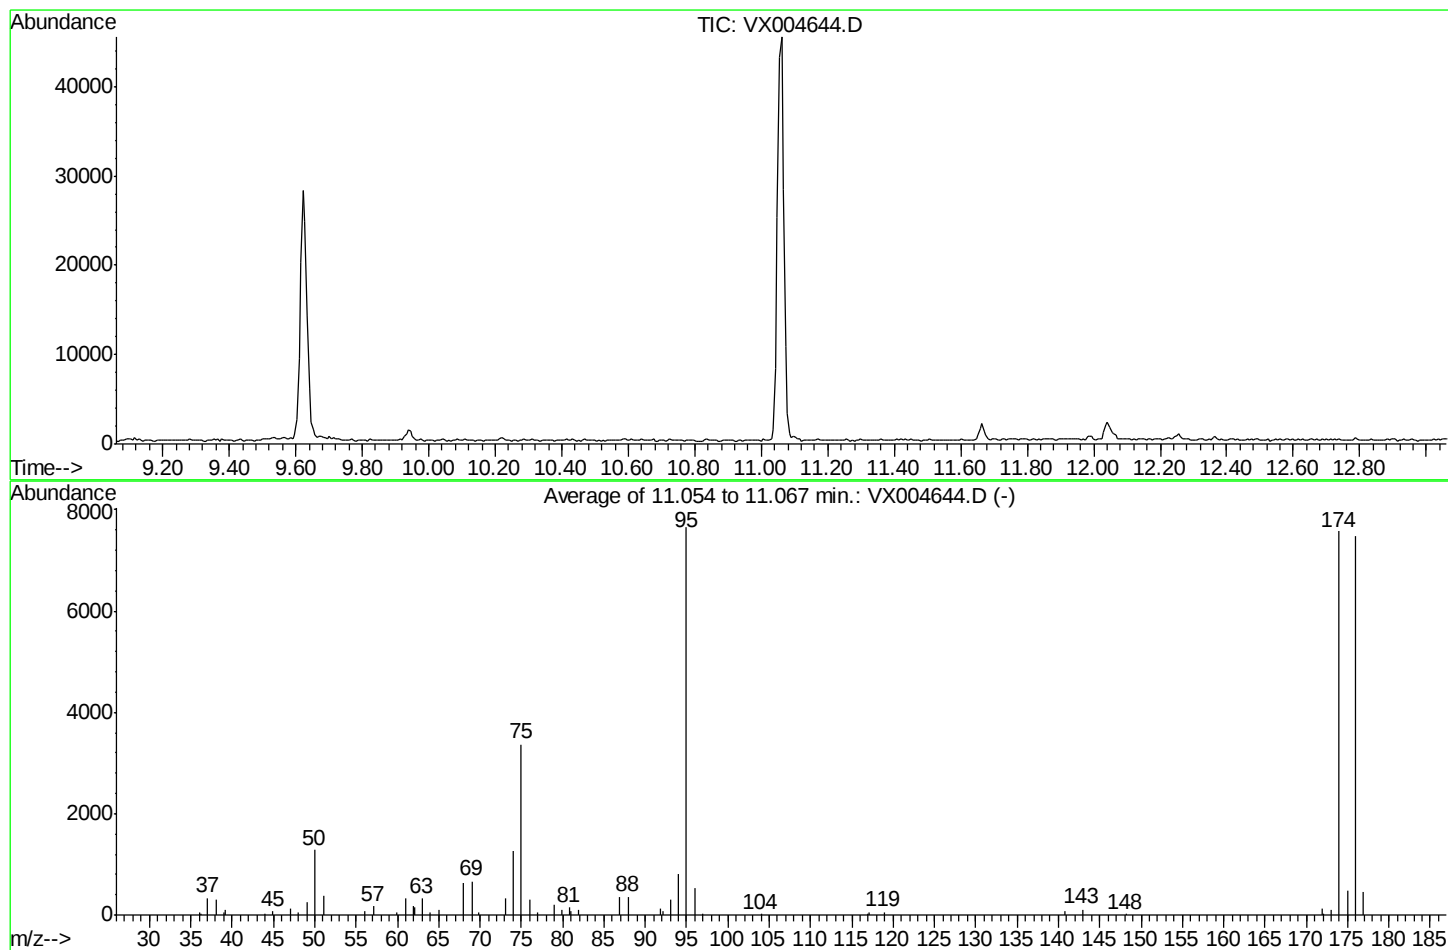

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	1279	PASS
75	95	30	60	44.0	3366	PASS
95	95	100	100	100.0	7651	PASS
96	95	5	9	7.0	533	PASS
173	174	0.00	2	1.5	110	PASS
174	95	50	100	99.0	7571	PASS
175	174	5	9	6.5	492	PASS
176	174	95	101	98.7	7476	PASS
177	176	5	9	6.1	459	PASS