


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX091818\
 Data File : VX004670.D
 Acq On : 18 Sep 2018 21:10
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091118W.M
 Title : SW846 8260
 Last Update : Wed Sep 12 02:17:23 2018

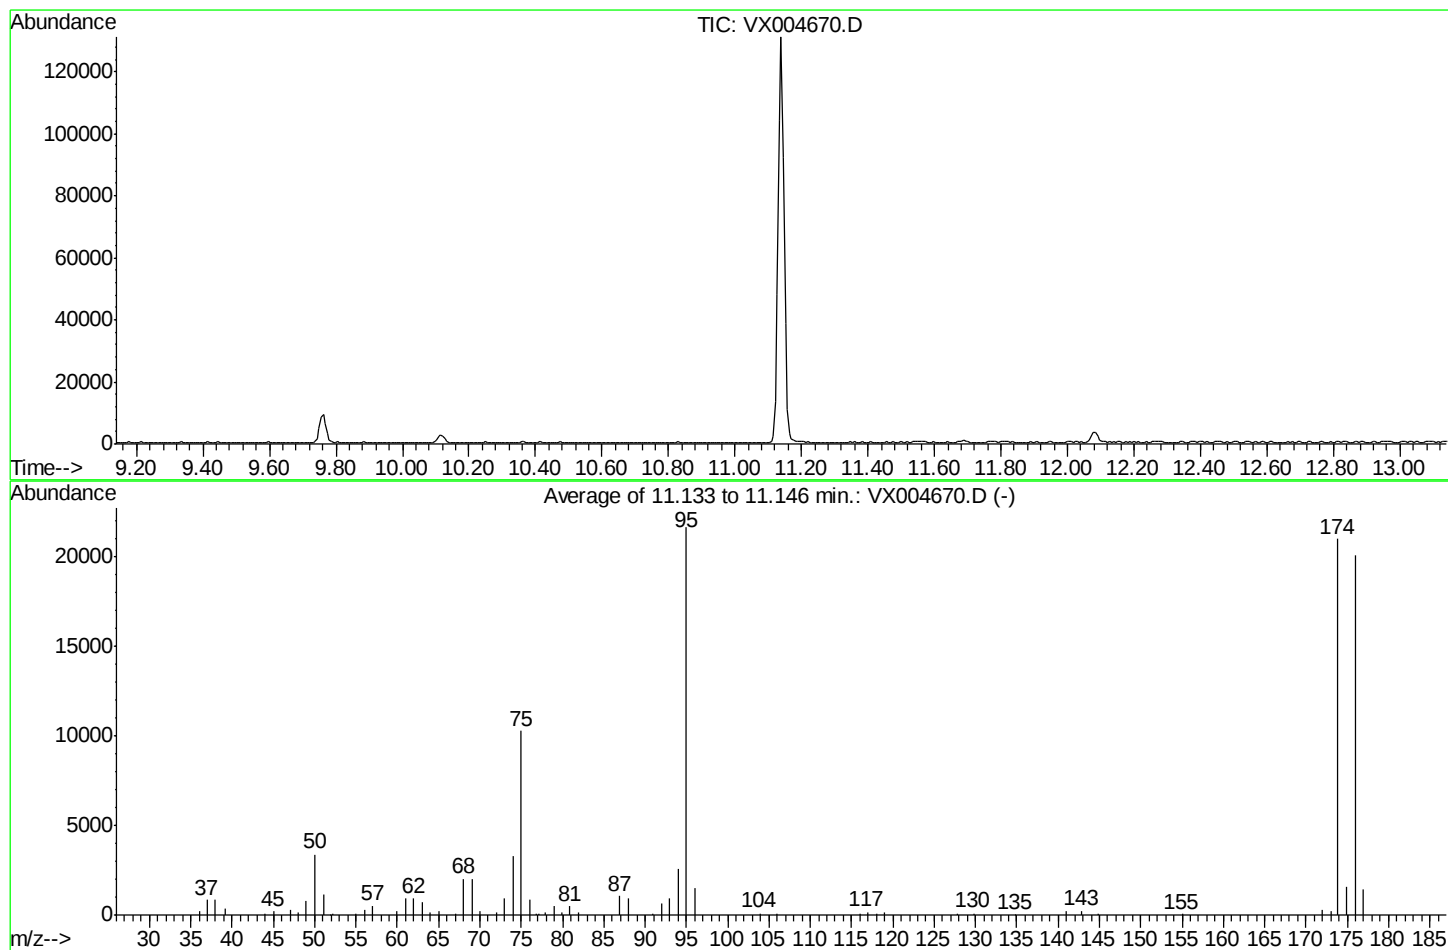

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	3378	PASS
75	95	30	60	47.5	10286	PASS
95	95	100	100	100.0	21642	PASS
96	95	5	9	6.9	1498	PASS
173	174	0.00	2	1.1	237	PASS
174	95	50	100	97.1	21005	PASS
175	174	5	9	7.4	1547	PASS
176	174	95	101	95.6	20080	PASS
177	176	5	9	7.2	1454	PASS