

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX091819\  
 Data File : VX012504.D  
 Acq On : 19 Sep 2019 03:51  
 Operator : JC/SP  
 Sample : K4858-09  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 46 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 RE122D3-20190909

## Integration Parameters: RTEINT.P

Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X091719W.M  
 Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.070       | 26            | 30          | 40           | rBV      | 292807         | 349242        | 36.91%          | 6.382%        |
| 2         | 1.265       | 58            | 62          | 69           | rBV      | 36702          | 44208         | 4.67%           | 0.808%        |
| 3         | 1.594       | 110           | 116         | 120          | rVB9     | 6481           | 11683         | 1.23%           | 0.214%        |
| 4         | 2.594       | 273           | 280         | 290          | rBV      | 27038          | 51856         | 5.48%           | 0.948%        |
| 5         | 5.490       | 742           | 755         | 768          | rBV      | 107046         | 306625        | 32.40%          | 5.603%        |
| 6         | 5.655       | 768           | 782         | 796          | rVV      | 211430         | 596876        | 63.07%          | 10.908%       |
| 7         | 6.051       | 839           | 847         | 857          | rBV      | 129122         | 338369        | 35.76%          | 6.184%        |
| 8         | 6.850       | 968           | 978         | 995          | rBV      | 307302         | 724239        | 76.53%          | 13.235%       |
| 9         | 7.209       | 1029          | 1037        | 1045         | rBV2     | 59730          | 128504        | 13.58%          | 2.348%        |
| 10        | 8.709       | 1276          | 1283        | 1294         | rBV      | 602381         | 946315        | 100.00%         | 17.293%       |
| 11        | 10.111      | 1507          | 1513        | 1519         | rBV      | 563679         | 777482        | 82.16%          | 14.208%       |
| 12        | 11.135      | 1675          | 1681        | 1690         | rBV      | 434897         | 566815        | 59.90%          | 10.358%       |
| 13        | 12.074      | 1830          | 1835        | 1842         | rBV      | 517926         | 629913        | 66.56%          | 11.511%       |


Sum of corrected areas: 5472127

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX091819\  
Data File : VX012504.D  
Acq On : 19 Sep 2019 03:51  
Operator : JC/SP  
Sample : K4858-09  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 46 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE122D3-20190909

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X091719W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

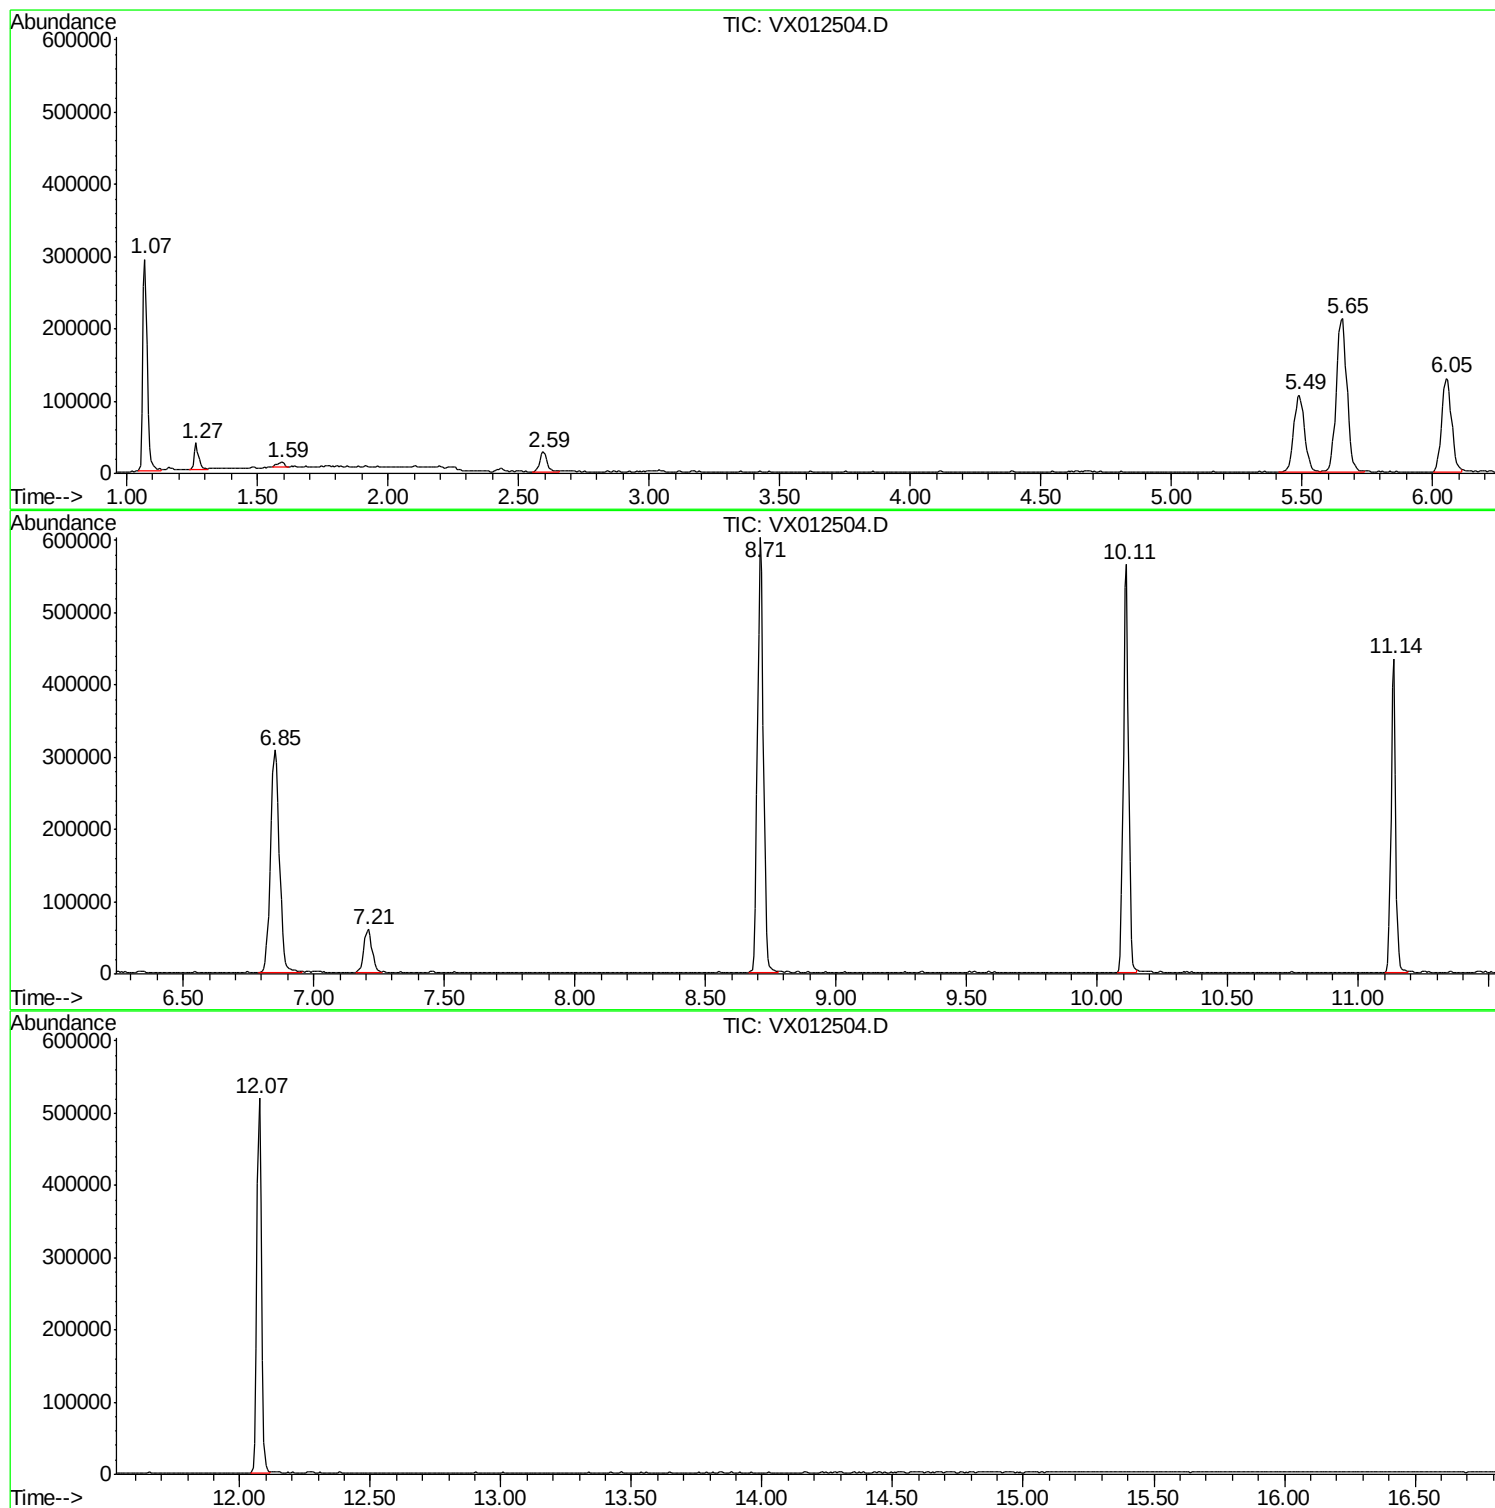

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX091819\  
Data File : VX012504.D  
Acq On : 19 Sep 2019 03:51  
Operator : JC/SP  
Sample : K4858-09  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 46 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE122D3-20190909

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X091719W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX091819\  
Data File : VX012504.D  
Acq On : 19 Sep 2019 03:51  
Operator : JC/SP  
Sample : K4858-09  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 46 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE122D3-20190909

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X091719W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | ---Internal Standard--- |
|------------------|----|---------|-------|----------|-------------------------|
|                  |    |         |       |          | # RT Resp Conc          |