


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX091819\
 Data File : VX012461.D
 Acq On : 18 Sep 2019 09:58
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091719W.M
 Title : SW846 8260
 Last Update : Tue Sep 17 15:27:10 2019

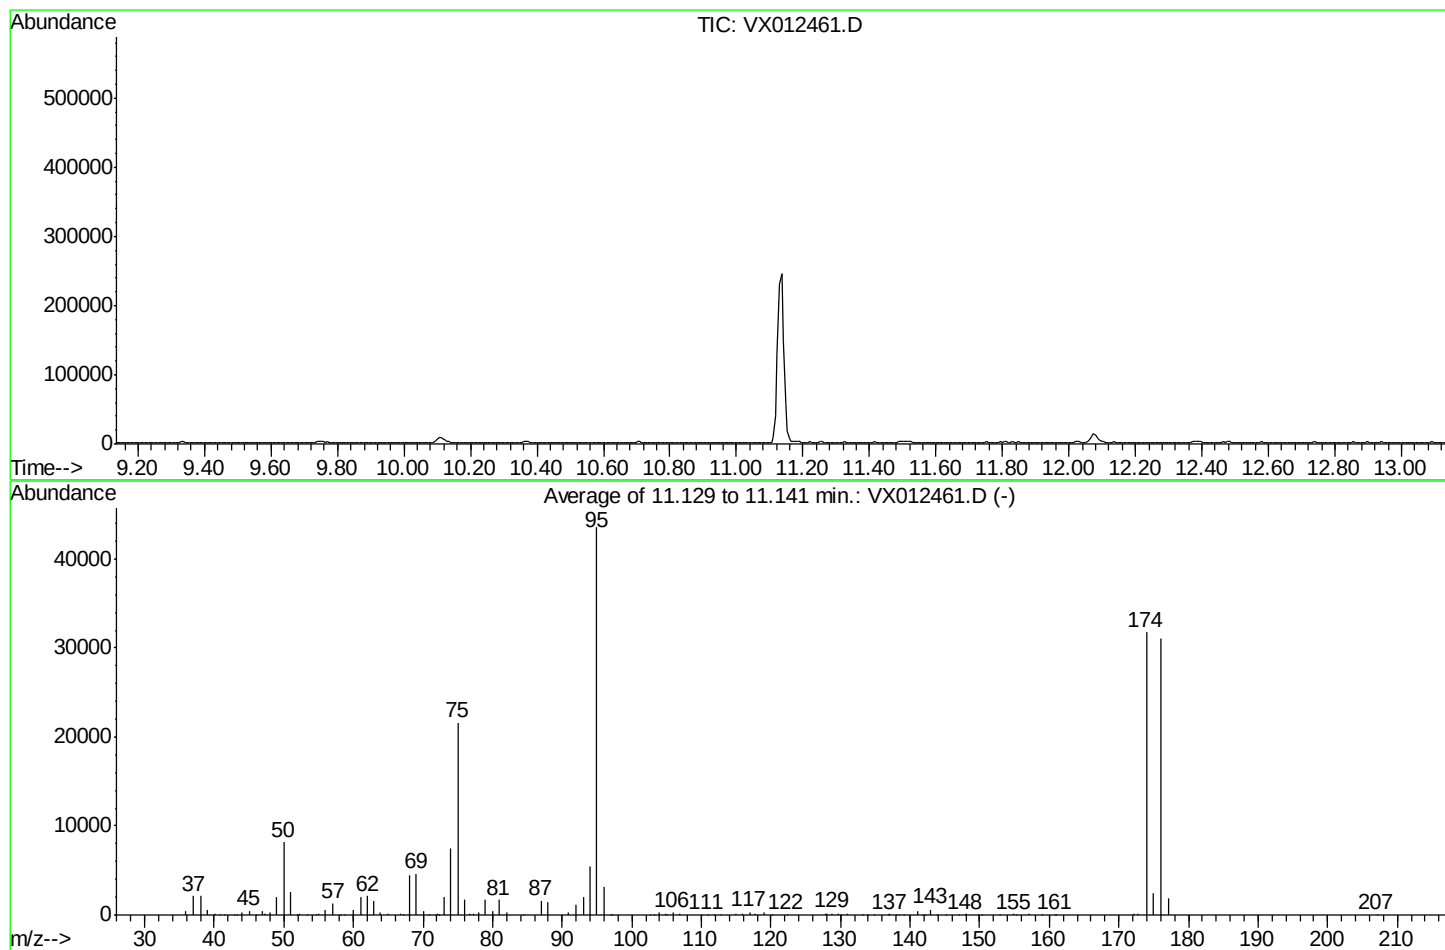

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	8146	PASS
75	95	30	60	49.6	21613	PASS
95	95	100	100	100.0	43554	PASS
96	95	5	9	7.2	3137	PASS
173	174	0.00	2	0.4	118	PASS
174	95	50	100	72.9	31738	PASS
175	174	5	9	7.7	2454	PASS
176	174	95	101	98.0	31112	PASS
177	176	5	9	5.9	1828	PASS