


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX091819\
Data File : VX012490.D
Acq On : 18 Sep 2019 22:01
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091719W.M
Title : SW846 8260
Last Update : Tue Sep 17 15:27:10 2019

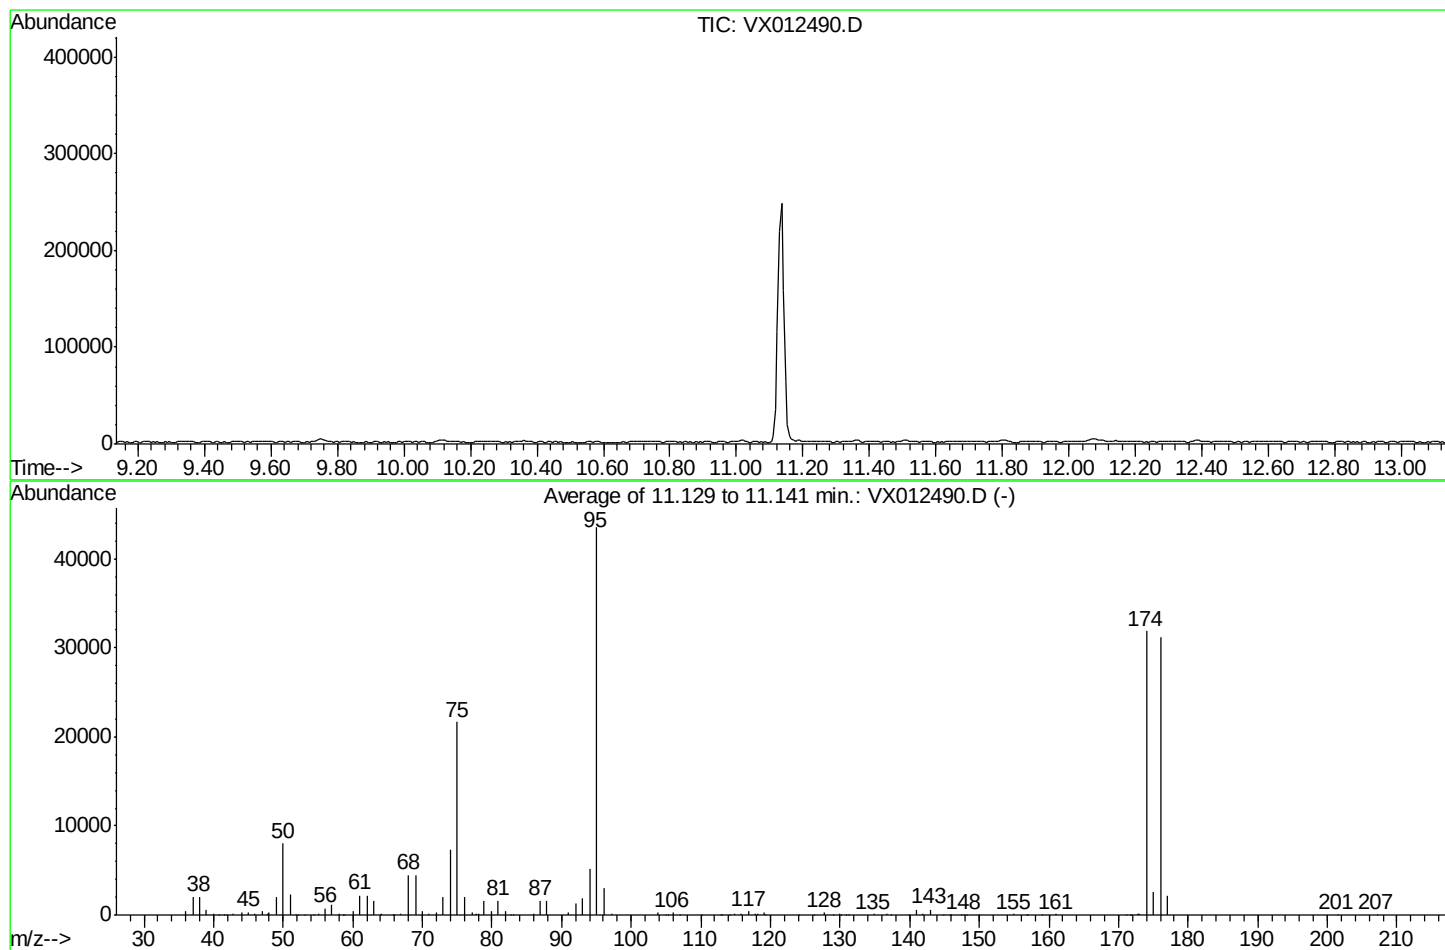

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	8012	PASS
75	95	30	60	49.8	21671	PASS
95	95	100	100	100.0	43520	PASS
96	95	5	9	6.9	2987	PASS
173	174	0.00	2	0.5	145	PASS
174	95	50	100	73.2	31877	PASS
175	174	5	9	8.1	2576	PASS
176	174	95	101	97.7	31146	PASS
177	176	5	9	6.9	2144	PASS