

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091823\
 Data File : VX037771.D
 Acq On : 18 Sep 2023 12:57
 Operator : JC/MD
 Sample : 04437-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1


Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-RW10A-GW-200-202

Quant Time: Sep 18 17:56:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 16 04:55:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	296836	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	483984	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	438774	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	200883	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	174814	44.824	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	89.640%		
35) Dibromofluoromethane	5.391	113	150729	46.545	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	93.080%		
50) Toluene-d8	8.653	98	573548	47.667	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	95.340%		
62) 4-Bromofluorobenzene	11.079	95	202554	46.326	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	92.660%		
Target Compounds						Qvalue
3) Chloromethane	1.307	50	881	0.259	ug/l	89
11) Tert butyl alcohol	2.959	59	1272	1.519	ug/l	96
13) Acrolein	2.233	56	624	0.755	ug/l	86
15) Acrylonitrile	3.087	53	461	0.248	ug/l #	86
16) Acetone	2.380	43	10505	5.599	ug/l	91
17) Carbon Disulfide	2.514	76	4168	0.574	ug/l	98
21) trans-1,2-Dichloroethene	3.099	96	728	0.226	ug/l #	84
25) 2-Butanone	4.593	43	1790	0.676	ug/l	92
31) Cyclohexane	5.556	56	6960	1.390	ug/l #	13
38) Carbon Tetrachloride	5.556	117	29373	6.293	ug/l #	15
49) 1,4-Dioxane	7.714	88	133	1.353	ug/l #	12
59) 2-Hexanone	9.439	43	1167	0.301	ug/l	95
68) m/p-Xylenes	10.305	106	1901	0.300	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	101408	21.826	ug/l #	39
77) Bromobenzene	11.201	156	785	0.215	ug/l	89
78) n-propylbenzene	11.305	91	4429	0.266	ug/l	100
79) 2-Chlorotoluene	11.366	91	2147	0.209	ug/l	90
81) trans-1,4-Dichloro-2-b...	11.079	75	101408	69.916	ug/l #	5
82) 4-Chlorotoluene	11.463	91	3198	0.277	ug/l	95
84) 1,2,4-Trimethylbenzene	11.756	105	2560	0.207	ug/l	96
85) sec-Butylbenzene	11.890	105	4100	0.269	ug/l	97
86) p-Isopropyltoluene	12.012	119	3746	0.295	ug/l	86
87) 1,3-Dichlorobenzene	11.975	146	2380	0.350	ug/l	93
88) 1,4-Dichlorobenzene	11.975	146	2380	0.342	ug/l	94
89) n-Butylbenzene	12.335	91	5379	0.483	ug/l	98
91) 1,2-Dichlorobenzene	12.335	146	1783	0.257	ug/l	96
93) 1,2,4-Trichlorobenzene	13.591	180	3293	0.805	ug/l	97
94) Hexachlorobutadiene	13.725	225	1671	0.875	ug/l	98
95) Naphthalene	13.774	128	10311	0.746	ug/l	99
96) 1,2,3-Trichlorobenzene	13.963	180	3361	0.799	ug/l	98





(#) = qualifier out of range (m) = manual integration (+) = signals summed

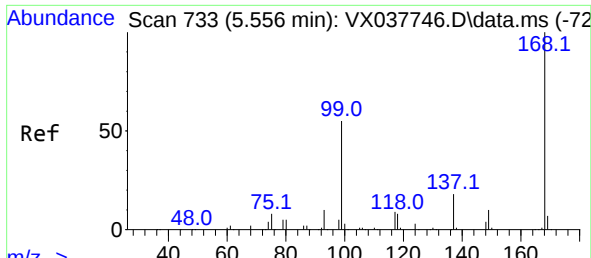

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-200-202


Tgt Ion:168 Resp: 296836
Ion Ratio Lower Upper
168 100
99 57.6 56.6 85.0

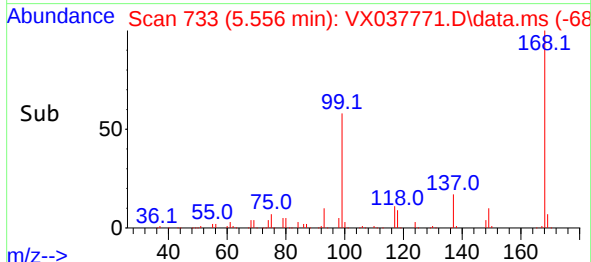

#3
Chloromethane
Concen: 0.259 ug/l
RT: 1.307 min Scan# 36
Delta R.T. 0.006 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57

Tgt Ion: 50 Resp: 881
Ion Ratio Lower Upper
50 100
52 37.8 25.5 38.3



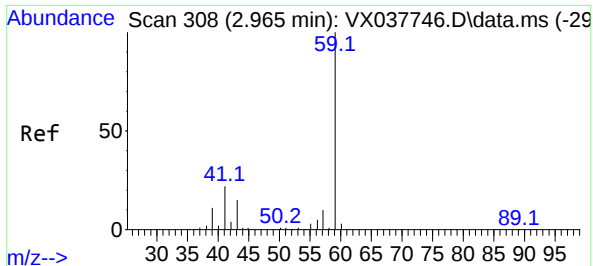

#11

Tert butyl alcohol

Concen: 1.519 ug/l

RT: 2.959 min Scan# 308

Delta R.T. -0.006 min

Lab File: VX037771.D

Acq: 18 Sep 2023 12:57

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB-RW10A-GW-200-202

Tgt Ion: 59 Resp: 1272

Ion Ratio Lower Upper

59 100

57 6.2 6.0 9.0

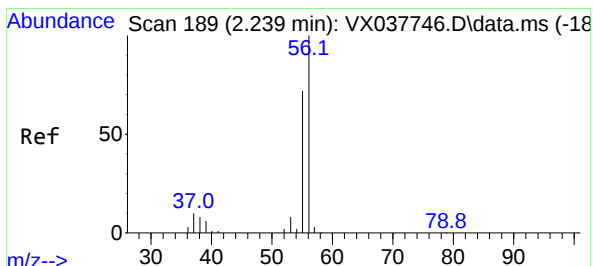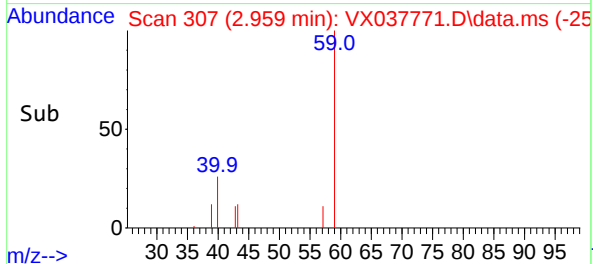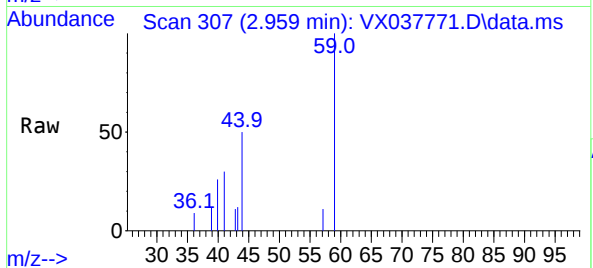

#13

Acrolein

Concen: 0.755 ug/l

RT: 2.233 min Scan# 188

Delta R.T. -0.006 min

Lab File: VX037771.D




Acq: 18 Sep 2023 12:57


Tgt Ion: 56 Resp: 624

Ion Ratio Lower Upper

56 100

55 60.1 57.1 85.7


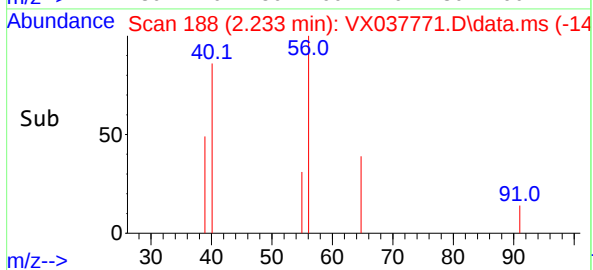

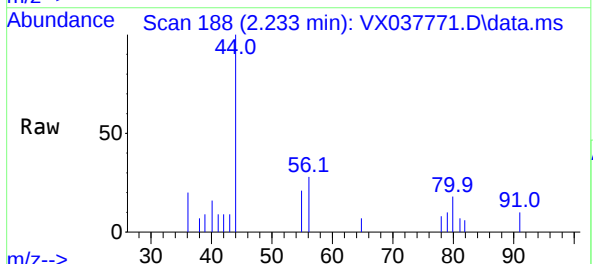




#15
Acrylonitrile
Concen: 0.248 ug/l
RT: 3.087 min Scan# 31
Delta R.T. 0.018 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-200-202


Tgt Ion: 53 Resp: 461
Ion Ratio Lower Upper
53 100
52 75.5 66.0 99.0
51 54.0 29.8 44.6#



#16
Acetone
Concen: 5.599 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57

Tgt Ion: 43 Resp: 10505
Ion Ratio Lower Upper
43 100
58 31.9 21.9 32.9

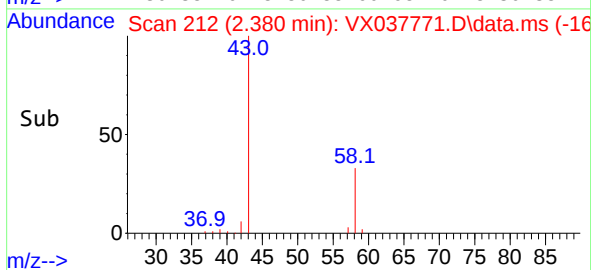



#17

Carbon Disulfide

Concen: 0.574 ug/l

RT: 2.514 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX037771.D

Acq: 18 Sep 2023 12:57

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB-RW10A-GW-200-202

Tgt Ion: 76 Resp: 4168

Ion Ratio Lower Upper

76 100

78 8.1 7.0 10.6

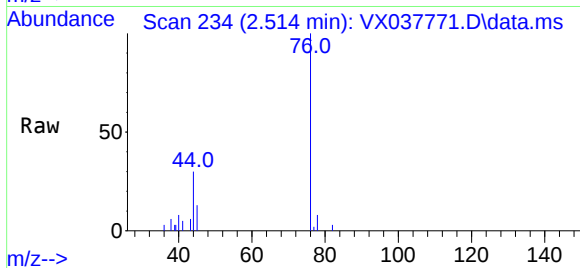

#21

trans-1,2-Dichloroethene

Concen: 0.226 ug/l

RT: 3.099 min Scan# 330

Delta R.T. 0.006 min

Lab File: VX037771.D

Acq: 18 Sep 2023 12:57




Tgt Ion: 96 Resp: 728


Ion Ratio Lower Upper

96 100

61 130.3 119.2 178.8

98 74.8 48.7 73.1#


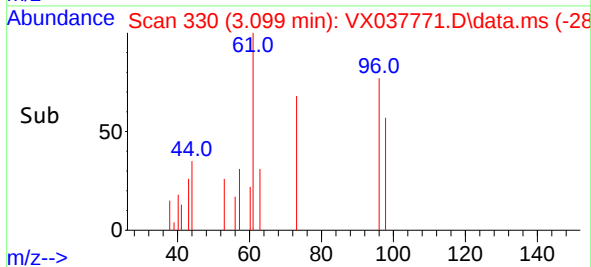

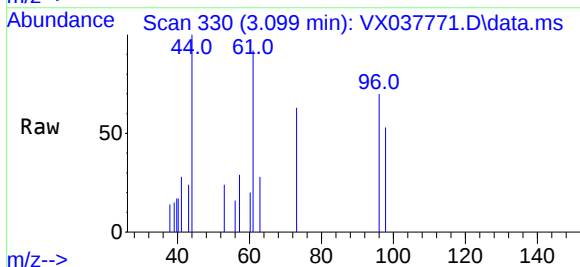


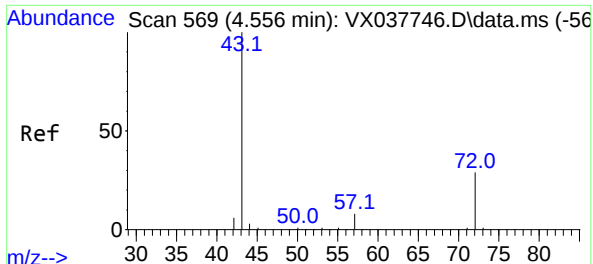

#25
2-Butanone
Concen: 0.676 ug/l
RT: 4.593 min Scan# 51
Delta R.T. 0.024 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-200-202


Tgt Ion: 43 Resp: 1790
Ion Ratio Lower Upper
43 100
72 20.5 19.4 29.2

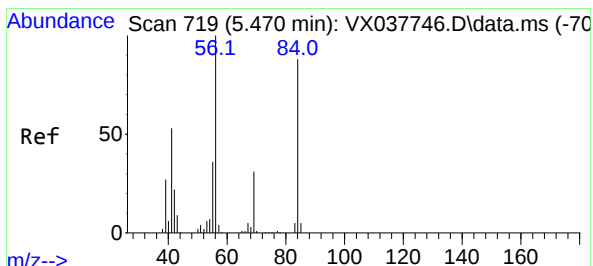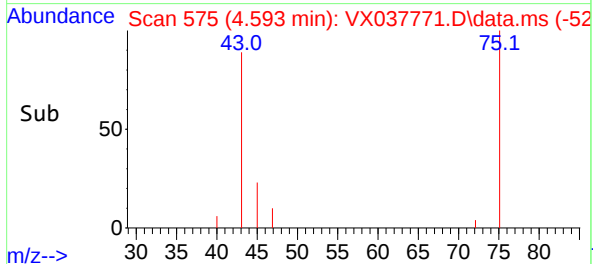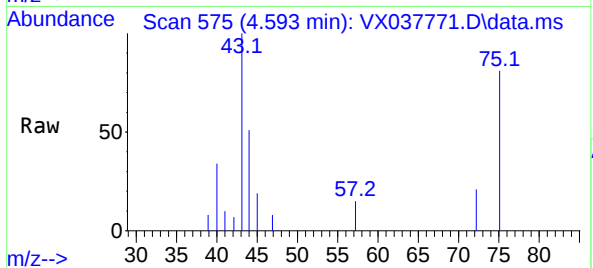

#31
Cyclohexane
Concen: 1.390 ug/l
RT: 5.556 min Scan# 733
Delta R.T. 0.085 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57

Tgt Ion: 56 Resp: 6960
Ion Ratio Lower Upper
56 100
69 146.0 23.4 35.2#
84 118.7 65.9 98.9#


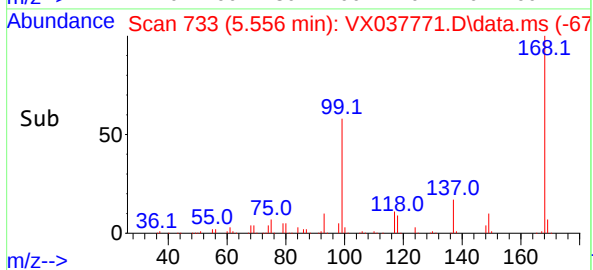

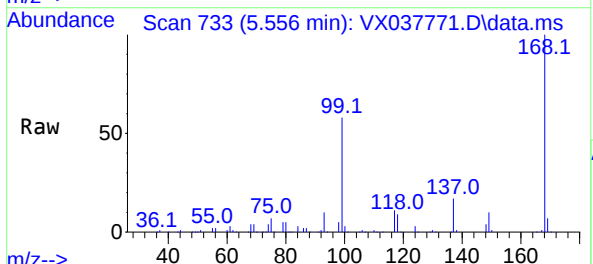




#33
1,2-Dichloroethane-d4
Concen: 44.824 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-200-202


Tgt Ion: 65 Resp: 174814
Ion Ratio Lower Upper
65 100
67 53.3 0.0 100.2



#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. -0.000 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57

Tgt Ion: 114 Resp: 483984
Ion Ratio Lower Upper
114 100
63 19.2 0.0 45.0
88 15.7 0.0 36.6

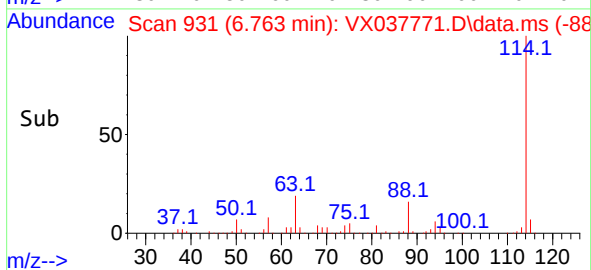

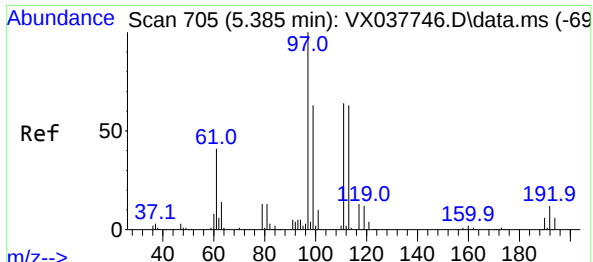

#35

Dibromofluoromethane

Concen: 46.545 ug/l

RT: 5.391 min Scan# 705

Delta R.T. 0.006 min

Lab File: VX037771.D


Acq: 18 Sep 2023 12:57

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB-RW10A-GW-200-202

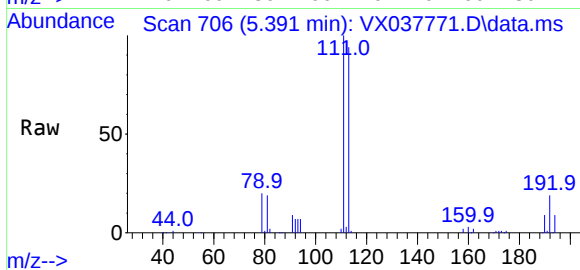




Tgt Ion:113 Resp: 150729

Ion Ratio Lower Upper

113 100

111 102.6 82.9 124.3

192 19.5 13.3 19.9

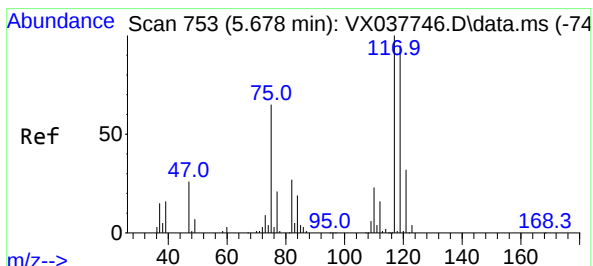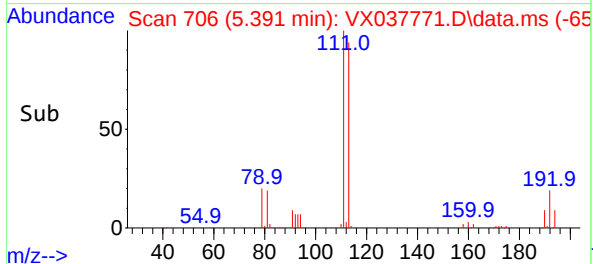

#38

Carbon Tetrachloride

Concen: 6.293 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.122 min

Lab File: VX037771.D

Acq: 18 Sep 2023 12:57




Tgt Ion:117 Resp: 29373


Ion Ratio Lower Upper

117 100

119 4.3 78.2 117.2#

121 0.0 24.4 36.6#

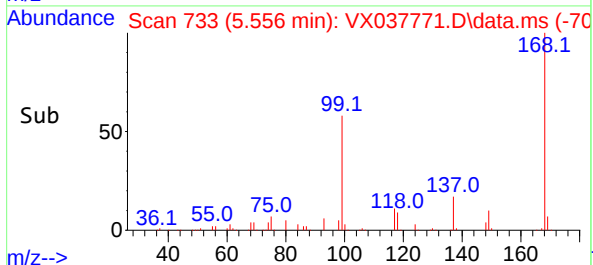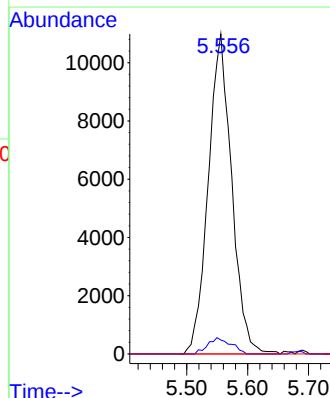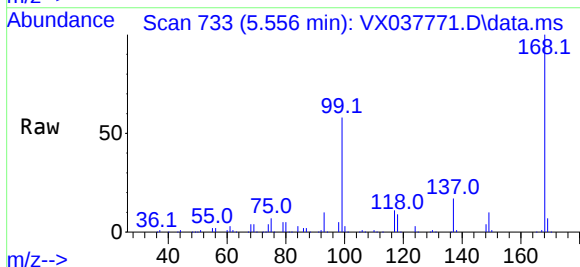

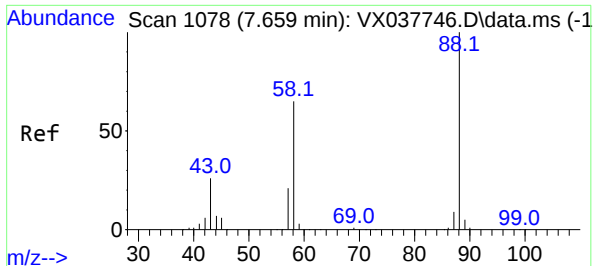

#49

1,4-Dioxane

Concen: 1.353 ug/l

RT: 7.714 min Scan# 1087

Delta R.T. 0.043 min

Lab File: VX037771.D

Acq: 18 Sep 2023 12:57

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB-RW10A-GW-200-202





Tgt Ion: 88 Resp: 133

Ion Ratio Lower Upper

88 100

43 17.3 0.0 0.0#

58 0.0 60.1 90.1#

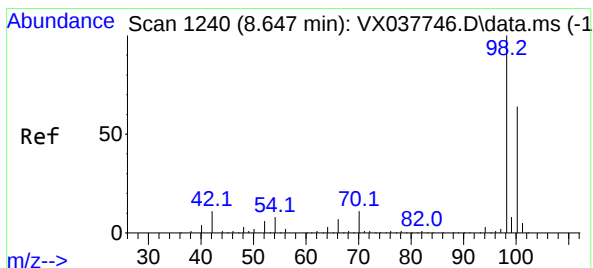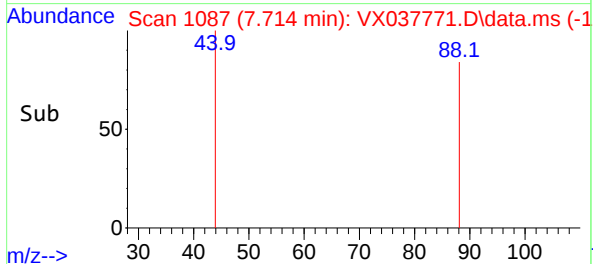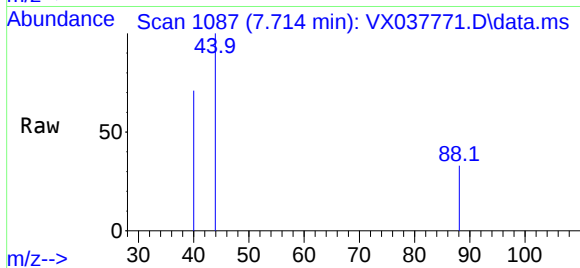

#50

Toluene-d8

Concen: 47.667 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.006 min

Lab File: VX037771.D




Acq: 18 Sep 2023 12:57


Tgt Ion: 98 Resp: 573548

Ion Ratio Lower Upper

98 100

100 63.3 53.1 79.7

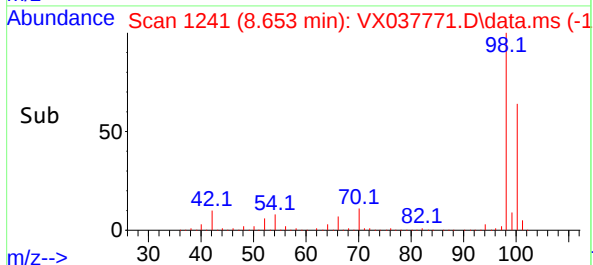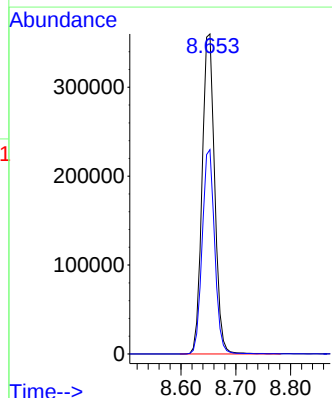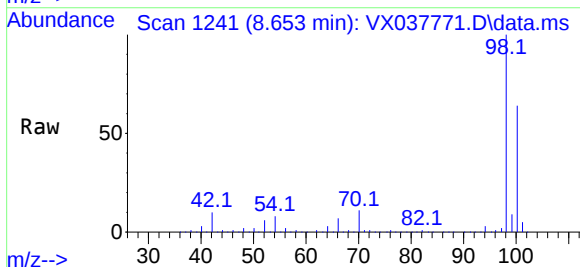

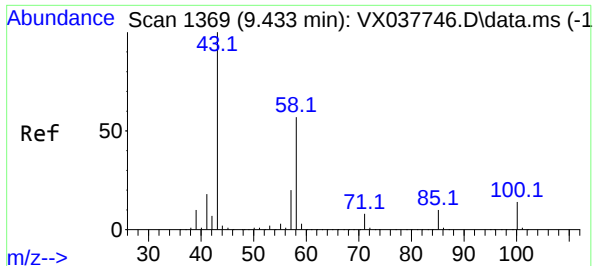

#59

2-Hexanone

Concen: 0.301 ug/l

RT: 9.439 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX037771.D

Acq: 18 Sep 2023 12:57

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB-RW10A-GW-200-202

Tgt Ion: 43 Resp: 1167

Ion Ratio Lower Upper

43 100

58 48.6 26.2 78.5

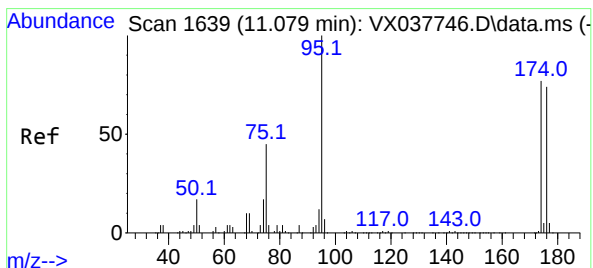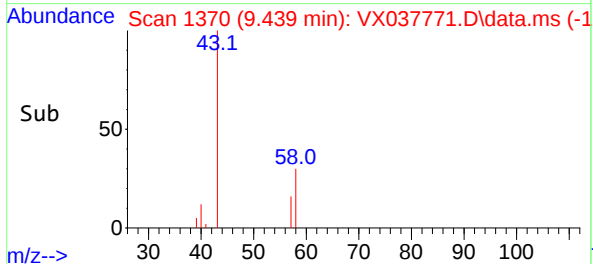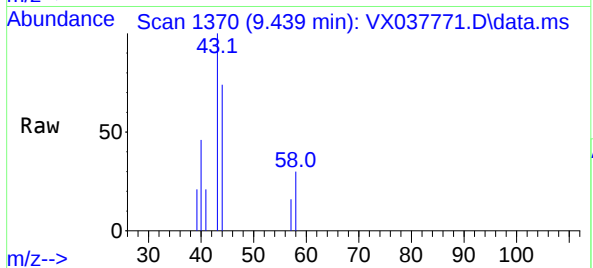

#62

4-Bromofluorobenzene

Concen: 46.326 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX037771.D

Acq: 18 Sep 2023 12:57




Tgt Ion: 95 Resp: 202554


Ion Ratio Lower Upper

95 100

174 82.6 0.0 135.6

176 79.5 0.0 131.0


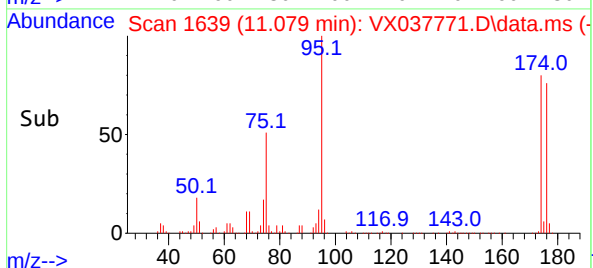
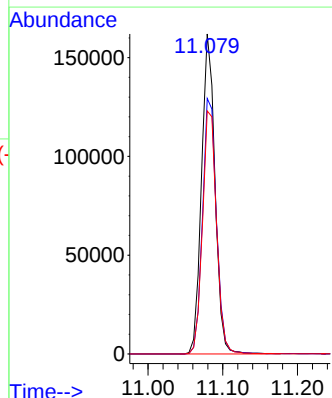
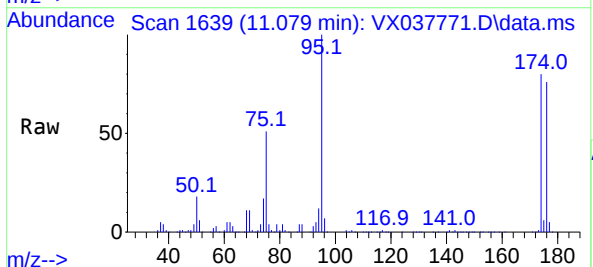




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-200-202


Tgt Ion:117 Resp: 438774
Ion Ratio Lower Upper
117 100
82 53.5 46.2 69.4
119 31.7 25.5 38.3

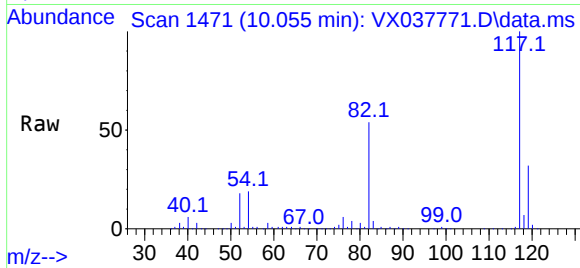

#68
m/p-Xylenes
Concen: 0.300 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57

Tgt Ion:106 Resp: 1901
Ion Ratio Lower Upper
106 100
91 206.0 165.5 248.3


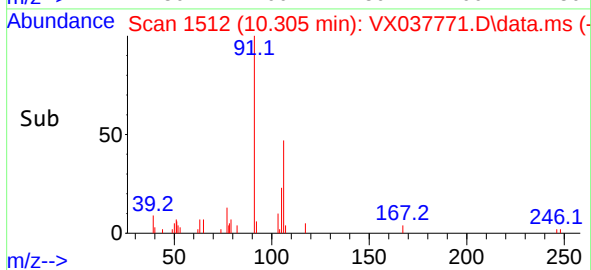

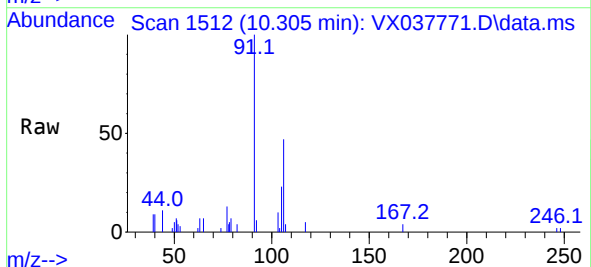




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-200-202


Tgt Ion:152 Resp: 200883
Ion Ratio Lower Upper
152 100
115 60.1 43.3 129.9
150 156.7 0.0 345.0

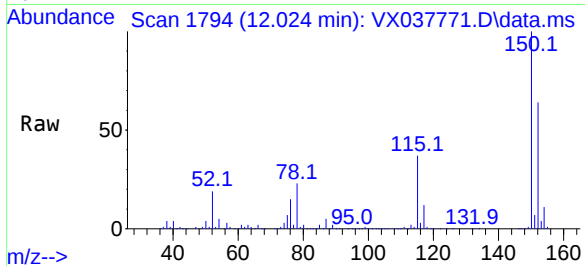

#76
1,2,3-Trichloropropane
Concen: 21.826 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57

Tgt Ion: 75 Resp: 101408
Ion Ratio Lower Upper
75 100
77 1.2 19.1 57.5#


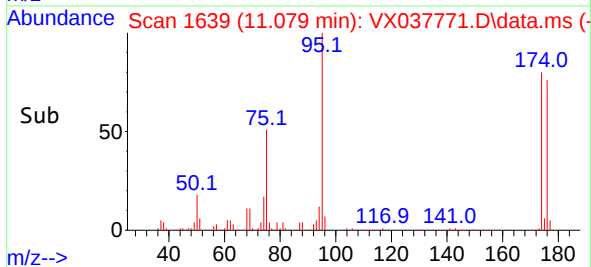

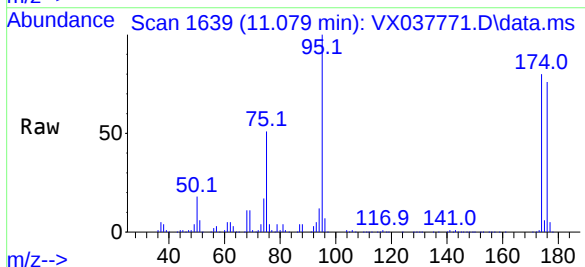




#77
Bromobenzene
Concen: 0.215 ug/l
RT: 11.201 min Scan# 1659
Delta R.T. -0.000 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-200-202


Tgt Ion:156 Resp: 785
Ion Ratio Lower Upper
156 100
77 154.8 88.4 265.3
158 97.6 48.0 144.0



#78
n-propylbenzene
Concen: 0.266 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57

Tgt Ion: 91 Resp: 4429
Ion Ratio Lower Upper
91 100
120 22.9 11.5 34.4









#79
2-Chlorotoluene
Concen: 0.209 ug/l
RT: 11.366 min Scan# 1686
Delta R.T. -0.000 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-200-202


Tgt Ion: 91 Resp: 2147
Ion Ratio Lower Upper
91 100
126 26.8 16.3 48.8

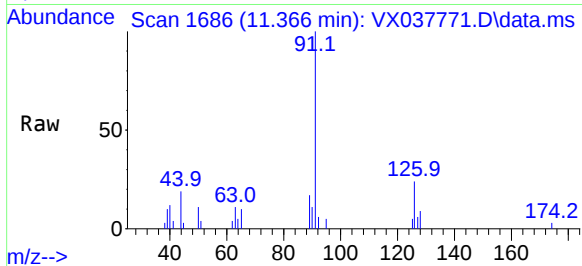

#81
trans-1,4-Dichloro-2-butene
Concen: 69.916 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57

Tgt Ion: 75 Resp: 101408
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#


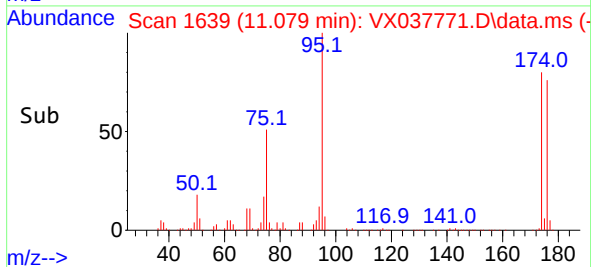

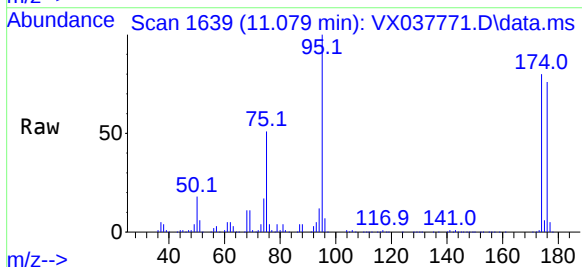




#82
4-Chlorotoluene
Concen: 0.277 ug/l
RT: 11.463 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-200-202


Tgt Ion: 91 Resp: 3198
Ion Ratio Lower Upper
91 100
126 31.3 14.2 42.6

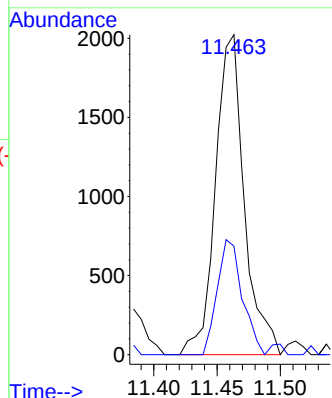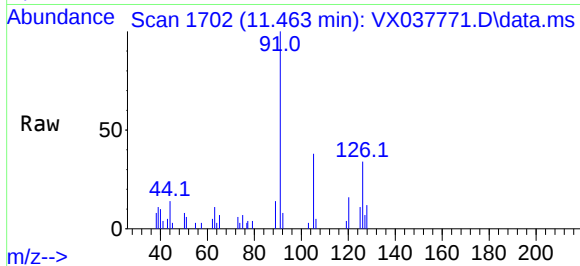

#84
1,2,4-Trimethylbenzene
Concen: 0.207 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57

Tgt Ion: 105 Resp: 2560
Ion Ratio Lower Upper
105 100
120 44.8 21.2 63.6



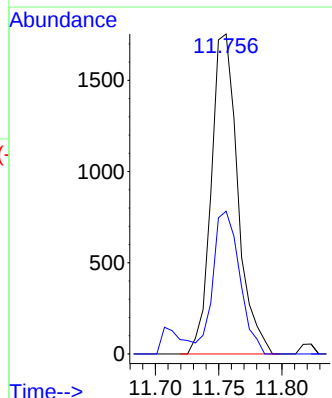
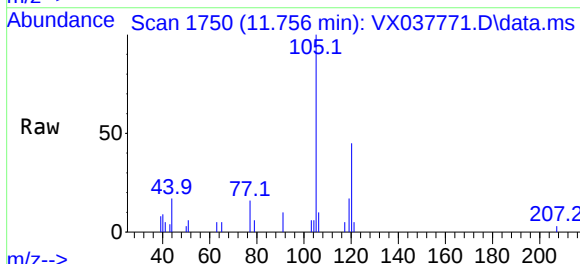




#85
 sec-Butylbenzene
 Concen: 0.269 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. -0.000 min
 Lab File: VX037771.D
 Acq: 18 Sep 2023 12:57




Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-RW10A-GW-200-202


Tgt Ion:105 Resp: 4100
 Ion Ratio Lower Upper
 105 100
 134 18.2 9.8 29.4



#86
 p-Isopropyltoluene
 Concen: 0.295 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. -0.000 min
 Lab File: VX037771.D
 Acq: 18 Sep 2023 12:57

Tgt Ion:119 Resp: 3746
 Ion Ratio Lower Upper
 119 100
 134 27.6 12.8 38.3
 91 38.6 13.1 39.3

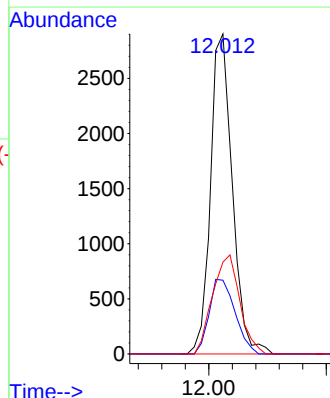



#87

1,3-Dichlorobenzene

Concen: 0.350 ug/l

RT: 11.975 min Scan# 1786

Delta R.T. 0.006 min

Lab File: VX037771.D

Acq: 18 Sep 2023 12:57

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB-RW10A-GW-200-202





Tgt Ion:146 Resp: 2380

Ion Ratio Lower Upper

146 100

111 41.6 22.1 66.1

148 70.7 31.8 95.3

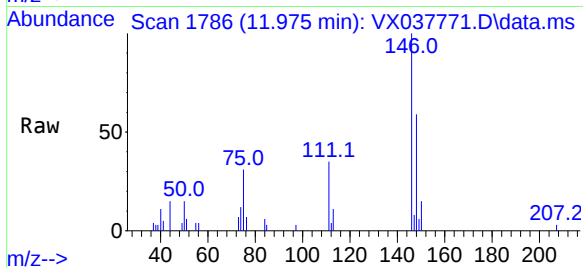

#88

1,4-Dichlorobenzene

Concen: 0.342 ug/l

RT: 11.975 min Scan# 1786

Delta R.T. -0.067 min

Lab File: VX037771.D

Acq: 18 Sep 2023 12:57




Tgt Ion:146 Resp: 2380


Ion Ratio Lower Upper

146 100

111 41.6 21.3 63.7

148 70.7 31.8 95.4


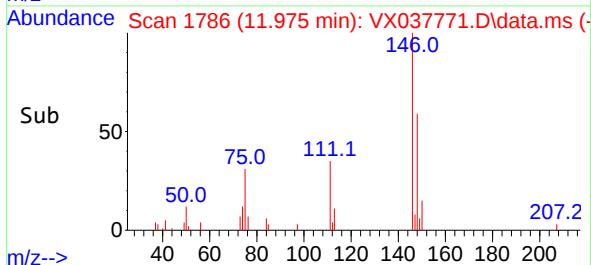
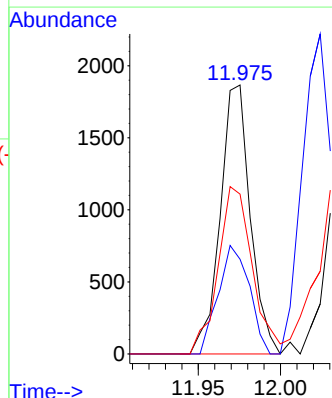
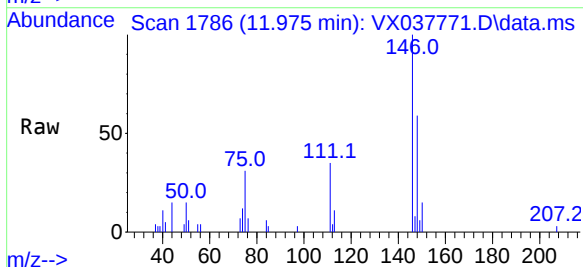




#89
n-Butylbenzene
Concen: 0.483 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. -0.000 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-200-202


Tgt Ion: 91	Resp:	5379	
Ion	Ratio	Lower	Upper
91	100		
92	53.3	27.4	82.0
134	26.4	12.6	37.8

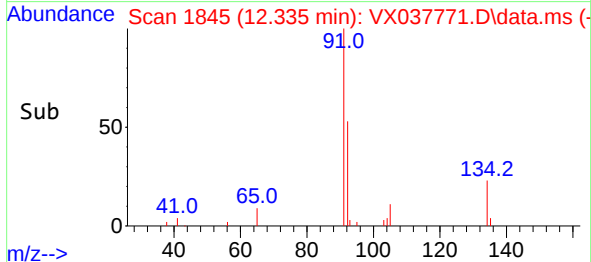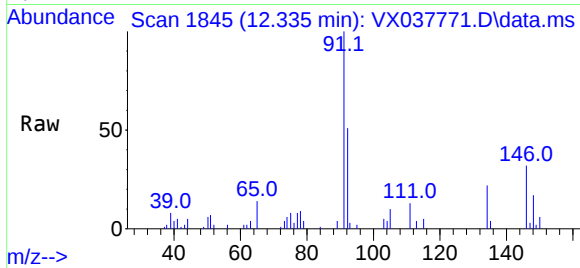

#91
1,2-Dichlorobenzene
Concen: 0.257 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. -0.000 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57

Tgt Ion:146	Resp:	1783	
Ion	Ratio	Lower	Upper
146	100		
111	47.2	22.4	67.0
148	59.8	31.6	95.0


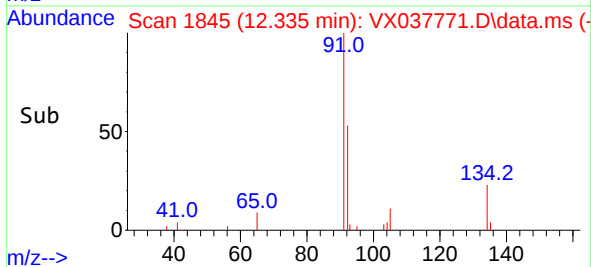

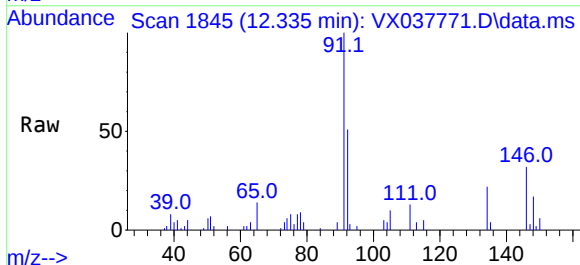




#93
1,2,4-Trichlorobenzene
Concen: 0.805 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. -0.000 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-200-202


Tgt Ion:	180	Resp:	3293
Ion	Ratio	Lower	Upper
180	100		
182	97.3	48.3	144.8
145	29.9	18.0	54.0

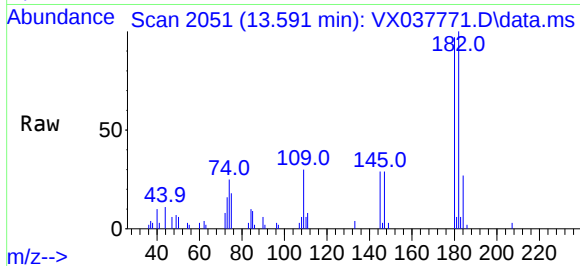

#94
Hexachlorobutadiene
Concen: 0.875 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. -0.000 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57

Tgt Ion:	225	Resp:	1671
Ion	Ratio	Lower	Upper
225	100		
223	62.9	31.1	93.2
227	66.6	32.5	97.5



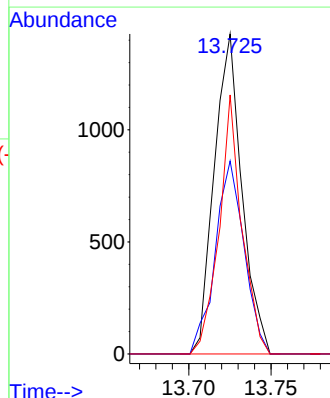
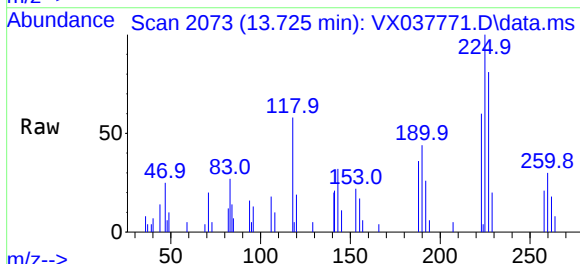




#95
Naphthalene
Concen: 0.746 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.006 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-200-202

Tgt Ion:	128	Resp:	10311
Ion Ratio	Lower	Upper	
128	100		
127	13.3	10.3	15.5
129	10.6	8.8	13.2

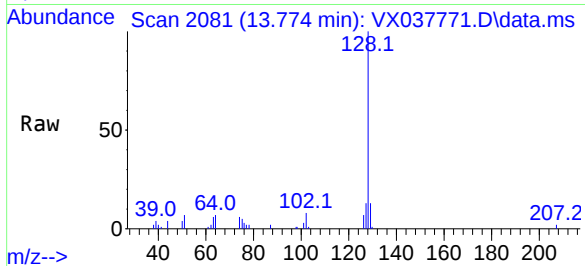

#96
1,2,3-Trichlorobenzene
Concen: 0.799 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. -0.000 min
Lab File: VX037771.D
Acq: 18 Sep 2023 12:57

Tgt Ion:	180	Resp:	3361
Ion Ratio	Lower	Upper	
180	100		
182	93.5	46.9	140.6
145	32.1	17.8	53.5

