

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091823\
 Data File : VX037787.D
 Acq On : 18 Sep 2023 19:33
 Operator : JC/MD
 Sample : 04408-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-16-0912

Quant Time: Sep 19 07:25:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 16 04:55:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	239187	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	406081	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	389801	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	198037	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	149029	47.423	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	94.840%
35) Dibromofluoromethane	5.391	113	123356	45.400	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	90.800%
50) Toluene-d8	8.647	98	494336	48.965	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.920%
62) 4-Bromofluorobenzene	11.079	95	184202	50.210	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	100.420%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091823\
Data File : VX037787.D
Acq On : 18 Sep 2023 19:33
Operator : JC/MD
Sample : 04408-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-16-0912

Quant Time: Sep 19 07:25:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 16 04:55:44 2023
Response via : Initial Calibration




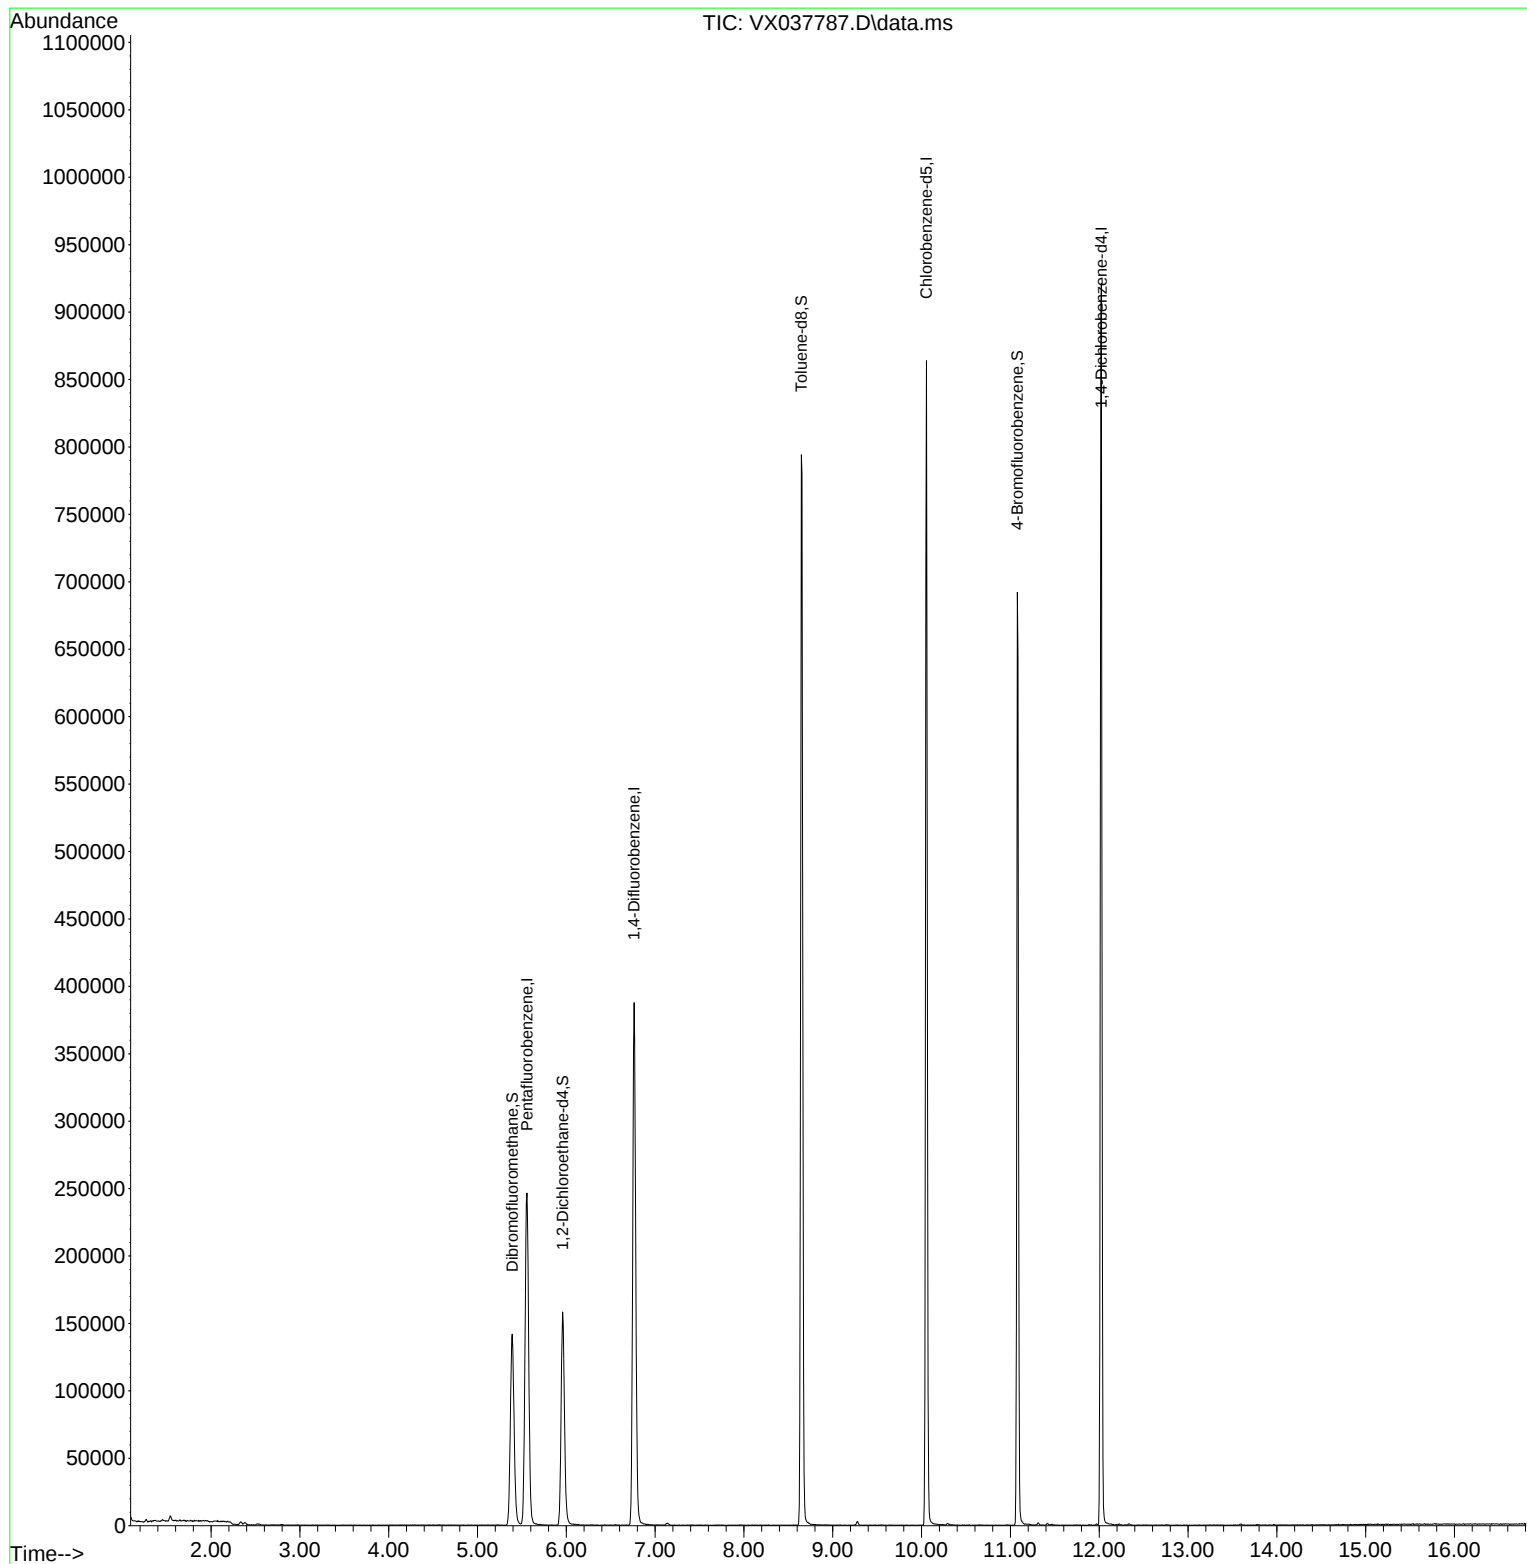




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 733
Delta R.T. 0.006 min
Lab File: VX037787.D
Acq: 18 Sep 2023 19:33




Instrument :
MSVOA_X
ClientSampleId :
MW-16-0912

Tgt Ion:168 Resp: 239187
Ion Ratio Lower Upper
168 100
99 57.2 56.6 85.0

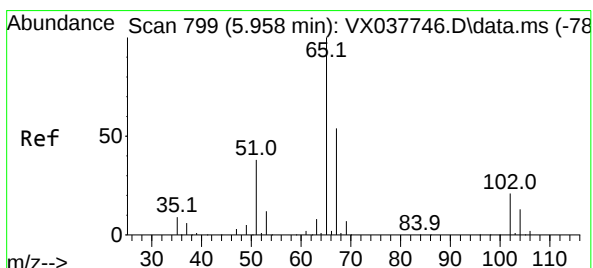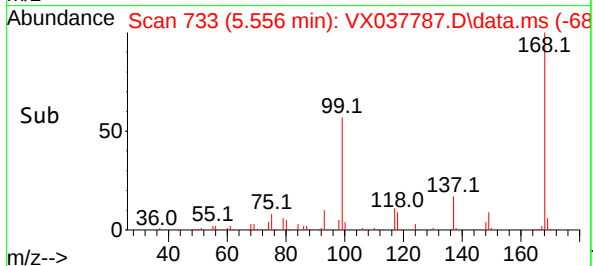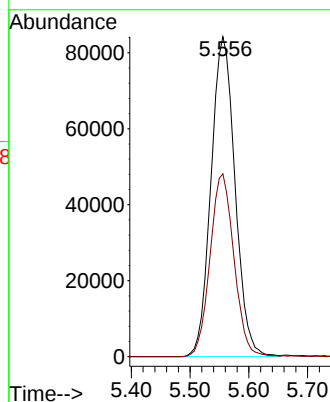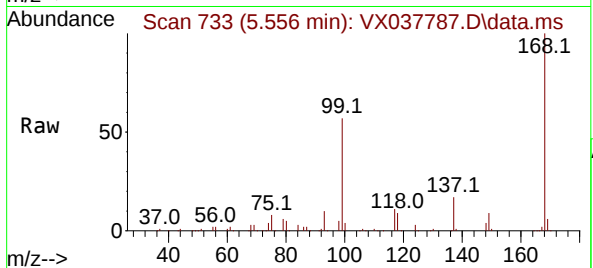

#33
1,2-Dichloroethane-d4
Concen: 47.423 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX037787.D
Acq: 18 Sep 2023 19:33

Tgt Ion: 65 Resp: 149029
Ion Ratio Lower Upper
65 100
67 53.1 0.0 100.2

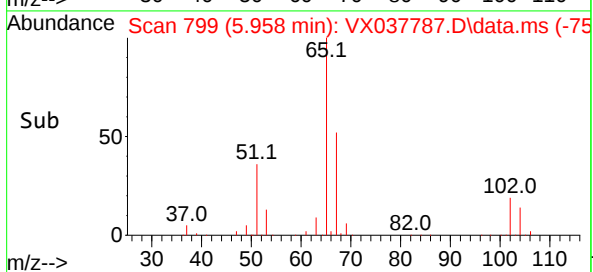
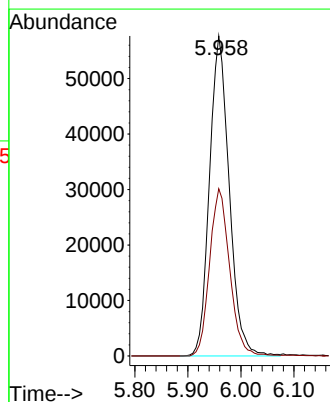
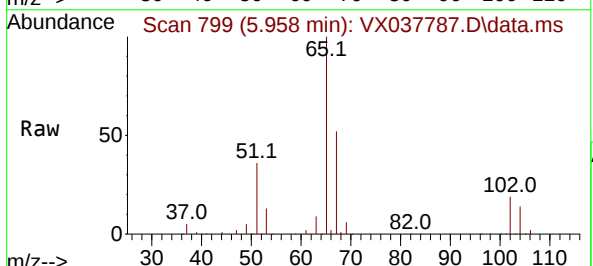




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX037787.D
Acq: 18 Sep 2023 19:33




Instrument :
MSVOA_X
ClientSampleId :
MW-16-0912


Tgt Ion:114 Resp: 406081
Ion Ratio Lower Upper
114 100
63 19.1 0.0 45.0
88 15.3 0.0 36.6

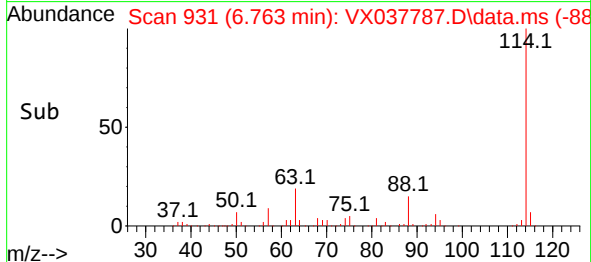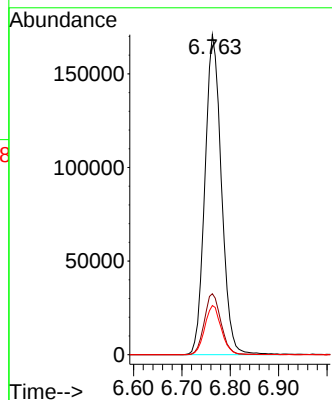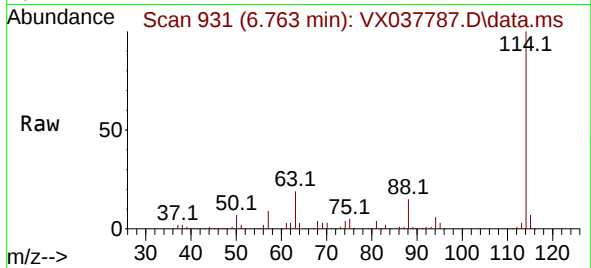

#35
Dibromofluoromethane
Concen: 45.400 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX037787.D
Acq: 18 Sep 2023 19:33

Tgt Ion:113 Resp: 123356
Ion Ratio Lower Upper
113 100
111 104.4 82.9 124.3
192 19.0 13.3 19.9

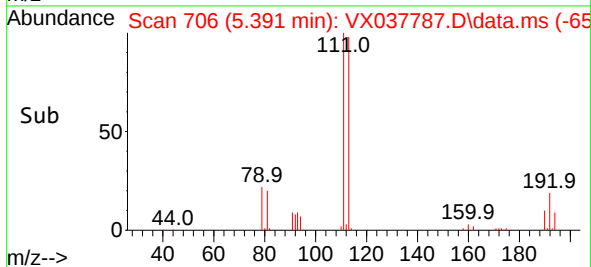
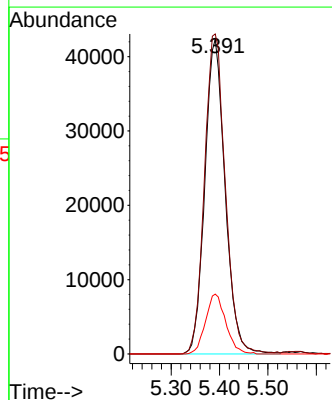
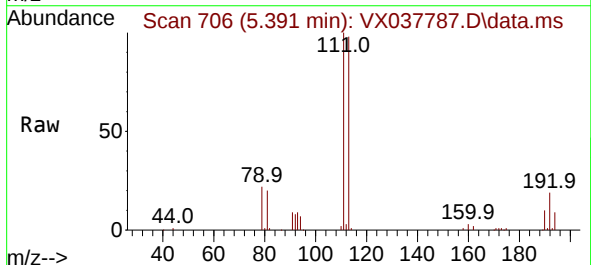


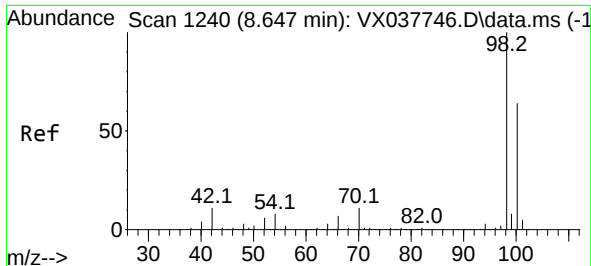

#50
Toluene-d8
Concen: 48.965 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX037787.D
Acq: 18 Sep 2023 19:33




Instrument :
MSVOA_X
ClientSampleId :
MW-16-0912

Tgt Ion: 98 Resp: 494336
Ion Ratio Lower Upper
98 100
100 63.6 53.1 79.7

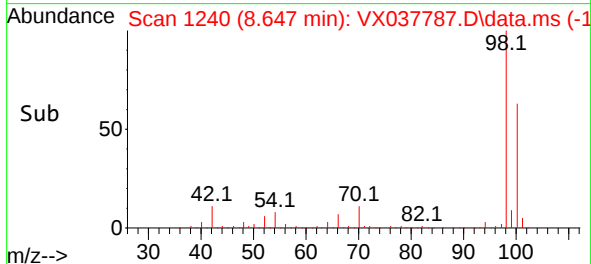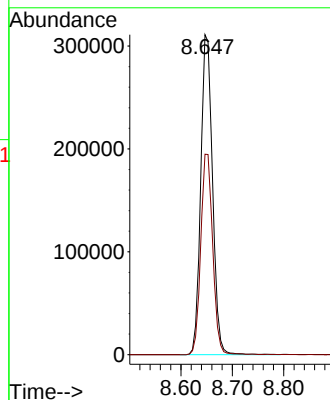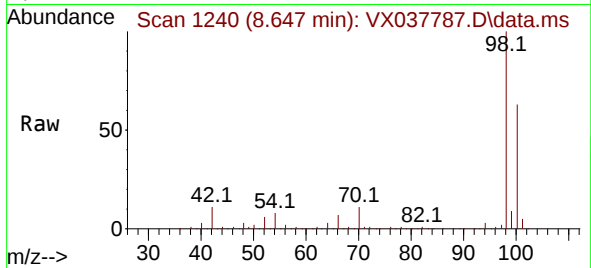

#62
4-Bromofluorobenzene
Concen: 50.210 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX037787.D
Acq: 18 Sep 2023 19:33

Tgt Ion: 95 Resp: 184202
Ion Ratio Lower Upper
95 100
174 81.6 0.0 135.6
176 78.5 0.0 131.0

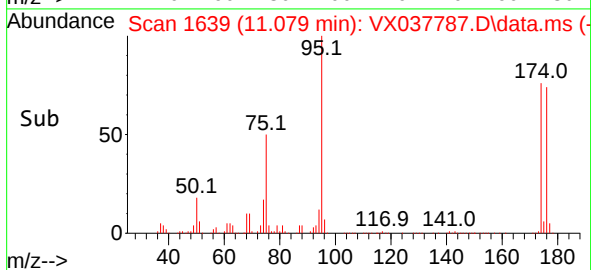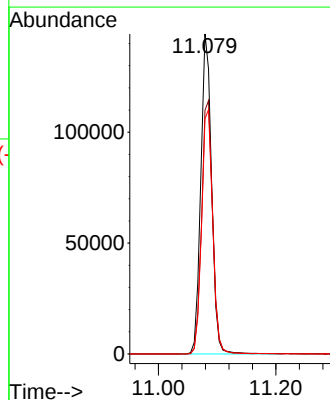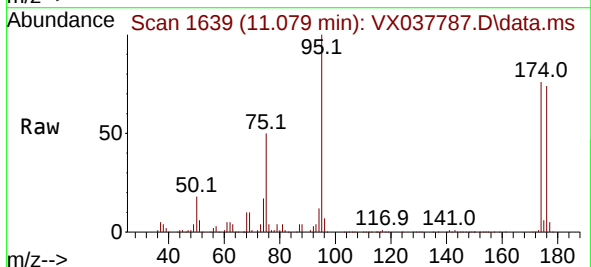



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX037787.D

Acq: 18 Sep 2023 19:33

Instrument :

MSVOA_X

ClientSampleId :

MW-16-0912





Tgt Ion:117 Resp: 389801

Ion Ratio Lower Upper

117 100

82 54.1 46.2 69.4

119 32.3 25.5 38.3

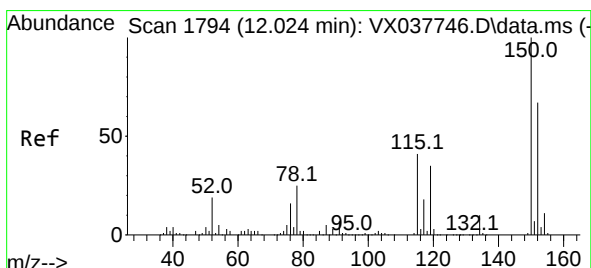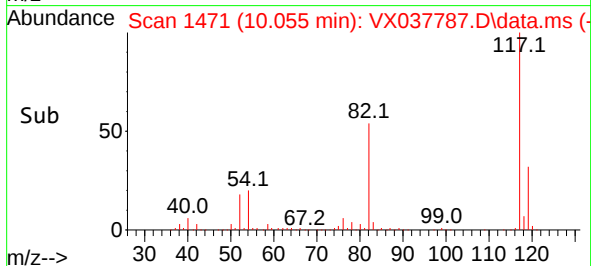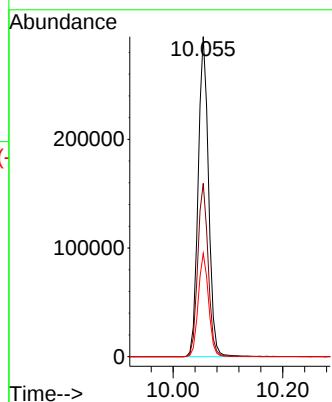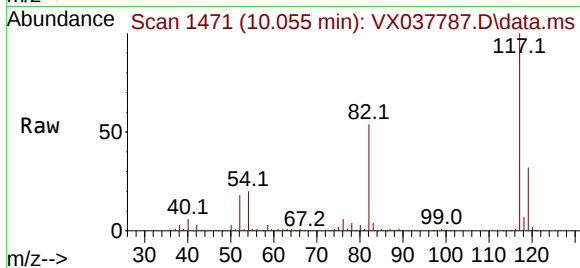

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX037787.D

Acq: 18 Sep 2023 19:33

Tgt Ion:152 Resp: 198037

Ion Ratio Lower Upper

152 100

115 60.1 43.3 129.9

150 155.1 0.0 345.0

