

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091825\
 Data File : VX047632.D
 Acq On : 18 Sep 2025 11:58
 Operator : JC/MD
 Sample : VX0918MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0918MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Title : SW846 8260

Signal : TIC: VX047632.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.538	556	566	573	rBV	4050	14003	1.51%	0.264%
2	5.367	690	702	718	rBV3	91700	294906	31.81%	5.553%
3	5.532	718	729	753	rVB	150351	458757	49.48%	8.639%
4	5.940	784	796	813	rBV	98346	291153	31.41%	5.483%
5	6.745	917	928	946	rBV	269690	710188	76.60%	13.373%
6	8.635	1231	1238	1252	rBV	515649	871604	94.02%	16.413%
7	10.037	1462	1468	1484	rBV	657263	921714	99.42%	17.356%
8	11.061	1631	1636	1648	rBV	480601	636493	68.66%	11.986%
9	11.433	1693	1697	1702	rVB2	8394	10923	1.18%	0.206%
10	11.695	1734	1740	1744	rBV2	7020	10079	1.09%	0.190%
11	11.872	1765	1769	1773	rVB	11003	13036	1.41%	0.245%
12	12.000	1785	1790	1805	rVB	703469	927087	100.00%	17.458%
13	12.317	1837	1842	1847	rVB	20169	24933	2.69%	0.470%
14	13.268	1993	1998	2004	rVB	12917	16238	1.75%	0.306%
15	13.567	2043	2047	2054	rVB2	14286	18620	2.01%	0.351%
16	13.707	2065	2070	2074	rVB3	27375	34168	3.69%	0.643%
17	13.756	2074	2078	2084	rVB	11045	14318	1.54%	0.270%
18	13.939	2103	2108	2114	rVB	14508	18305	1.97%	0.345%
19	15.670	2386	2392	2397	rBV5	12140	23969	2.59%	0.451%




Sum of corrected areas: 5310494

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091825\
Data File : VX047632.D
Acq On : 18 Sep 2025 11:58
Operator : JC/MD
Sample : VX0918MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0918MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

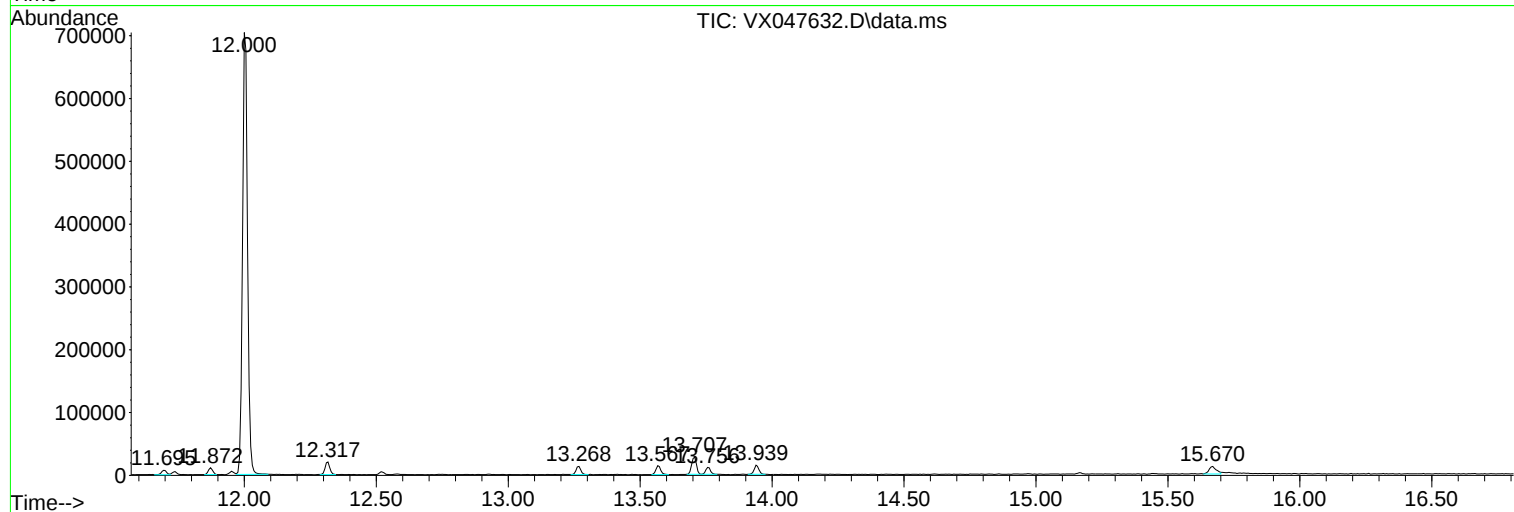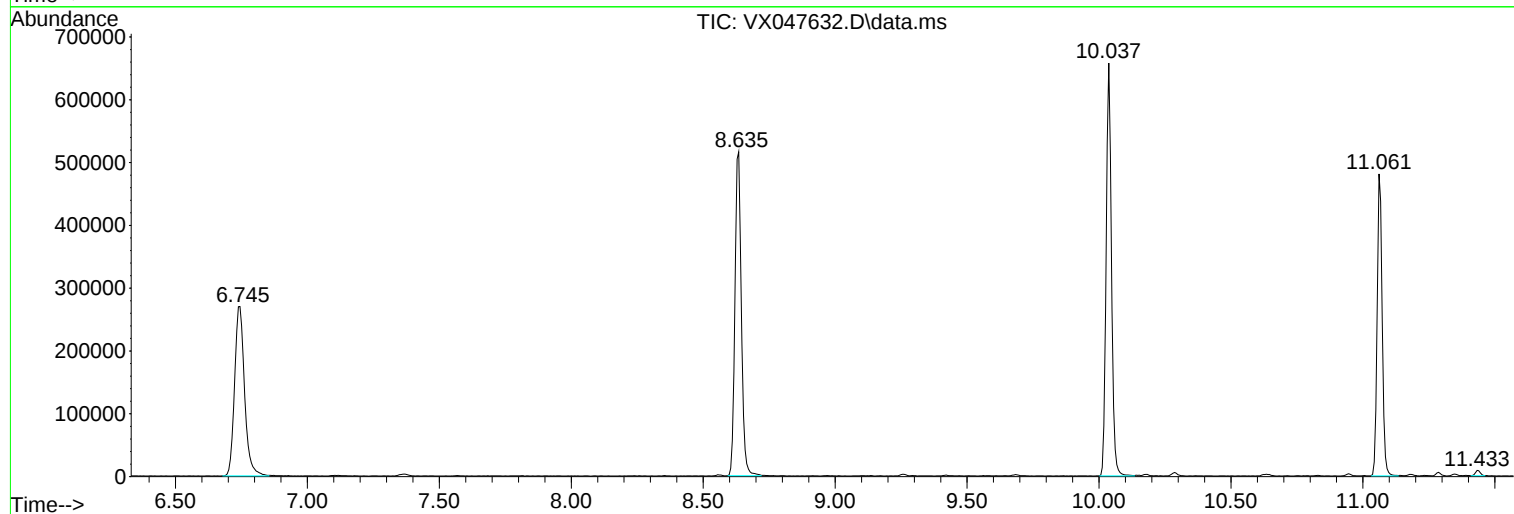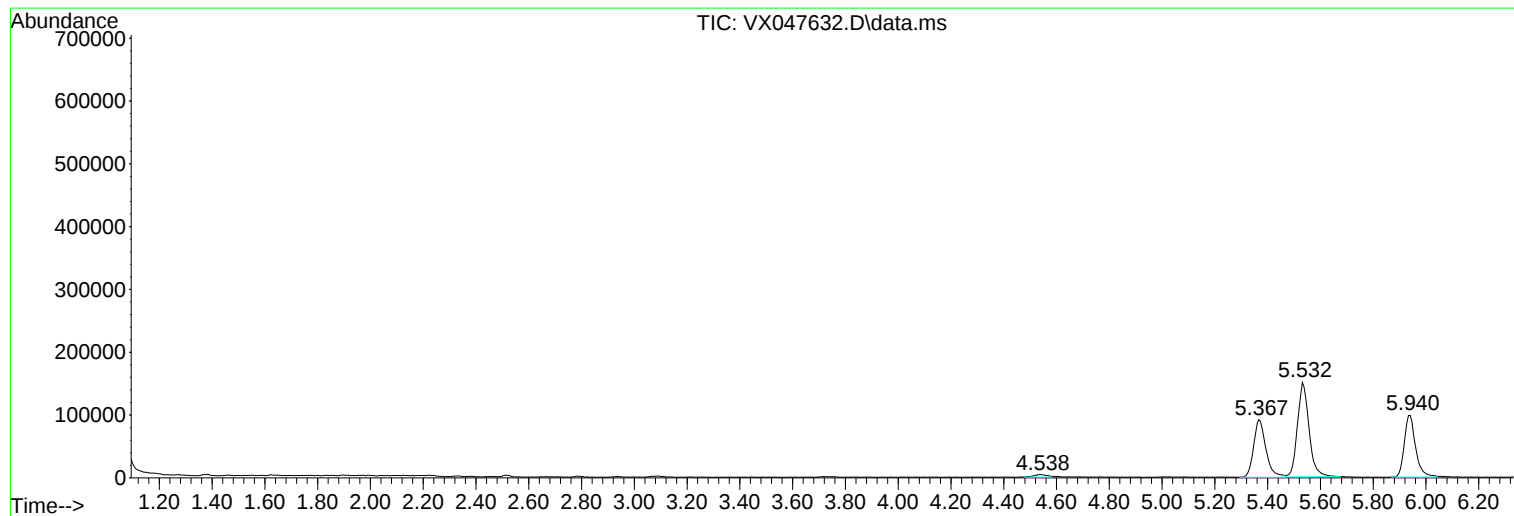

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091825\
Data File : VX047632.D
Acq On : 18 Sep 2025 11:58
Operator : JC/MD
Sample : VX0918MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0918MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091825\
Data File : VX047632.D
Acq On : 18 Sep 2025 11:58
Operator : JC/MD
Sample : VX0918MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0918MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc