


# Chloroethane

Response Ratio

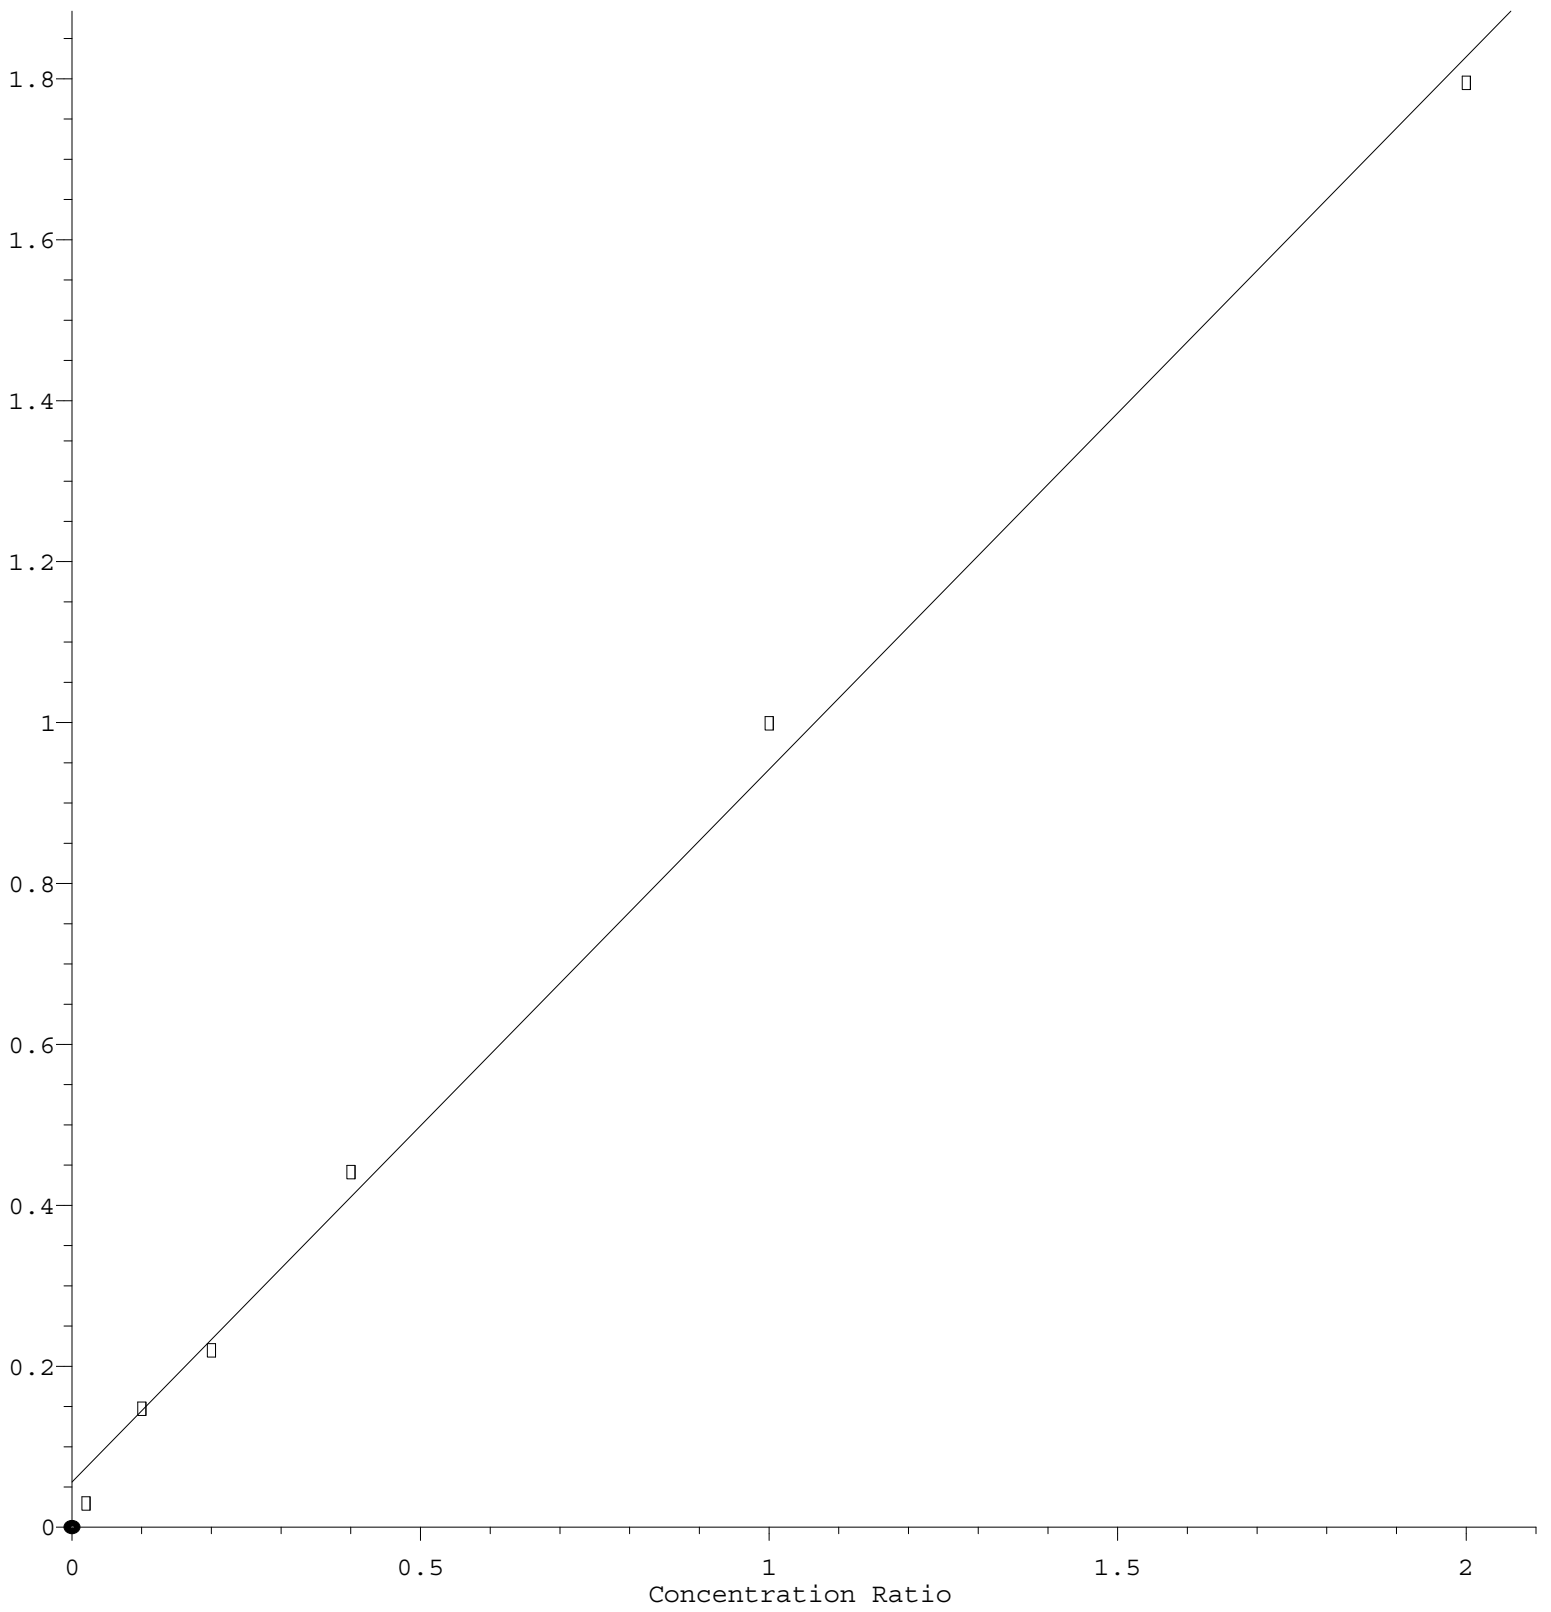


$$\text{Response} = 8.860\text{e-}001 * \text{Amt} + 5.591\text{e-}002$$

Coef of Det ( $r^2$ ) = 0.996740 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091922W.M

Calibration Table Last Updated: Tue Sep 20 09:45:29 2022


## Hexachlorobutadiene

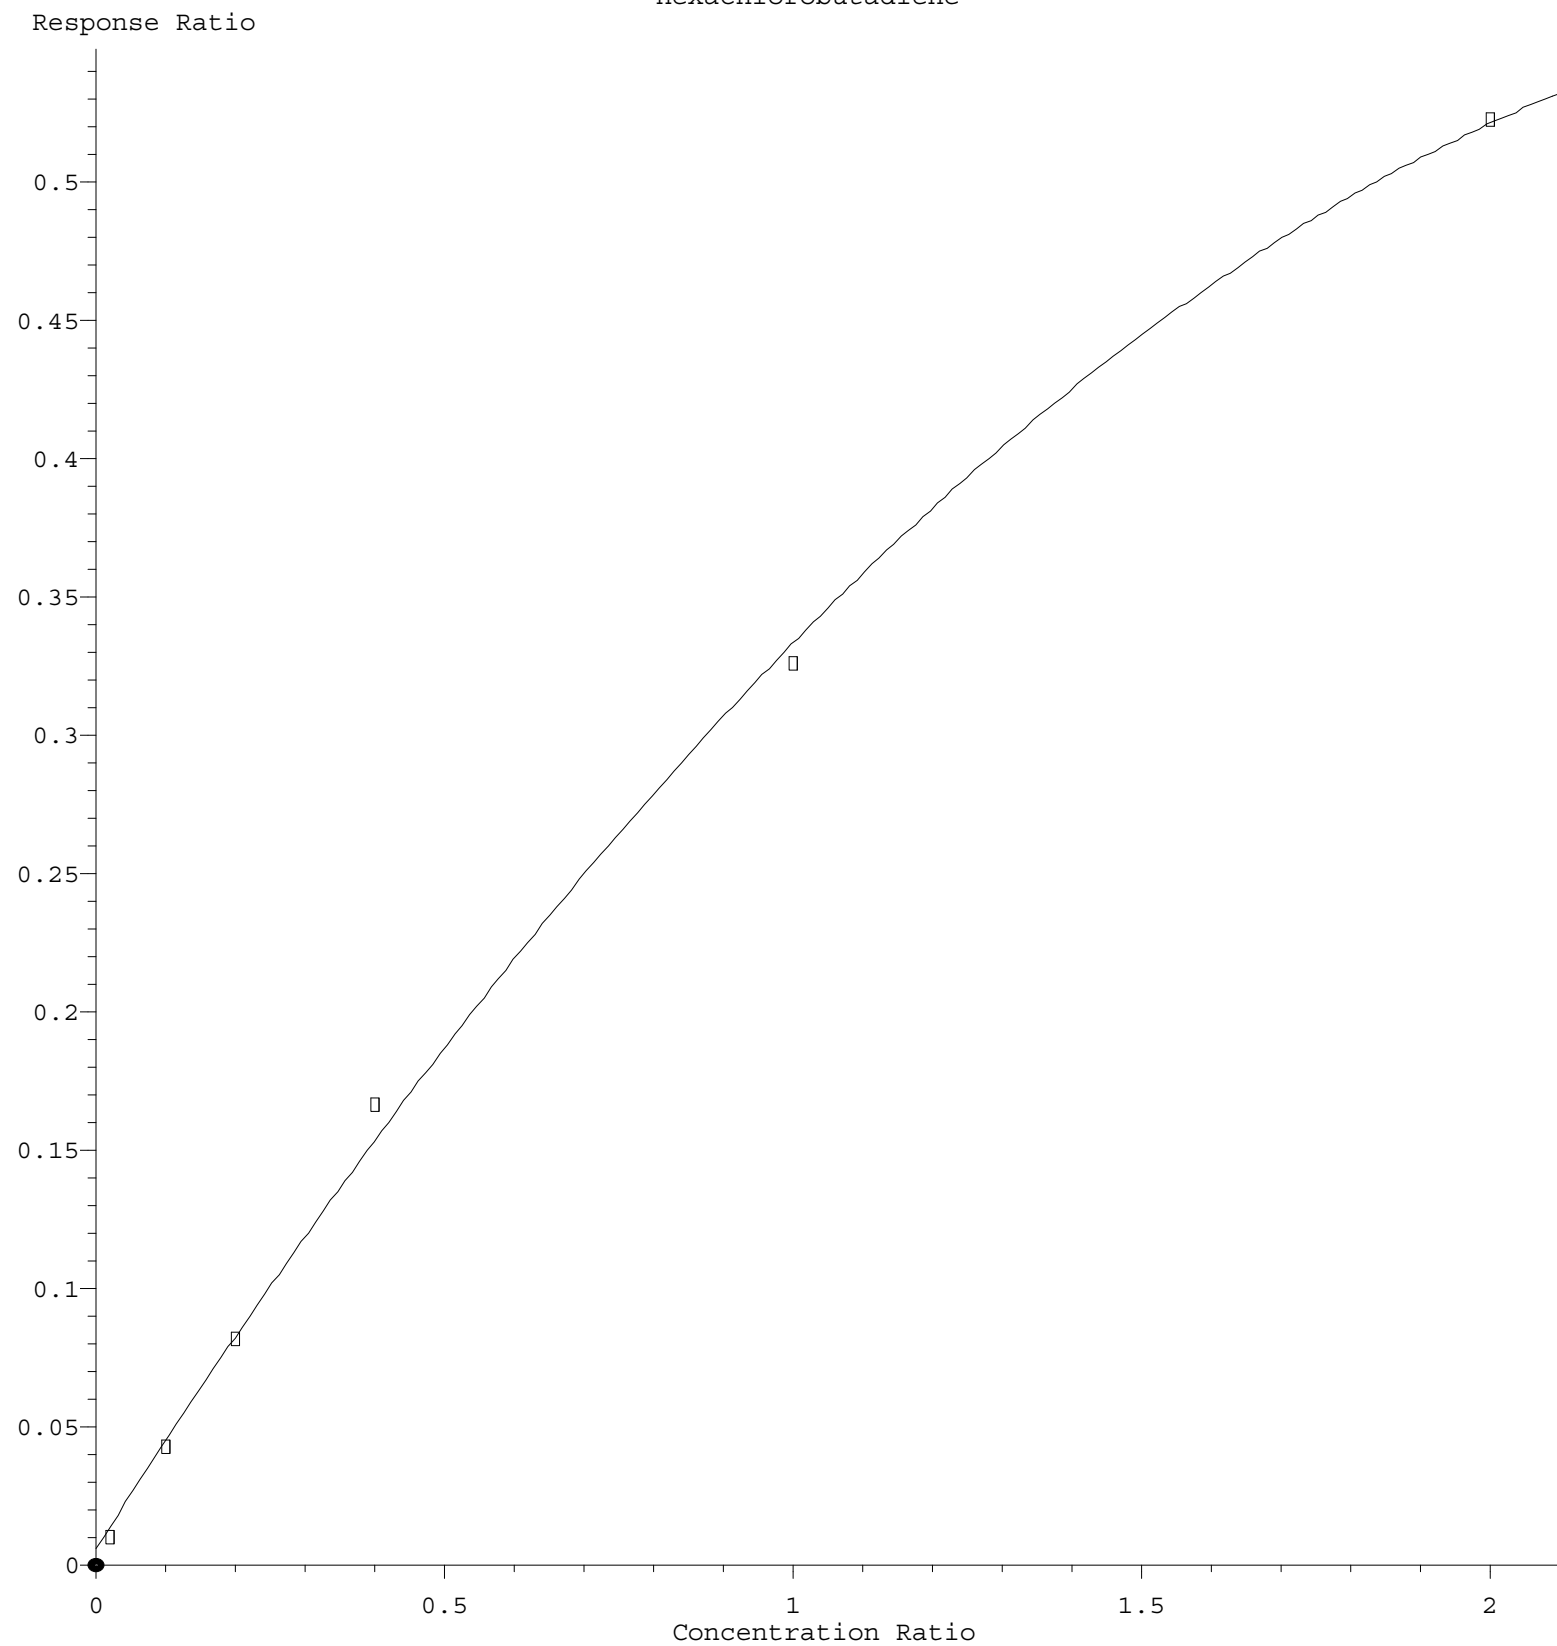

$R = -6.970e-002 A^2 + 3.970e-001 A + 5.986e-003$   
Coef of Det ( $r^2$ ) = 0.998772    Curve Fit: Quadratic  
Method Name:    Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091922W.M  
Calibration Table Last Updated: Tue Sep 20 09:45:29 2022

# 1,1,1,2-Tetrachloroethane

Response Ratio

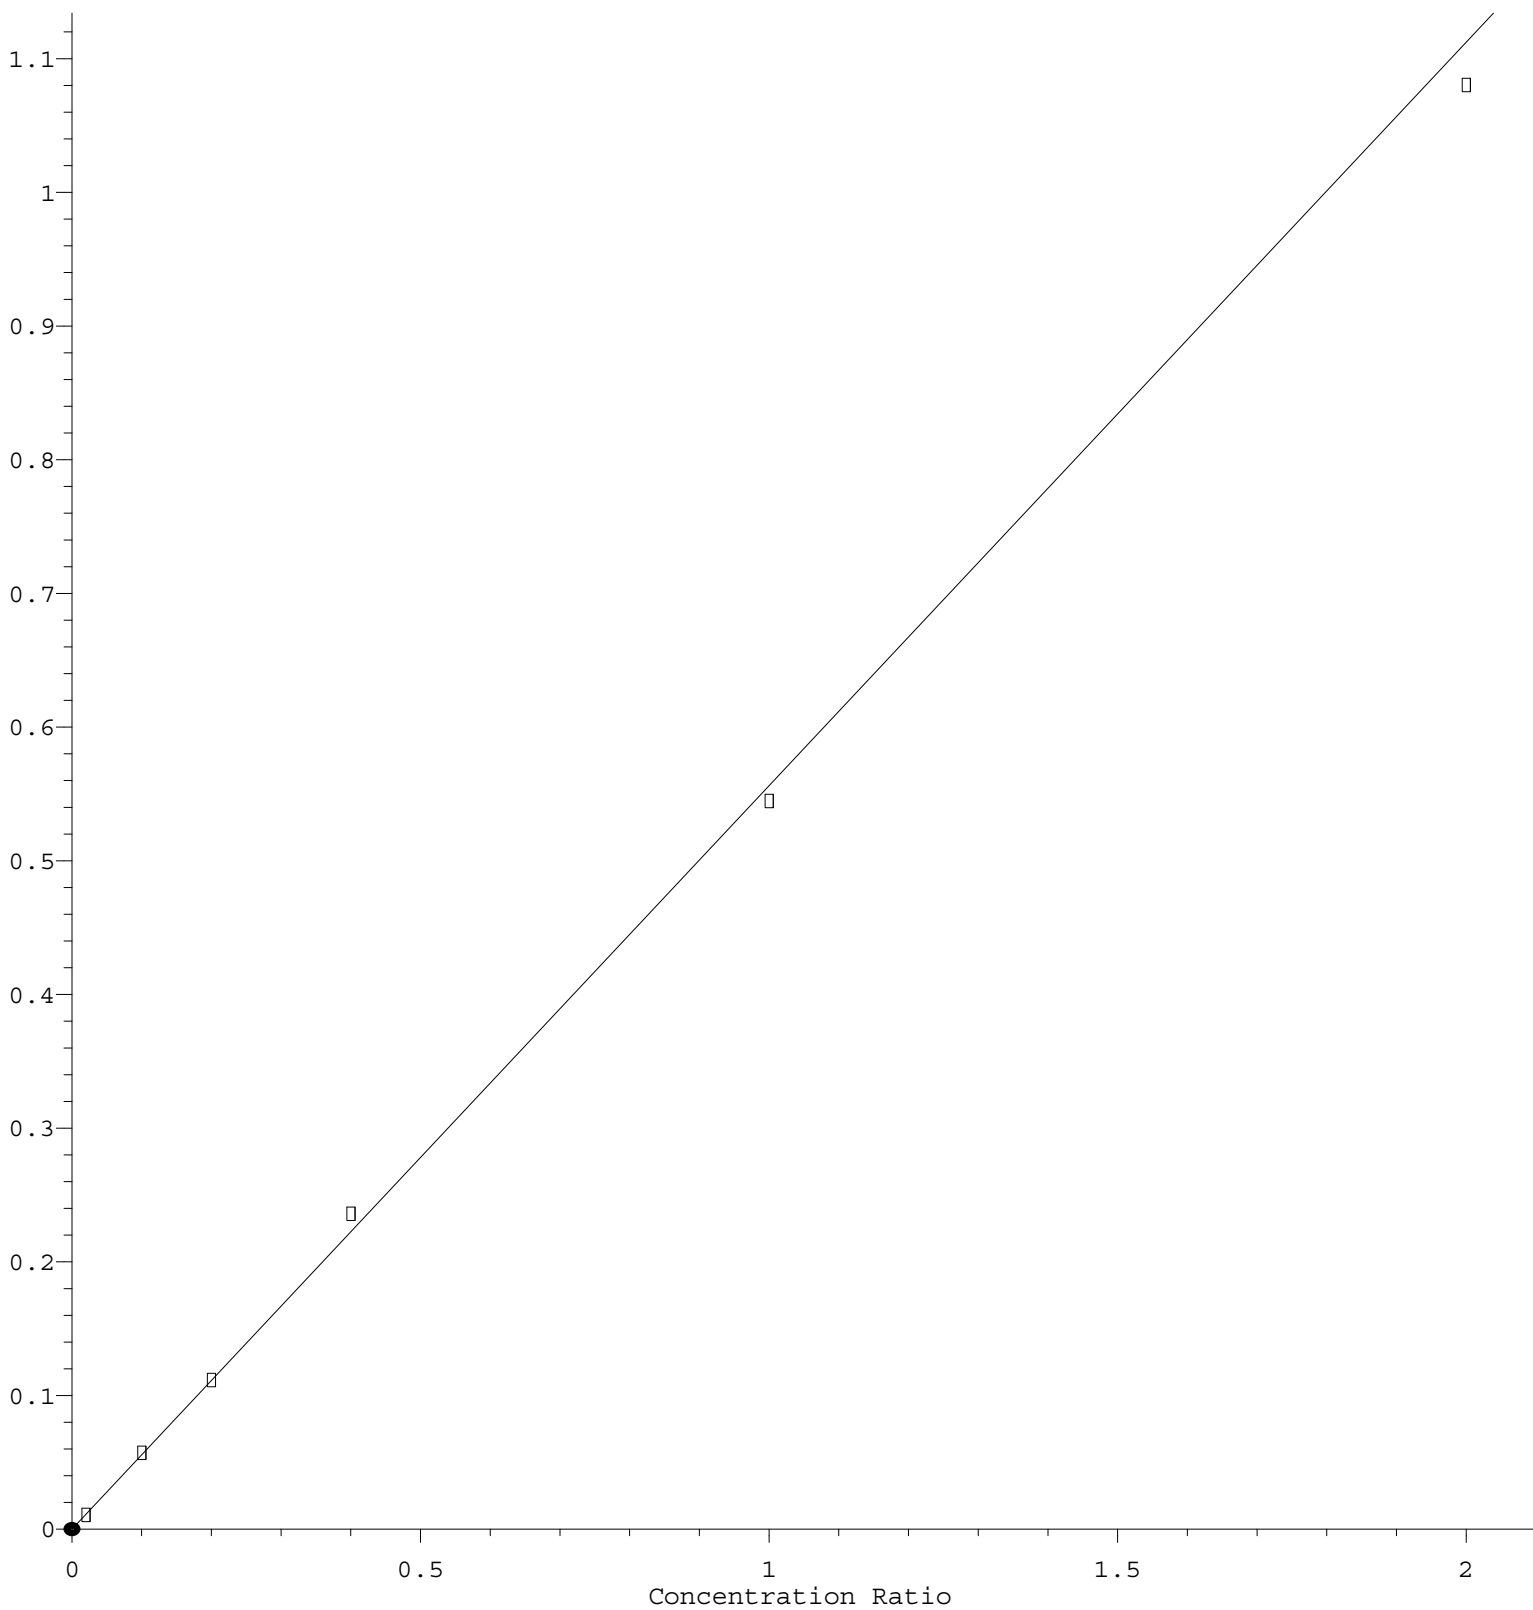

$$\text{Response} = 5.563\text{e-}001 * \text{Amt}$$


RF Rel Std Dev = 3.735% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091922W.M

Calibration Table Last Updated: Tue Sep 20 09:45:29 2022

# Tetrachloroethene

Response Ratio

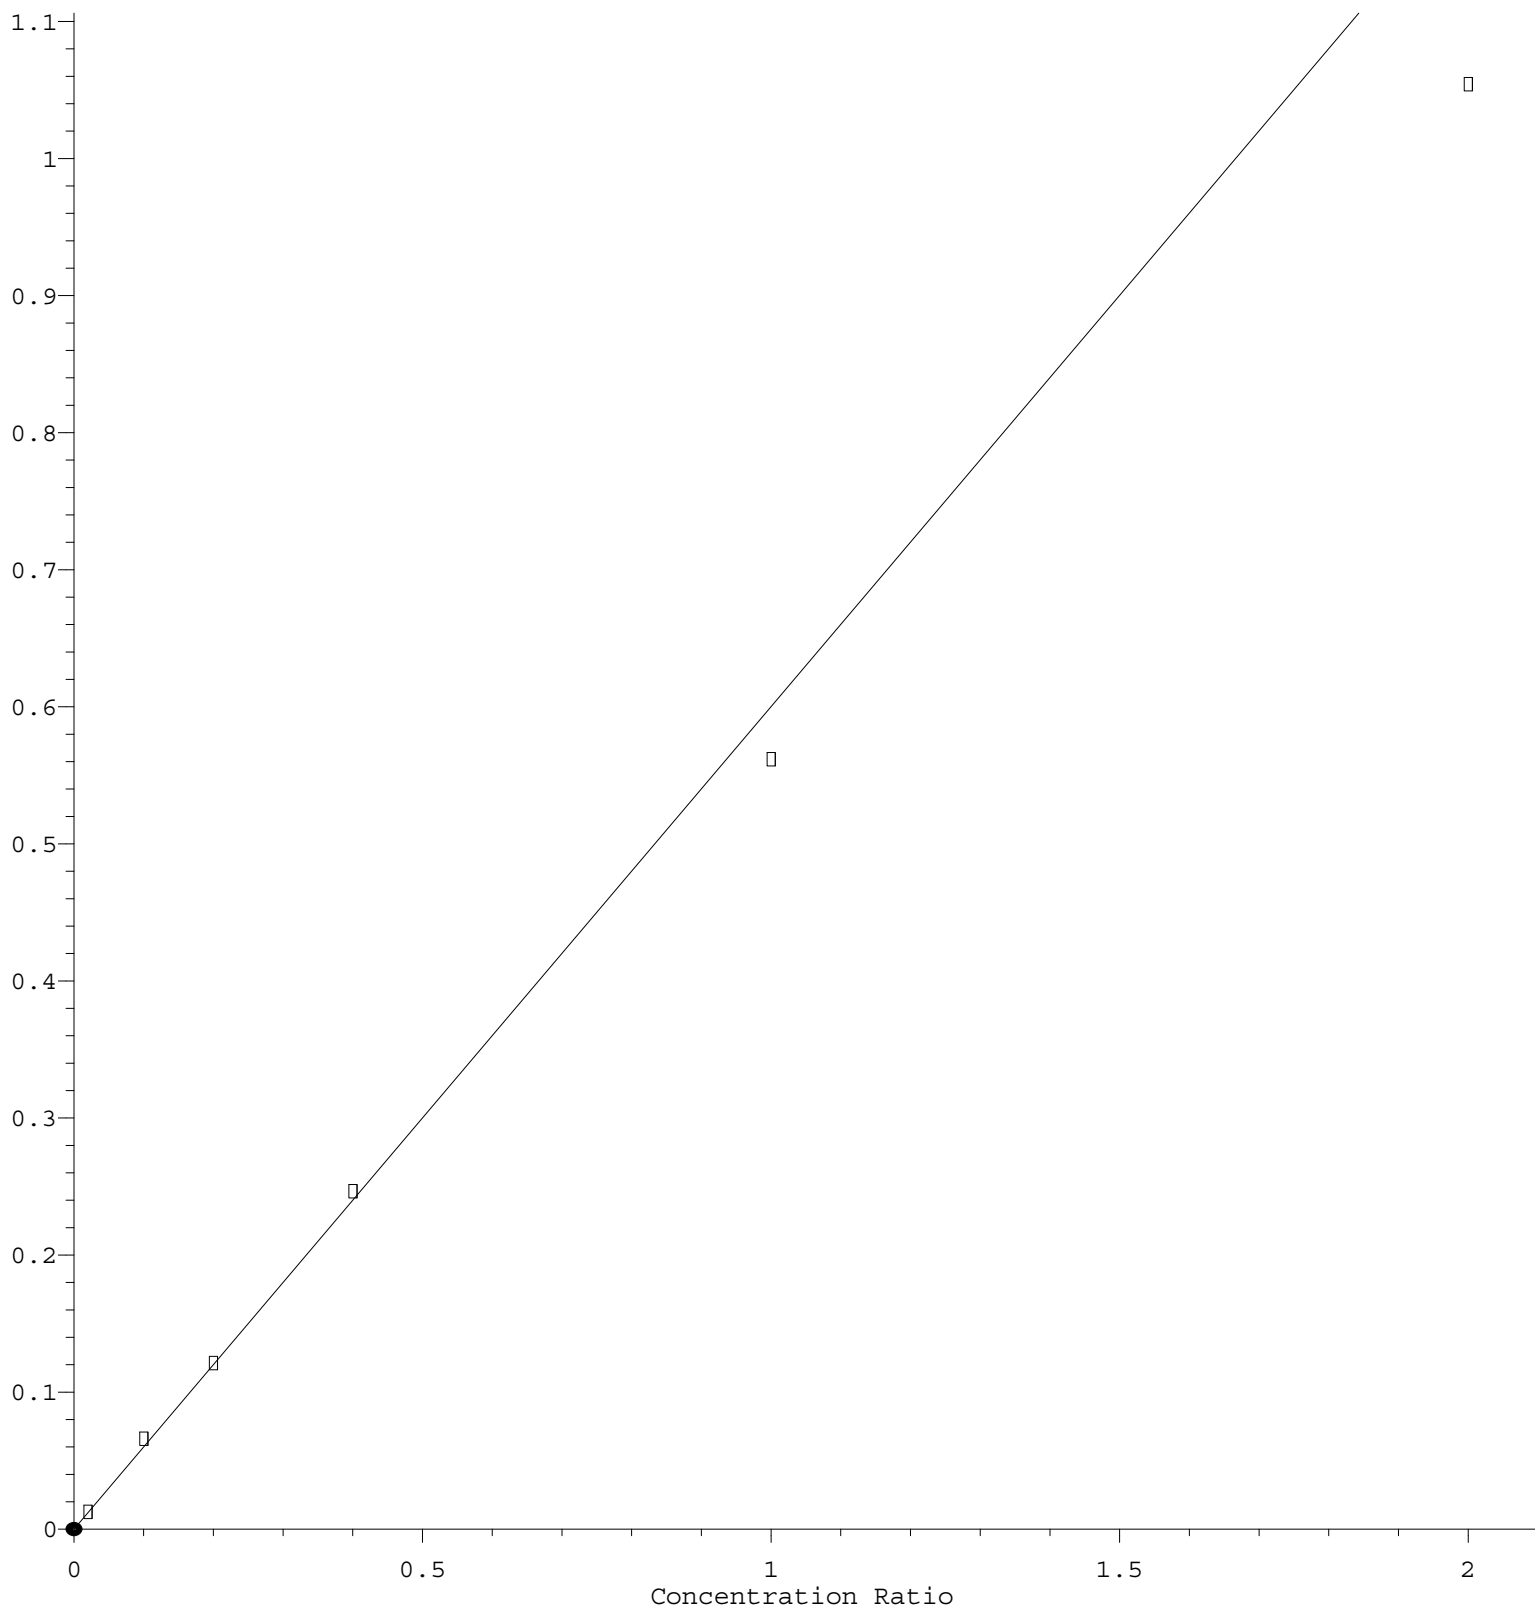

$$\text{Response} = 6.006\text{e-}001 * \text{Amt}$$


RF Rel Std Dev = 8.069% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091922W.M

Calibration Table Last Updated: Tue Sep 20 09:45:29 2022

# Dibromofluoromethane


Response Ratio

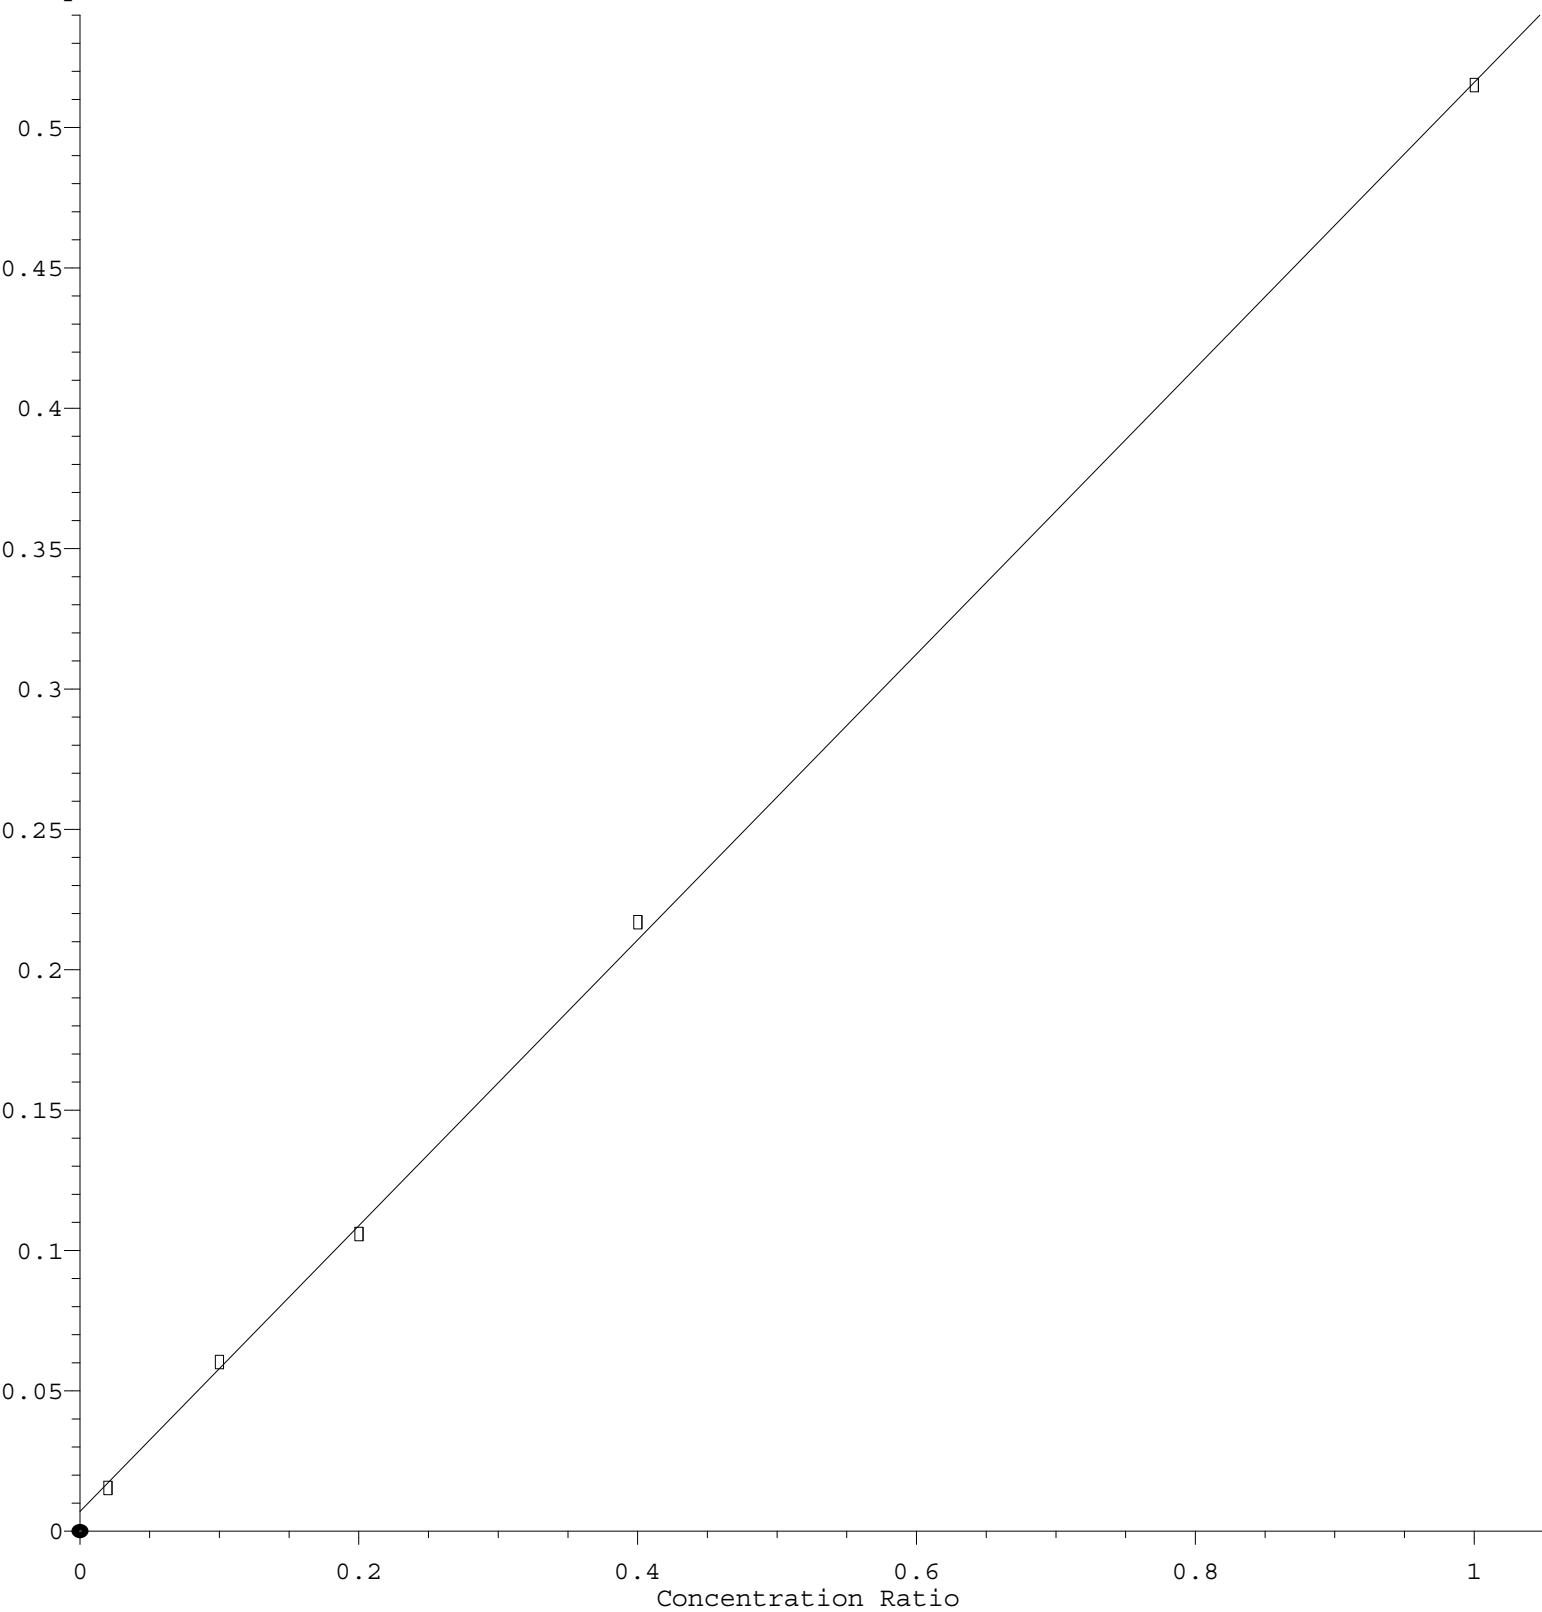

Response = 5.093e-001 \* Amt + 7.494e-003  
 Coef of Det (r^2) = 0.999651 Curve Fit: Linear  
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091922W.M  
 Calibration Table Last Updated: Tue Sep 20 09:45:29 2022

## 1,2-Dichloroethane-d4

Response Ratio

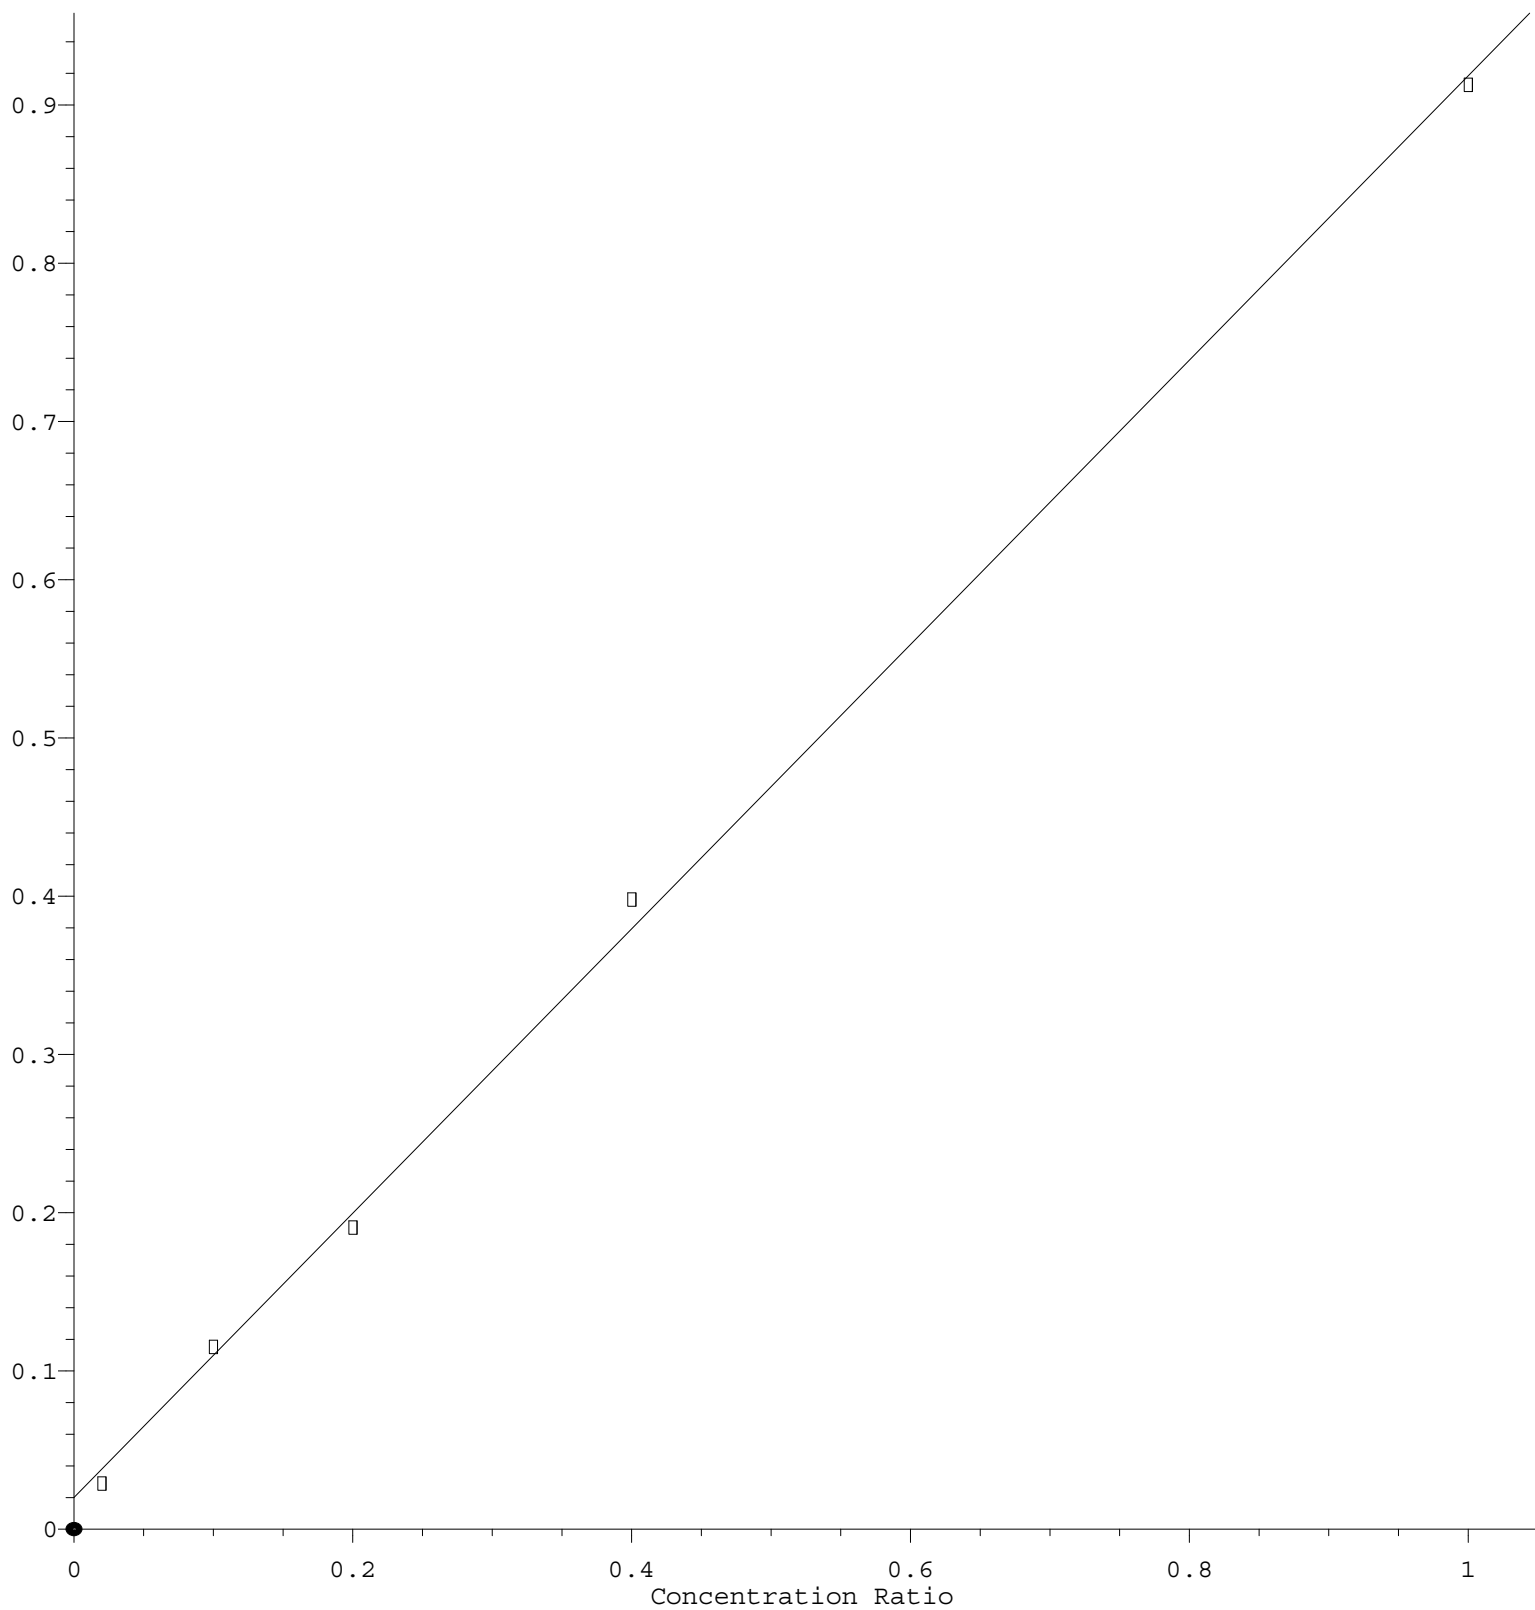

$$\text{Response} = 8.989\text{e-}001 * \text{Amt} + 1.980\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.998861 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091922W.M

Calibration Table Last Updated: Tue Sep 20 09:45:29 2022

# Methylene Chloride


Response Ratio

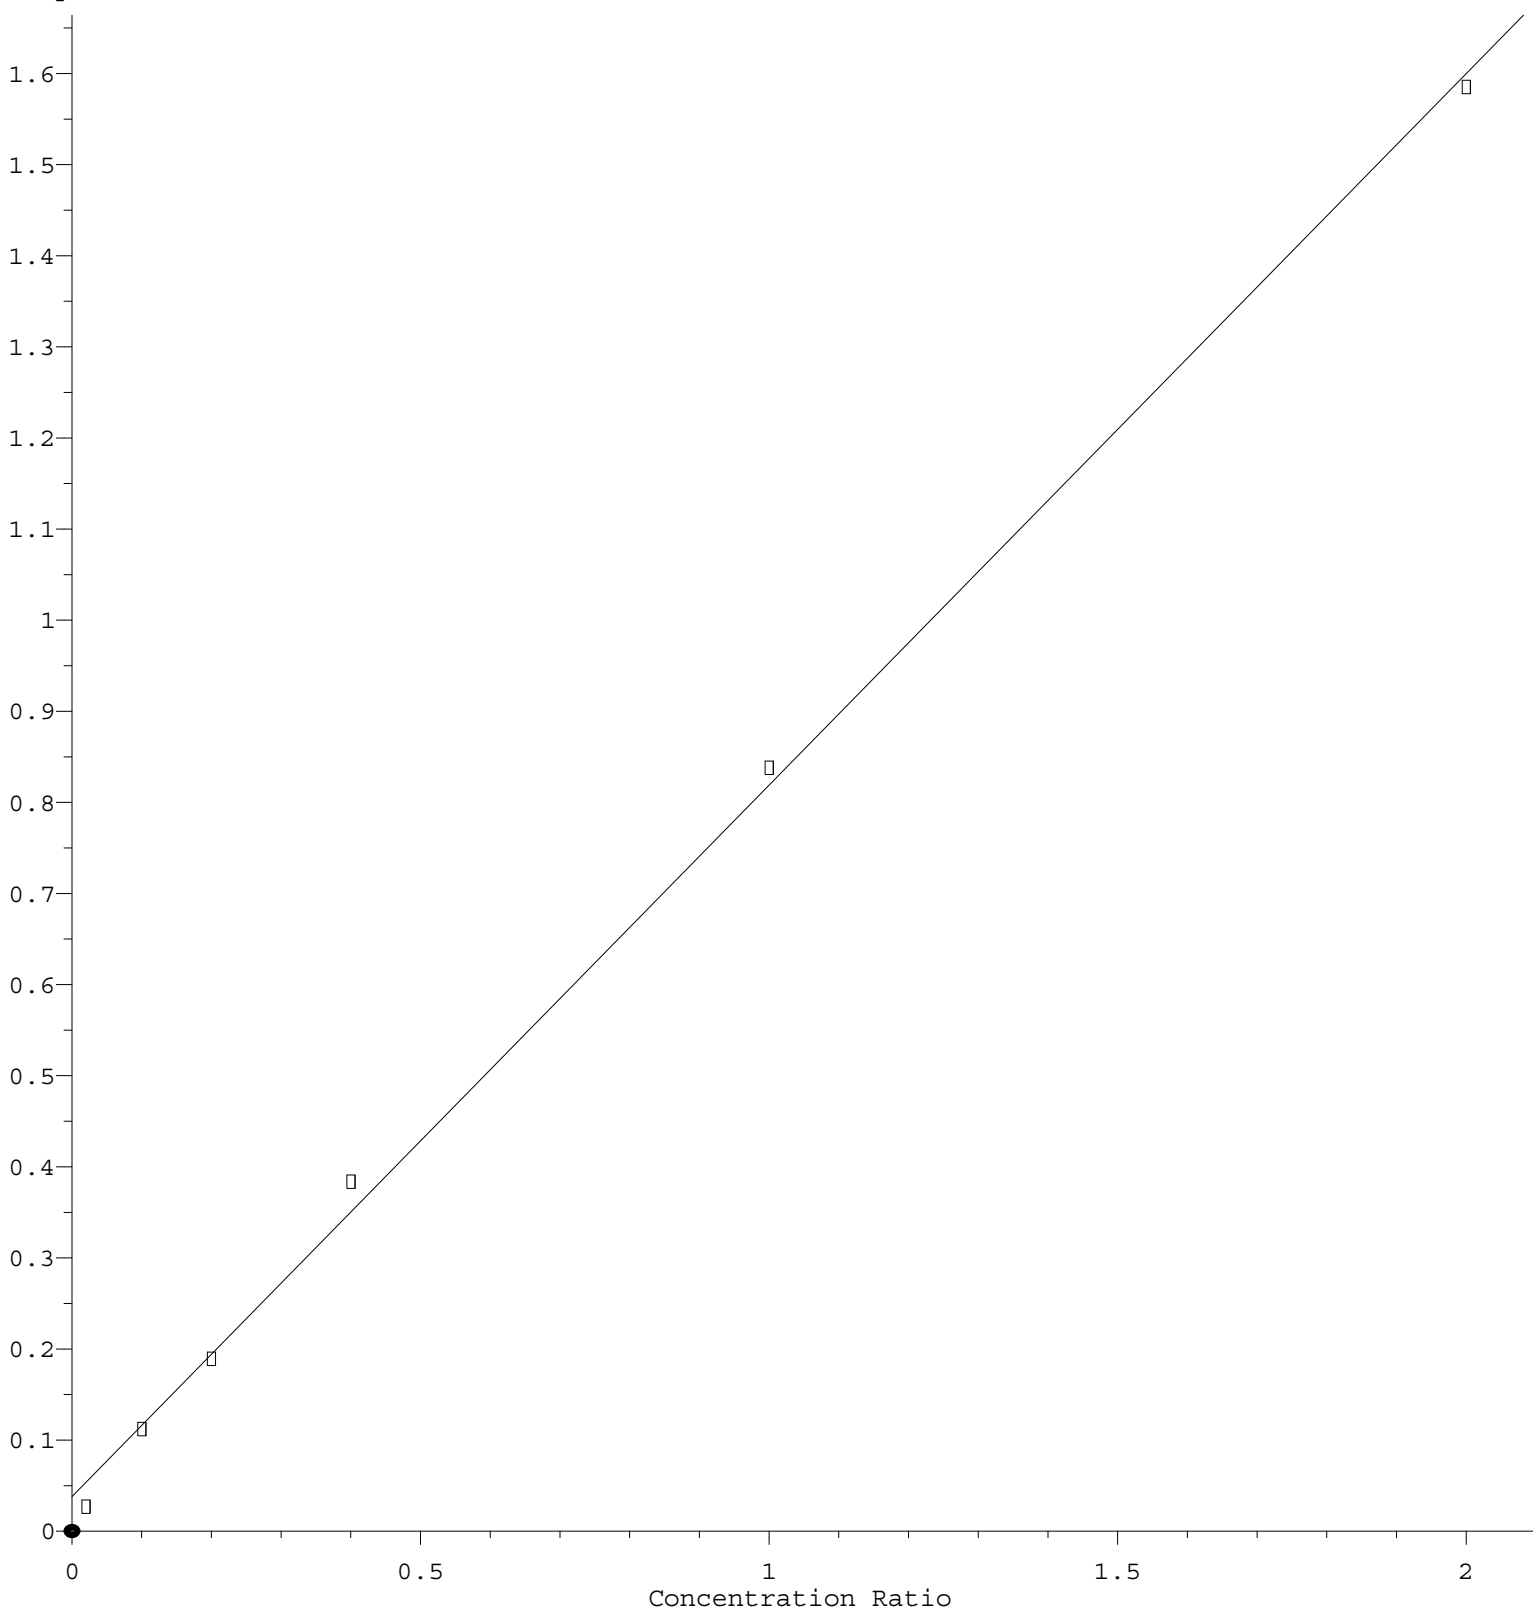

Response =  $7.809e-001 \cdot \text{Amt} + 3.831e-002$   
 Coef of Det ( $r^2$ ) = 0.998624    Curve Fit: Linear  
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091922W.M  
 Calibration Table Last Updated: Tue Sep 20 09:45:29 2022

# Acetone


Response Ratio

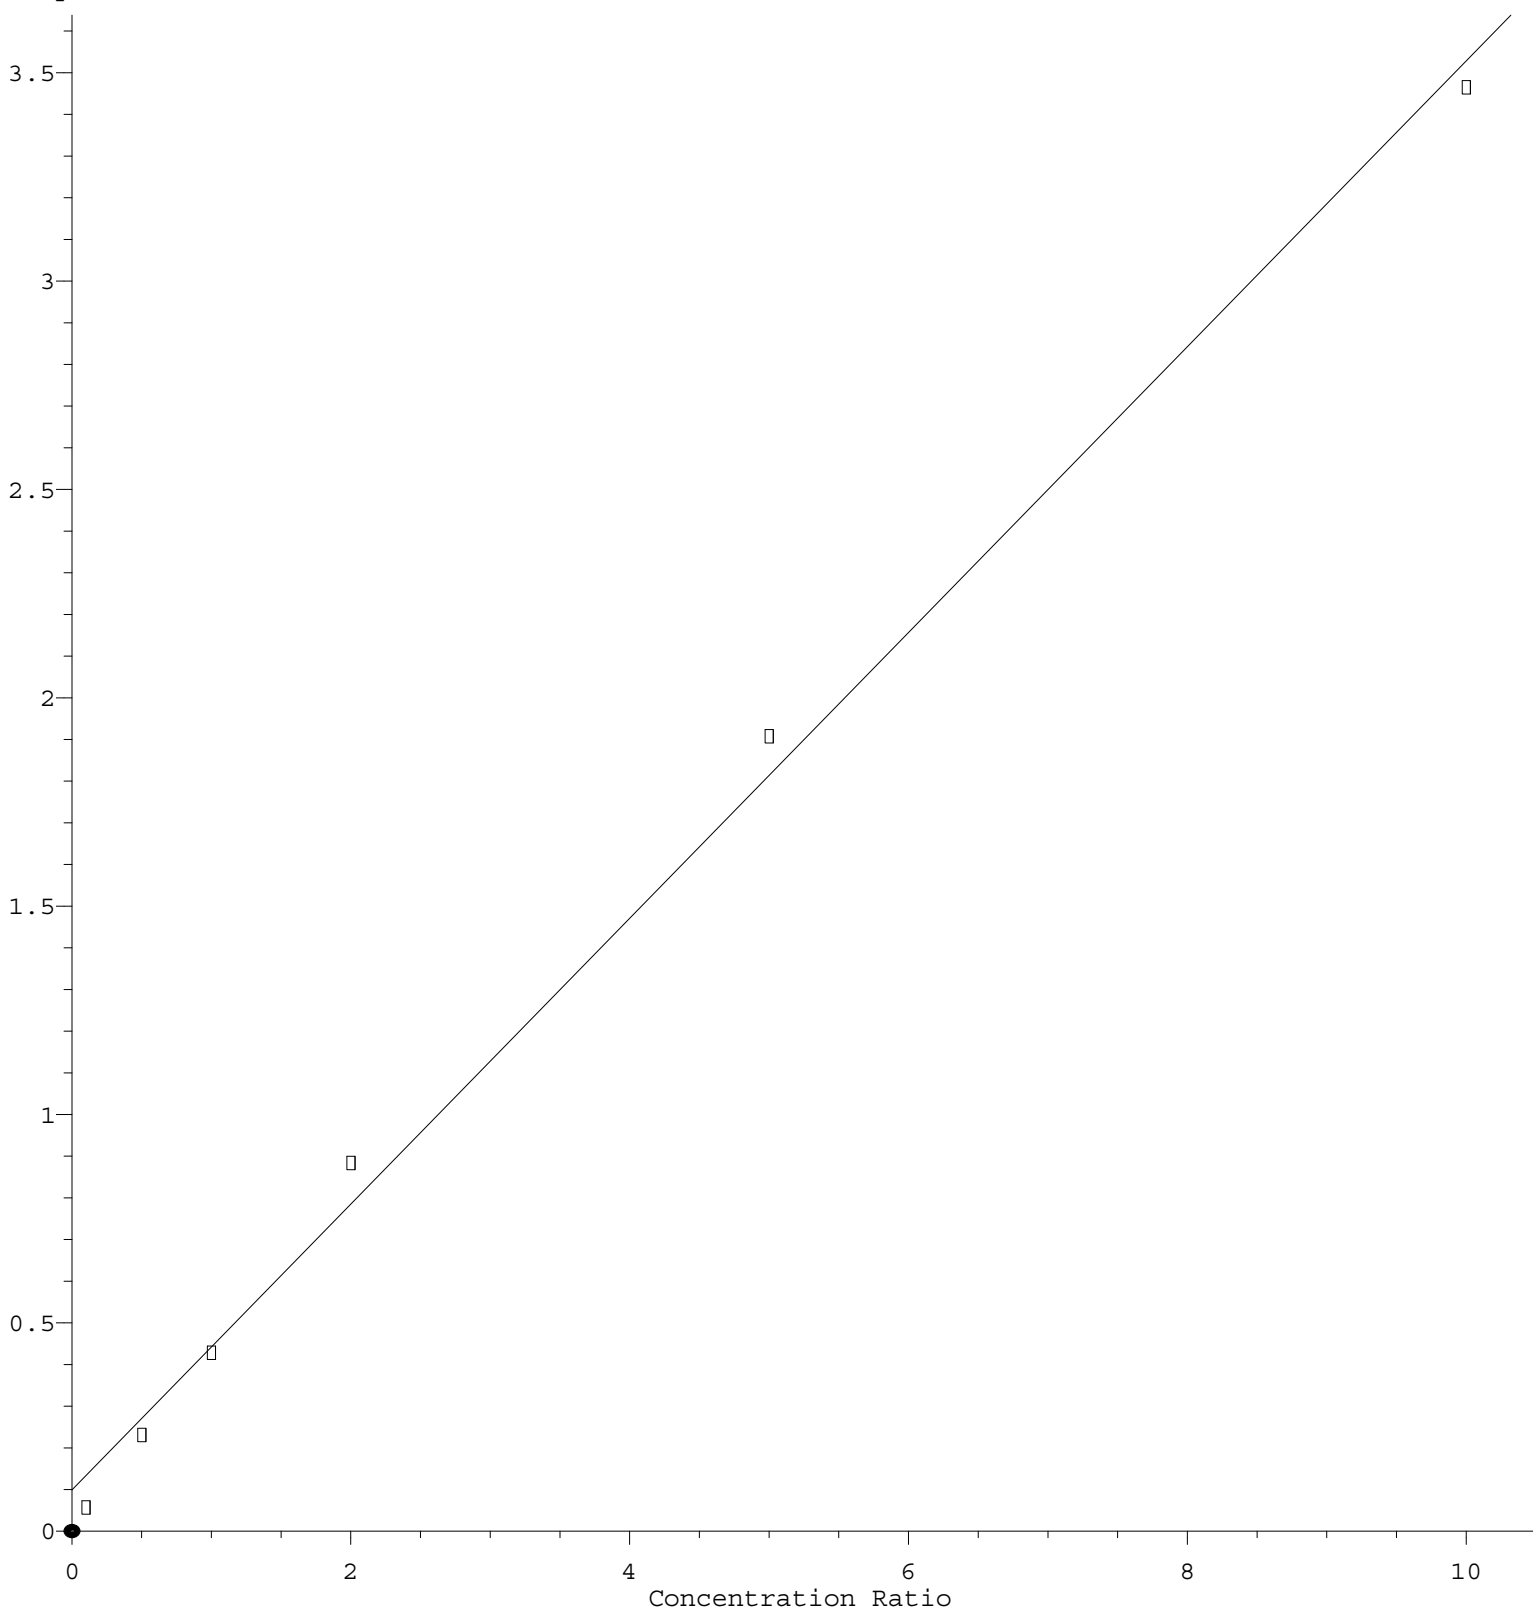

Response = 3.429e-001 \* Amt + 9.906e-002  
 Coef of Det (r^2) = 0.996478    Curve Fit: Linear  
 Method Name:    Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091922W.M  
 Calibration Table Last Updated: Tue Sep 20 09:45:29 2022

# Acrolein

Response Ratio

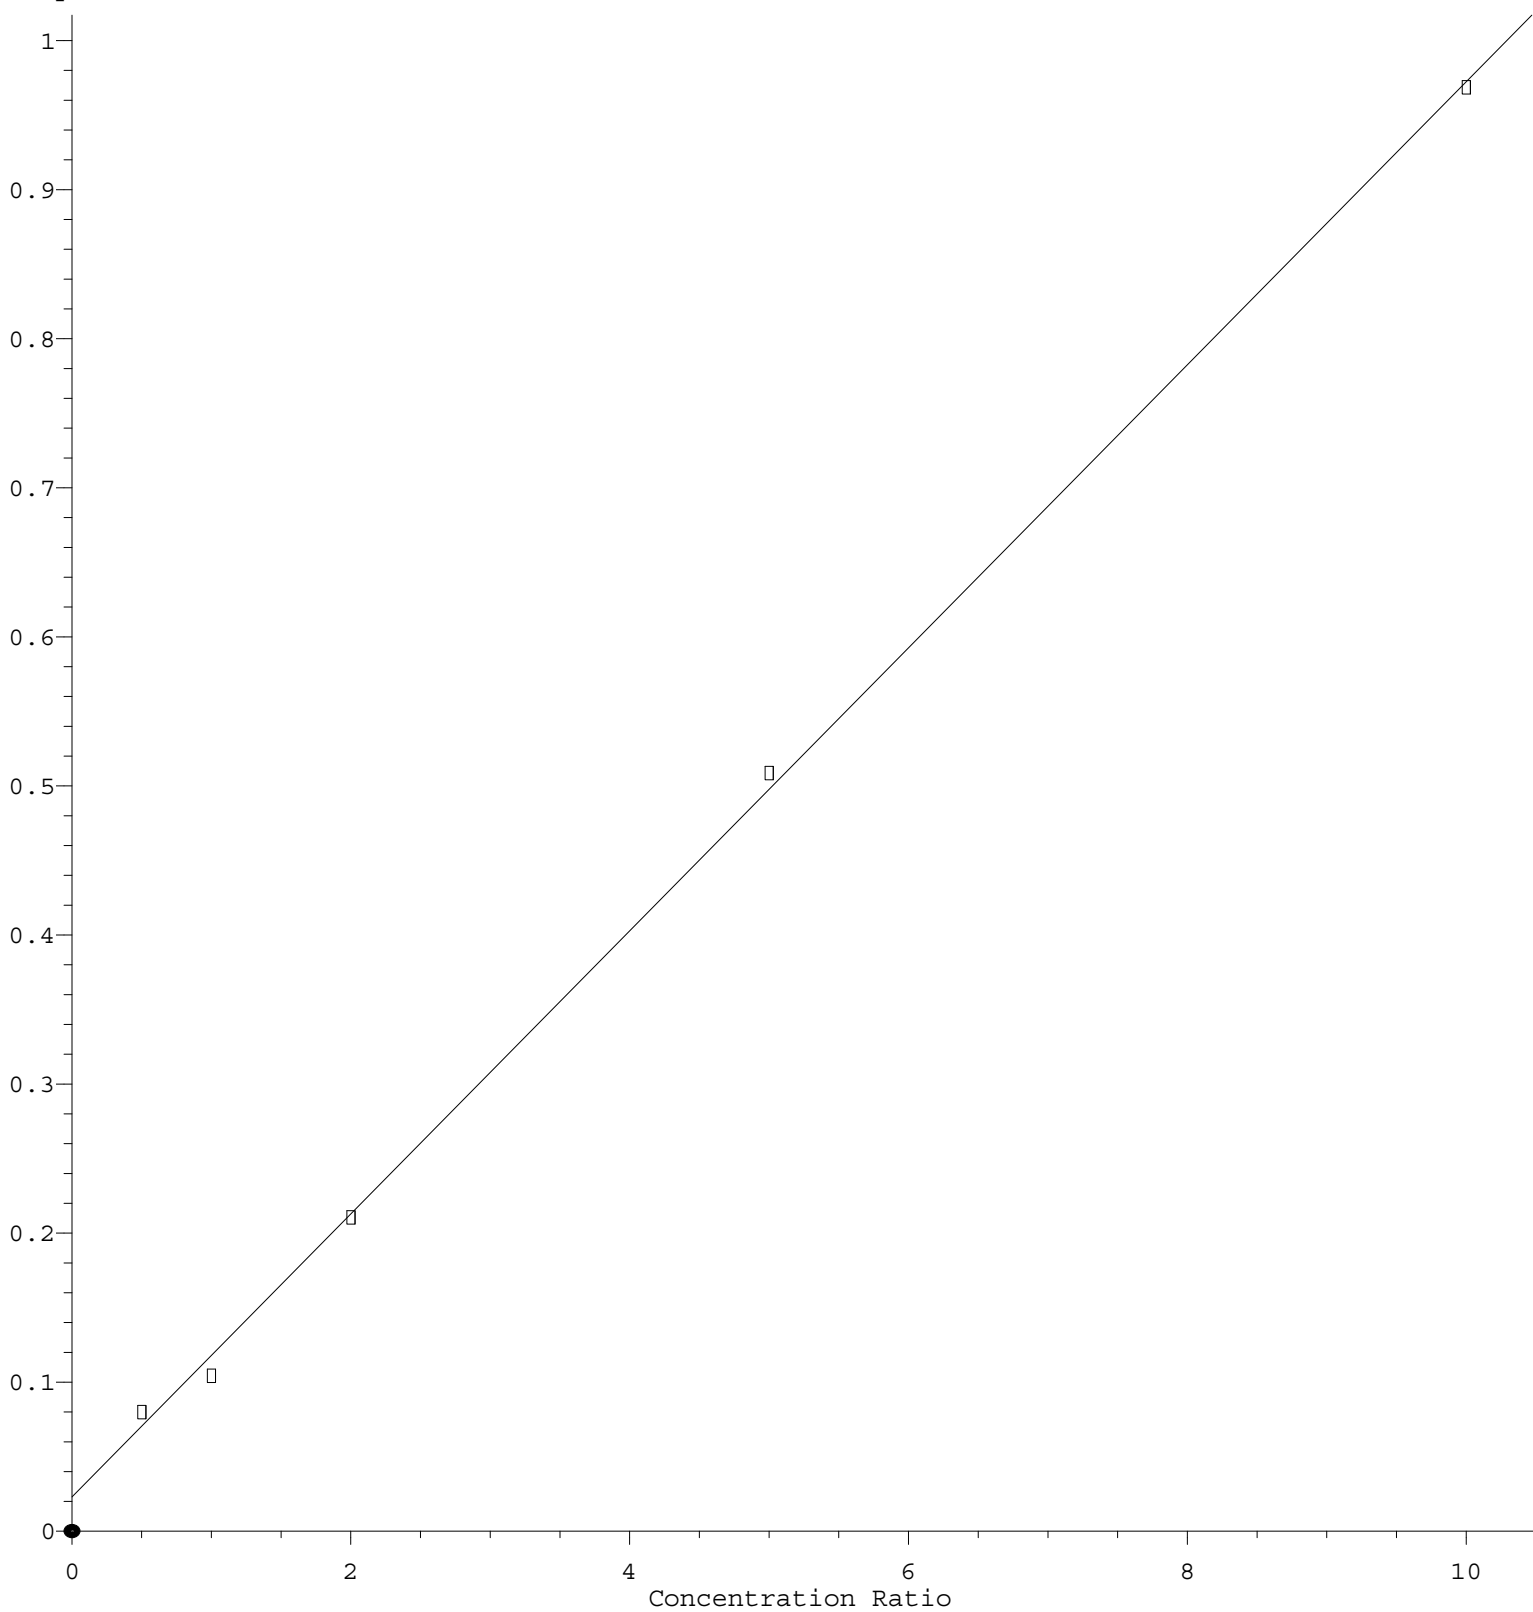

$$\text{Response} = 9.496\text{e-}002 * \text{Amt} + 2.300\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.999258 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091922W.M

Calibration Table Last Updated: Tue Sep 20 09:45:29 2022

## Tert butyl alcohol

Response Ratio

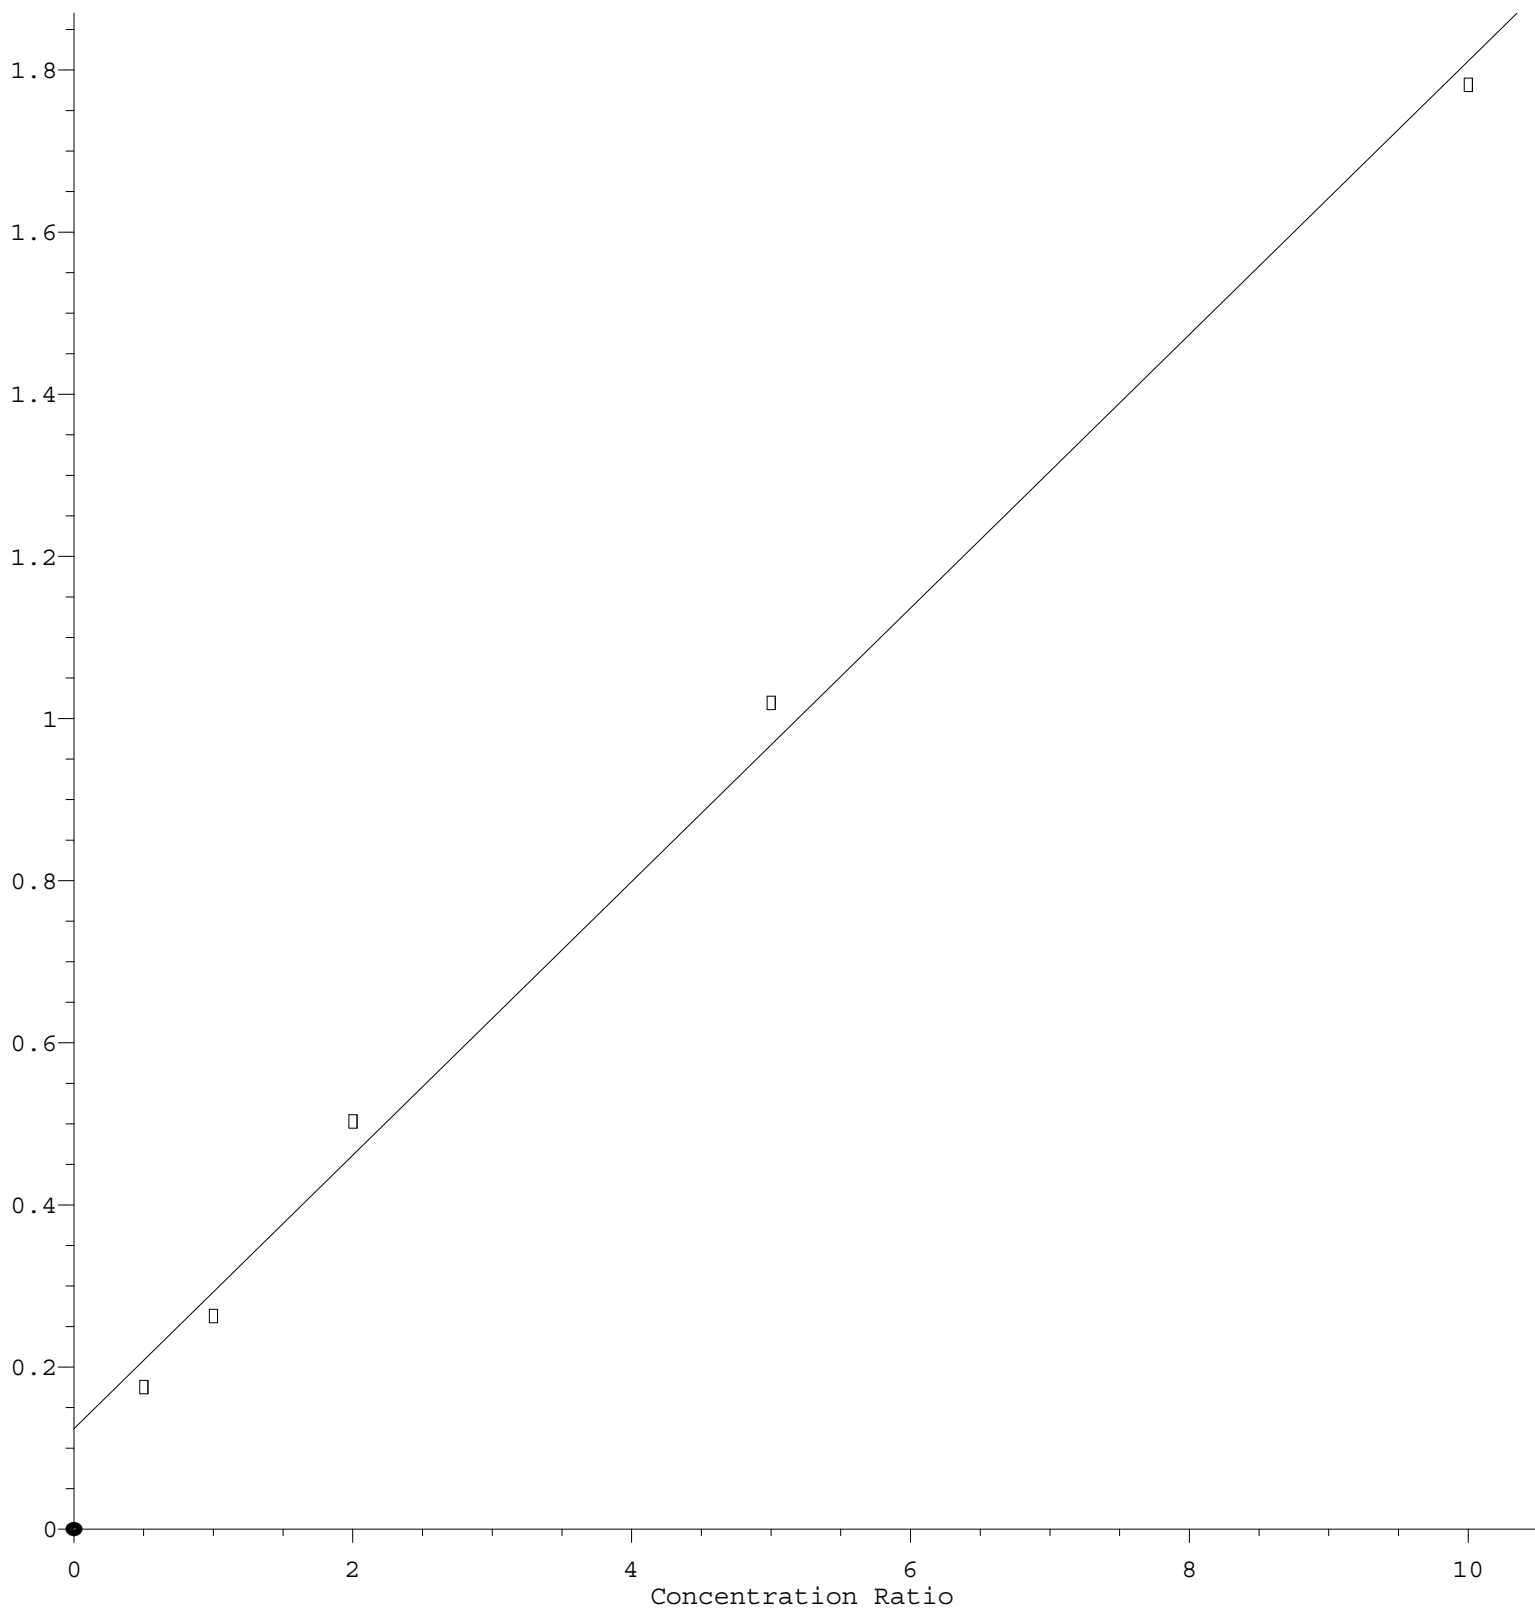

$$\text{Response} = 1.687\text{e-}001 * \text{Amt} + 1.243\text{e-}001$$

Coef of Det ( $r^2$ ) = 0.995907 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X091922W.M

Calibration Table Last Updated: Tue Sep 20 09:45:29 2022