

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091922\
 Data File : VX031473.D
 Acq On : 19 Sep 2022 20:23
 Operator : JC/MD
 Sample : N4558-09RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-RW5-GW-278-280RE

Quant Time: Sep 20 09:50:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 20 09:45:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	67798	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	113348	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	104699	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	46284	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	74672	60.163	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	120.320%
35) Dibromofluoromethane	5.391	113	62693	53.564	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	107.120%
50) Toluene-d8	8.653	98	238205	52.748	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	105.500%
62) 4-Bromofluorobenzene	11.085	95	72977	47.708	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	95.420%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091922\
Data File : VX031473.D
Acq On : 19 Sep 2022 20:23
Operator : JC/MD
Sample : N4558-09RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW5-GW-278-280RE


Quant Time: Sep 20 09:50:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 09:45:29 2022
Response via : Initial Calibration

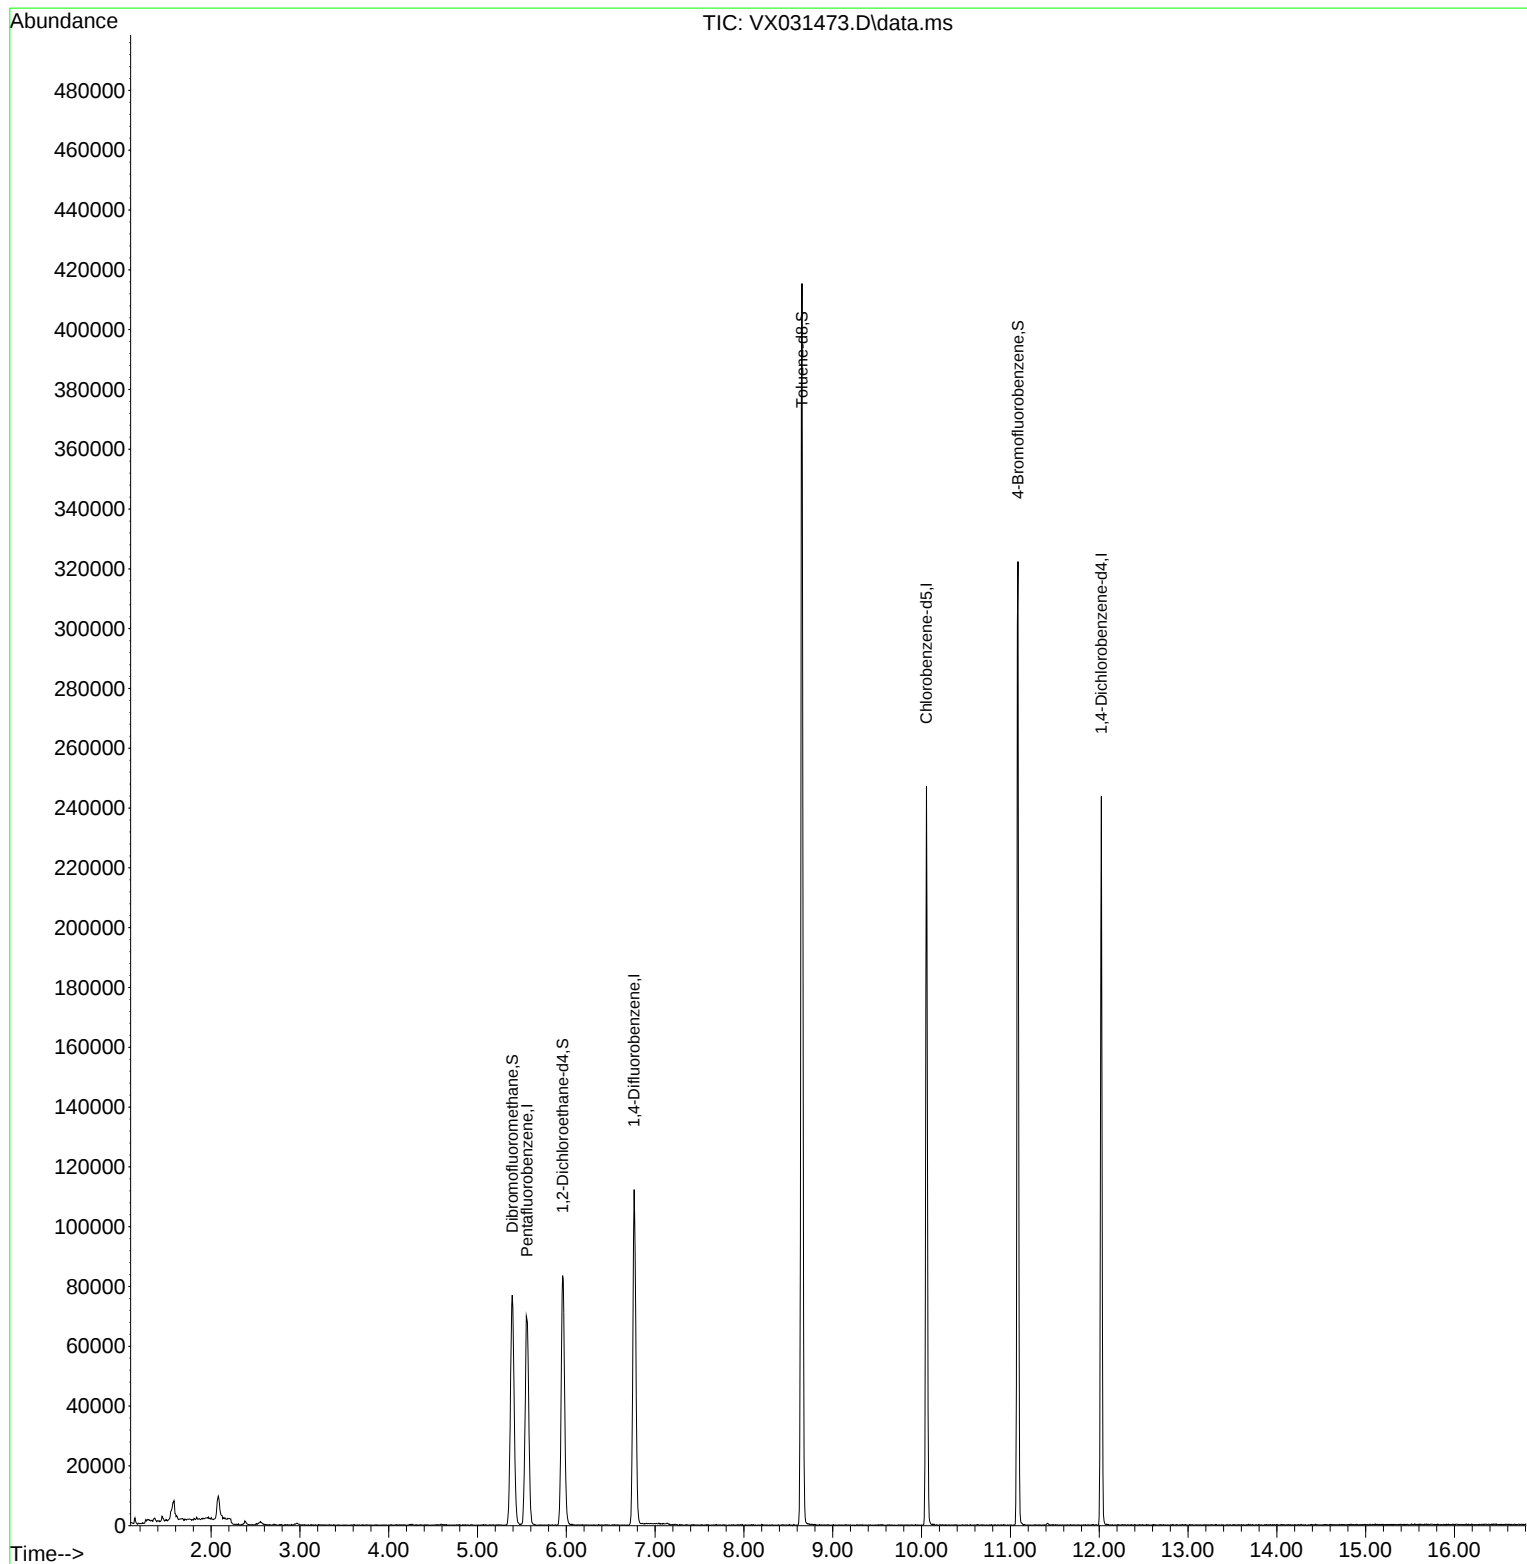



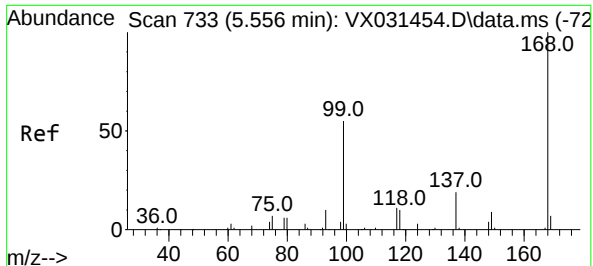


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.000 min
Lab File: VX031473.D
Acq: 19 Sep 2022 20:23

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW5-GW-278-280RE



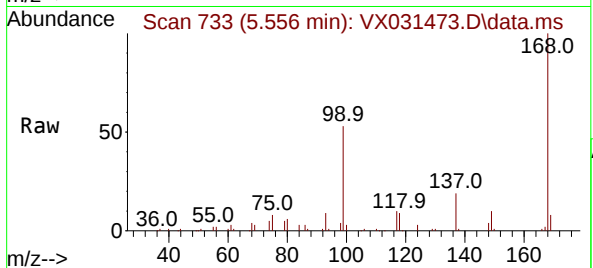


Tgt Ion:168 Resp: 67798
Ion Ratio Lower Upper
168 100
99 52.9 48.8 73.2

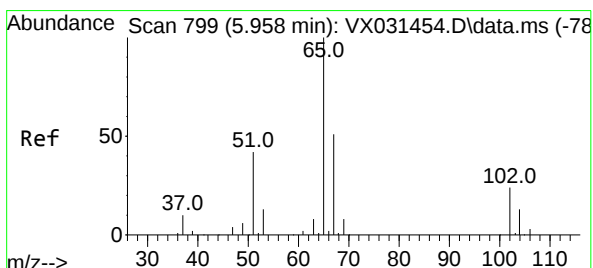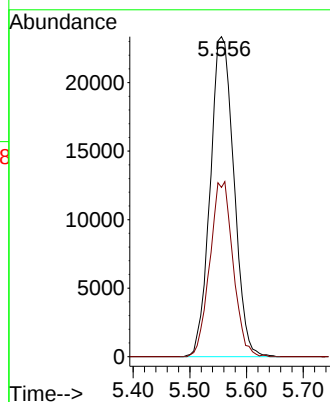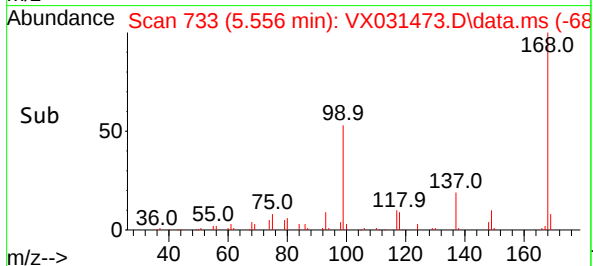

#33
1,2-Dichloroethane-d4
Concen: 60.163 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX031473.D
Acq: 19 Sep 2022 20:23

Tgt Ion: 65 Resp: 74672
Ion Ratio Lower Upper
65 100
67 51.3 0.0 102.4


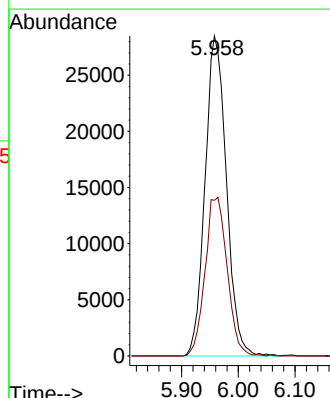
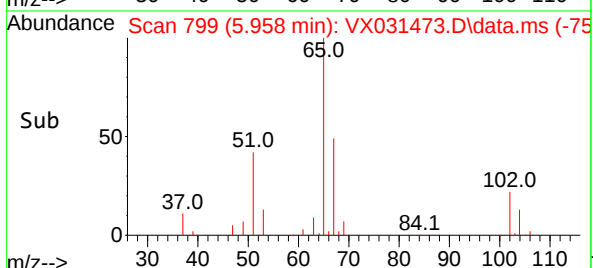
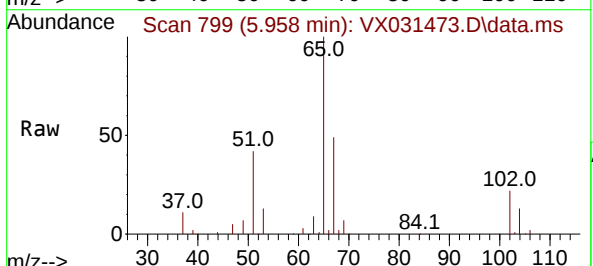




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX031473.D
Acq: 19 Sep 2022 20:23




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW5-GW-278-280RE


Tgt Ion:114 Resp: 113348
Ion Ratio Lower Upper
114 100
63 18.4 0.0 42.6
88 14.5 0.0 33.0

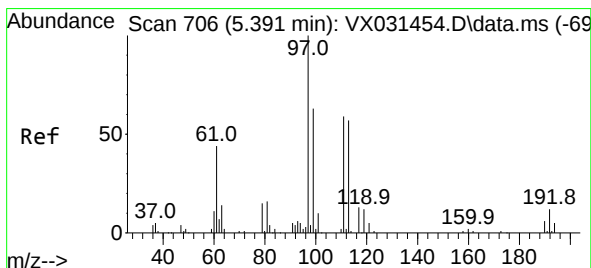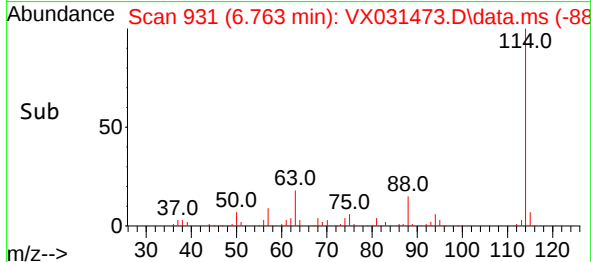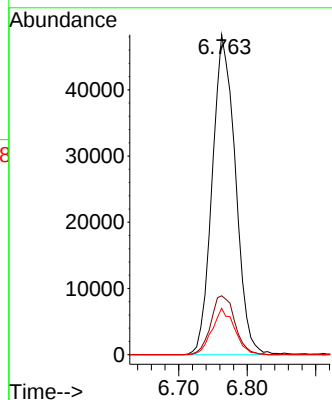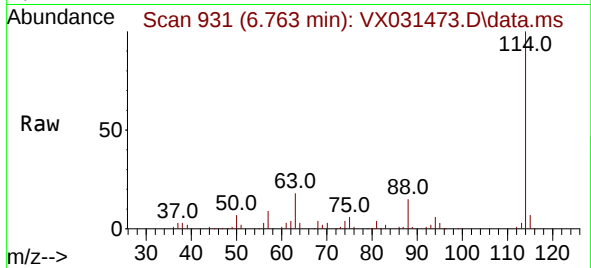

#35
Dibromofluoromethane
Concen: 53.564 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.000 min
Lab File: VX031473.D
Acq: 19 Sep 2022 20:23

Tgt Ion:113 Resp: 62693
Ion Ratio Lower Upper
113 100
111 103.8 82.4 123.6
192 19.5 14.1 21.1


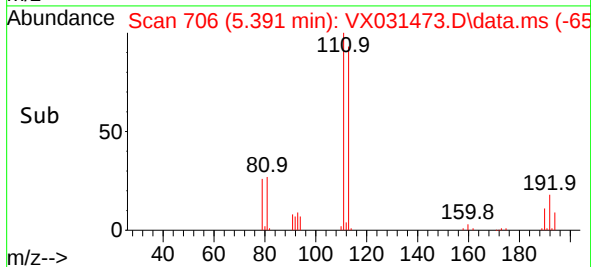
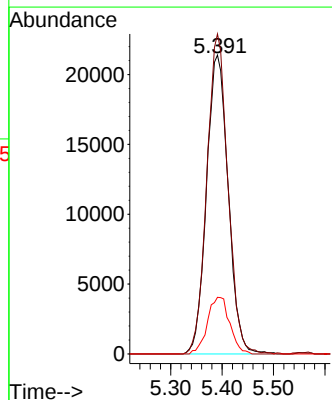
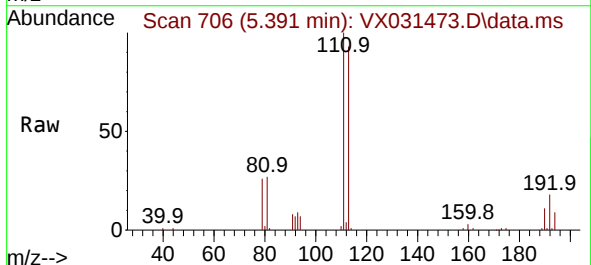


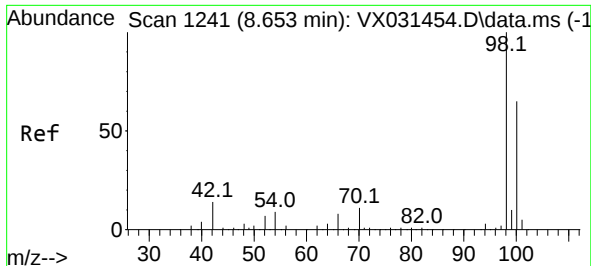

#50
Toluene-d8
Concen: 52.748 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX031473.D
Acq: 19 Sep 2022 20:23




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW5-GW-278-280RE


Tgt Ion: 98 Resp: 238205
Ion Ratio Lower Upper
98 100
100 64.2 52.5 78.7

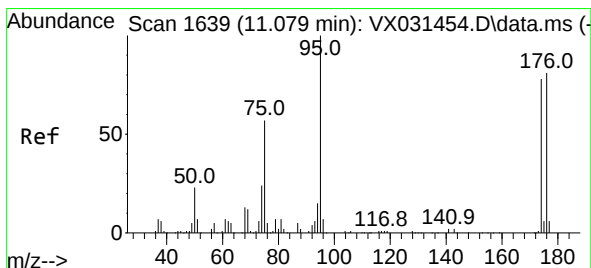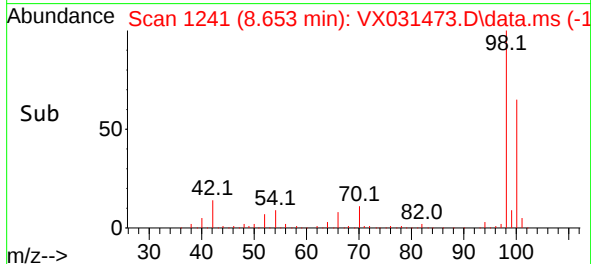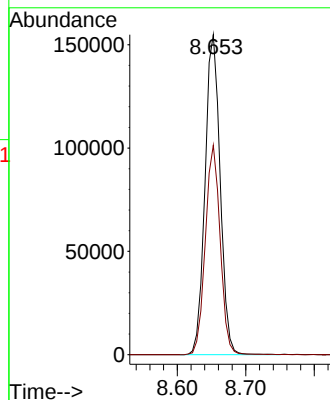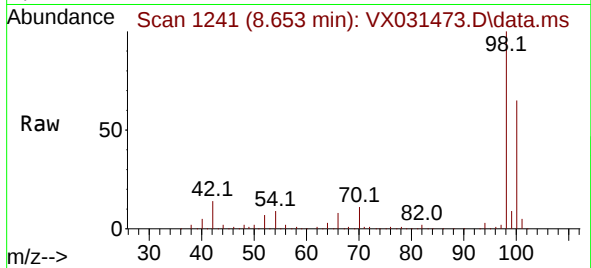

#62
4-Bromofluorobenzene
Concen: 47.708 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX031473.D
Acq: 19 Sep 2022 20:23

Tgt Ion: 95 Resp: 72977
Ion Ratio Lower Upper
95 100
174 90.0 0.0 153.2
176 85.0 0.0 144.0


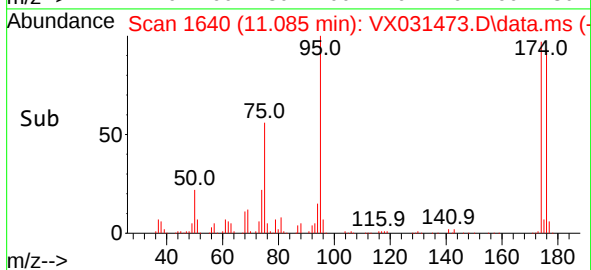
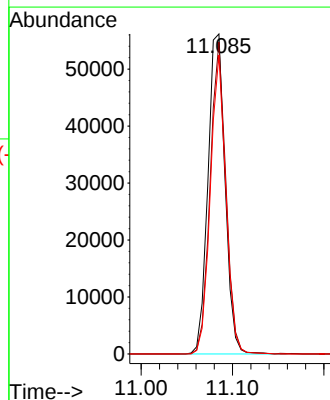
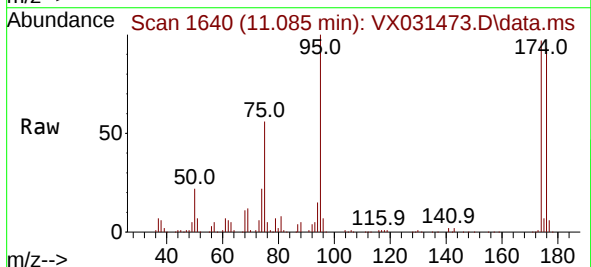


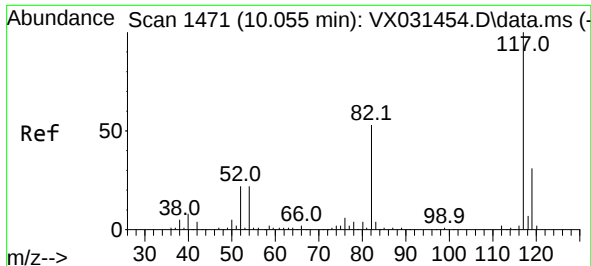

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX031473.D
Acq: 19 Sep 2022 20:23

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW5-GW-278-280RE

Tgt Ion:117 Resp: 104699
Ion Ratio Lower Upper
117 100
82 53.6 46.8 70.2
119 30.9 26.4 39.6

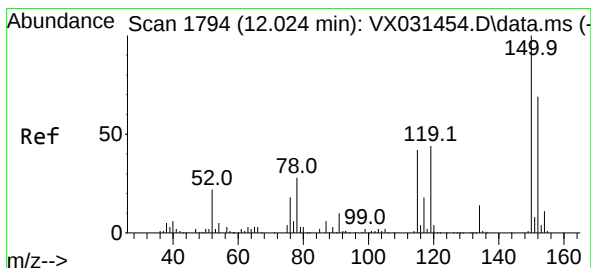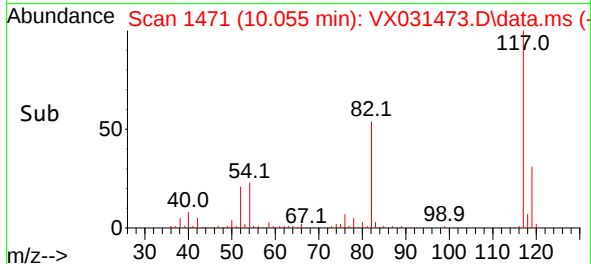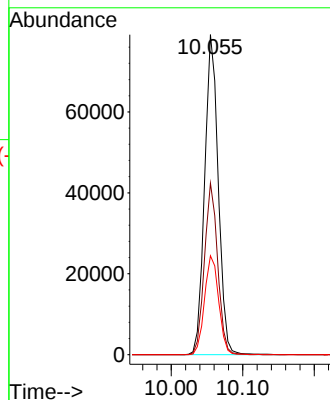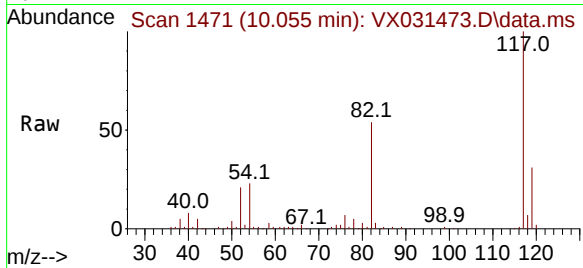

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX031473.D
Acq: 19 Sep 2022 20:23

Tgt Ion:152 Resp: 46284
Ion Ratio Lower Upper
152 100
115 57.1 43.4 130.1
150 160.0 0.0 346.8

