
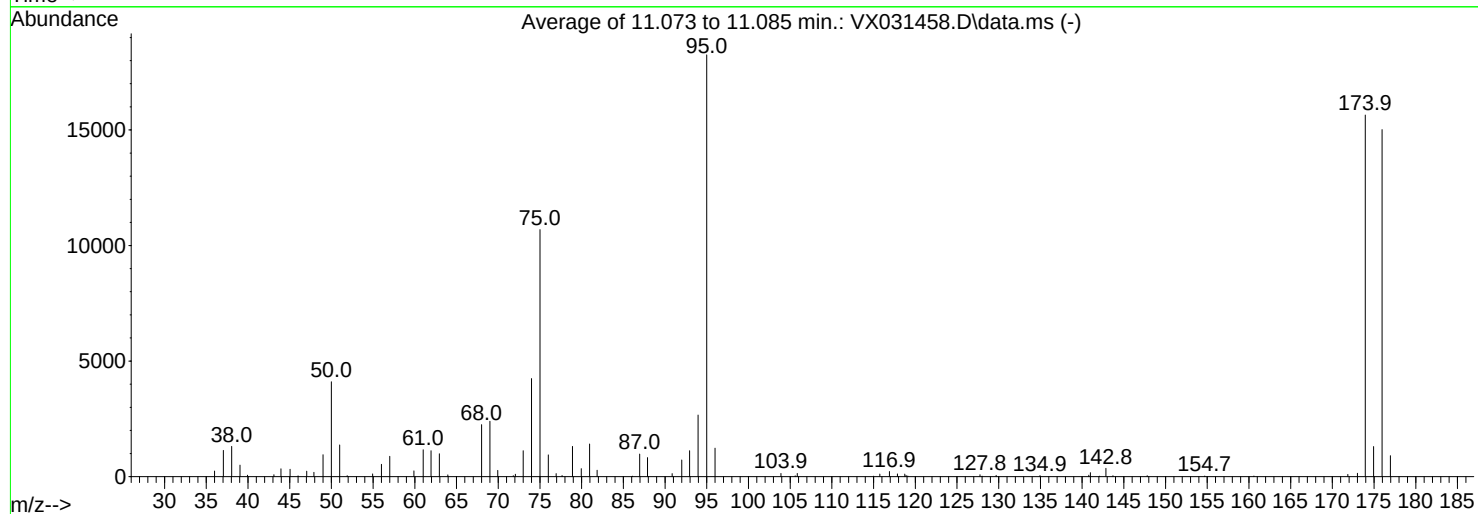


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091922\
Data File : VX031458.D
Acq On : 19 Sep 2022 13:59
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Title : SW846 8260
Last Update : Tue Sep 20 09:45:29 2022

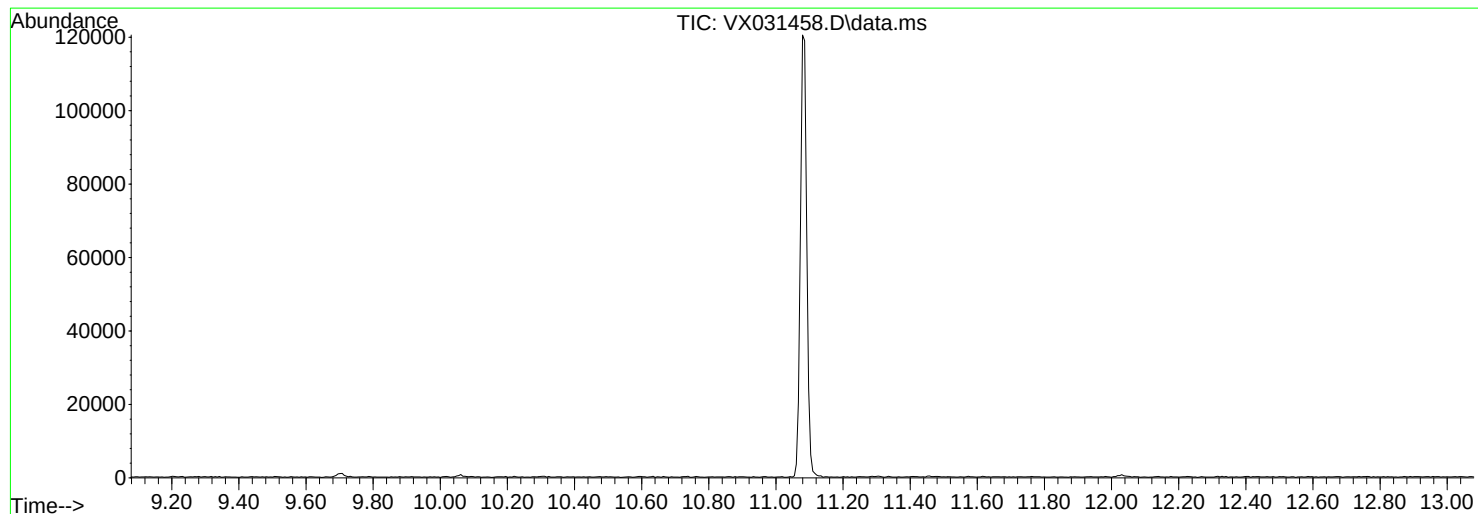

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.5	4105	PASS
75	95	30	60	58.6	10689	PASS
95	95	100	100	100.0	18250	PASS
96	95	5	9	6.7	1230	PASS
173	174	0.00	2	0.9	146	PASS
174	95	50	100	85.7	15647	PASS
175	174	5	9	8.3	1299	PASS
176	174	95	101	96.0	15019	PASS
177	176	5	9	6.1	910	PASS