

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX091923\  
Data File : VX037804.D  
Acq On : 19 Sep 2023 14:30  
Operator : JC/MD  
Sample : 04491-10  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TB-9-15

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091523W.M

Title : SW846 8260

Signal : TIC: VX037804.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.391       | 695           | 706         | 721          | rBV      | 135274         | 393091        | 32.80%          | 6.003%        |
| 2         | 5.556       | 722           | 733         | 749          | rVB      | 233762         | 659172        | 55.00%          | 10.067%       |
| 3         | 5.958       | 788           | 799         | 817          | rBV      | 147191         | 397710        | 33.19%          | 6.074%        |
| 4         | 6.763       | 921           | 931         | 952          | rBV      | 362323         | 869324        | 72.54%          | 13.276%       |
| 5         | 8.647       | 1234          | 1240        | 1259         | rBV      | 742831         | 1198457       | 100.00%         | 18.303%       |
| 6         | 10.055      | 1465          | 1471        | 1487         | rBV      | 811569         | 1080792       | 90.18%          | 16.506%       |
| 7         | 11.079      | 1634          | 1639        | 1652         | rBV      | 663652         | 838431        | 69.96%          | 12.804%       |
| 8         | 12.024      | 1788          | 1794        | 1804         | rBV      | 869622         | 1111014       | 92.70%          | 16.967%       |




Sum of corrected areas: 6547991

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX091923\  
Data File : VX037804.D  
Acq On : 19 Sep 2023 14:30  
Operator : JC/MD  
Sample : 04491-10  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TB-9-15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091523W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

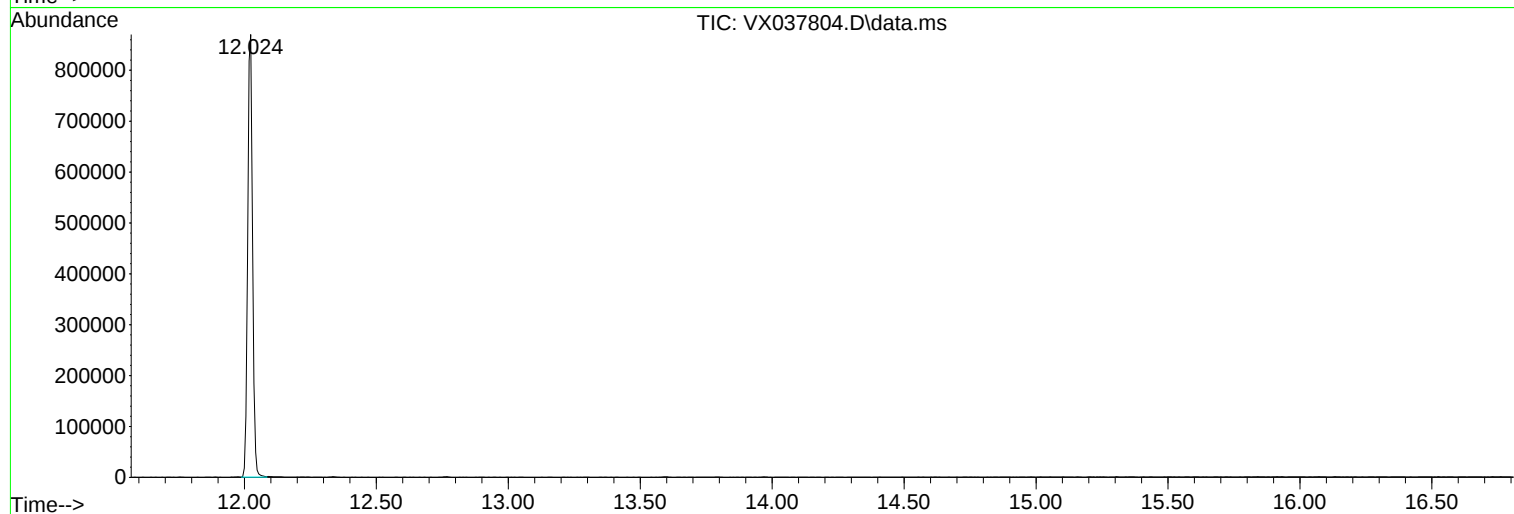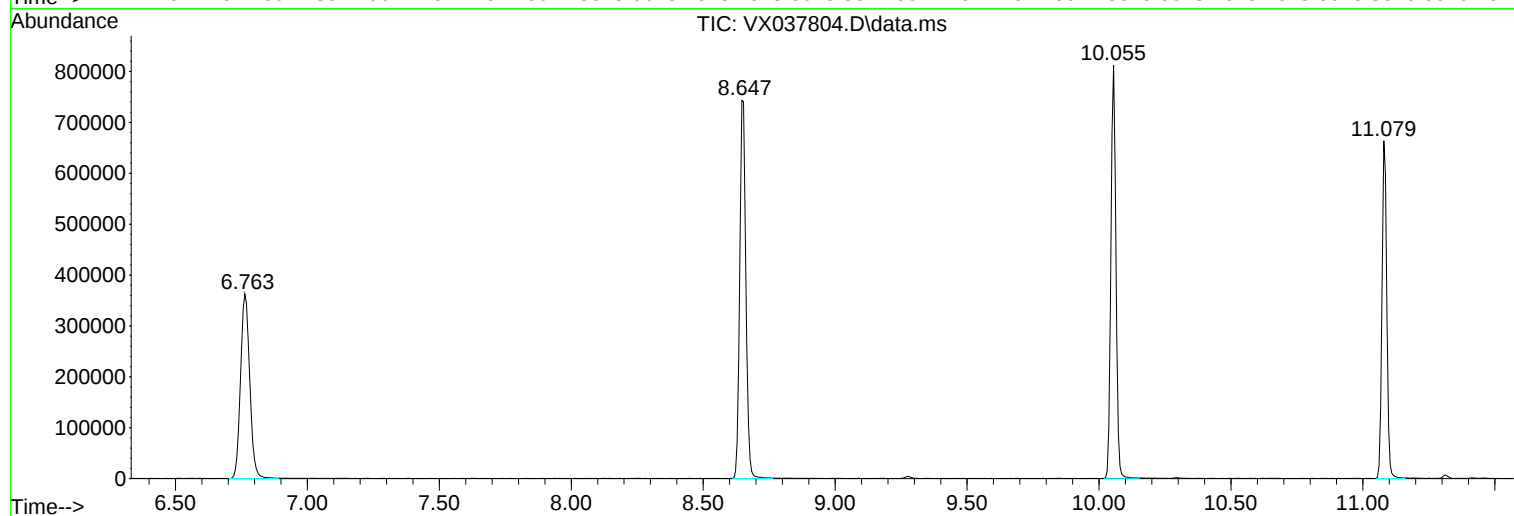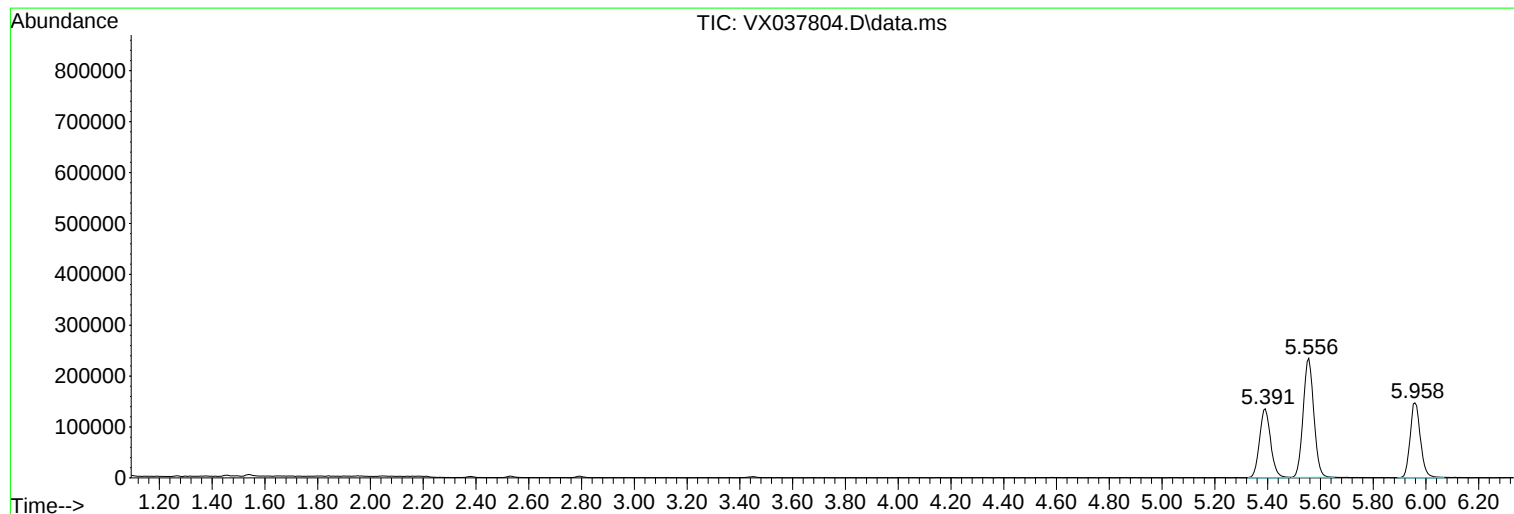

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX091923\  
Data File : VX037804.D  
Acq On : 19 Sep 2023 14:30  
Operator : JC/MD  
Sample : 04491-10  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TB-9-15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091523W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX091923\  
Data File : VX037804.D  
Acq On : 19 Sep 2023 14:30  
Operator : JC/MD  
Sample : 04491-10  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TB-9-15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091523W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|