



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091923\
Data File : VX037791.D
Acq On : 19 Sep 2023 09:09
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Title : SW846 8260
Last Update : Sat Sep 16 04:55:44 2023

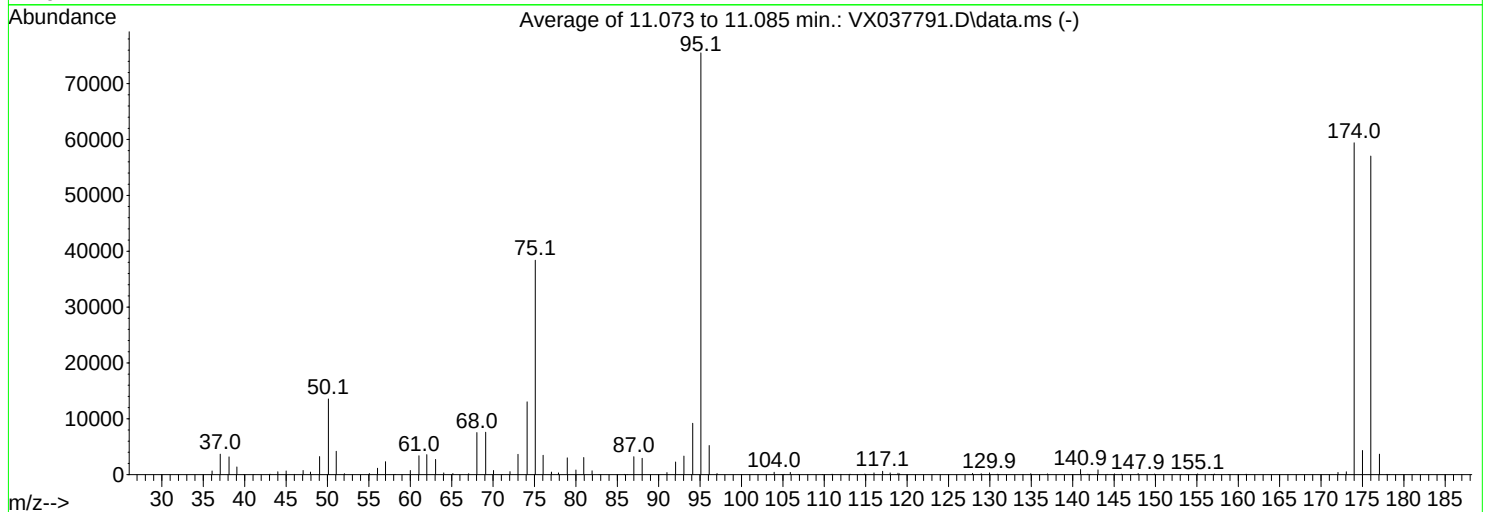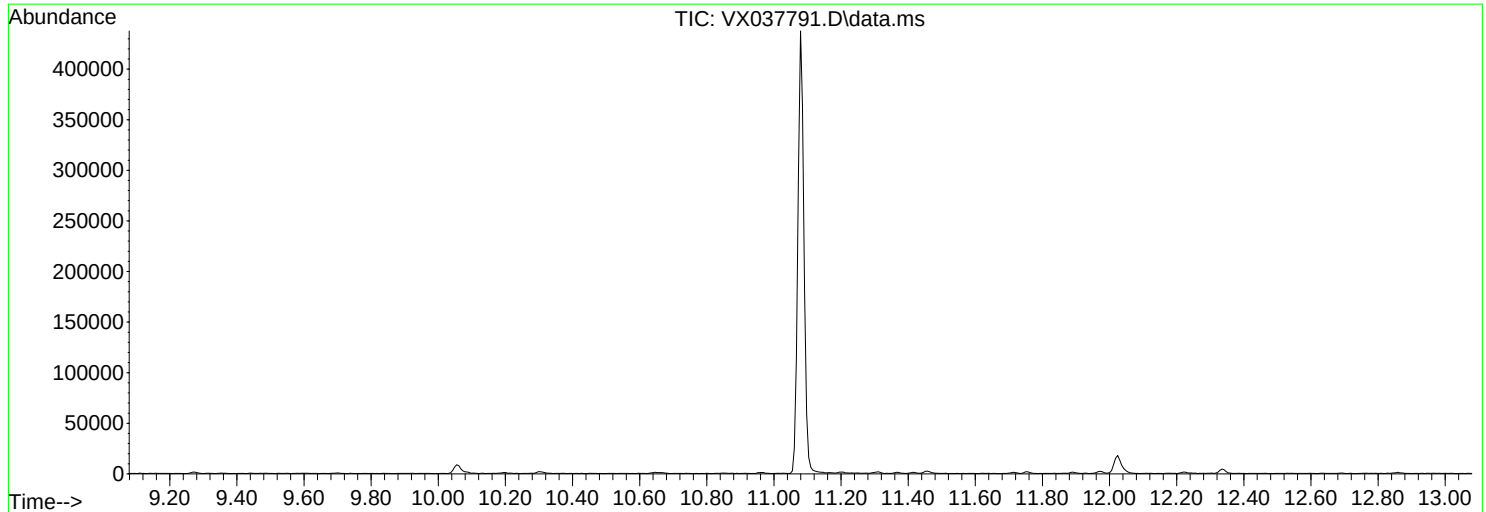

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	13546	PASS
75	95	30	60	50.9	38403	PASS
95	95	100	100	100.0	75517	PASS
96	95	5	9	6.9	5215	PASS
173	174	0.00	2	0.9	517	PASS
174	95	50	100	78.7	59419	PASS
175	174	5	9	7.3	4335	PASS
176	174	95	101	96.0	57027	PASS
177	176	5	9	6.4	3678	PASS