


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX092019\
 Data File : VX012544.D
 Acq On : 20 Sep 2019 08:59
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091719W.M
 Title : SW846 8260
 Last Update : Tue Sep 17 15:27:10 2019

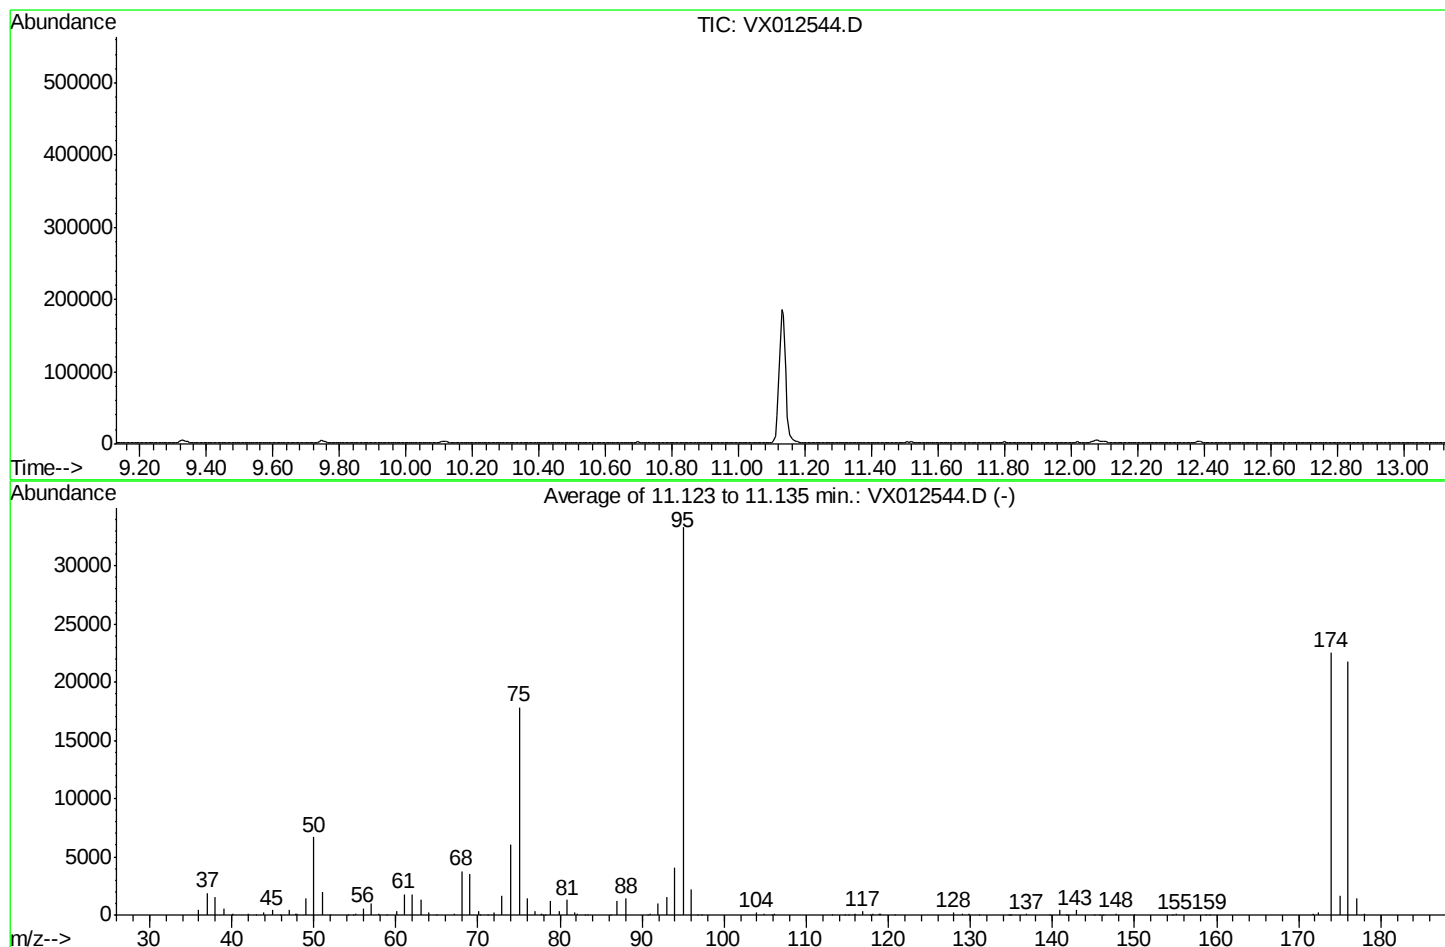

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1670

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	6707	PASS
75	95	30	60	53.6	17856	PASS
95	95	100	100	100.0	33312	PASS
96	95	5	9	6.6	2215	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	67.6	22535	PASS
175	174	5	9	7.4	1670	PASS
176	174	95	101	96.4	21733	PASS
177	176	5	9	6.7	1462	PASS