


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX092019\  
 Data File : VX012571.D  
 Acq On : 20 Sep 2019 21:02  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 29 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X091719W.M  
 Title : SW846 8260  
 Last Update : Tue Sep 17 15:27:10 2019

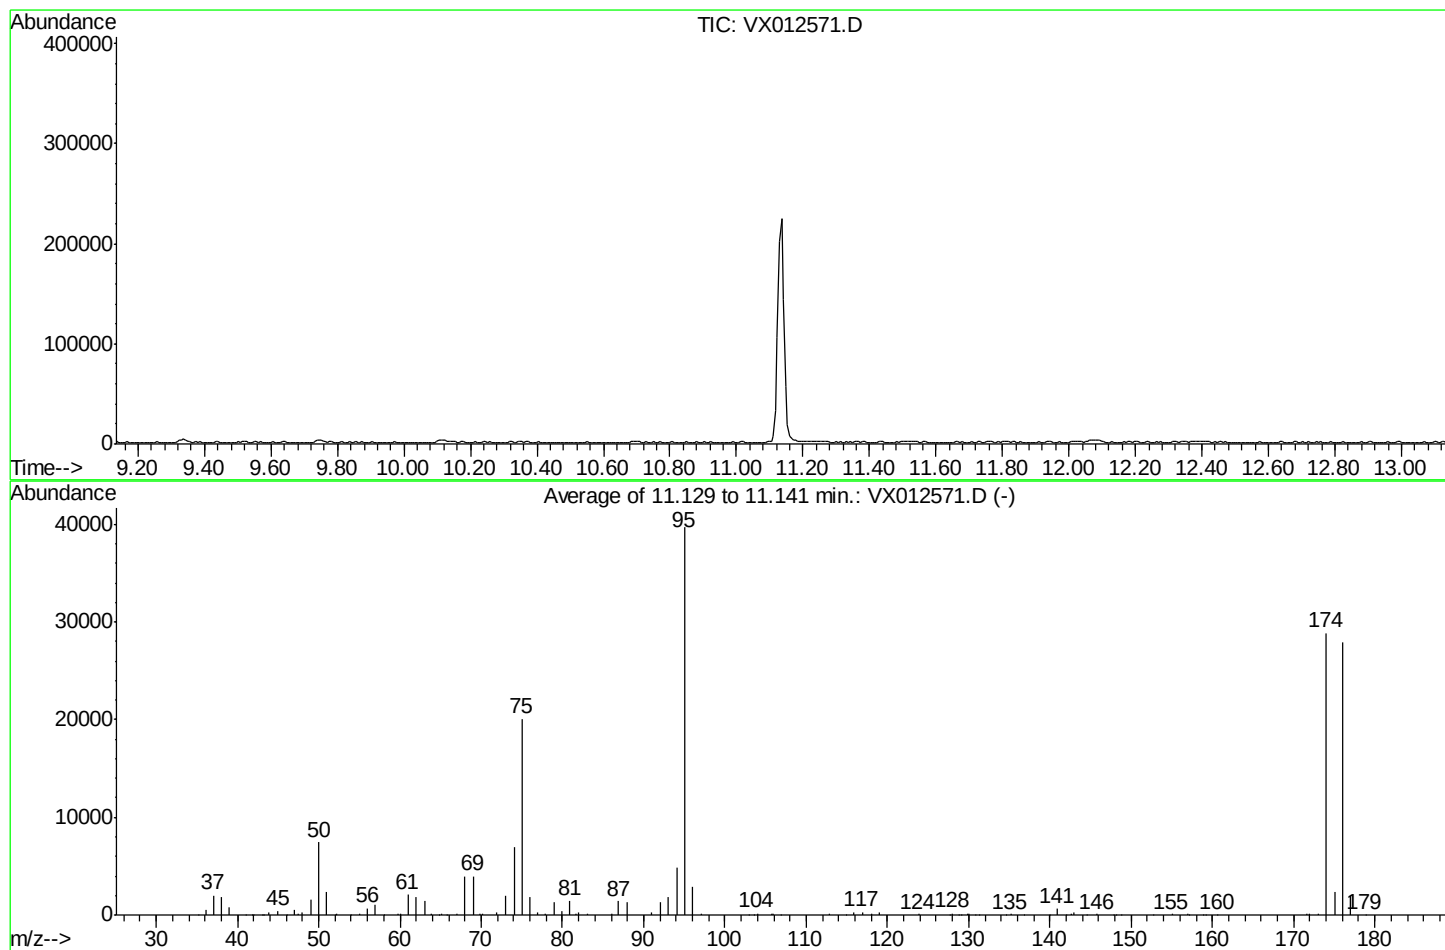

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1673

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 18.8      | 7447    | PASS             |
| 75          | 95           | 30           | 60           | 50.5      | 20048   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 39685   | PASS             |
| 96          | 95           | 5            | 9            | 7.1       | 2824    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.6       | 161     | PASS             |
| 174         | 95           | 50           | 100          | 72.7      | 28864   | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 2309    | PASS             |
| 176         | 174          | 95           | 101          | 96.7      | 27909   | PASS             |
| 177         | 176          | 5            | 9            | 7.1       | 1987    | PASS             |