

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092021\
 Data File : VX024362.D
 Acq On : 20 Sep 2021 19:37
 Operator : JC/MD
 Sample : M3782-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE132D7-20210914

Quant Time: Sep 21 08:43:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 14 12:18:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	139236	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	244704	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	195111	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	88755	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	103877	52.319	ug/l	0.00
Spiked Amount	50.000	Range 78 - 117	Recovery	= 104.640%		
35) Dibromofluoromethane	5.397	113	81236	49.501	ug/l	0.00
Spiked Amount	50.000	Range 75 - 124	Recovery	= 99.000%		
50) Toluene-d8	8.653	98	255166	42.681	ug/l	0.00
Spiked Amount	50.000	Range 92 - 112	Recovery	= 85.360%#		
62) 4-Bromofluorobenzene	11.085	95	102850	44.206	ug/l	0.00
Spiked Amount	50.000	Range 83 - 123	Recovery	= 88.420%		
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.172	85	546	0.408	ug/l	81
3) Chloromethane	1.294	50	342	0.245	ug/l #	42
6) Chloroethane	1.709	64	80	2.070	ug/l #	43
9) 1,1,2-Trichlorotrifluo...	2.331	101	31157	22.730	ug/l	92
11) Tert butyl alcohol	2.959	59	418	Below Cal	#	73
12) 1,1-Dichloroethene	2.325	96	8941	6.964	ug/l	98
14) Allyl chloride	2.550	41	597	0.256	ug/l #	38
16) Acetone	2.392	43	1285	1.518	ug/l	88
20) Methylene Chloride	2.794	84	579	0.356	ug/l	94
24) 1,1-Dichloroethane	3.623	63	4641	1.726	ug/l	99
27) cis-1,2-Dichloroethene	4.501	96	5916	3.645	ug/l	93
28) Bromochloromethane	5.105	49	264	0.241	ug/l #	9
29) Tetrahydrofuran	5.038	42	410	0.525	ug/l #	81
30) Chloroform	5.105	83	4283	1.498	ug/l	98
31) Cyclohexane	5.562	56	2977	1.282	ug/l #	15
32) 1,1,1-Trichloroethane	5.391	97	1106	0.432	ug/l #	46
36) 1,1-Dichloropropene	5.562	75	10805	4.803	ug/l #	50
38) Carbon Tetrachloride	5.684	117	3865	1.526	ug/l #	93
39) Methylcyclohexane	7.135	83	29669	11.045	ug/l #	1
42) 1,2-Dichloroethane	6.092	62	769	0.286	ug/l #	73
44) Trichloroethene	7.135	130	2487929	1372.259	ug/l	99
49) 1,4-Dioxane	7.671	88	494	11.331	ug/l #	87
51) 4-Methyl-2-Pentanone	8.647	43	1306	0.491	ug/l #	1
55) 1,1,2-Trichloroethane	9.159	97	1479	0.821	ug/l	91
60) Dibromochloromethane	9.275	129	3652	3.452	ug/l #	11
64) Tetrachloroethene	9.275	164	3797	2.512	ug/l	93
76) 1,2,3-Trichloropropane	11.085	75	54236	26.575	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	54236	78.158	ug/l #	12
95) Naphthalene	13.780	128	97	1.302	ug/l #	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092021\
Data File : VX024362.D
Acq On : 20 Sep 2021 19:37
Operator : JC/MD
Sample : M3782-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914

Quant Time: Sep 21 08:43:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 14 12:18:04 2021
Response via : Initial Calibration




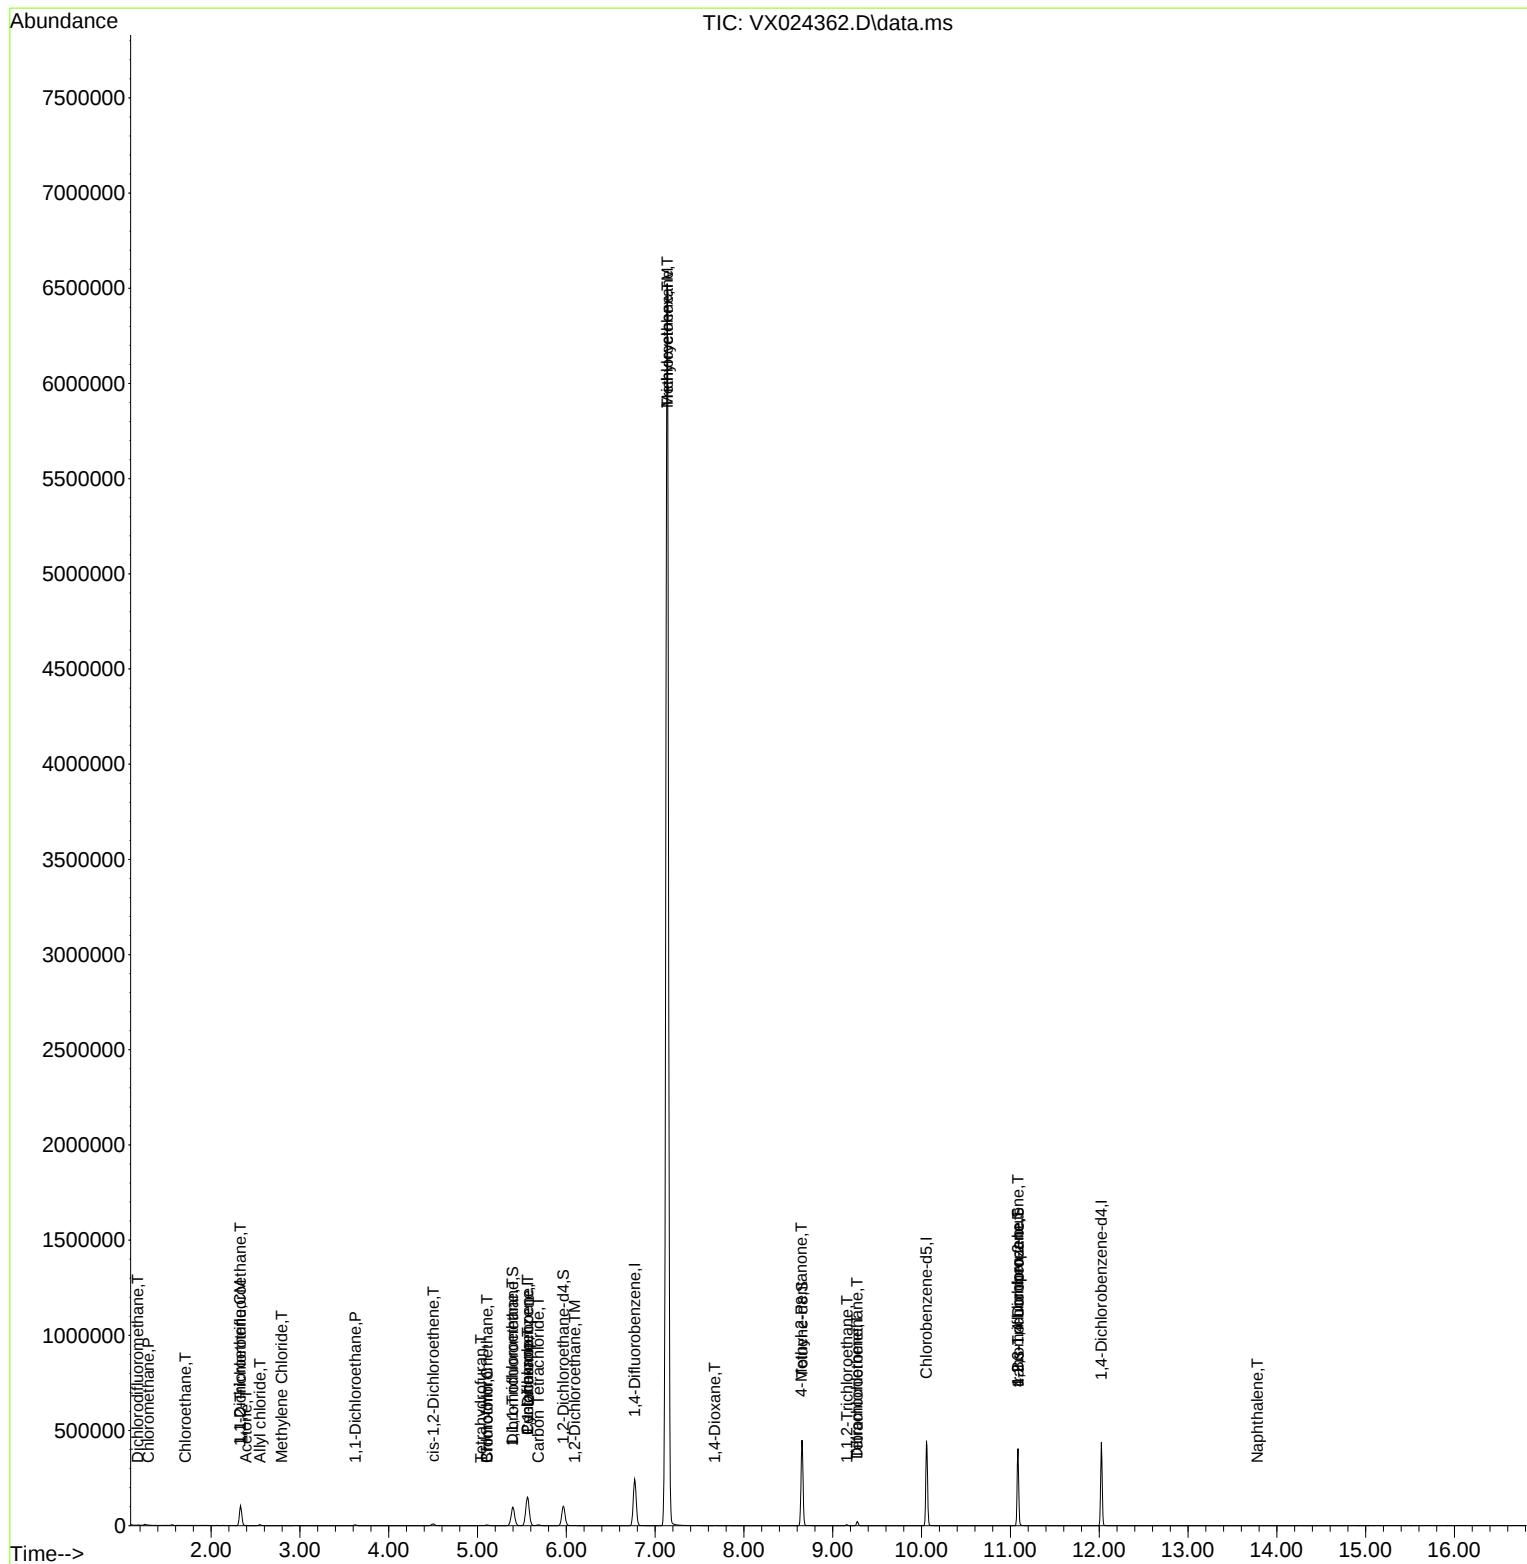




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914


Tgt Ion:168 Resp: 139236
Ion Ratio Lower Upper
168 100
99 63.2 45.8 68.6

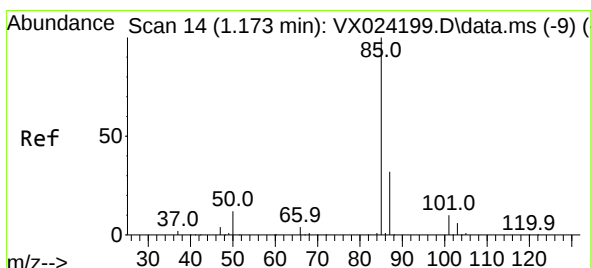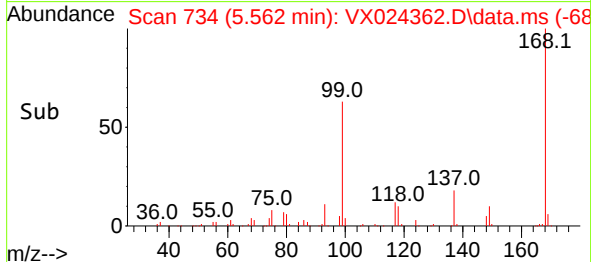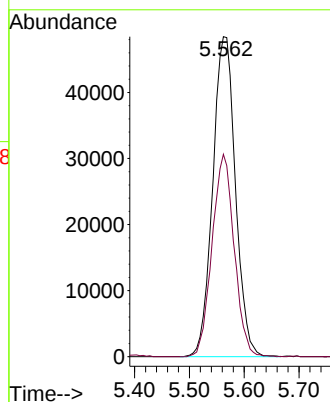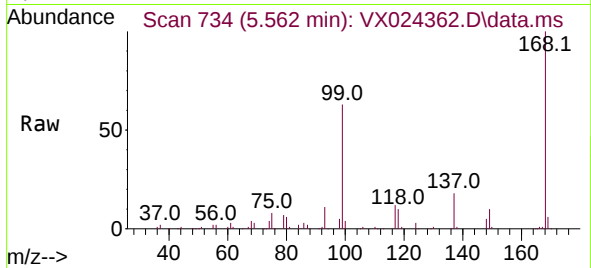

#2
Dichlorodifluoromethane
Concen: 0.408 ug/l
RT: 1.172 min Scan# 14
Delta R.T. -0.001 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Tgt Ion: 85 Resp: 546
Ion Ratio Lower Upper
85 100
87 22.0 16.4 49.2


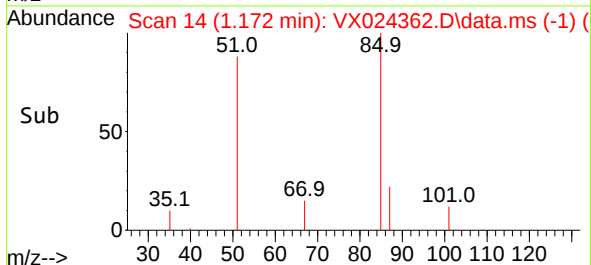

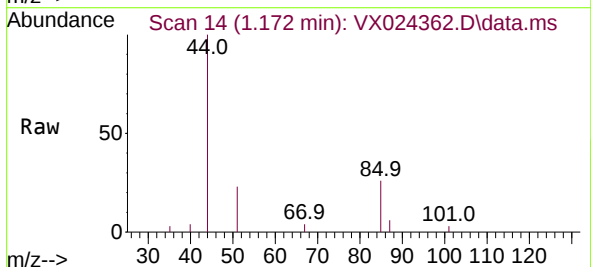


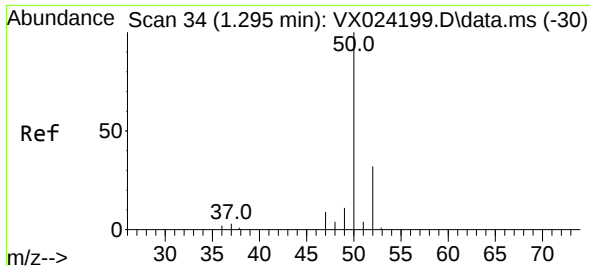

#3
Chloromethane
Concen: 0.245 ug/l
RT: 1.294 min Scan# 34
Delta R.T. -0.001 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914


Tgt Ion: 50 Resp: 342
Ion Ratio Lower Upper
50 100
52 0.0 26.4 39.6#

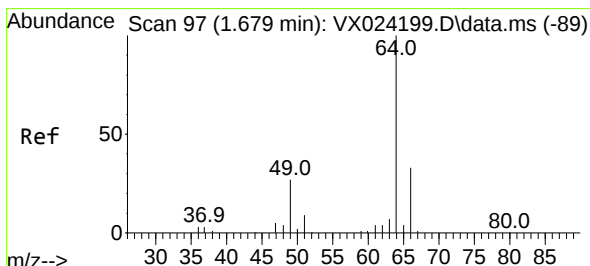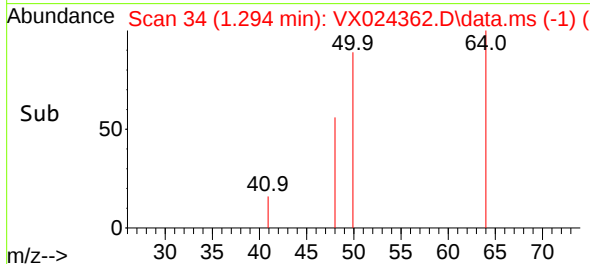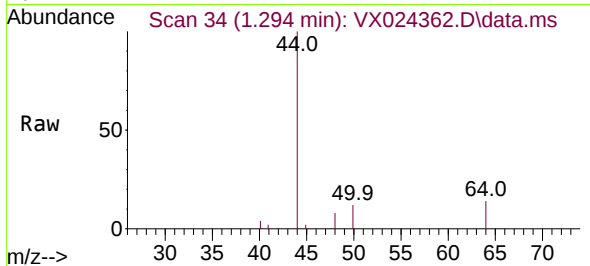

#6
Chloroethane
Concen: 2.070 ug/l
RT: 1.709 min Scan# 102
Delta R.T. 0.030 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Tgt Ion: 64 Resp: 80
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.0#


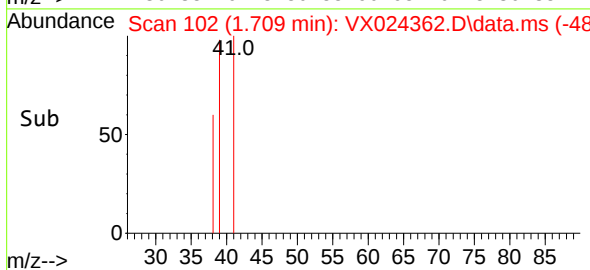
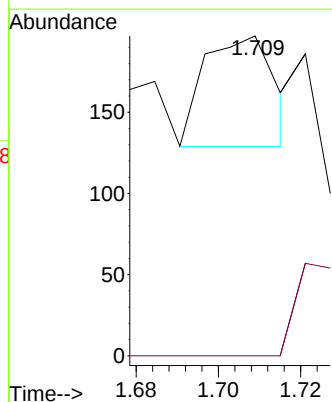
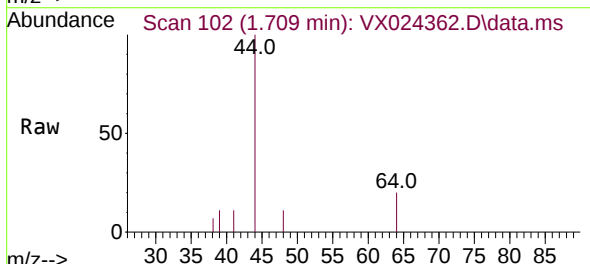




#9
1,1,2-Trichlorotrifluoroethane
Concen: 22.730 ug/l
RT: 2.331 min Scan# 204
Delta R.T. -0.000 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914


Tgt Ion:101 Resp: 31157
Ion Ratio Lower Upper
101 100
85 48.5 34.9 52.3
151 84.5 61.4 92.2

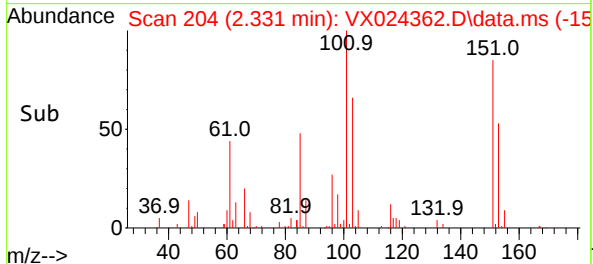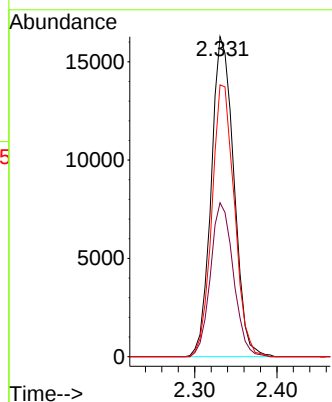

#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.959 min Scan# 307
Delta R.T. -0.024 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Tgt Ion: 59 Resp: 418
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#



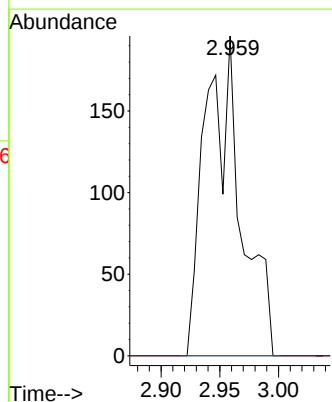
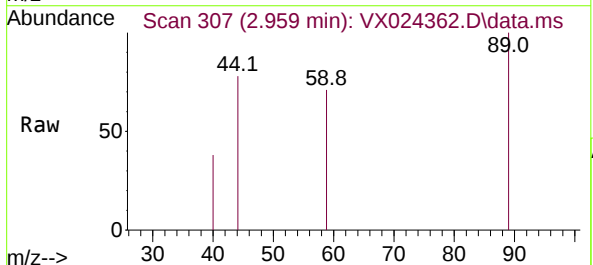




#12
1,1-Dichloroethene
Concen: 6.964 ug/l
RT: 2.325 min Scan# 203
Delta R.T. 0.006 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914


Tgt Ion: 96 Resp: 8941
Ion Ratio Lower Upper
96 100
61 152.2 124.6 187.0
98 63.4 50.6 76.0

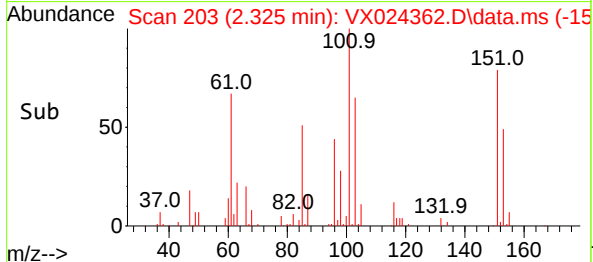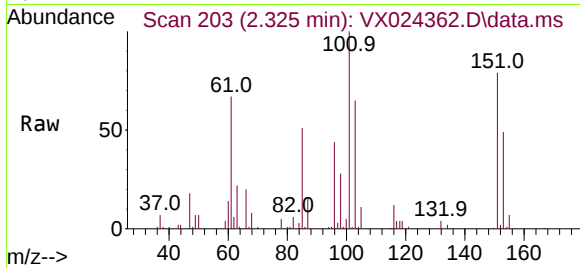

#14
Allyl chloride
Concen: 0.256 ug/l
RT: 2.550 min Scan# 240
Delta R.T. -0.116 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Tgt Ion: 41 Resp: 597
Ion Ratio Lower Upper
41 100
39 113.1 51.6 77.4#
76 0.0 30.5 45.7#




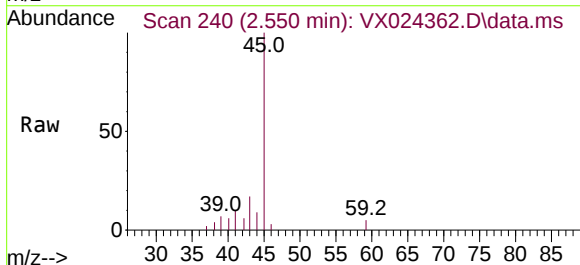


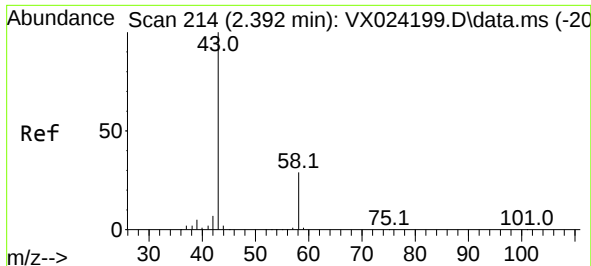

#16
Acetone
Concen: 1.518 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914


Tgt Ion: 43 Resp: 1285
Ion Ratio Lower Upper
43 100
58 27.9 27.8 41.8

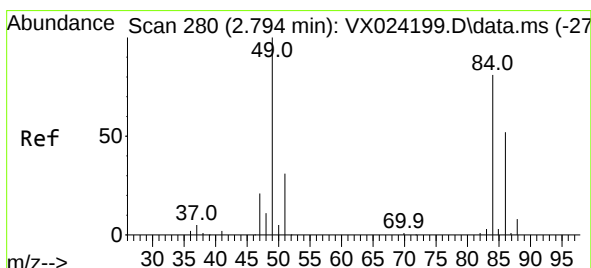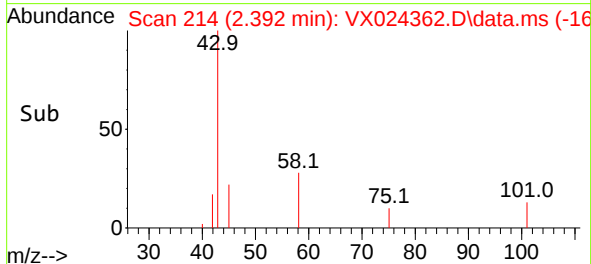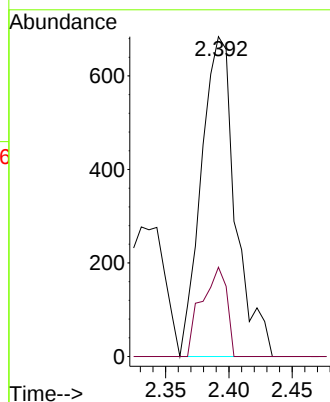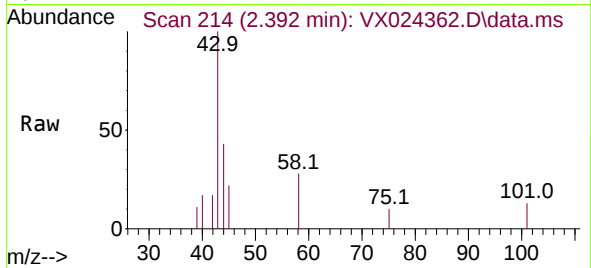

#20
Methylene Chloride
Concen: 0.356 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Tgt Ion: 84 Resp: 579
Ion Ratio Lower Upper
84 100
49 104.1 88.6 132.8
51 33.4 27.0 40.6
86 70.6 50.3 75.5


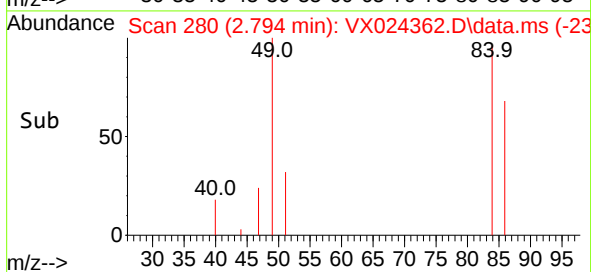
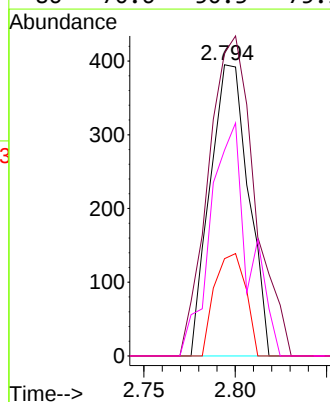
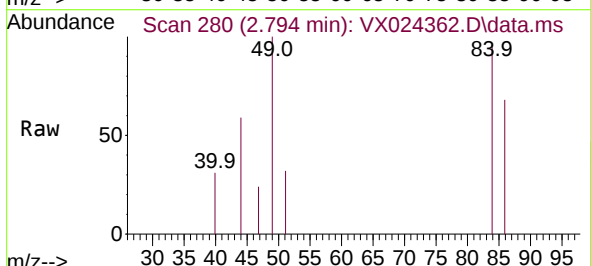




#24
1,1-Dichloroethane
Concen: 1.726 ug/l
RT: 3.623 min Scan# 416
Delta R.T. 0.006 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914


Tgt Ion: 63	Resp: 4641
Ion Ratio	Lower Upper
63 100	
98 7.2	3.8 11.2
100 5.3	2.5 7.5

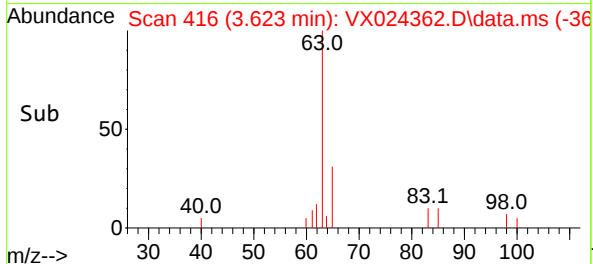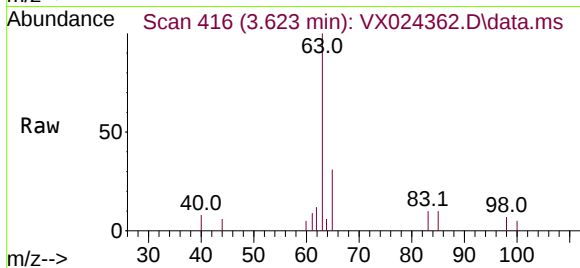

#27
cis-1,2-Dichloroethene
Concen: 3.645 ug/l
RT: 4.501 min Scan# 560
Delta R.T. 0.006 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Tgt Ion: 96	Resp: 5916
Ion Ratio	Lower Upper
96 100	
61 131.6	0.0 285.6
98 64.1	0.0 129.6




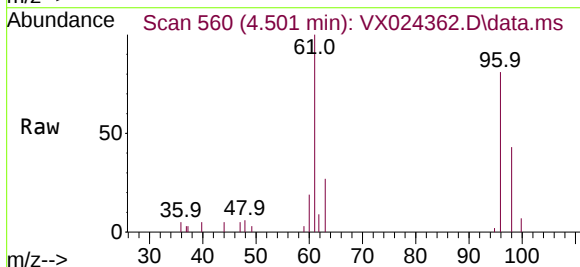




#28
Bromochloromethane
Concen: 0.241 ug/l
RT: 5.105 min Scan# 659
Delta R.T. 0.195 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914


Tgt Ion: 49 Resp: 264
Ion Ratio Lower Upper
49 100
129 0.0 0.0 4.0
130 0.0 68.2 102.2#

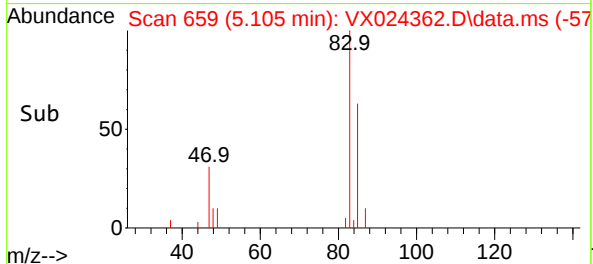

#29
Tetrahydrofuran
Concen: 0.525 ug/l
RT: 5.038 min Scan# 648
Delta R.T. 0.019 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Tgt Ion: 42 Resp: 410
Ion Ratio Lower Upper
42 100
72 31.0 41.7 62.5#
71 43.7 38.4 57.6





#30

Chloroform

Concen: 1.498 ug/l

RT: 5.105 min Scan# 659

Delta R.T. -0.000 min

Lab File: VX024362.D

Acq: 20 Sep 2021 19:37

Tgt Ion: 83 Resp: 4283

Ion Ratio Lower Upper

83 100





85 63.2 52.0 78.0

Instrument :

MSVOA_X

ClientSampleId :

RE132D7-20210914

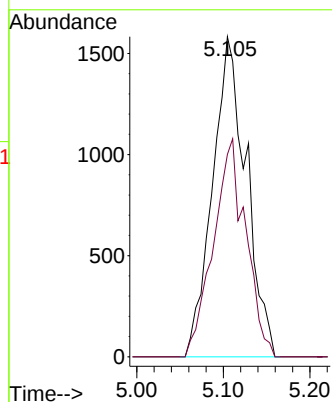

#31

Cyclohexane

Concen: 1.282 ug/l

RT: 5.562 min Scan# 734

Delta R.T. 0.085 min

Lab File: VX024362.D

Acq: 20 Sep 2021 19:37




Tgt Ion: 56 Resp: 2977


Ion Ratio Lower Upper

56 100

69 164.0 25.3 37.9#

84 117.7 71.4 107.0#

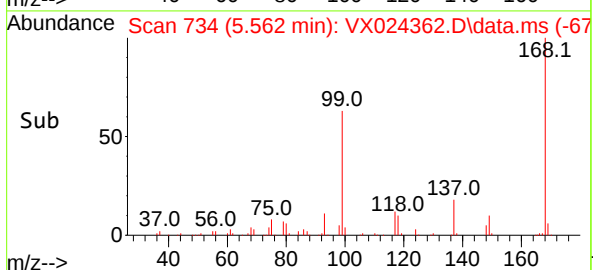







#32

1,1,1-Trichloroethane
Concen: 0.432 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914




Tgt Ion: 97 Resp: 1106
Ion Ratio Lower Upper
97 100
99 0.0 51.5 77.3#
61 51.0 34.2 51.4

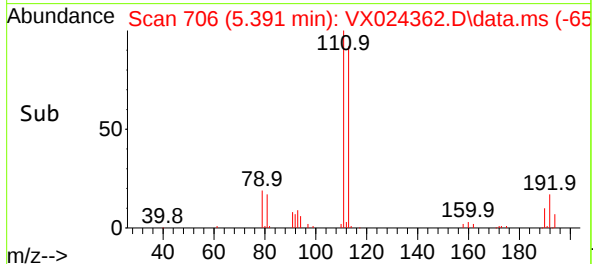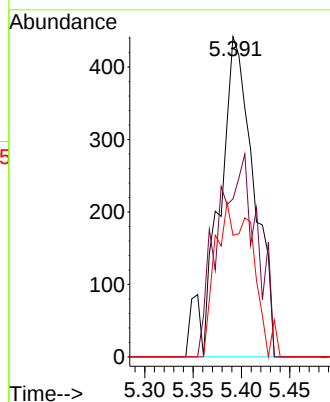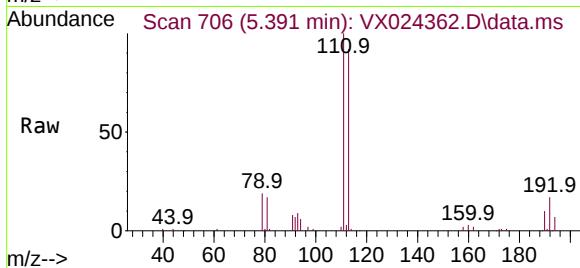


#33

1,2-Dichloroethane-d4
Concen: 52.319 ug/l
RT: 5.964 min Scan# 800
Delta R.T. -0.007 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Tgt Ion: 65 Resp: 103877
Ion Ratio Lower Upper
65 100
67 51.6 0.0 105.4



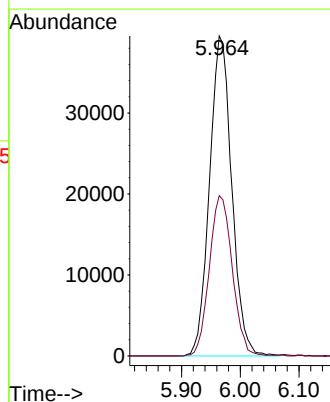
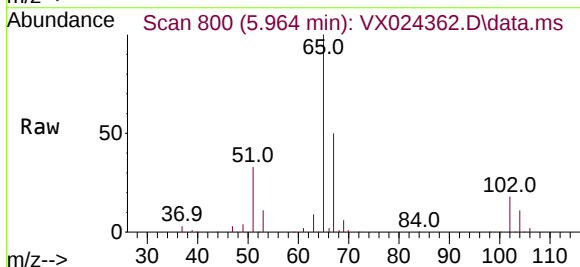




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914


Tgt Ion:114 Resp: 244704
Ion Ratio Lower Upper
114 100
63 20.9 0.0 40.8
88 16.3 0.0 32.8

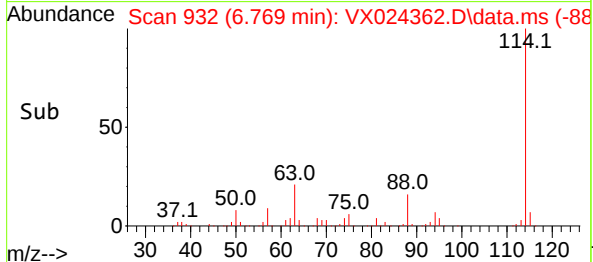

#35
Dibromofluoromethane
Concen: 49.501 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Tgt Ion:113 Resp: 81236
Ion Ratio Lower Upper
113 100
111 102.5 81.9 122.9
192 19.4 16.7 25.1




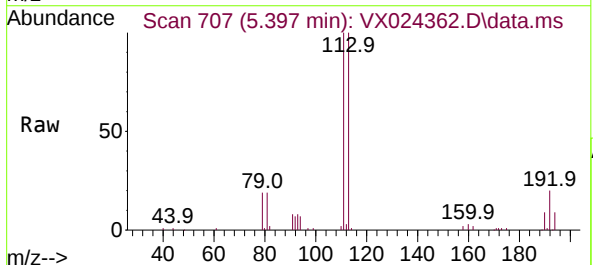


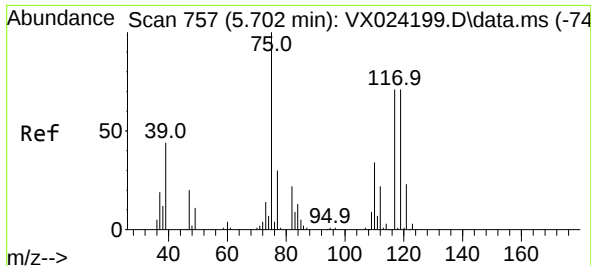

#36
1,1-Dichloropropene
Concen: 4.803 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.140 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914


Tgt Ion: 75 Resp: 10805
Ion Ratio Lower Upper
75 100
110 9.8 18.1 54.4#
77 0.0 25.3 37.9#

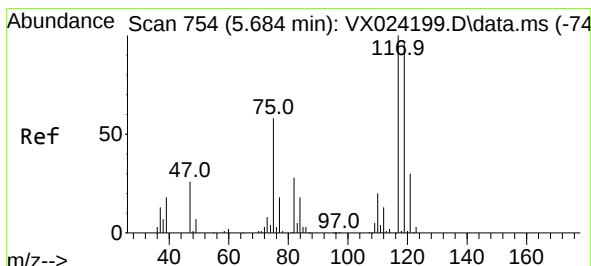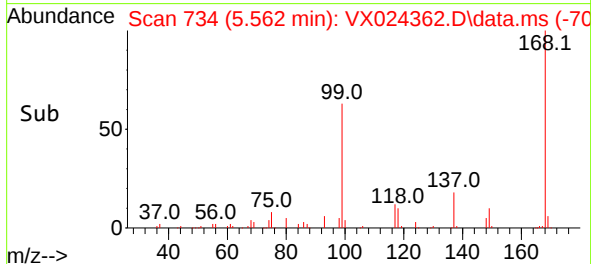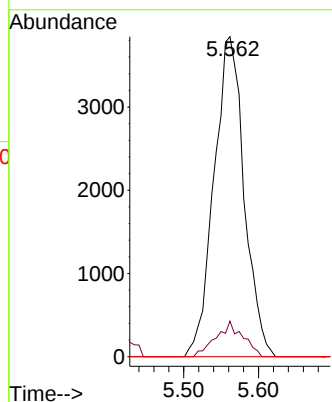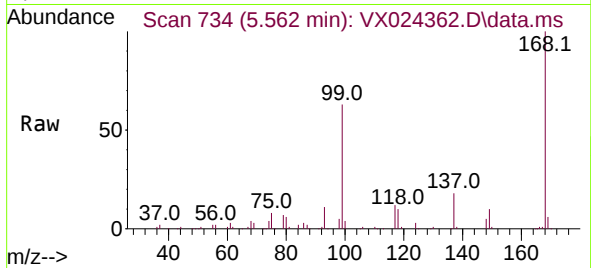

#38
Carbon Tetrachloride
Concen: 1.526 ug/l
RT: 5.684 min Scan# 754
Delta R.T. -0.000 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Tgt Ion: 117 Resp: 3865
Ion Ratio Lower Upper
117 100
119 92.0 76.2 114.2
121 20.1 24.8 37.2#

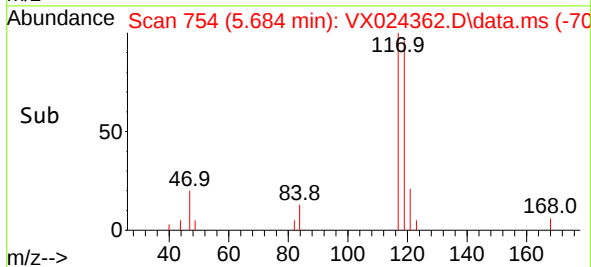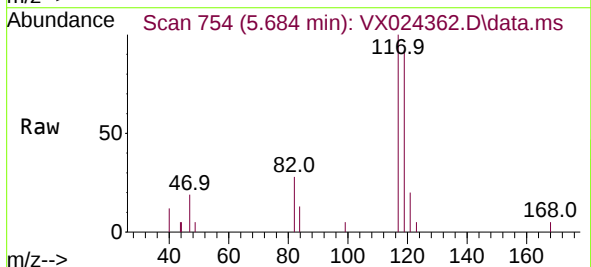



#39

Methylcyclohexane

Concen: 11.045 ug/l

RT: 7.135 min Scan# 992

Delta R.T. -0.250 min

Lab File: VX024362.D

Acq: 20 Sep 2021 19:37





Tgt Ion: 83 Resp: 29669

Ion Ratio Lower Upper

83 100

55 0.0 58.9 88.3#

98 214.0 38.1 57.1#

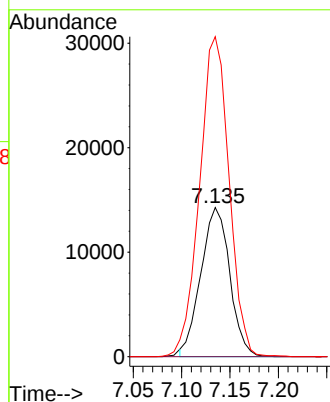

#42

1,2-Dichloroethane

Concen: 0.286 ug/l

RT: 6.092 min Scan# 821

Delta R.T. -0.007 min

Lab File: VX024362.D




Acq: 20 Sep 2021 19:37


Tgt Ion: 62 Resp: 769

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.2


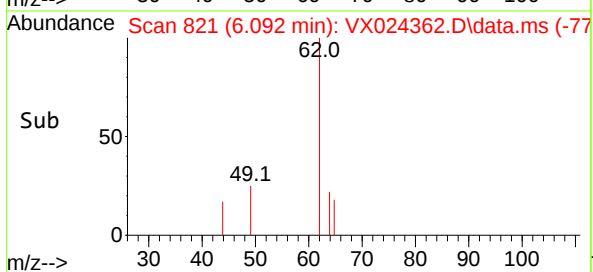
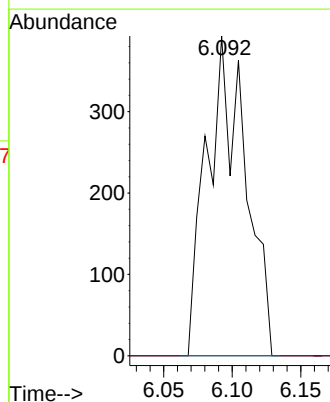





#44
Trichloroethene
Concen: 1372.259 ug/l
RT: 7.135 min Scan# 992
Delta R.T. -0.000 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914


Tgt Ion:130 Resp: 2487929
Ion Ratio Lower Upper
130 100
95 99.9 0.0 198.0

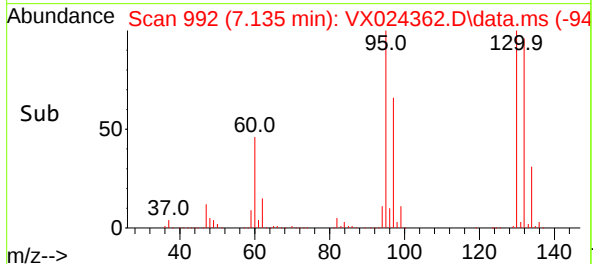

#49
1,4-Dioxane
Concen: 11.331 ug/l
RT: 7.671 min Scan# 1080
Delta R.T. 0.006 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Tgt Ion: 88 Resp: 494
Ion Ratio Lower Upper
88 100
43 19.2 23.2 34.8#
58 59.9 55.0 82.4

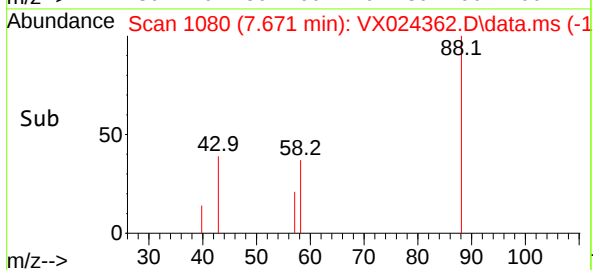



#50

Toluene-d8

Concen: 42.681 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX024362.D





Acq: 20 Sep 2021 19:37

Tgt Ion: 98 Resp: 255166

Ion Ratio Lower Upper

98 100

100 63.6 51.9 77.9

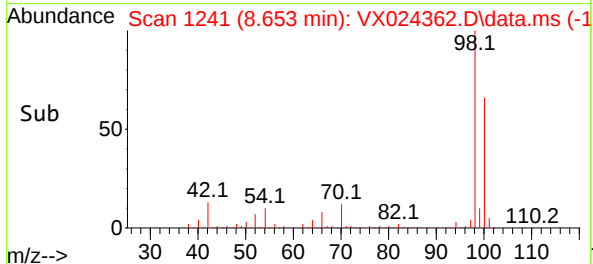

#51

4-Methyl-2-Pentanone

Concen: 0.491 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.067 min

Lab File: VX024362.D




Acq: 20 Sep 2021 19:37


Tgt Ion: 43 Resp: 1306

Ion Ratio Lower Upper

43 100

58 165.4 35.4 53.0#









#55
1,1,2-Trichloroethane
Concen: 0.821 ug/l
RT: 9.159 min Scan# 1324
Delta R.T. -0.000 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914


Tgt Ion: 97	Resp: 1479
Ion Ratio	Lower Upper
97 100	
83 79.7	69.3 103.9
85 46.0	44.3 66.5
99 56.7	50.3 75.5

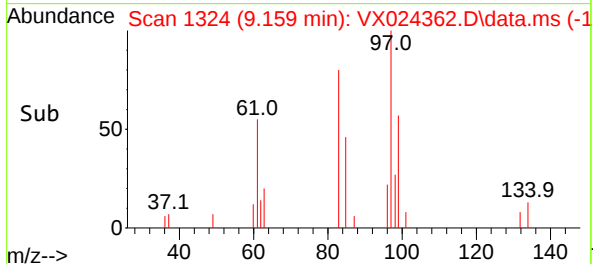

#60
Dibromochloromethane
Concen: 3.452 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.250 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Tgt Ion:129	Resp:	3652	
Ion	Ratio	Lower	Upper
129	100		
127	0.0	38.4	115.2#


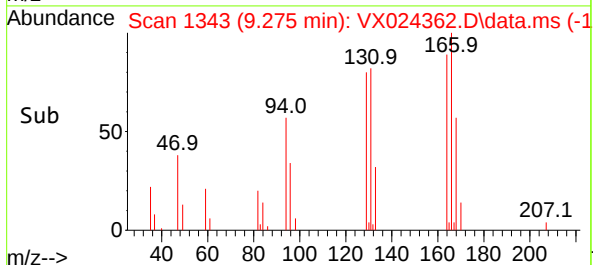
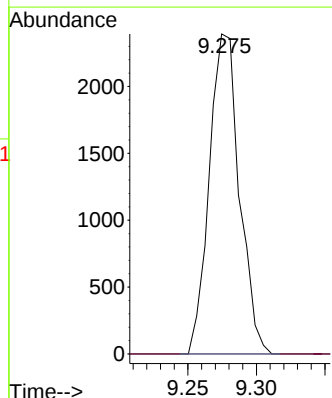



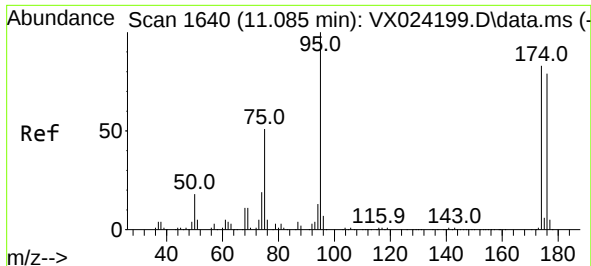

#62
4-Bromofluorobenzene
Concen: 44.206 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914


Tgt Ion: 95 Resp: 102850
Ion Ratio Lower Upper
95 100
174 79.1 0.0 154.6
176 75.2 0.0 155.8

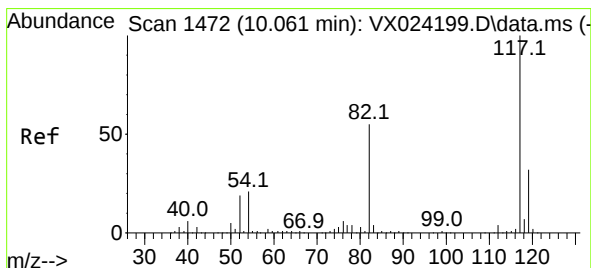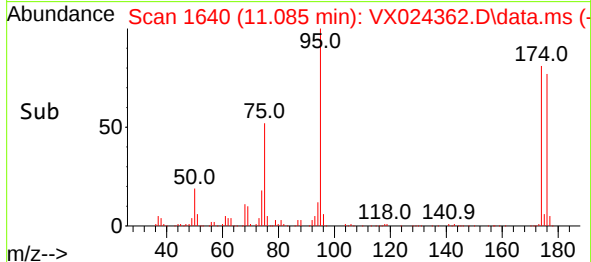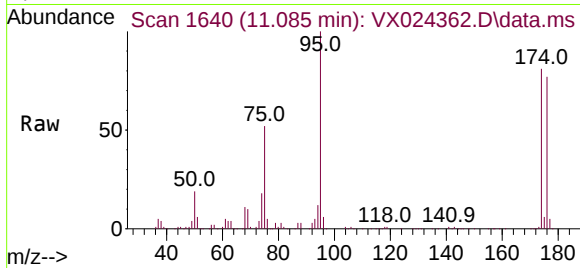

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Tgt Ion: 117 Resp: 195111
Ion Ratio Lower Upper
117 100
82 57.6 47.4 71.2
119 31.0 26.6 39.8

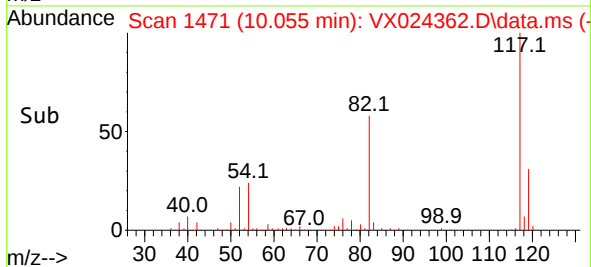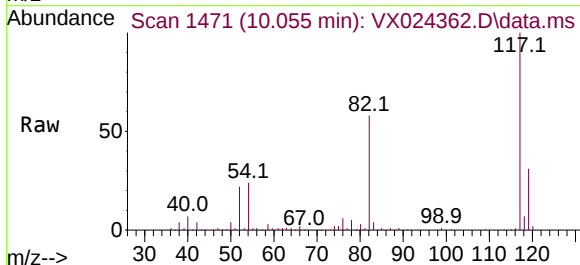




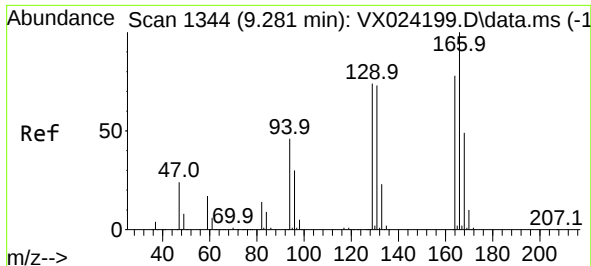


#64
Tetrachloroethene
Concen: 2.512 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.006 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914

Tgt Ion:164 Resp: 3797




Ion	Ratio	Lower	Upper
164	100		
166	113.0	103.4	155.2
129	90.6	70.8	106.2
131	93.2	72.5	108.7

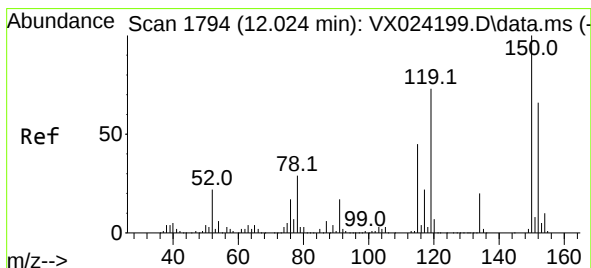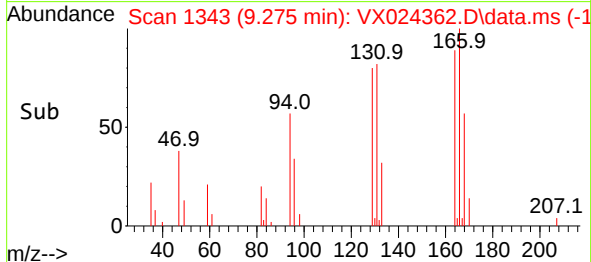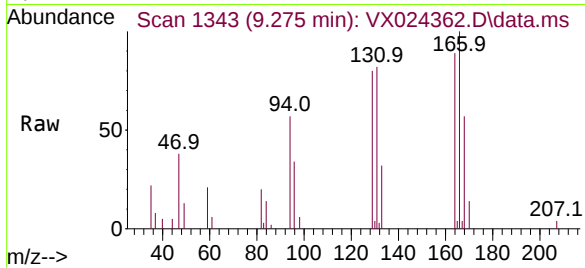


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Tgt Ion:152 Resp: 88755

Ion	Ratio	Lower	Upper
152	100		
115	60.9	41.1	123.3
150	157.4	0.0	349.0


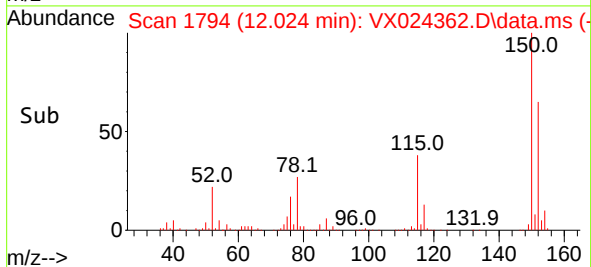

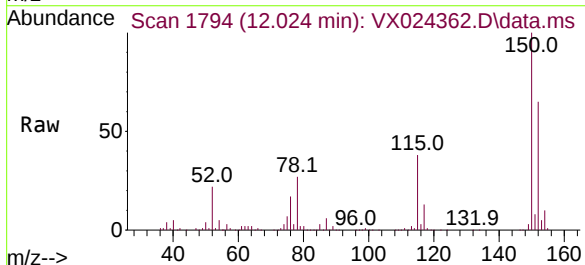


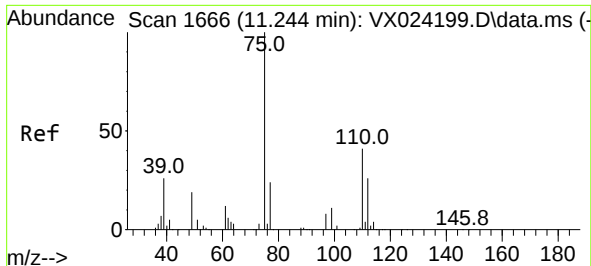

#76
1,2,3-Trichloropropane
Concen: 26.575 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37




Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914


Tgt Ion: 75 Resp: 54236
Ion Ratio Lower Upper
75 100
77 1.0 19.1 57.5#

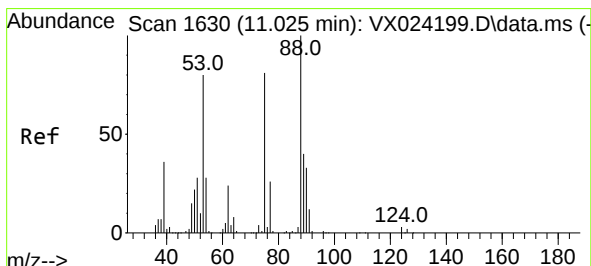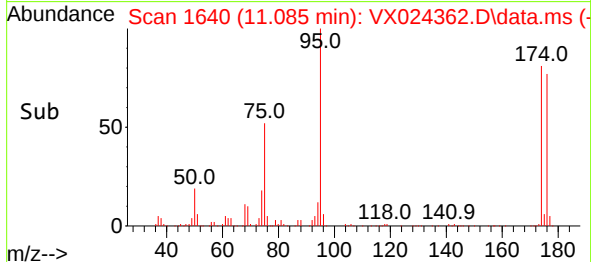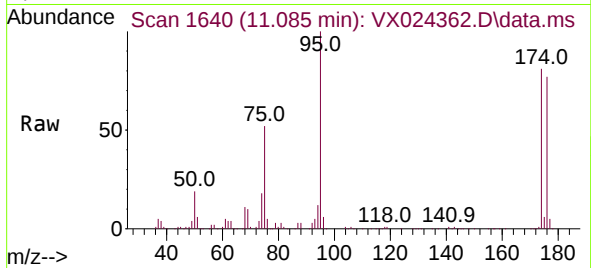

#81
trans-1,4-Dichloro-2-butene
Concen: 78.158 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.060 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37


Tgt Ion: 75 Resp: 54236
Ion Ratio Lower Upper
75 100
53 0.1 74.5 111.7#
89 0.0 37.9 56.9#

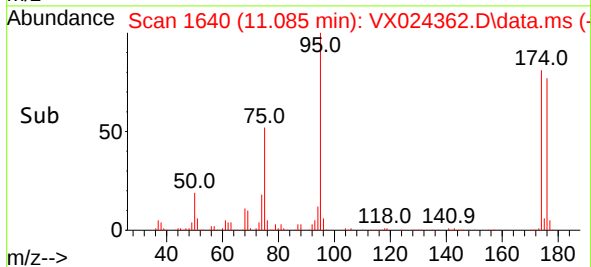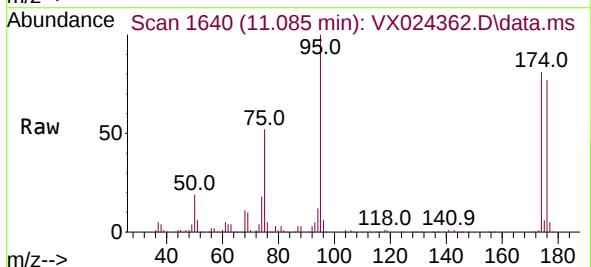

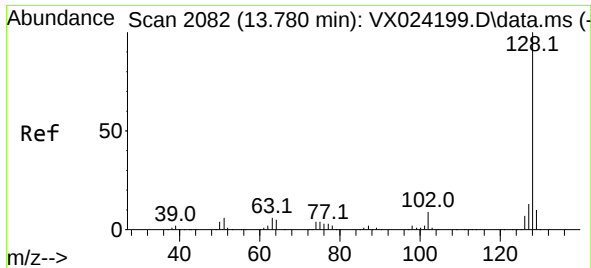

#95
Naphthalene
Concen: 1.302 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX024362.D
Acq: 20 Sep 2021 19:37

Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20210914

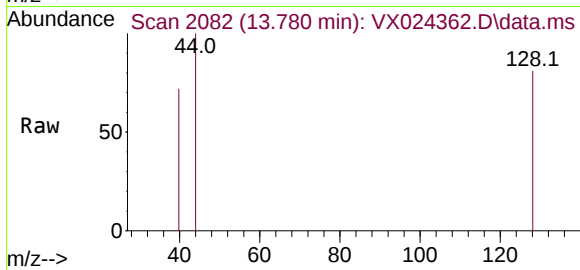

Tgt Ion:	128	Resp:	97
Ion	Ratio	Lower	Upper
128	100		
127	0.0	10.3	15.5#
129	0.0	8.8	13.2#

