
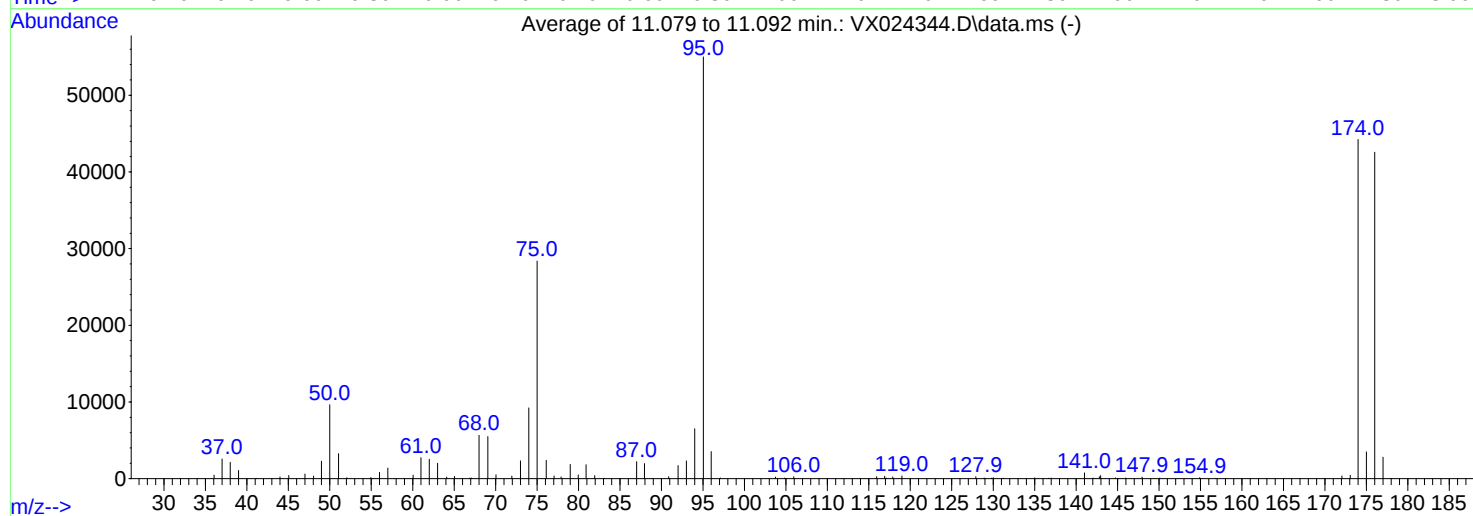


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092021\
 Data File : VX024344.D
 Acq On : 20 Sep 2021 09:21
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
 Title : SW846 8260
 Last Update : Tue Sep 21 10:52:48 2021

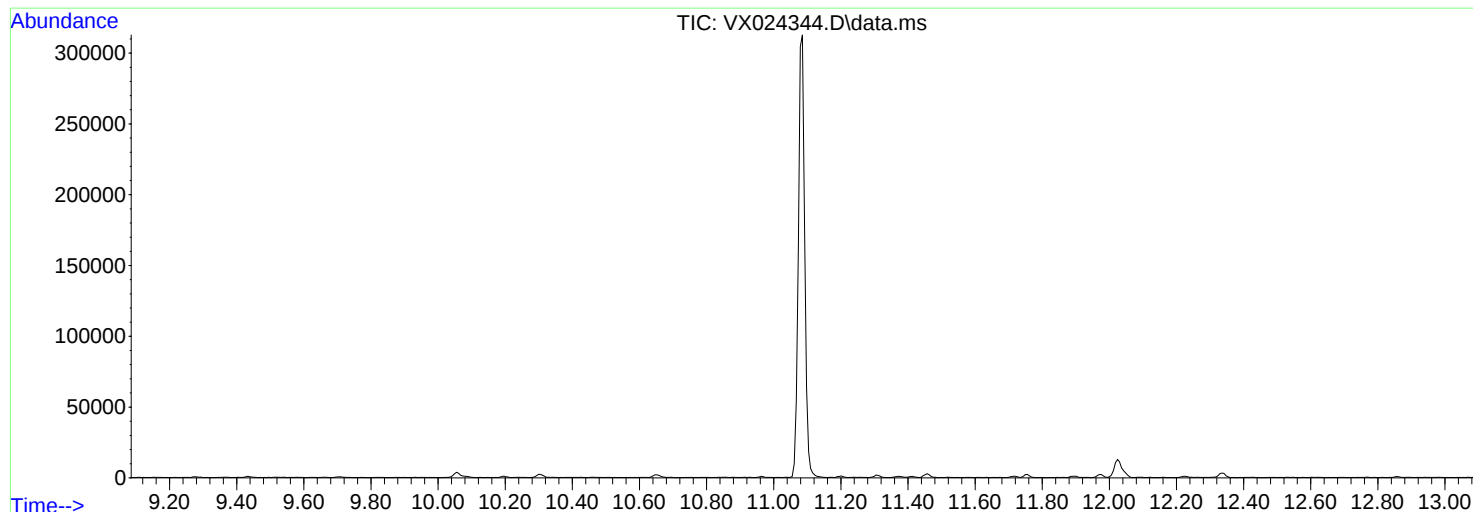

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	9645	PASS
75	95	30	60	51.6	28376	PASS
95	95	100	100	100.0	55011	PASS
96	95	5	9	6.4	3532	PASS
173	174	0.00	2	1.0	445	PASS
174	95	50	100	80.4	44235	PASS
175	174	5	9	7.9	3487	PASS
176	174	95	101	96.2	42573	PASS
177	176	5	9	6.6	2800	PASS