

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092023\
 Data File : VX037824.D
 Acq On : 20 Sep 2023 11:37
 Operator : JC/MD
 Sample : 04511-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 50093

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M

Title : SW846 8260

Signal : TIC: VX037824.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.051	152	158	194	rVB	591408	1014319	81.39%	12.544%
2	4.721	588	596	608	rBV	26381	75477	6.06%	0.933%
3	5.385	694	705	722	rBV	138964	410744	32.96%	5.080%
4	5.556	722	733	748	rVB	243251	686968	55.12%	8.496%
5	5.958	787	799	809	rBV	149591	407040	32.66%	5.034%
6	6.044	809	813	822	rVB2	12395	28607	2.30%	0.354%
7	6.763	922	931	949	rBV	379481	899250	72.15%	11.121%
8	7.214	999	1005	1015	rBV2	13408	33689	2.70%	0.417%
9	8.647	1234	1240	1248	rBV	793446	1246286	100.00%	15.413%
10	8.720	1248	1252	1264	rVB	48032	78110	6.27%	0.966%
11	10.055	1465	1471	1488	rBV	829909	1122566	90.07%	13.883%
12	10.305	1506	1512	1520	rBV2	13452	22003	1.77%	0.272%
13	10.647	1564	1568	1579	rVB3	7588	13936	1.12%	0.172%
14	11.079	1634	1639	1650	rBV	698347	873792	70.11%	10.806%
15	12.024	1788	1794	1803	rBV	896779	1173073	94.13%	14.508%




Sum of corrected areas: 8085860

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092023\
Data File : VX037824.D
Acq On : 20 Sep 2023 11:37
Operator : JC/MD
Sample : 04511-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50093

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

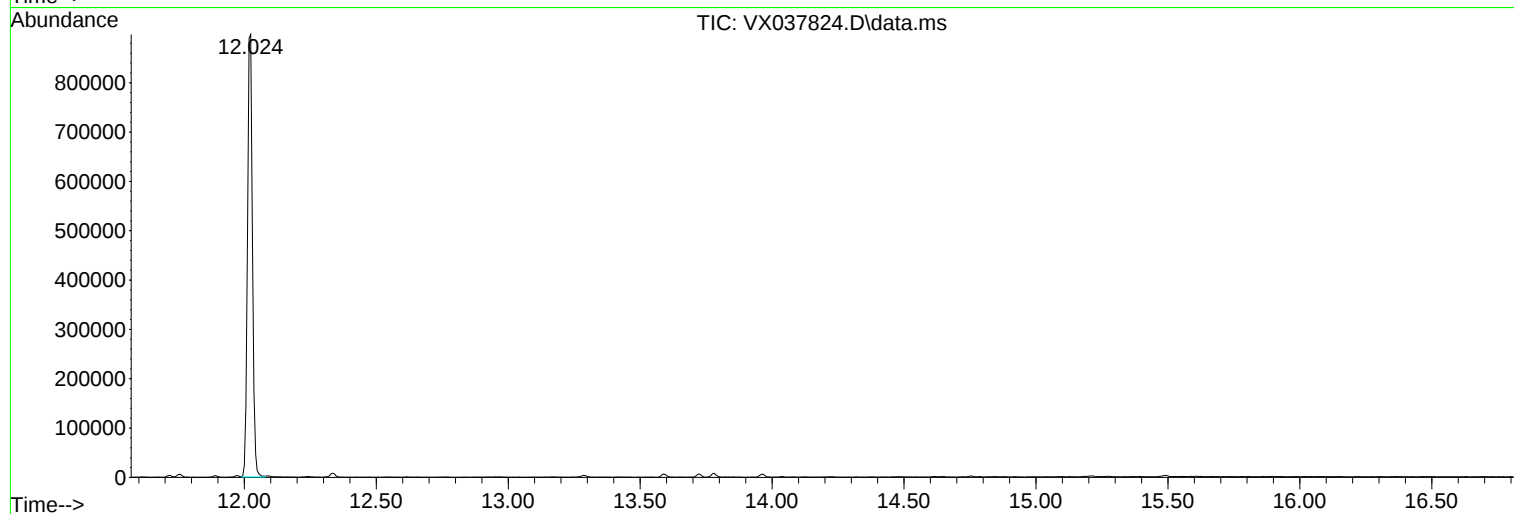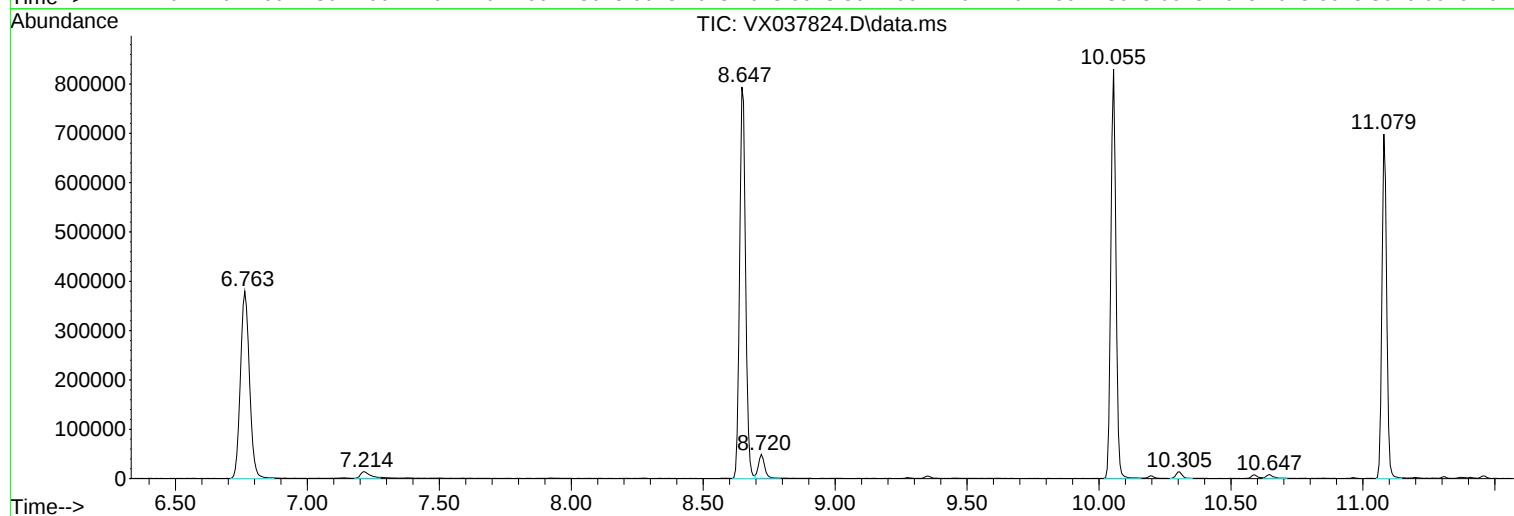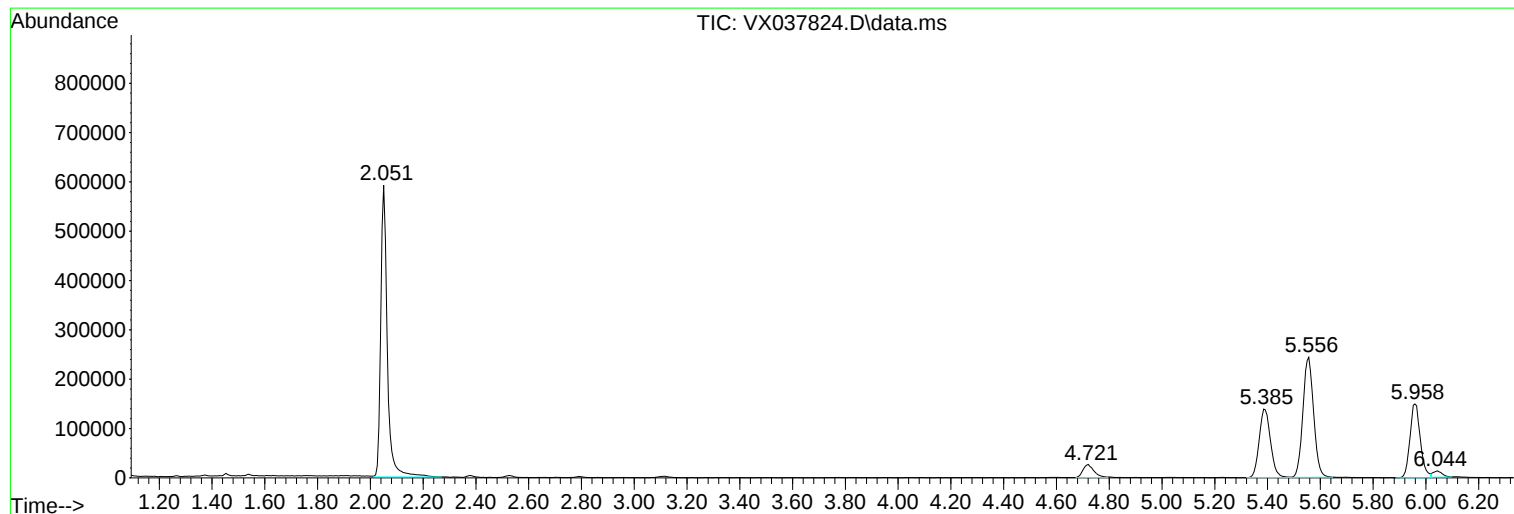

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092023\
Data File : VX037824.D
Acq On : 20 Sep 2023 11:37
Operator : JC/MD
Sample : 04511-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50093










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.051	73.83 ug/l	1014320	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Ethanol			46	C2H6O	000064-17-5	64
2	Dimethyl ether			46	C2H6O	000115-10-6	9
3	Methane, nitroso-			45	CH3NO	000865-40-7	4
4	Formic acid			46	CH2O2	000064-18-6	4
5	Oxalic acid			90	C2H2O4	000144-62-7	4

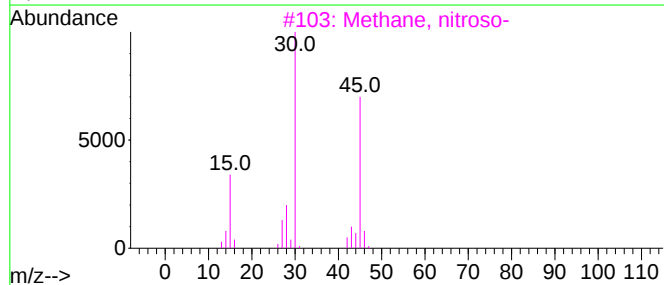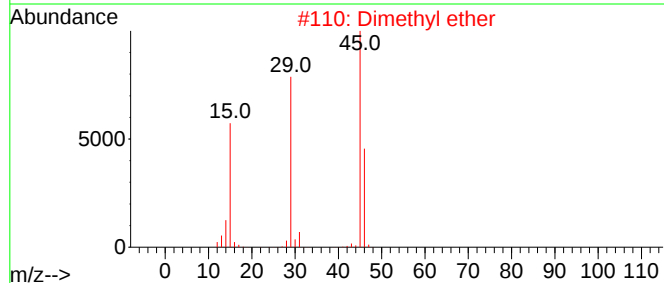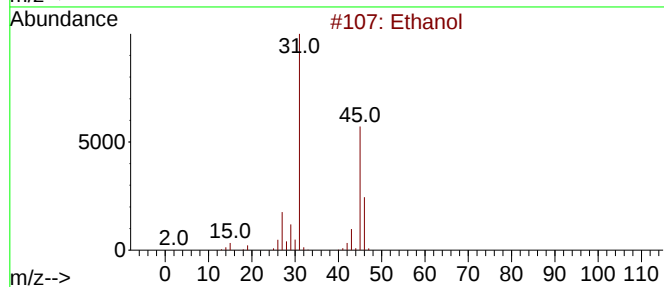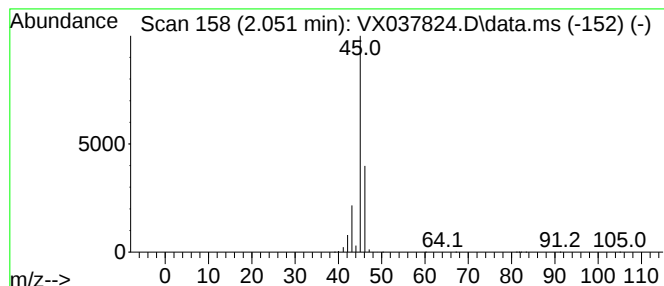

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092023\
Data File : VX037824.D
Acq On : 20 Sep 2023 11:37
Operator : JC/MD
Sample : 04511-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50093

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol	2.051	73.8	ug/l	1014320	1	5.556	686968	50.0