

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092023\
 Data File : VX037833.D
 Acq On : 20 Sep 2023 15:06
 Operator : JC/MD
 Sample : 04526-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-RW10A-GW-420-422

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M

Title : SW846 8260

Signal : TIC: VX037833.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	17	rBV	32931	33373	2.45%	0.437%
2	1.374	41	47	52	rBV2	11390	20114	1.47%	0.263%
3	1.453	57	60	65	rBV	13678	14970	1.10%	0.196%
4	5.385	693	705	722	rBV	155661	461546	33.82%	6.044%
5	5.556	722	733	748	rVB	265072	754733	55.31%	9.884%
6	5.958	787	799	815	rBV	169001	452003	33.12%	5.919%
7	6.763	922	931	949	rBV	418792	987491	72.37%	12.932%
8	8.647	1234	1240	1250	rBV	846931	1364546	100.00%	17.870%
9	10.055	1465	1471	1490	rBV	911251	1238993	90.80%	16.226%
10	11.079	1634	1639	1653	rBV	779053	989424	72.51%	12.958%
11	12.024	1788	1794	1805	rBV	1014197	1318706	96.64%	17.270%




Sum of corrected areas: 7635899

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092023\
Data File : VX037833.D
Acq On : 20 Sep 2023 15:06
Operator : JC/MD
Sample : 04526-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-420-422

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

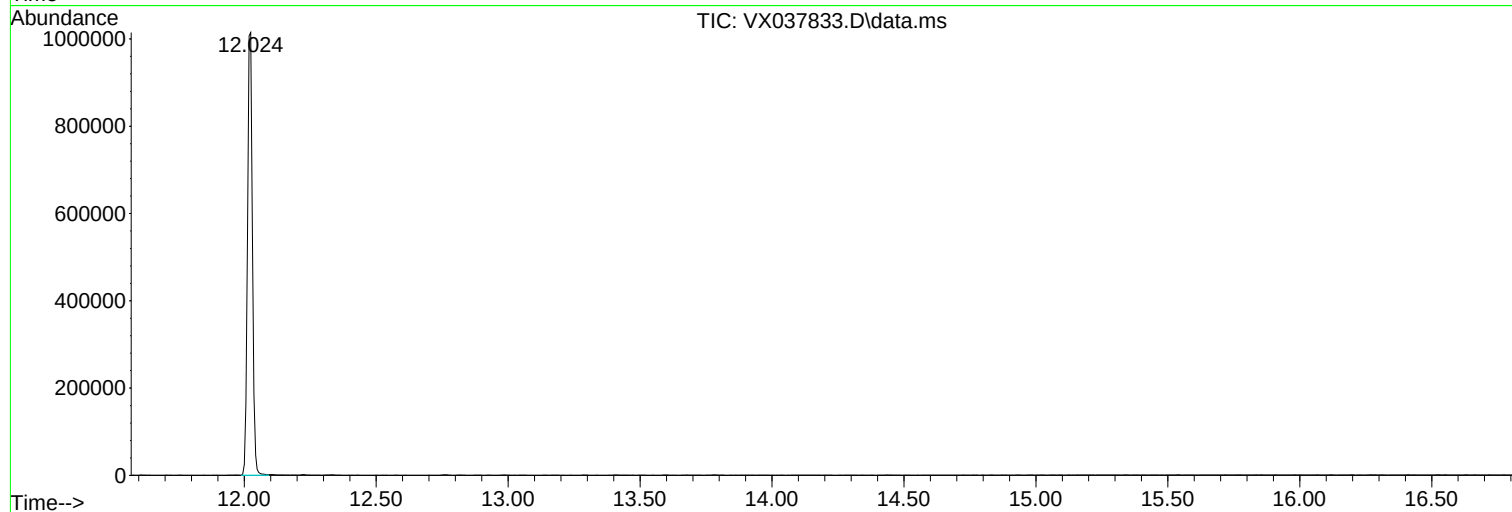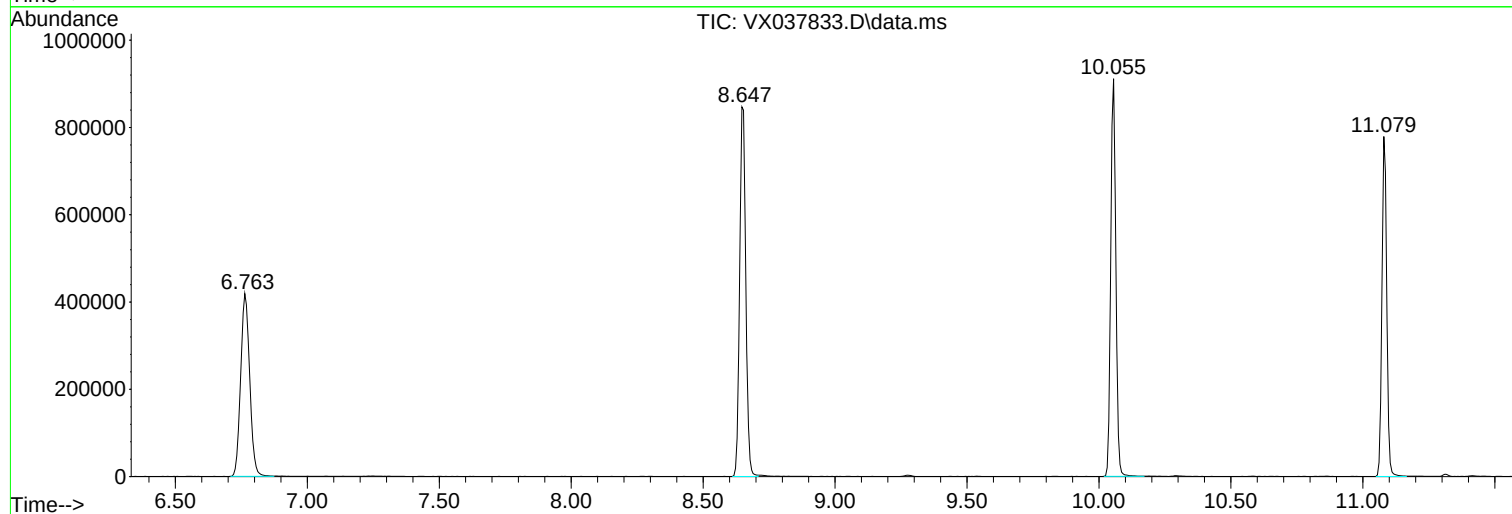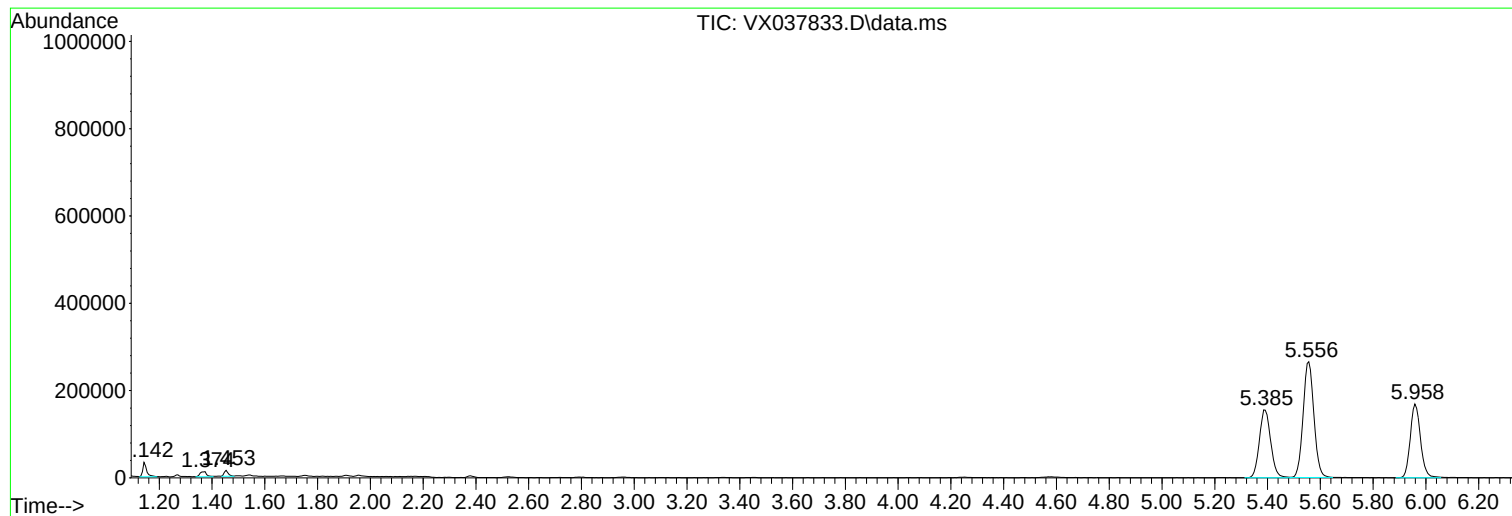

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092023\
Data File : VX037833.D
Acq On : 20 Sep 2023 15:06
Operator : JC/MD
Sample : 04526-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-420-422

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092023\
Data File : VX037833.D
Acq On : 20 Sep 2023 15:06
Operator : JC/MD
Sample : 04526-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-420-422

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------