
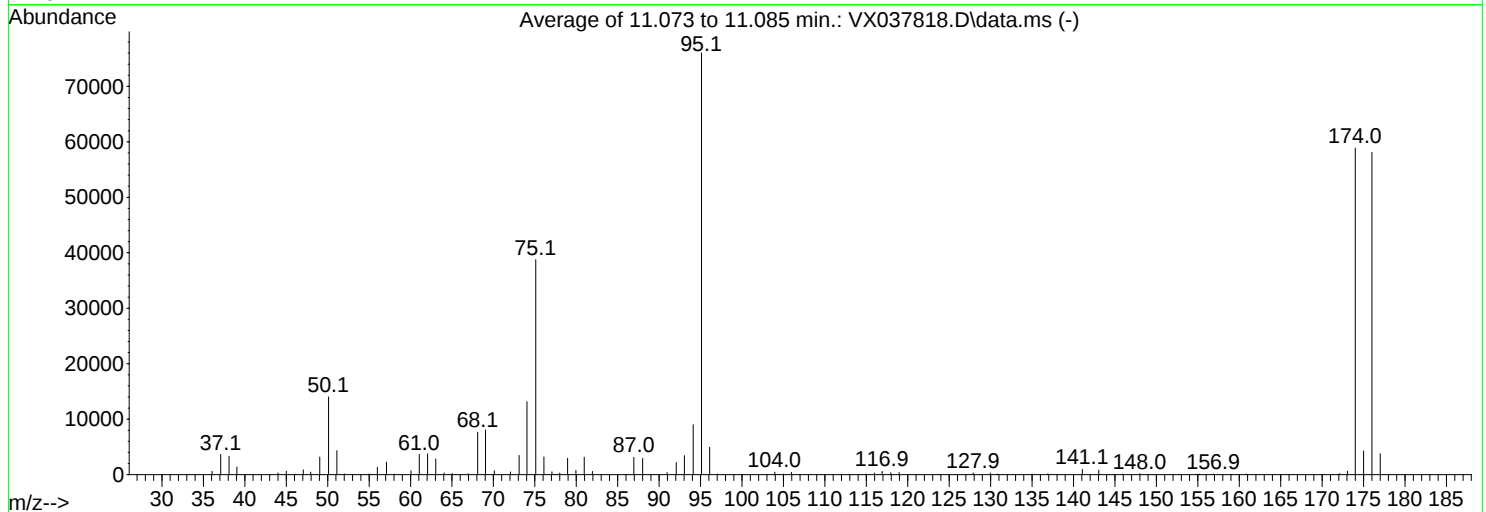


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092023\
Data File : VX037818.D
Acq On : 20 Sep 2023 08:57
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Title : SW846 8260
Last Update : Sat Sep 16 04:55:44 2023

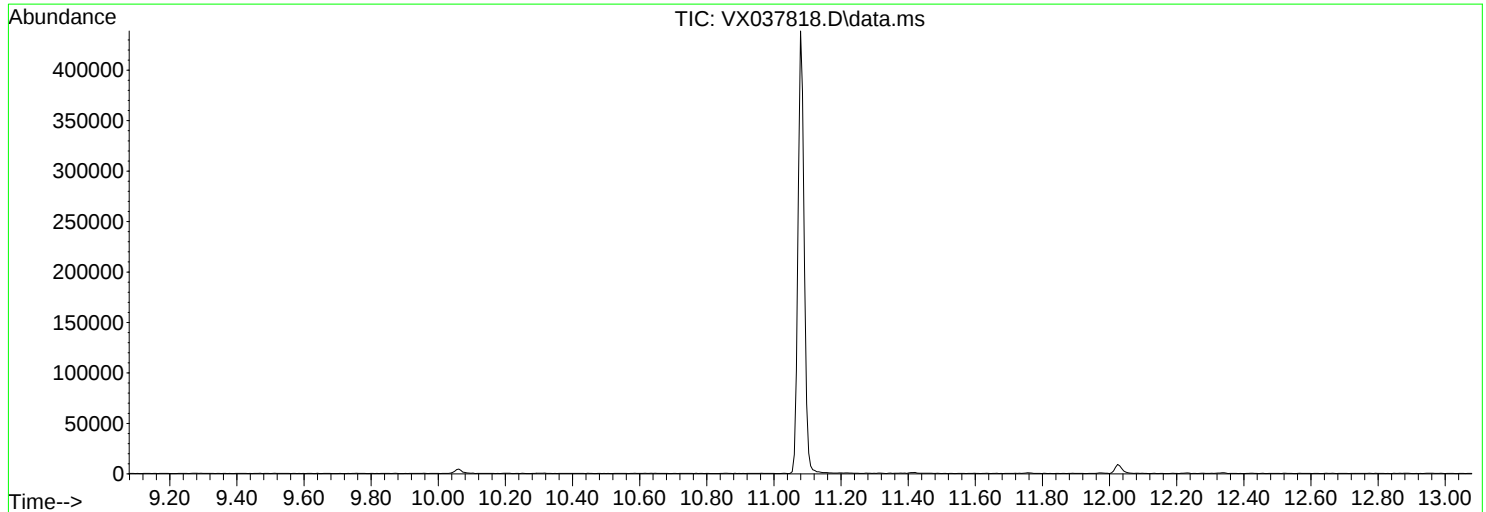

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	14012	PASS
75	95	30	60	51.0	38787	PASS
95	95	100	100	100.0	76048	PASS
96	95	5	9	6.5	4932	PASS
173	174	0.00	2	1.1	626	PASS
174	95	50	100	77.4	58891	PASS
175	174	5	9	7.2	4266	PASS
176	174	95	101	98.7	58099	PASS
177	176	5	9	6.5	3784	PASS