
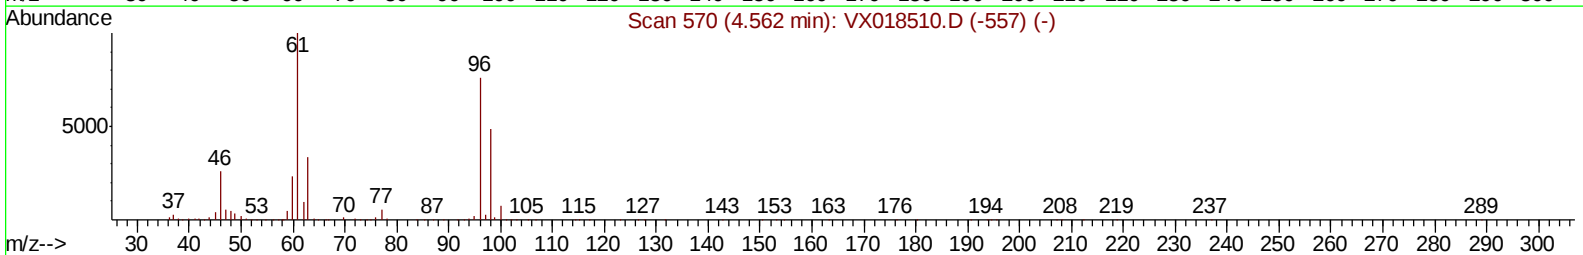
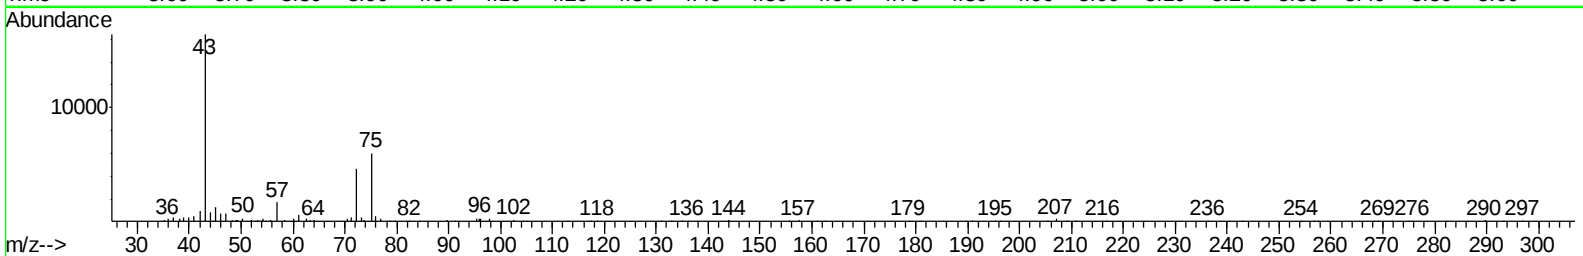


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092120\
Data File : VX018511.D
Acq On : 21 Sep 2020 13:09
Operator : JC/SP
Sample : VSTD100404
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Sep 22 01:06:51 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXMLM092120WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 22 00:58:36 2020
Response via : Initial Calibration

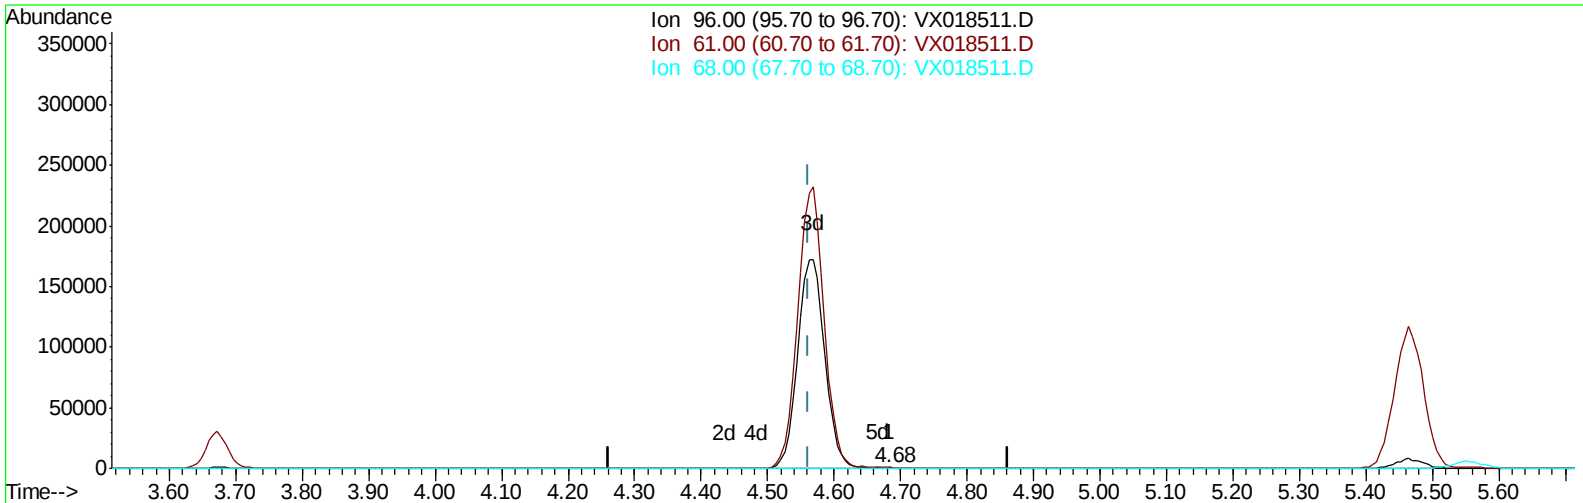

TIC: VX018511.D

(20) cis-1,2-Dichloroethene (T)

4.684min (+0.122) 0.15ug/L

response 731

Ion	Exp%	Act%
96.00	100	100
61.00	131.20	105.66
68.00	0.00	0.00
0.00	0.00	0.00