
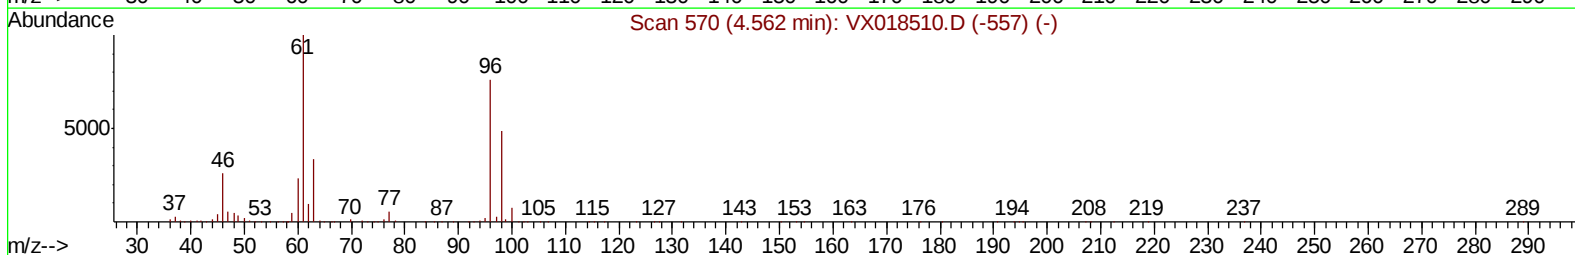
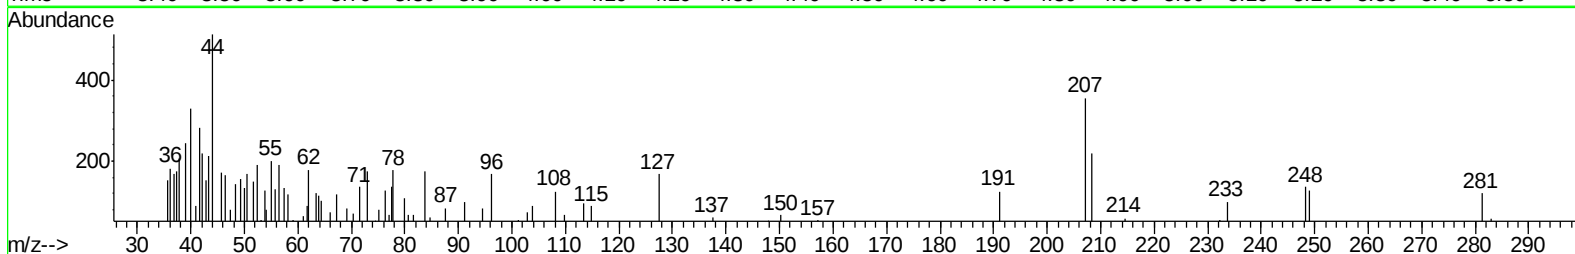


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092120\
Data File : VX018513.D
Acq On : 21 Sep 2020 14:19
Operator : JC/SP
Sample : VSTDICV050
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Sep 22 01:53:56 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM092120WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 22 01:45:38 2020
Response via : Initial Calibration

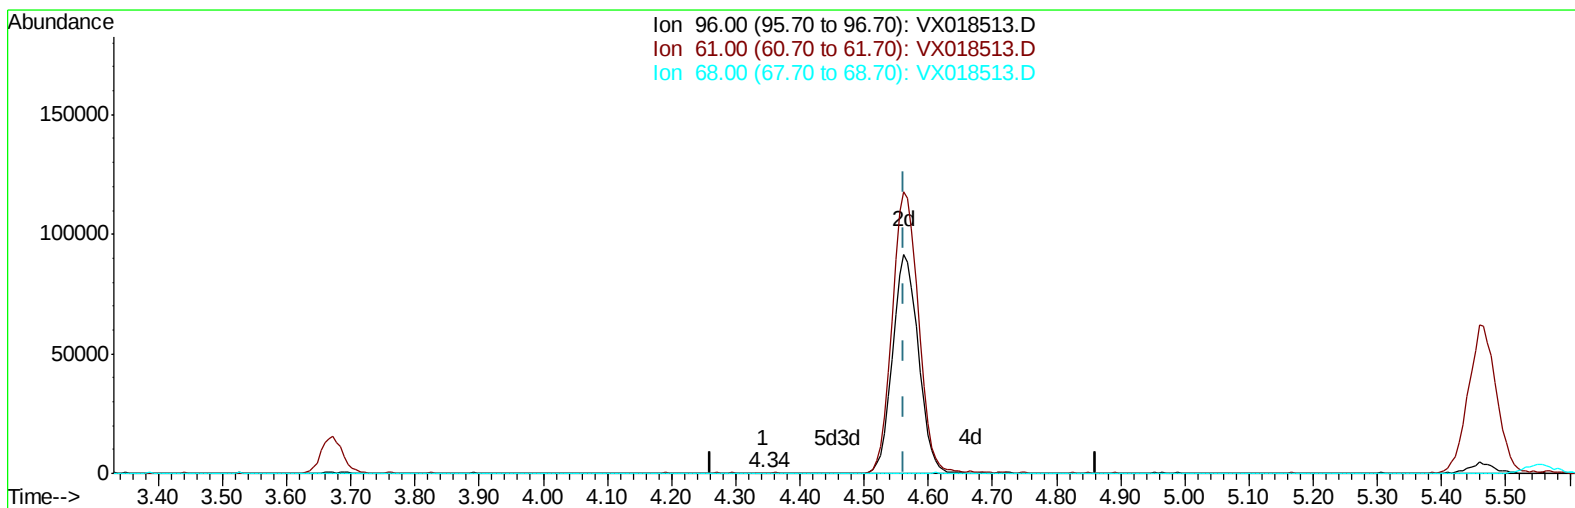

TIC: VX018513.D

(20) cis-1,2-Dichloroethene (T)

4.343min (-0.219) 0.03ug/L

response 135

Ion	Exp%	Act%
96.00	100	100
61.00	131.20	92.22
68.00	0.00	0.00
0.00	0.00	0.00