
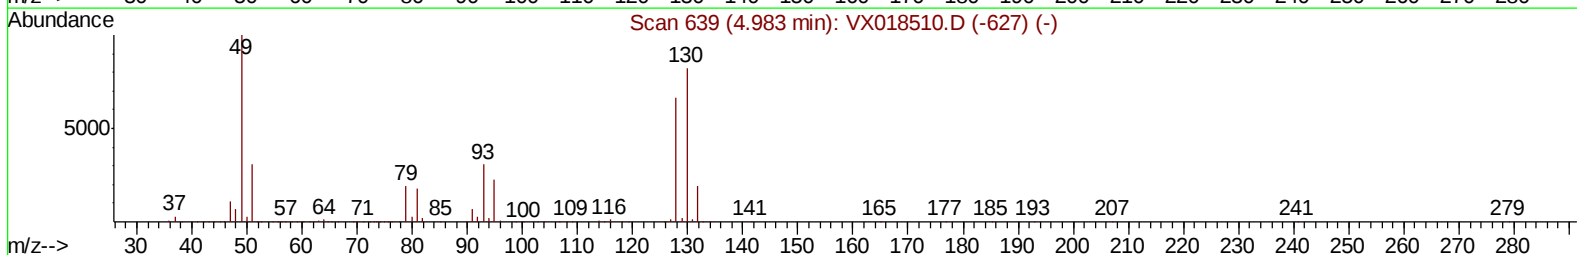
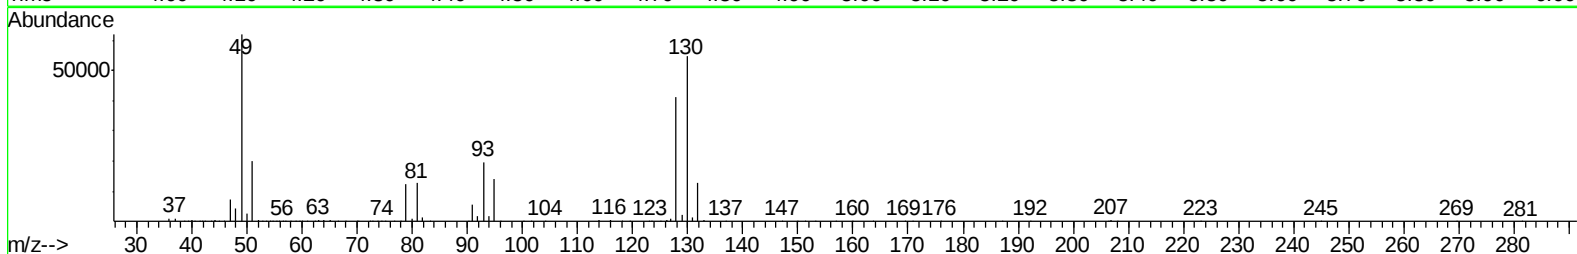


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092120\
 Data File : VX018518.D
 Acq On : 21 Sep 2020 18:05
 Operator : JC/SP
 Sample : VSTDCCC050EC
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Sep 22 02:24:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM092120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 22 02:17:51 2020
 Response via : Initial Calibration

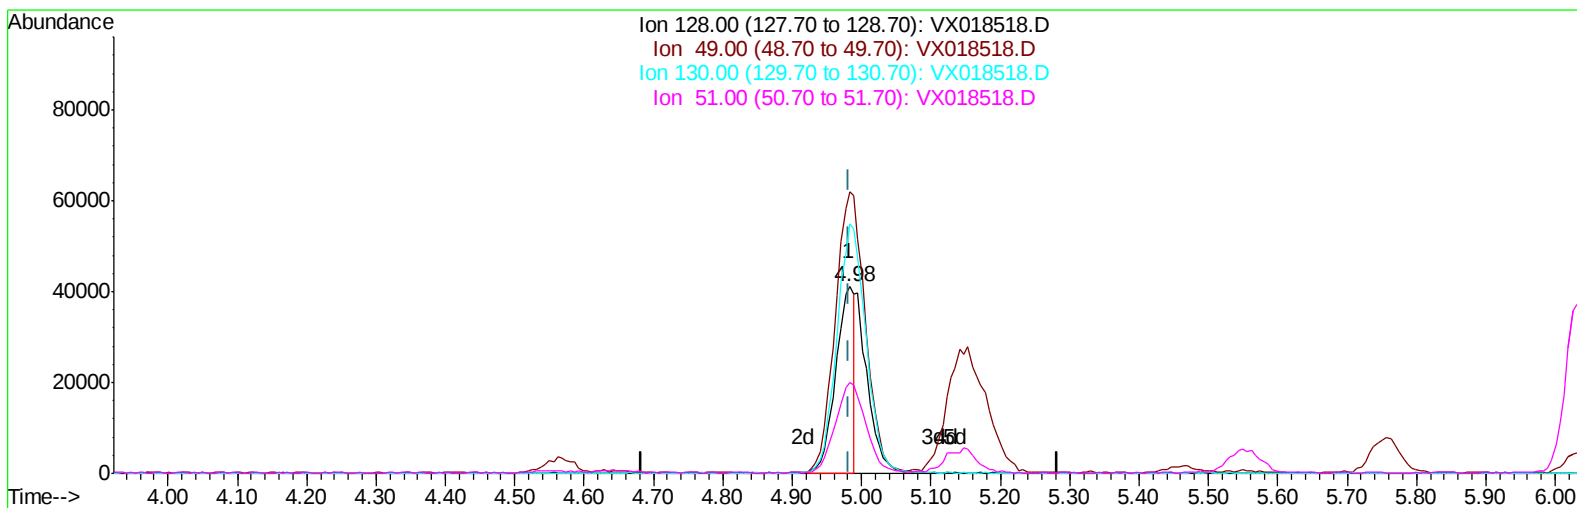

TIC: VX018518.D

(23) Bromochloromethane (T)

4.983min (0.000) 30.19ug/L

response 77763

Ion	Exp%	Act%
128.00	100	100
49.00	149.80	151.07
130.00	123.60	133.78
51.00	46.30	49.10