
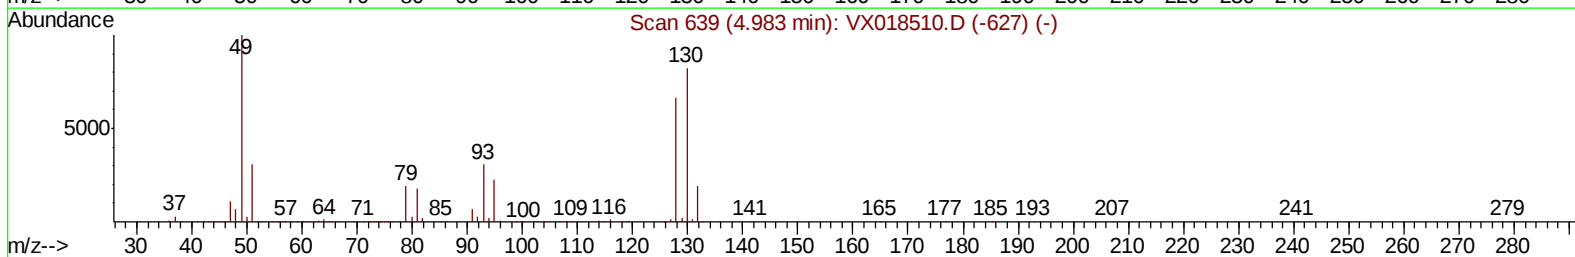
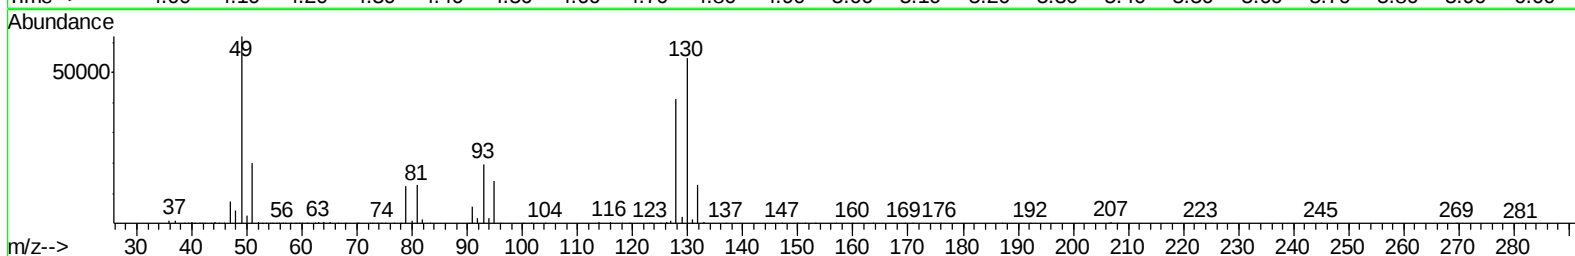


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092120\  
Data File : VX018518.D  
Acq On : 21 Sep 2020 18:05  
Operator : JC/SP  
Sample : VSTDCCC050EC  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Sep 22 02:24:31 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\SFAMXLM092120WMA.M  
Quant Title : VOC Analysis  
QLast Update : Tue Sep 22 02:17:51 2020  
Response via : Initial Calibration

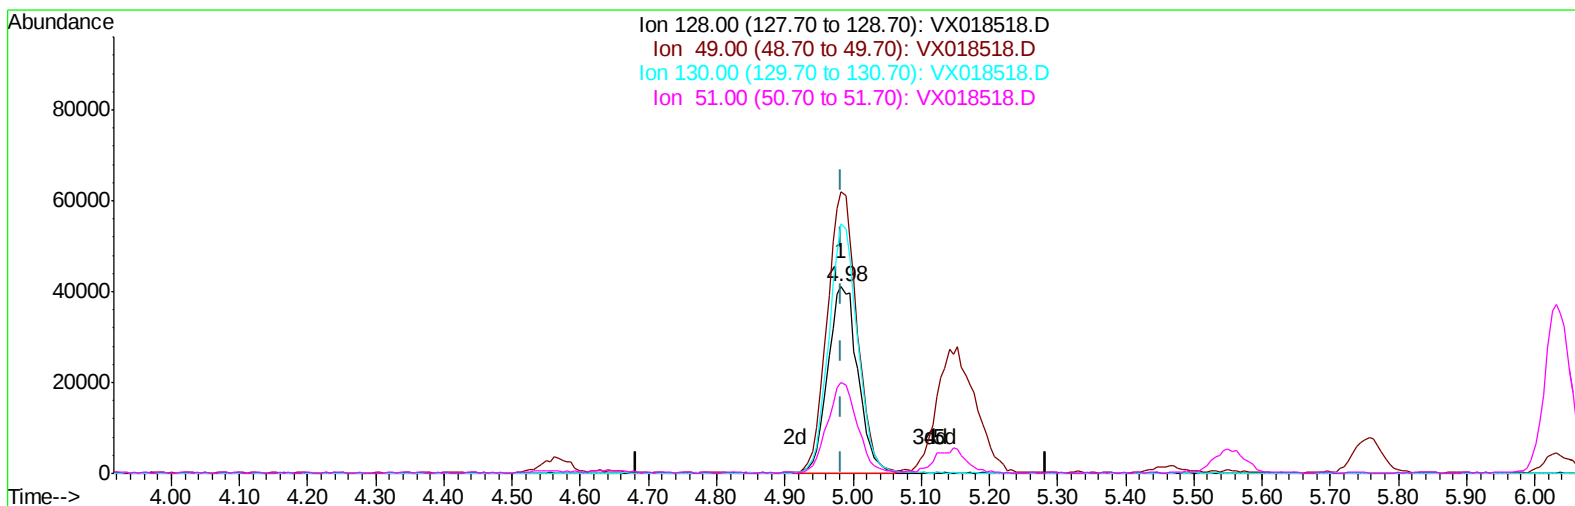

TIC: VX018518.D

(23) Bromochloromethane (T)

4.983min (0.000) 48.69ug/L m

response 125402

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 128.00 | 100    | 100    |
| 49.00  | 149.80 | 151.07 |
| 130.00 | 123.60 | 133.78 |
| 51.00  | 46.30  | 49.10  |