

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092120\
 Data File : VX018514.D
 Acq On : 21 Sep 2020 16:01
 Operator : JC/SP
 Sample : VX0921WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK401

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML092120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.386	46	49	58	rVB	329763	347366	13.64%	1.712%
2	1.697	96	100	108	rVB	257738	303495	11.91%	1.496%
3	2.343	199	206	220	rBV	577339	951579	37.35%	4.689%
4	2.538	236	238	247	rVB3	5088	9928	0.39%	0.049%
5	2.727	268	269	273	rVB4	3129	2352	0.09%	0.012%
6	2.831	284	286	287	rBV2	2635	2283	0.09%	0.011%
7	3.050	319	322	325	rBV4	1961	2110	0.08%	0.010%
8	3.191	343	345	348	rBV4	1965	2042	0.08%	0.010%
9	3.319	365	366	369	rVB3	2687	1790	0.07%	0.009%
10	3.367	369	374	375	rBV4	2009	3069	0.12%	0.015%
11	3.465	388	390	393	rVB4	2694	2335	0.09%	0.012%
12	3.818	447	448	450	rBV2	2157	2017	0.08%	0.010%
13	4.221	512	514	516	rBV3	2322	2347	0.09%	0.012%
14	4.318	527	530	532	rBV4	2089	2220	0.09%	0.011%
15	4.410	540	545	546	rBV5	2795	2544	0.10%	0.013%
16	4.538	557	566	578	rBV	151626	444803	17.46%	2.192%
17	4.763	602	603	608	rBV5	2254	2885	0.11%	0.014%
18	4.898	624	625	627	rBV2	2885	1994	0.08%	0.010%
19	5.044	646	649	650	rBV2	3050	2572	0.10%	0.013%
20	5.141	654	665	679	rVV	330851	1036688	40.69%	5.109%
21	5.306	690	692	694	rVB3	3418	2827	0.11%	0.014%
22	5.343	696	698	701	rVB4	1723	1889	0.07%	0.009%
23	5.373	701	703	706	rBV4	2021	2406	0.09%	0.012%
24	5.446	711	715	717	rBV5	3670	5104	0.20%	0.025%
25	5.684	752	754	757	rBV4	2124	2600	0.10%	0.013%
26	5.727	757	761	763	rBV5	1364	2144	0.08%	0.011%
27	5.751	763	765	770	rVB6	2738	3505	0.14%	0.017%
28	5.897	786	789	795	rBV8	1745	2794	0.11%	0.014%
29	6.044	799	813	828	rBV2	860515	2547584	100.00%	12.554%
30	6.196	836	838	840	rBV3	2074	2108	0.08%	0.010%
31	6.281	850	852	853	rBV2	2020	2067	0.08%	0.010%
32	6.409	871	873	875	rBV3	2000	2305	0.09%	0.011%
33	6.653	911	913	916	rVB4	2763	2606	0.10%	0.013%
34	6.726	923	925	926	rBV2	2258	2023	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092120\
 Data File : VX018514.D
 Acq On : 21 Sep 2020 16:01
 Operator : JC/SP
 Sample : VX0921WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK401

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML092120WMA.M
 Title : VOC Analysis

35	6.830	931	942	954	rBV	735495	1774992	69.67%	8.747%
36	6.934	957	959	962	rVV4	4163	5054	0.20%	0.025%
37	7.123	987	990	991	rBV3	1937	2026	0.08%	0.010%
38	7.172	993	998	1006	rVB8	14050	34376	1.35%	0.169%
39	7.232	1006	1008	1010	rBV3	3060	2667	0.10%	0.013%
40	7.367	1022	1030	1045	rVB	535661	1142914	44.86%	5.632%
41	7.684	1079	1082	1084	rBV4	2782	2898	0.11%	0.014%
42	7.708	1084	1086	1089	rBV4	2190	2285	0.09%	0.011%
43	7.745	1091	1092	1094	rBV2	2201	1884	0.07%	0.009%
44	7.879	1112	1114	1116	rBV3	2418	1804	0.07%	0.009%
45	7.903	1116	1118	1120	rVB3	2493	2079	0.08%	0.010%
46	7.940	1120	1124	1126	rBV4	2675	3717	0.15%	0.018%
47	7.976	1126	1130	1136	rBV8	3809	6110	0.24%	0.030%
48	8.373	1189	1195	1205	rBV	389818	626486	24.59%	3.087%
49	8.446	1205	1207	1209	rVB3	3949	2851	0.11%	0.014%
50	8.470	1209	1211	1214	rBV4	2351	2362	0.09%	0.012%
51	8.555	1224	1225	1229	rVB4	2792	3655	0.14%	0.018%
52	8.696	1241	1248	1258	rBV	1361926	2068396	81.19%	10.193%
53	8.946	1286	1289	1290	rBV2	2135	2310	0.09%	0.011%
54	8.994	1291	1297	1304	rBV	306921	446322	17.52%	2.199%
55	9.092	1311	1313	1317	rBV5	2059	2904	0.11%	0.014%
56	9.220	1332	1334	1337	rVB3	3096	2711	0.11%	0.013%
57	9.427	1362	1368	1375	rBV	720608	1015736	39.87%	5.005%
58	9.738	1415	1419	1425	rVB5	9753	16056	0.63%	0.079%
59	9.909	1445	1447	1452	rBV5	1932	3101	0.12%	0.015%
60	10.098	1471	1478	1488	rVV	1553279	2161018	84.83%	10.649%
61	10.390	1525	1526	1530	rVB3	3830	2921	0.11%	0.014%
62	10.451	1534	1536	1538	rVV3	2532	2366	0.09%	0.012%
63	10.494	1541	1543	1547	rVV5	2033	2043	0.08%	0.010%
64	10.537	1548	1550	1553	rVB4	2711	2223	0.09%	0.011%
65	10.628	1563	1565	1568	rBV3	2476	2027	0.08%	0.010%
66	10.689	1571	1575	1582	rVB10	5517	14260	0.56%	0.070%
67	10.750	1583	1585	1588	rBV4	2155	2157	0.08%	0.011%
68	11.006	1622	1627	1630	rVB6	4932	7769	0.30%	0.038%
69	11.122	1642	1646	1652	rVB7	6222	11118	0.44%	0.055%
70	11.171	1652	1654	1657	rVB4	3675	3218	0.13%	0.016%
71	11.232	1657	1664	1674	rBV	877254	1133844	44.51%	5.587%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092120\
 Data File : VX018514.D
 Acq On : 21 Sep 2020 16:01
 Operator : JC/SP
 Sample : VX0921WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK401

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM092120WMA.M
 Title : VOC Analysis

72	11.500	1703	1708	1709	rBV4	4053	5613	0.22%	0.028%
73	11.713	1741	1743	1745	rBV3	3930	3568	0.14%	0.018%
74	11.750	1747	1749	1753	rVV5	4376	5488	0.22%	0.027%
75	11.793	1753	1756	1758	rVV4	3468	4290	0.17%	0.021%
76	11.976	1783	1786	1787	rBV3	2588	2864	0.11%	0.014%
77	12.006	1789	1791	1795	rVV5	4926	6243	0.25%	0.031%
78	12.061	1795	1800	1809	rBV	1706593	2048420	80.41%	10.094%
79	12.360	1844	1849	1856	rBV	1514875	1894587	74.37%	9.336%
80	12.530	1875	1877	1880	rVB4	2605	2062	0.08%	0.010%
81	12.555	1880	1881	1884	rBV3	2619	2667	0.10%	0.013%
82	12.597	1886	1888	1890	rBV3	1807	1838	0.07%	0.009%
83	13.152	1975	1979	1986	rVB9	6563	11603	0.46%	0.057%
84	13.487	2031	2034	2036	rVV4	1463	1813	0.07%	0.009%
85	13.628	2052	2057	2061	rVB8	8841	15152	0.59%	0.075%
86	13.731	2071	2074	2076	rBV4	3235	3278	0.13%	0.016%
87	13.817	2085	2088	2092	rBV3	5470	7628	0.30%	0.038%
88	13.951	2108	2110	2114	rVV4	4617	5595	0.22%	0.028%
89	14.000	2114	2118	2122	rVV7	7439	12583	0.49%	0.062%
90	14.054	2126	2127	2132	rVV5	2838	2484	0.10%	0.012%
91	14.097	2132	2134	2136	rVV3	2183	2586	0.10%	0.013%
92	14.121	2136	2138	2142	rVB5	3508	3337	0.13%	0.016%
93	14.164	2142	2145	2148	rBV4	2620	3795	0.15%	0.019%
94	14.262	2158	2161	2163	rVB4	2231	2320	0.09%	0.011%
95	14.378	2178	2180	2183	rVB4	3327	2536	0.10%	0.012%
96	14.414	2183	2186	2187	rBV3	2403	1915	0.08%	0.009%
97	14.743	2238	2240	2242	rBV2	2231	1850	0.07%	0.009%
98	14.841	2253	2256	2258	rBV4	2429	2747	0.11%	0.014%
99	14.871	2258	2261	2262	rBV3	2536	2154	0.08%	0.011%
100	16.712	2561	2563	2565	rBV3	2567	2476	0.10%	0.012%


Sum of corrected areas: 20292533

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX092120\
Data File : VX018514.D
Acq On : 21 Sep 2020 16:01
Operator : JC/SP
Sample : VX0921WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK401

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM092120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

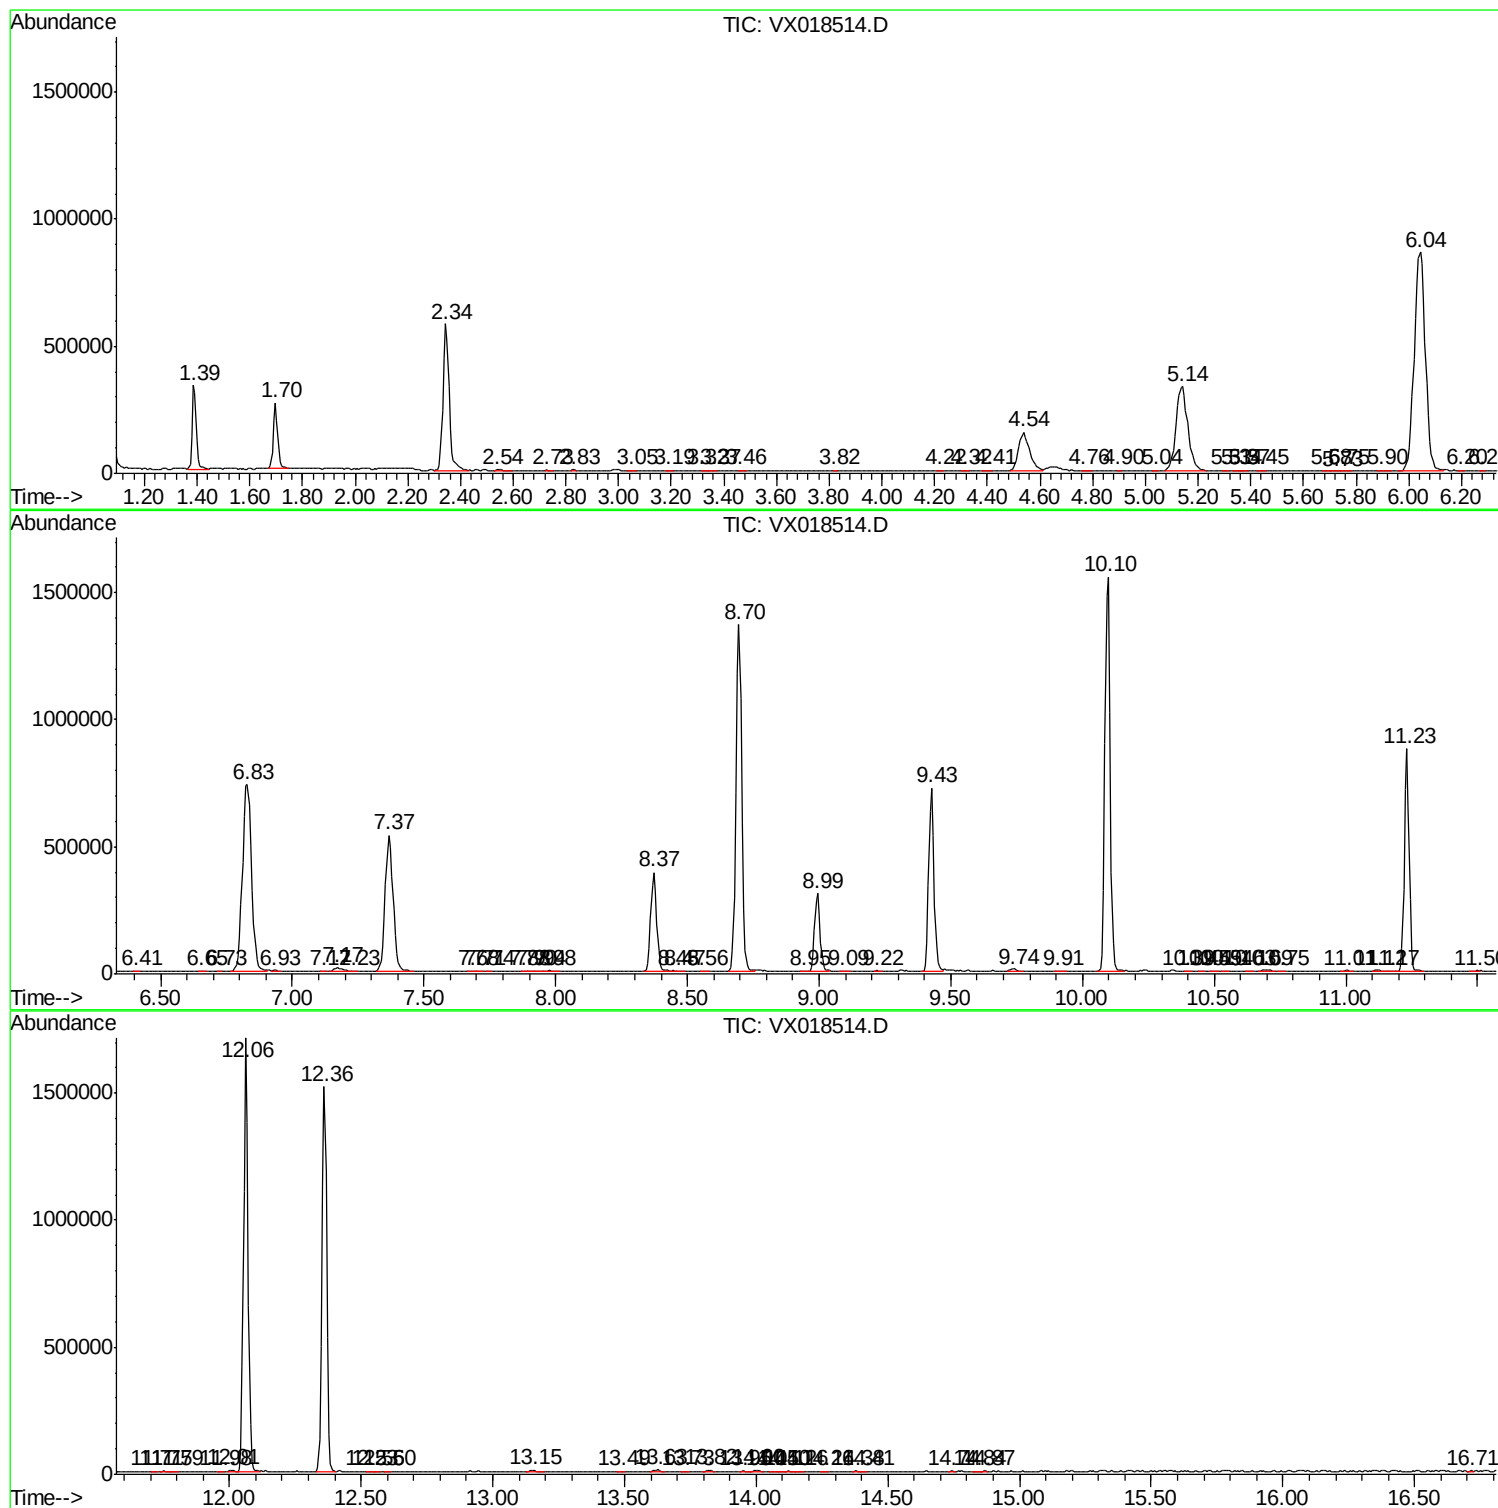

Data_Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX092120\
Data_File : VX018514.D
Acq_On : 21-Sep-2020 16:011
Operator : JC/SPP
Sample : VX0921WBL011
Misc : 5.0mL/MSVOA_X/WATER
ALS_Vial : 11 Sample_Multiplier: 11

Instrument :
MSVOA_X
ClientSampleId :
VBLK401

Quant_Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SEAMXLM092120WMA.MM
Quant_Title : VOC_Analysis

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
