

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092120\
 Data File : VX018515.D
 Acq On : 21 Sep 2020 16:27
 Operator : JC/SP
 Sample : VX0921WBL02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK402

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM092120WMA.M

Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.386	46	49	56	rVB	322491	341299	13.24%	1.745%
2	1.697	96	100	107	rBV	257340	298251	11.57%	1.525%
3	2.343	200	206	223	rVB	572146	948125	36.77%	4.847%
4	2.623	250	252	253	rBV2	2689	1425	0.06%	0.007%
5	2.837	283	287	290	rVB6	4920	6047	0.23%	0.031%
6	2.989	307	312	317	rBV7	7781	13733	0.53%	0.070%
7	3.075	324	326	327	rBV2	2297	1390	0.05%	0.007%
8	3.215	348	349	352	rBV3	2341	2157	0.08%	0.011%
9	3.343	368	370	371	rBV2	2733	1685	0.07%	0.009%
10	3.416	381	382	384	rBV2	2095	1431	0.06%	0.007%
11	3.440	384	386	389	rVB3	2580	1982	0.08%	0.010%
12	3.629	415	417	418	rBV2	2238	1699	0.07%	0.009%
13	3.843	449	452	458	rBV8	2847	6430	0.25%	0.033%
14	3.916	461	464	466	rVB4	2279	2196	0.09%	0.011%
15	4.013	478	480	484	rVB5	3120	3387	0.13%	0.017%
16	4.050	484	486	487	rBV2	2555	2170	0.08%	0.011%
17	4.093	491	493	495	rBV3	2498	2431	0.09%	0.012%
18	4.117	495	497	498	rVB3	2593	1198	0.05%	0.006%
19	4.300	525	527	531	rVB5	1922	1818	0.07%	0.009%
20	4.331	531	532	535	rBV3	1699	1701	0.07%	0.009%
21	4.446	550	551	553	rBV2	2346	1790	0.07%	0.009%
22	4.538	557	566	577	rBV2	146316	436727	16.94%	2.233%
23	4.922	627	629	632	rVB4	2003	2161	0.08%	0.011%
24	4.946	632	633	637	rVB4	2297	2759	0.11%	0.014%
25	4.989	637	640	642	rBV3	1990	2306	0.09%	0.012%
26	5.013	642	644	647	rBV3	1711	1993	0.08%	0.010%
27	5.141	655	665	678	rVB	333758	1036741	40.21%	5.300%
28	5.330	692	696	699	rBV6	1862	2744	0.11%	0.014%
29	5.422	709	711	714	rBV4	2107	2545	0.10%	0.013%
30	5.532	725	729	730	rBV4	2908	3339	0.13%	0.017%
31	5.763	764	767	768	rBV3	1854	1982	0.08%	0.010%
32	5.824	774	777	780	rVB5	2361	3151	0.12%	0.016%
33	6.044	799	813	827	rBV2	878292	2578189	100.00%	13.181%
34	6.220	841	842	845	rVV3	3147	1687	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092120\
 Data File : VX018515.D
 Acq On : 21 Sep 2020 16:27
 Operator : JC/SP
 Sample : VX0921WBL02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK402

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML092120WMA.M
 Title : VOC Analysis

35	6.391	869	870	871	rBV	1986	1412	0.05%	0.007%
36	6.452	878	880	882	rBV3	1918	1384	0.05%	0.007%
37	6.702	919	921	923	rVB3	3247	2253	0.09%	0.012%
38	6.830	932	942	956	rBV2	658569	1582889	61.40%	8.092%
39	7.037	974	976	977	rBV2	2433	2271	0.09%	0.012%
40	7.367	1021	1030	1044	rBV	525487	1136134	44.07%	5.808%
41	7.653	1074	1077	1078	rBV3	2645	2861	0.11%	0.015%
42	7.726	1087	1089	1091	rBV3	2219	2207	0.09%	0.011%
43	8.153	1157	1159	1160	rBV2	2538	1984	0.08%	0.010%
44	8.183	1162	1164	1165	rVB2	2261	1308	0.05%	0.007%
45	8.269	1176	1178	1181	rBV4	3729	4934	0.19%	0.025%
46	8.372	1188	1195	1204	rBV	400787	622588	24.15%	3.183%
47	8.519	1217	1219	1221	rBV3	2501	1786	0.07%	0.009%
48	8.696	1241	1248	1255	rBV	1379503	2070872	80.32%	10.587%
49	8.994	1291	1297	1307	rBB	308081	445173	17.27%	2.276%
50	9.135	1317	1320	1323	rBV5	2257	3771	0.15%	0.019%
51	9.317	1346	1350	1354	rBV7	4453	5332	0.21%	0.027%
52	9.427	1362	1368	1376	rBV	733724	1012489	39.27%	5.176%
53	9.738	1414	1419	1425	rBV8	8984	14582	0.57%	0.075%
54	9.933	1449	1451	1452	rBV2	2448	1777	0.07%	0.009%
55	10.025	1465	1466	1470	rBV4	1717	1597	0.06%	0.008%
56	10.098	1472	1478	1489	rVB	1446924	1943539	75.38%	9.936%
57	10.384	1522	1525	1526	rBV3	1566	1328	0.05%	0.007%
58	10.433	1531	1533	1534	rBV2	1960	1486	0.06%	0.008%
59	10.512	1541	1546	1549	rVB7	3399	6229	0.24%	0.032%
60	10.549	1549	1552	1553	rBV3	2007	2322	0.09%	0.012%
61	10.659	1566	1570	1571	rBV4	1562	2118	0.08%	0.011%
62	10.689	1573	1575	1578	rVV4	2211	2172	0.08%	0.011%
63	10.823	1595	1597	1599	rBV3	1408	1250	0.05%	0.006%
64	10.884	1605	1607	1608	rBV2	2521	1341	0.05%	0.007%
65	10.982	1621	1623	1625	rBV3	1838	1832	0.07%	0.009%
66	11.073	1635	1638	1641	rBV5	3410	5369	0.21%	0.027%
67	11.122	1643	1646	1649	rVV5	5806	7996	0.31%	0.041%
68	11.152	1649	1651	1654	rVB4	2532	2715	0.11%	0.014%
69	11.232	1659	1664	1671	rVB	900472	1124111	43.60%	5.747%
70	11.427	1694	1696	1699	rVB4	2716	2238	0.09%	0.011%
71	11.457	1699	1701	1703	rVB3	2904	2320	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092120\
 Data File : VX018515.D
 Acq On : 21 Sep 2020 16:27
 Operator : JC/SP
 Sample : VX0921WBL02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK402

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM092120WMA.M
 Title : VOC Analysis

72	11.500	1703	1708	1709	rBV5	3600	4906	0.19%	0.025%
73	11.628	1727	1729	1731	rVB3	2290	1210	0.05%	0.006%
74	11.872	1767	1769	1770	rBV2	2598	2328	0.09%	0.012%
75	11.915	1774	1776	1779	rVV4	2538	3127	0.12%	0.016%
76	11.963	1781	1784	1787	rBV5	2448	3131	0.12%	0.016%
77	12.061	1795	1800	1808	rVB	1485843	1819059	70.56%	9.300%
78	12.244	1828	1830	1831	rBV2	1961	1614	0.06%	0.008%
79	12.317	1841	1842	1843	rBV	2171	1226	0.05%	0.006%
80	12.360	1844	1849	1856	rVV	1555322	1912434	74.18%	9.777%
81	12.585	1881	1886	1887	rBV5	2271	3470	0.13%	0.018%
82	12.853	1928	1930	1931	rBV2	3310	1910	0.07%	0.010%
83	12.963	1946	1948	1950	rVB3	3059	2811	0.11%	0.014%
84	12.988	1950	1952	1953	rBV2	1922	1334	0.05%	0.007%
85	13.048	1957	1962	1963	rBV5	2686	3756	0.15%	0.019%
86	13.201	1985	1987	1990	rBV4	3450	4860	0.19%	0.025%
87	13.268	1996	1998	1999	rVB2	2411	1698	0.07%	0.009%
88	13.378	2015	2016	2018	rBV2	1916	1724	0.07%	0.009%
89	13.469	2029	2031	2033	rBV3	2452	1743	0.07%	0.009%
90	13.561	2044	2046	2048	rVB3	2435	1431	0.06%	0.007%
91	13.585	2048	2050	2052	rBV3	3036	2416	0.09%	0.012%
92	13.622	2054	2056	2063	rVB8	5945	8825	0.34%	0.045%
93	13.725	2072	2073	2075	rBV2	1702	1322	0.05%	0.007%
94	13.902	2099	2102	2105	rVB5	4134	5388	0.21%	0.028%
95	14.012	2114	2120	2124	rVB8	4381	8468	0.33%	0.043%
96	14.048	2124	2126	2130	rVV4	2781	3679	0.14%	0.019%
97	14.097	2132	2134	2136	rVB3	2308	1836	0.07%	0.009%
98	14.286	2162	2165	2166	rBV3	2365	2599	0.10%	0.013%
99	14.877	2260	2262	2264	rBV3	2178	2015	0.08%	0.010%
100	15.444	2353	2355	2356	rBV2	4442	3154	0.12%	0.016%


Sum of corrected areas: 19560113

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX092120\
Data File : VX018515.D
Acq On : 21 Sep 2020 16:27
Operator : JC/SP
Sample : VX0921WBL02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK402

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM092120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

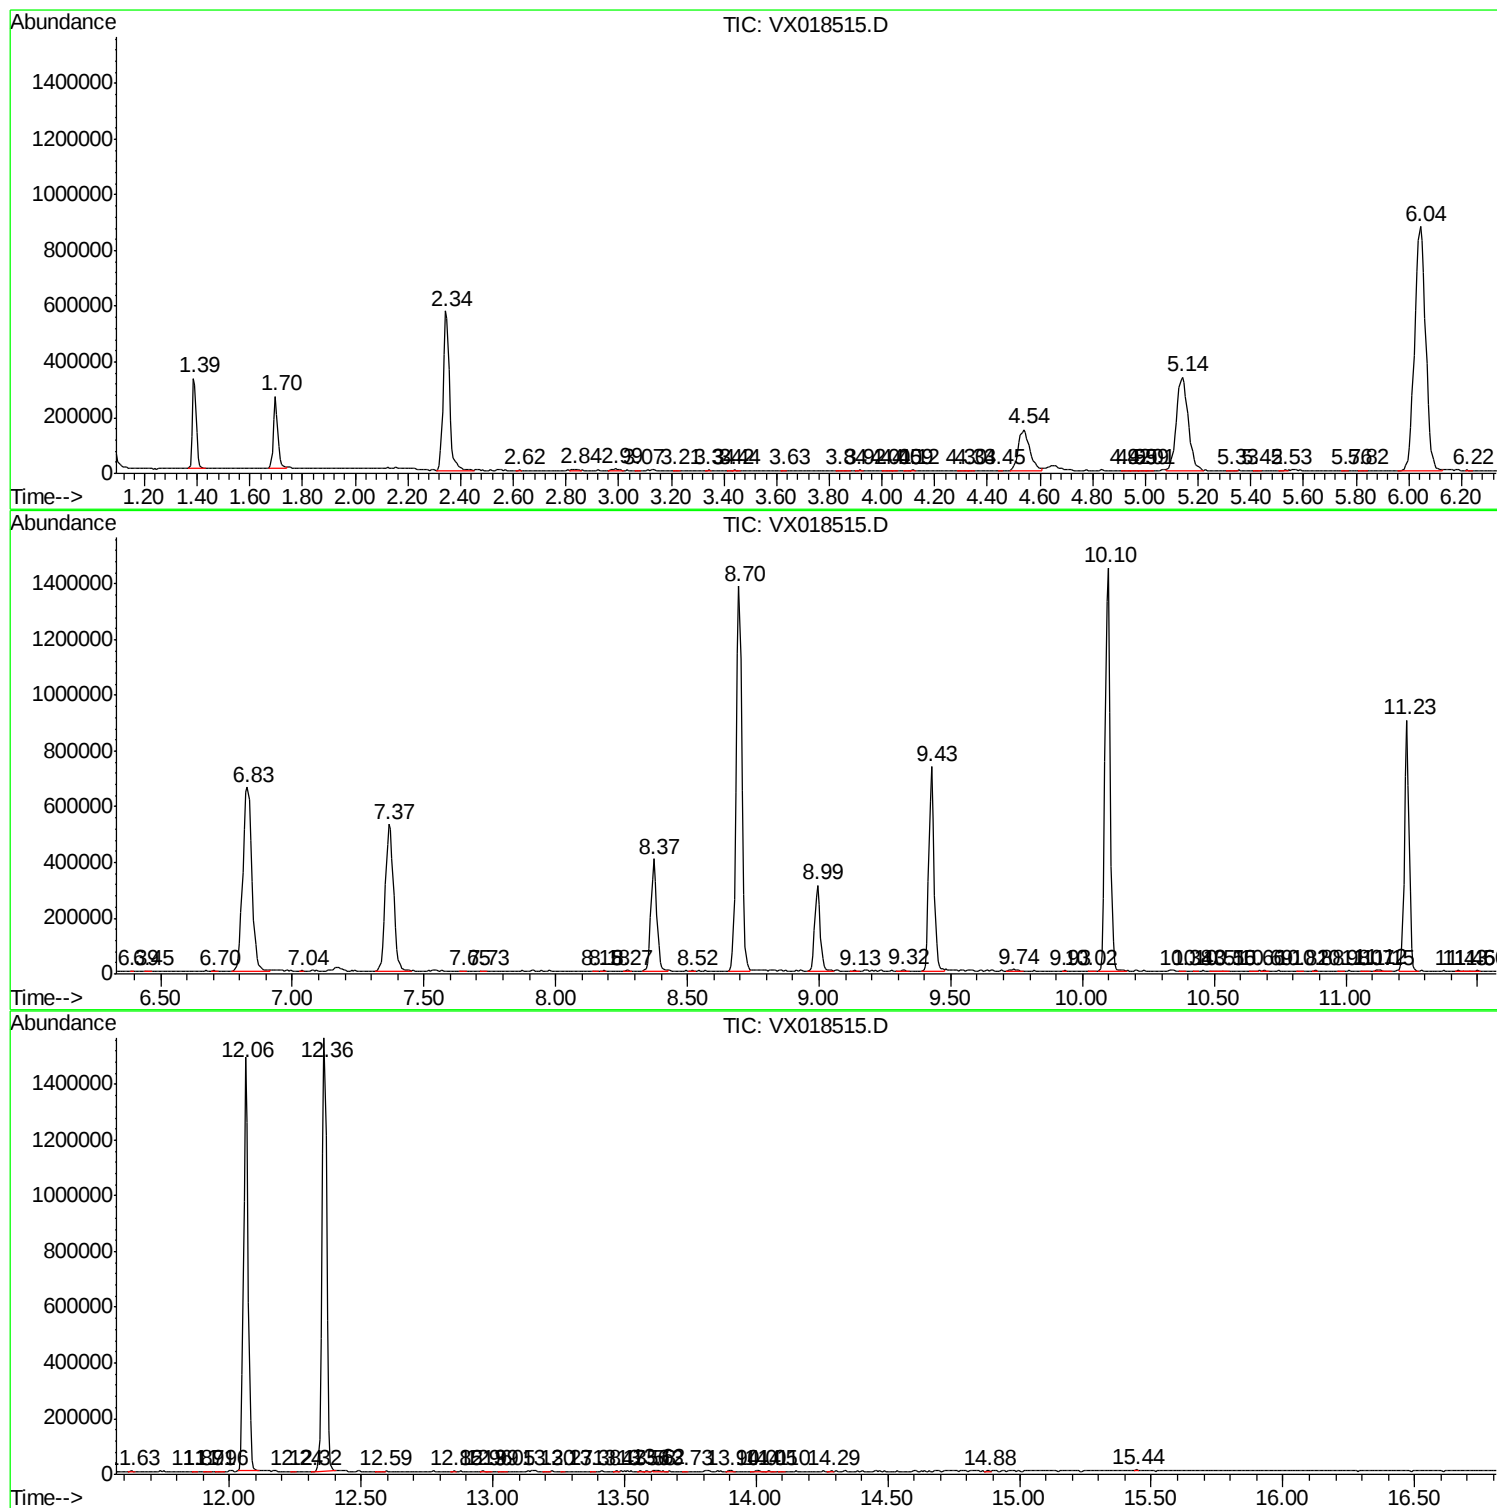

Data_Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX092120\
Data_File : VX018515.D
Acq_On : 21-Sep-2020 16:277
Operator : JC/SPP
Sample : VX0921WBL022
Misc : 5.0mL/MSVOA_X/WATER
ALS_Vial : 12 Sample_Multiplier: 11

Instrument :
MSVOA_X
ClientSampleId :
VBLK402

Quant_Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SEAMXLM092120WMA.M
Quant_Title : VOC_Analysis

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
