

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092120\
 Data File : VX018521.D
 Acq On : 22 Sep 2020 11:36
 Operator : JC/SP
 Sample : VX0921WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK403

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML092120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.386	46	49	57	rVB	358585	376765	13.57%	1.769%
2	1.697	96	100	107	rVB	282161	330867	11.92%	1.553%
3	2.343	200	206	216	rBV	619936	1007951	36.30%	4.732%
4	2.538	236	238	239	rBV2	3071	2024	0.07%	0.010%
5	2.721	266	268	269	rBV2	2147	1903	0.07%	0.009%
6	2.794	277	280	281	rBV3	2593	2439	0.09%	0.011%
7	2.940	302	304	305	rBV2	3046	1974	0.07%	0.009%
8	3.221	348	350	351	rBV2	1438	1452	0.05%	0.007%
9	3.239	351	353	354	rVB2	3145	1764	0.06%	0.008%
10	3.294	360	362	364	rBV3	1727	2184	0.08%	0.010%
11	3.343	369	370	371	rBV	2690	1713	0.06%	0.008%
12	3.404	378	380	385	rVB6	2639	3922	0.14%	0.018%
13	3.453	385	388	391	rBV5	1714	2608	0.09%	0.012%
14	3.520	397	399	402	rBV3	1393	1788	0.06%	0.008%
15	3.611	413	414	418	rBV4	1808	2387	0.09%	0.011%
16	3.855	452	454	456	rBV3	2125	1861	0.07%	0.009%
17	3.922	463	465	468	rBV4	2491	2048	0.07%	0.010%
18	3.946	468	469	473	rBV4	2561	2870	0.10%	0.013%
19	4.184	506	508	510	rVB3	2864	2032	0.07%	0.010%
20	4.209	510	512	514	rBV3	2457	1506	0.05%	0.007%
21	4.306	525	528	529	rBV3	2622	2166	0.08%	0.010%
22	4.532	556	565	577	rBV	176984	517446	18.64%	2.429%
23	4.794	606	608	609	rBV2	2350	1799	0.06%	0.008%
24	4.812	609	611	612	rVB2	2707	1514	0.05%	0.007%
25	4.830	612	614	616	rBV3	2053	1443	0.05%	0.007%
26	4.904	624	626	627	rBV2	3281	2738	0.10%	0.013%
27	4.965	634	636	638	rBV3	2476	1979	0.07%	0.009%
28	5.062	650	652	653	rBV2	2429	2326	0.08%	0.011%
29	5.135	653	664	677	rVV2	378711	1149880	41.41%	5.398%
30	5.251	681	683	684	rBV2	2445	2187	0.08%	0.010%
31	5.855	781	782	784	rBV2	1685	1409	0.05%	0.007%
32	5.903	788	790	795	rVB6	2187	2138	0.08%	0.010%
33	6.044	799	813	827	rBV2	929627	2776634	100.00%	13.034%
34	6.391	867	870	872	rBV4	2147	2490	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092120\
 Data File : VX018521.D
 Acq On : 22 Sep 2020 11:36
 Operator : JC/SP
 Sample : VX0921WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK403

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXMLM092120WMA.M
 Title : VOC Analysis

35	6.409	872	873	877	rVV5	2975	3072	0.11%	0.014%
36	6.659	912	914	920	rBV7	1491	2124	0.08%	0.010%
37	6.830	932	942	957	rBV	762381	1792045	64.54%	8.412%
38	7.123	987	990	991	rBV3	4390	4003	0.14%	0.019%
39	7.171	992	998	1008	rVB4	18328	45898	1.65%	0.215%
40	7.367	1020	1030	1040	rBV	581729	1253459	45.14%	5.884%
41	7.635	1071	1074	1075	rBV3	1719	1900	0.07%	0.009%
42	7.708	1084	1086	1087	rBV2	2716	1749	0.06%	0.008%
43	7.757	1090	1094	1095	rBV3	2712	3864	0.14%	0.018%
44	8.043	1139	1141	1143	rBV3	2062	1601	0.06%	0.008%
45	8.068	1143	1145	1147	rBV3	2296	2436	0.09%	0.011%
46	8.372	1188	1195	1202	rBV	415297	675165	24.32%	3.169%
47	8.696	1241	1248	1255	rBV	1452044	2232236	80.39%	10.479%
48	8.994	1291	1297	1306	rBV	327765	486652	17.53%	2.285%
49	9.262	1339	1341	1343	rVB3	2634	1703	0.06%	0.008%
50	9.366	1356	1358	1359	rBV2	1956	1595	0.06%	0.007%
51	9.427	1362	1368	1382	rVV	842959	1173195	42.25%	5.507%
52	9.616	1396	1399	1402	rBV5	2331	2628	0.09%	0.012%
53	9.689	1410	1411	1413	rVB2	2805	1614	0.06%	0.008%
54	9.738	1413	1419	1422	rBV5	9936	16950	0.61%	0.080%
55	9.945	1449	1453	1454	rBV4	2556	2976	0.11%	0.014%
56	10.092	1472	1477	1485	rBV	1530439	2127964	76.64%	9.989%
57	10.445	1533	1535	1539	rVB5	1758	1642	0.06%	0.008%
58	10.531	1546	1549	1553	rBV6	1842	3767	0.14%	0.018%
59	10.585	1556	1558	1561	rVV4	1923	2221	0.08%	0.010%
60	10.646	1566	1568	1569	rBV2	2009	1594	0.06%	0.007%
61	10.689	1571	1575	1580	rVV8	3366	7280	0.26%	0.034%
62	10.750	1583	1585	1587	rBV3	2307	2012	0.07%	0.009%
63	10.793	1591	1592	1595	rBV3	2258	2622	0.09%	0.012%
64	11.000	1624	1626	1628	rBV3	3319	3842	0.14%	0.018%
65	11.116	1644	1645	1647	rBV2	3016	2743	0.10%	0.013%
66	11.177	1653	1655	1656	rBV2	2470	1507	0.05%	0.007%
67	11.232	1658	1664	1670	rVV	965816	1234872	44.47%	5.797%
68	11.445	1697	1699	1702	rVB4	3631	3551	0.13%	0.017%
69	11.494	1702	1707	1712	rBV9	5571	11068	0.40%	0.052%
70	11.573	1718	1720	1722	rBV3	1506	1569	0.06%	0.007%
71	11.750	1744	1749	1752	rBV7	4535	7570	0.27%	0.036%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092120\
 Data File : VX018521.D
 Acq On : 22 Sep 2020 11:36
 Operator : JC/SP
 Sample : VX0921WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK403

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM092120WMA.M
 Title : VOC Analysis

72	11.786	1752	1755	1759	rBV5	3705	6095	0.22%	0.029%
73	11.860	1764	1767	1768	rBV3	3121	3048	0.11%	0.014%
74	11.951	1779	1782	1785	rBV4	4015	6129	0.22%	0.029%
75	12.061	1795	1800	1806	rBV	1545389	1917081	69.04%	8.999%
76	12.219	1824	1826	1827	rBV2	2147	1393	0.05%	0.007%
77	12.360	1844	1849	1856	rVB	1605814	1955903	70.44%	9.182%
78	12.542	1877	1879	1882	rBV3	2603	2112	0.08%	0.010%
79	12.683	1900	1902	1904	rVB3	2455	2054	0.07%	0.010%
80	12.713	1904	1907	1908	rBV3	1828	1451	0.05%	0.007%
81	12.829	1925	1926	1929	rBV3	2036	2612	0.09%	0.012%
82	12.933	1940	1943	1945	rBV4	2739	2737	0.10%	0.013%
83	12.994	1949	1953	1954	rVB4	2276	2451	0.09%	0.012%
84	13.079	1965	1967	1968	rBV2	2318	2197	0.08%	0.010%
85	13.115	1972	1973	1976	rVV3	1752	1683	0.06%	0.008%
86	13.158	1976	1980	1984	rVB5	6646	8727	0.31%	0.041%
87	13.189	1984	1985	1988	rBV3	1522	1607	0.06%	0.008%
88	13.250	1993	1995	1996	rBV2	2757	2180	0.08%	0.010%
89	13.628	2054	2057	2063	rVB8	8792	12462	0.45%	0.059%
90	13.695	2066	2068	2071	rBV4	1923	1469	0.05%	0.007%
91	13.817	2086	2088	2092	rVB2	5994	5766	0.21%	0.027%
92	14.170	2144	2146	2148	rVB3	3383	2113	0.08%	0.010%
93	14.225	2153	2155	2158	rVB4	3034	2577	0.09%	0.012%
94	14.256	2158	2160	2162	rBV3	3286	3677	0.13%	0.017%
95	14.505	2199	2201	2203	rBV3	3004	2669	0.10%	0.013%
96	14.536	2203	2206	2208	rVV4	2347	3024	0.11%	0.014%
97	14.646	2223	2224	2226	rBV2	2048	1535	0.06%	0.007%
98	15.694	2394	2396	2398	rBV3	2848	2737	0.10%	0.013%
99	16.066	2455	2457	2458	rBV2	3344	2262	0.08%	0.011%
100	16.298	2493	2495	2496	rBV2	2492	1653	0.06%	0.008%


Sum of corrected areas: 21302300

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX092120\
Data File : VX018521.D
Acq On : 22 Sep 2020 11:36
Operator : JC/SP
Sample : VX0921WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK403

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM092120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

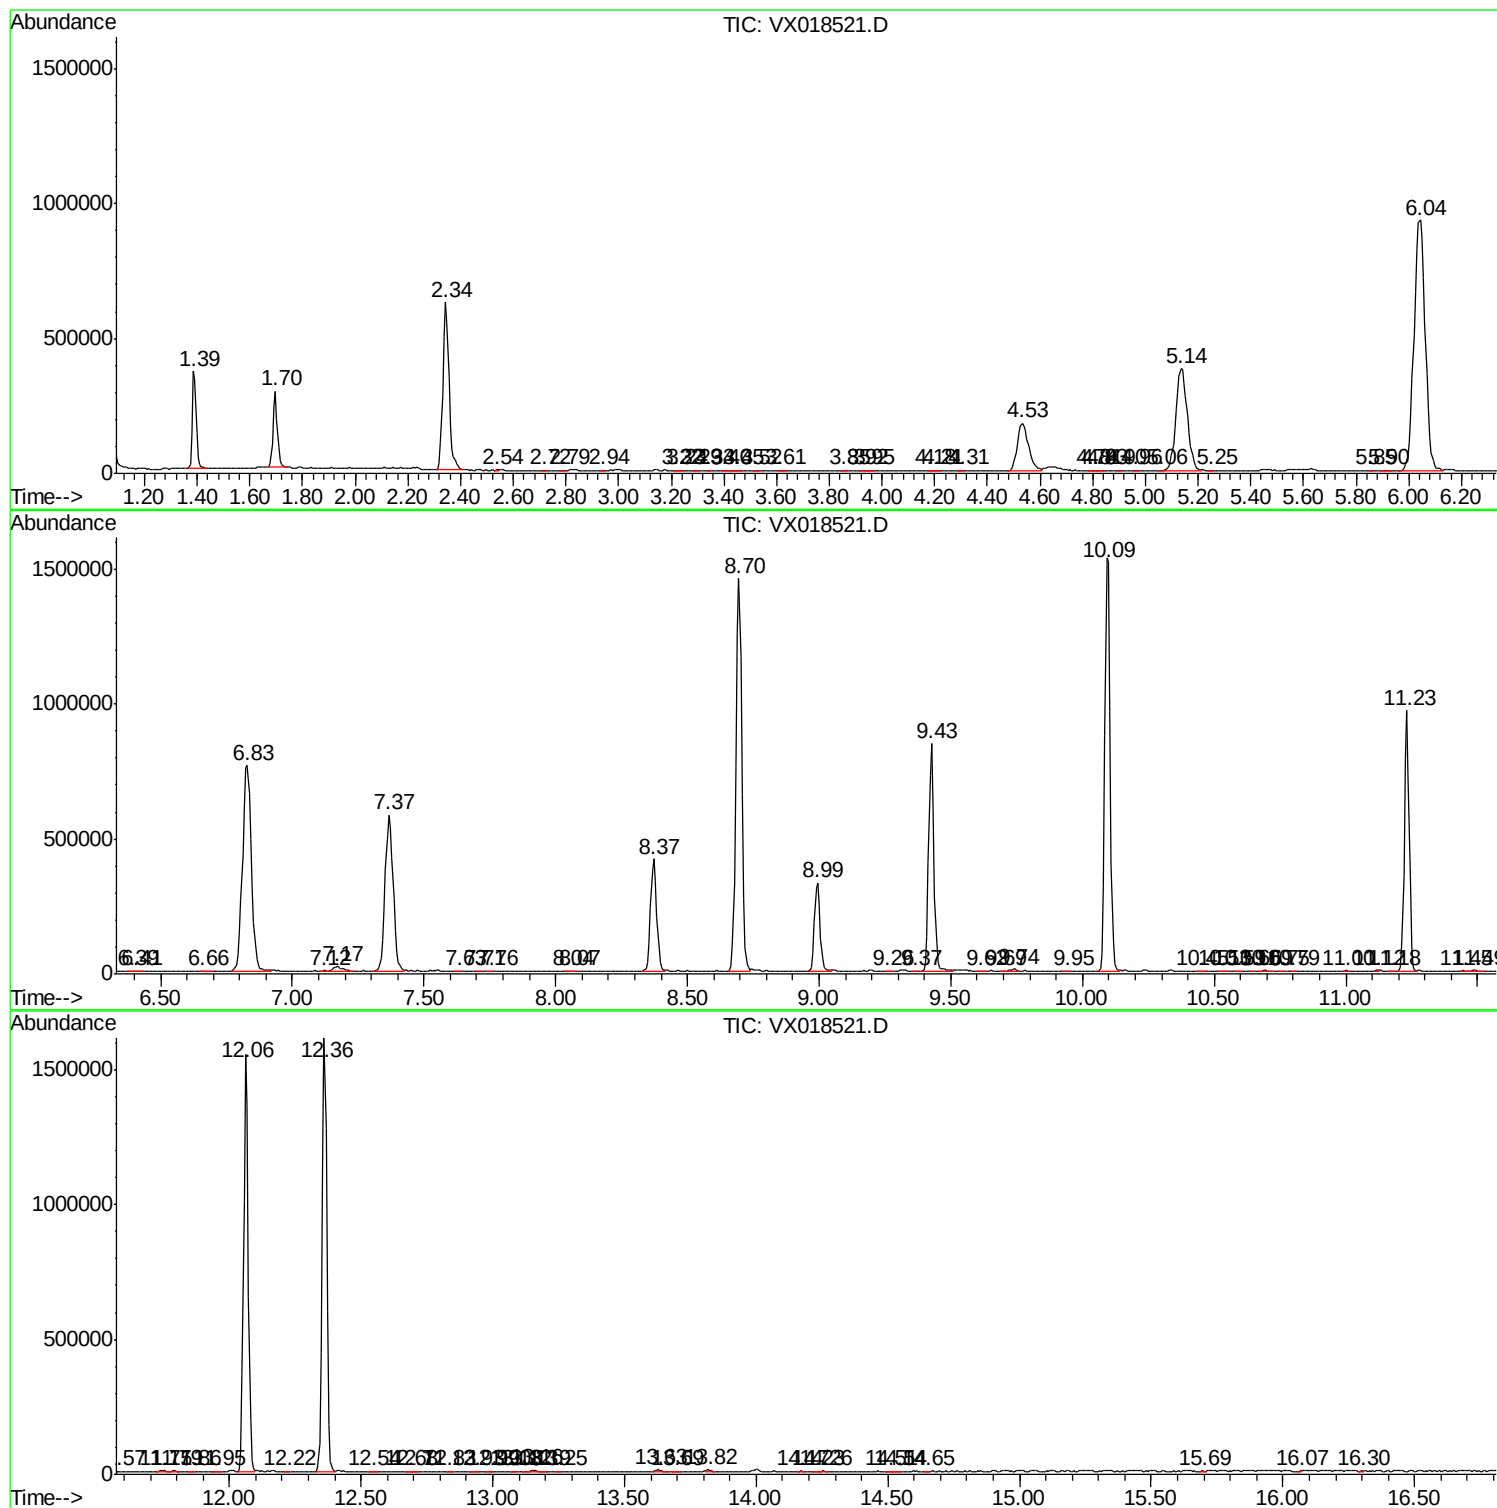

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX092120\
Data File : VX018521.D
Acq On : 22 Sep 2020 11:36
Operator : JC/SP
Sample : VX0921WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK403

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM092120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX092120\
Data File : VX018521.D
Acq On : 22 Sep 2020 11:36
Operator : JC/SP
Sample : VX0921WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK403

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM092120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc