


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX092120\
 Data File : VX018507.D
 Acq On : 21 Sep 2020 09:55
 Operator : JC/SP
 Sample : BFB401
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB401

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Oct 01 17:22:05 2020

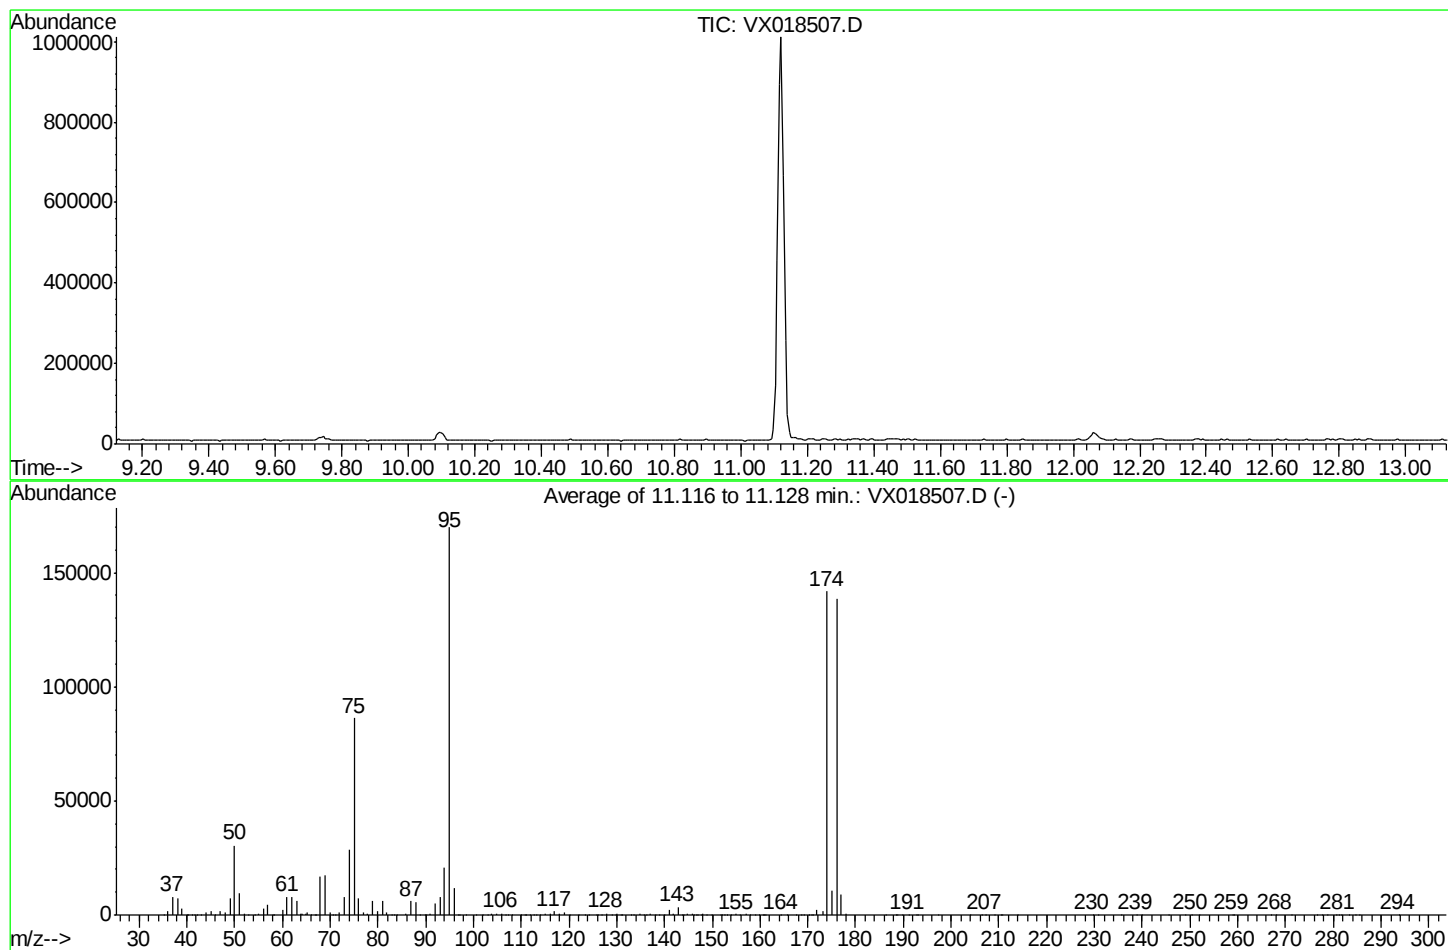

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	30492	PASS
75	95	30	80	50.7	86115	PASS
95	95	100	100	100.0	169834	PASS
96	95	5	9	6.8	11554	PASS
173	174	0.00	2	1.3	1818	PASS
174	95	50	120	83.5	141781	PASS
175	174	5	9	7.6	10798	PASS
176	174	95	101	97.6	138360	PASS
177	176	5	9	6.6	9175	PASS

m/z	Abundance
36.00	2224.0
37.00	10176.0
38.10	8448.0
39.00	4054.0
39.80	383.0
40.20	412.0
41.20	128.0
41.70	212.0
42.10	142.0
42.90	162.0
44.00	1692.0
45.00	1813.0
46.00	473.0
47.00	1756.0
47.90	1150.0
49.10	7528.0
50.00	33664.0
51.00	11113.0
52.10	602.0
52.90	287.0
53.60	113.0
54.20	221.0
55.10	515.0
56.10	2921.0
57.00	5214.0
58.00	327.0
58.80	127.0
60.00	2235.0
61.00	9060.0
62.00	9357.0
63.00	7902.0
64.00	1169.0
64.90	1754.0
65.90	277.0
66.80	399.0
68.00	18816.0
69.00	19248.0
70.00	1384.0
70.70	369.0
71.20	176.0
72.00	1308.0
73.00	8103.0
74.00	31152.0
75.00	94136.0
76.10	7819.0
77.20	1153.0
77.90	795.0
78.90	6764.0
80.00	1806.0
80.90	6961.0
81.90	1447.0
82.90	321.0
83.90	82.0
85.30	85.0
86.00	219.0
87.00	7376.0
88.00	6373.0
88.90	256.0
89.90	194.0
90.90	984.0
92.10	5791.0
93.00	8280.0
94.00	22944.0
95.00	188928.0
96.00	12636.0
96.90	202.0
101.70	71.0
102.00	66.0
102.90	177.0
104.00	720.0
104.90	379.0
106.00	628.0
106.70	241.0
108.20	56.0
109.80	194.0
111.10	371.0
112.00	315.0
112.60	229.0
113.20	131.0
115.10	442.0
115.90	759.0
117.10	1578.0
117.90	816.0
119.00	1483.0
123.30	89.0
124.10	160.0
125.80	134.0
126.70	147.0
127.90	745.0
128.90	205.0
129.90	744.0
130.80	264.0

Instrument :
MSVOA_X
ClientSampleId :
BFB401

133.10	59.0
134.80	338.0
136.10	86.0
136.90	494.0
138.00	209.0
139.90	122.0
140.90	2215.0
141.90	368.0
142.90	4054.0
143.80	200.0
144.80	753.0
145.90	467.0
146.70	124.0
147.20	176.0
148.00	599.0
148.90	100.0
150.00	260.0
151.90	120.0
154.00	219.0
155.00	520.0
157.10	265.0
158.00	72.0
159.00	250.0
160.70	120.0
169.30	131.0
170.60	332.0
171.10	286.0
171.90	2275.0
173.10	1537.0
174.00	133568.0
175.00	9865.0
176.00	126544.0
177.00	9744.0
178.10	450.0
186.30	67.0
188.70	60.0
191.00	120.0
192.80	103.0
193.10	94.0
197.20	82.0
207.20	233.0
208.00	58.0
238.80	59.0
239.90	68.0
276.50	56.0
277.60	56.0
281.20	197.0
285.50	146.0

Instrument :
MSVOA_X
ClientSampleId :
BFB401

m/z	Abundance
35.30	222.0
35.80	1619.0
37.00	8607.0
38.00	8689.0
39.10	3767.0
39.90	793.0
41.00	247.0
41.50	221.0
41.80	258.0
43.00	307.0
43.90	2300.0
45.00	2133.0
46.10	252.0
47.00	1878.0
48.00	1204.0
49.00	8246.0
50.00	37104.0
51.00	10758.0
52.00	675.0
53.00	187.0
55.00	415.0
56.00	3289.0
57.00	5144.0
57.90	189.0
58.20	192.0
60.00	2605.0
61.00	9445.0
62.00	9815.0
63.00	7088.0
64.20	953.0
65.10	1716.0
66.00	291.0
67.10	677.0
68.00	20312.0
69.00	20928.0
70.00	2017.0
71.00	157.0
72.00	1267.0
73.00	9080.0
74.00	35432.0
75.00	104056.0
76.00	8443.0
77.00	1112.0
77.90	833.0
78.90	6649.0
79.90	2038.0
80.90	7373.0
81.80	1841.0
83.40	135.0
83.90	99.0
84.60	157.0
85.10	66.0
85.90	438.0
86.90	7290.0
87.90	7199.0
88.80	283.0
90.10	194.0
90.80	839.0
92.00	6615.0
93.00	9191.0
94.00	24008.0
95.00	195072.0
96.00	13545.0
97.10	418.0
98.30	64.0
102.90	240.0
103.80	928.0
104.80	538.0
105.90	1192.0
107.20	184.0
109.90	272.0
110.80	330.0
111.80	194.0
112.60	122.0
113.10	479.0
113.90	58.0
114.90	261.0
116.00	744.0
116.90	1622.0
118.00	869.0
119.00	1221.0
122.00	72.0
123.40	56.0
124.10	182.0
125.80	188.0
126.90	89.0
127.90	1182.0
129.00	355.0
129.90	542.0
130.10	551.0
130.80	283.0
132.90	125.0

Instrument :
MSVOA_X
ClientSampleId :
BFB401

134.70	448.0
136.10	65.0
137.00	629.0
139.00	182.0
140.00	269.0
140.90	2640.0
142.00	414.0
142.90	4126.0
144.00	350.0
144.90	727.0
146.00	421.0
147.00	133.0
148.10	611.0
148.90	59.0
149.90	508.0
151.80	78.0
152.50	81.0
153.00	153.0
153.90	181.0
155.00	730.0
155.70	50.0
157.00	490.0
158.80	275.0
159.80	53.0
160.90	470.0
164.40	68.0
167.60	53.0
168.60	59.0
169.30	168.0
170.30	221.0
170.70	278.0
171.90	2574.0
172.90	1787.0
174.00	166784.0
175.00	13086.0
176.00	168448.0
177.00	10282.0
177.90	338.0
186.30	69.0
188.30	107.0
189.90	64.0
191.00	151.0
193.10	128.0
206.50	175.0
207.10	226.0
208.00	118.0
213.80	62.0
221.30	141.0
238.70	67.0
245.50	61.0
248.90	64.0
252.00	61.0
268.00	95.0
278.70	61.0
281.00	310.0
284.70	54.0
293.70	69.0

Instrument :
MSVOA_X
ClientSampleId :
BFB401

m/z	Abundance
35.30	362.0
36.00	1463.0
37.00	5269.0
38.00	4940.0
38.90	1900.0
40.00	417.0
41.10	192.0
42.20	254.0
43.00	134.0
44.10	1146.0
44.90	948.0
45.90	611.0
47.00	1585.0
48.10	997.0
49.10	5423.0
50.00	21152.0
51.10	7090.0
51.90	307.0
53.10	263.0
54.10	117.0
54.90	418.0
56.00	1933.0
56.90	3534.0
57.80	272.0
59.20	113.0
59.90	1402.0
61.00	5656.0
62.10	4883.0
63.00	4143.0
63.90	783.0
65.10	1561.0
66.10	157.0
66.70	271.0
67.20	265.0
68.00	11894.0
69.00	12230.0
70.00	894.0
71.00	256.0
72.10	660.0
73.00	6498.0
74.00	20176.0
75.00	60560.0
76.10	5990.0
76.90	679.0
77.80	677.0
78.90	4840.0
79.90	1529.0
80.90	3663.0
81.90	1364.0
82.90	148.0
84.60	124.0
85.80	292.0
87.00	3683.0
88.00	4037.0
89.80	133.0
90.80	630.0
92.00	3368.0
93.00	5578.0
94.00	15170.0
95.00	125504.0
96.00	8483.0
97.00	324.0
100.60	100.0
101.10	99.0
103.00	97.0
103.90	612.0
104.90	398.0
105.80	711.0
106.70	251.0
107.20	351.0
108.00	60.0
109.90	180.0
111.10	178.0
112.30	158.0
113.00	206.0
113.90	92.0
114.90	212.0
116.10	475.0
117.00	1239.0
117.90	817.0
119.00	864.0
120.10	77.0
122.00	70.0
124.30	164.0
126.00	197.0
127.00	54.0
127.90	617.0
129.10	331.0
130.00	898.0
131.10	284.0
132.90	114.0
133.60	74.0

Instrument :
MSVOA_X
ClientSampleId :
BFB401

134.80	522.0
135.70	124.0
136.90	407.0
138.80	187.0
139.90	152.0
140.80	1465.0
142.00	463.0
143.00	2410.0
143.90	150.0
145.00	627.0
145.90	336.0
146.20	330.0
146.90	133.0
147.80	459.0
148.80	234.0
149.90	129.0
152.10	56.0
153.10	119.0
153.80	363.0
155.00	499.0
155.80	59.0
157.00	370.0
159.00	262.0
161.10	268.0
164.30	52.0
165.80	82.0
167.50	63.0
169.30	67.0
170.80	362.0
171.90	2141.0
173.10	2130.0
174.00	124992.0
175.00	9444.0
176.00	120088.0
177.00	7500.0
178.00	370.0
188.40	59.0
203.90	108.0
207.10	408.0
208.00	87.0
209.20	116.0
210.30	104.0
210.80	65.0
221.30	53.0
229.70	89.0
230.70	62.0
235.70	92.0
250.20	73.0
258.80	97.0
259.30	74.0
267.00	63.0
267.90	64.0
271.20	64.0
278.80	73.0
280.70	75.0
281.10	259.0
281.60	101.0
283.30	110.0
293.70	69.0

Instrument :
MSVOA_X
ClientSampleId :
BFB401

m/z	Abundance
35.30	148.0
35.90	155.0
37.80	294.0
39.00	348.0
39.90	449.0
41.40	196.0
41.90	95.0
42.60	171.0
43.90	816.0
45.00	145.0
45.80	156.0
46.70	105.0
47.30	109.0
48.30	110.0
49.80	148.0
50.70	124.0
51.50	119.0
52.30	125.0
53.30	92.0
53.80	107.0
55.70	192.0
57.10	87.0
58.80	96.0
59.40	120.0
60.20	64.0
60.70	86.0
61.50	65.0
63.10	116.0
64.70	73.0
65.30	120.0
67.20	104.0
70.20	78.0
72.30	68.0
73.00	265.0
74.10	92.0
75.00	135.0
75.50	94.0
76.00	55.0
76.50	103.0
78.10	126.0
78.80	56.0
79.30	99.0
81.70	188.0
82.50	111.0
84.50	101.0
85.20	137.0
88.40	57.0
94.70	118.0
101.10	51.0
101.70	118.0
102.60	70.0
111.50	104.0
112.20	74.0
118.00	94.0
118.70	60.0
124.50	84.0
127.10	67.0
129.80	147.0
130.30	55.0
143.80	58.0
148.10	52.0
149.60	103.0
150.80	62.0
153.10	67.0
155.10	78.0
156.10	56.0
169.20	60.0
170.80	63.0
206.80	136.0
208.00	120.0
218.60	59.0
220.00	96.0
221.20	125.0
249.20	60.0
270.30	89.0
281.20	115.0
288.10	98.0
292.80	64.0

Instrument :
MSVOA_X
ClientSampleId :
BFB401