


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX092120\
 Data File : VX018519.D
 Acq On : 22 Sep 2020 09:55
 Operator : JC/SP
 Sample : BFB402
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB402

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Oct 01 17:22:05 2020

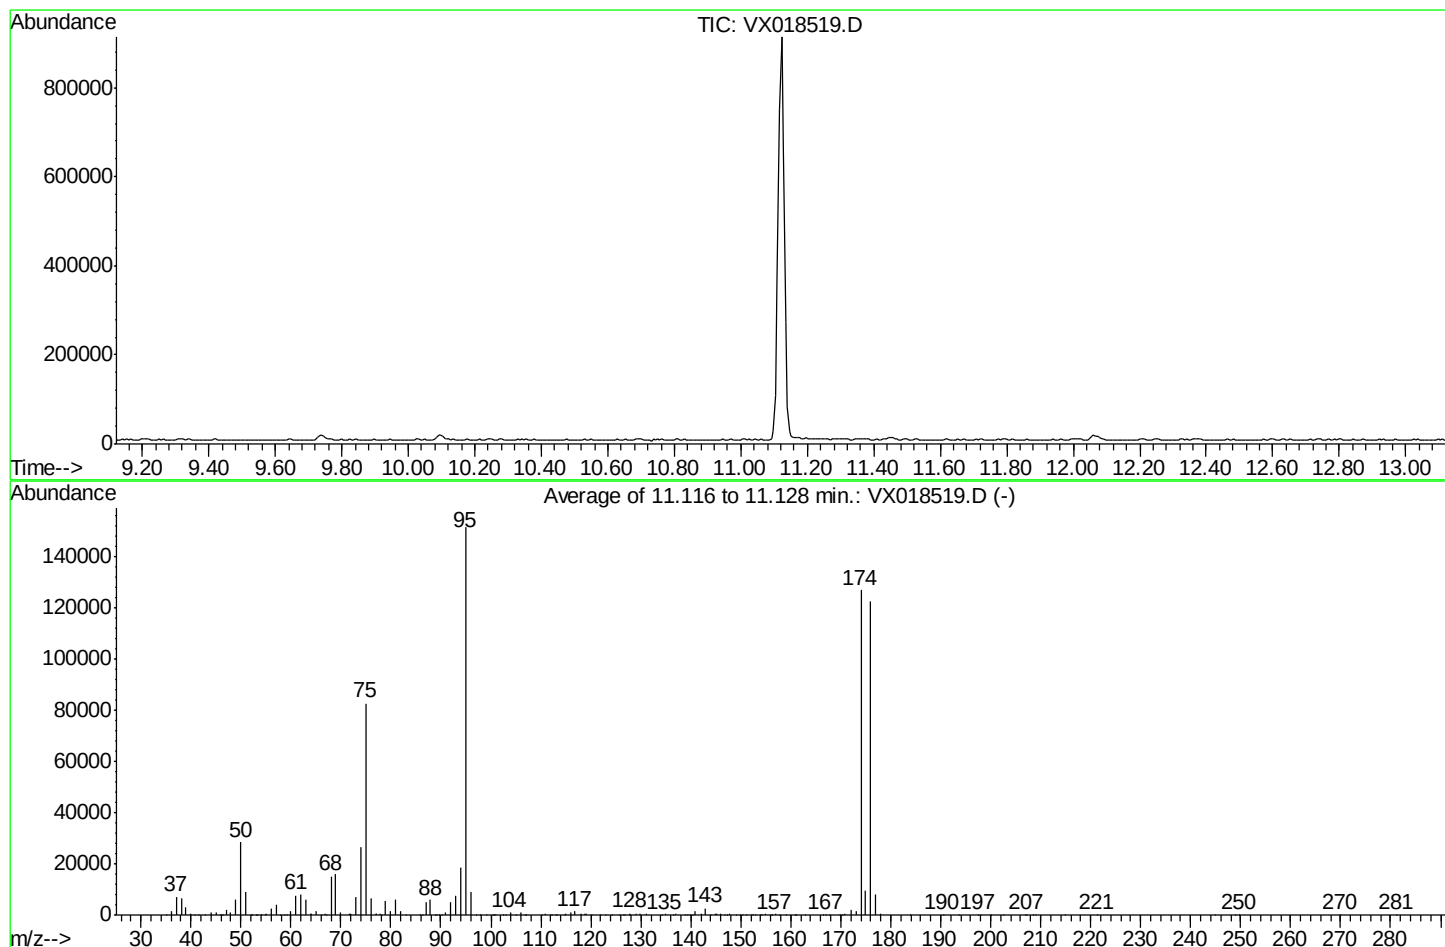

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	28450	PASS
75	95	30	80	54.5	82650	PASS
95	95	100	100	100.0	151517	PASS
96	95	5	9	6.1	9170	PASS
173	174	0.00	2	1.4	1744	PASS
174	95	50	120	83.8	126909	PASS
175	174	5	9	7.6	9624	PASS
176	174	95	101	96.8	122789	PASS
177	176	5	9	6.4	7826	PASS

m/z	Abundance
35.10	189.0
36.00	1664.0
37.00	8629.0
38.10	6695.0
39.00	3706.0
40.10	609.0
40.60	213.0
41.40	138.0
42.80	221.0
43.90	1672.0
44.90	1147.0
47.00	1323.0
48.00	1195.0
49.00	7570.0
50.00	30992.0
51.00	10178.0
52.10	581.0
52.90	171.0
53.30	286.0
53.90	60.0
54.80	670.0
56.00	3212.0
57.00	3892.0
58.00	279.0
58.70	114.0
59.20	110.0
60.00	1891.0
61.00	8401.0
62.00	8155.0
63.00	7233.0
63.90	1337.0
64.90	1571.0
66.00	269.0
66.90	561.0
68.00	14803.0
69.00	17376.0
70.00	978.0
70.90	174.0
72.00	1022.0
73.00	6688.0
74.00	27872.0
75.00	84952.0
76.10	6126.0
77.00	1083.0
77.90	881.0
78.90	5589.0
80.00	1398.0
81.00	5700.0
81.90	1558.0
83.10	189.0
85.90	324.0
86.90	4871.0
88.00	6115.0
90.10	170.0
90.90	746.0
92.10	4993.0
93.00	7952.0
94.00	19088.0
95.00	153152.0
96.00	10283.0
97.90	52.0
100.60	188.0
102.40	97.0
103.10	152.0
104.00	948.0
104.90	148.0
105.80	812.0
106.80	229.0
110.00	261.0
110.90	279.0
111.90	237.0
112.80	171.0
113.30	56.0
115.10	373.0
115.90	770.0
116.80	936.0
118.00	940.0
118.80	1133.0
122.90	97.0
124.30	195.0
126.80	152.0
127.70	455.0
129.10	295.0
129.90	464.0
131.00	202.0
134.00	54.0
134.80	364.0
136.90	416.0
140.20	221.0
141.00	1559.0
142.00	399.0
142.90	2743.0

Instrument :
MSVOA_X
ClientSampleId :
BFB402

144.00	216.0
144.90	833.0
145.90	448.0
147.10	102.0
147.80	519.0
149.00	123.0
149.80	151.0
151.20	87.0
152.00	144.0
152.80	170.0
153.80	203.0
154.90	488.0
157.00	462.0
157.80	61.0
158.90	340.0
160.90	160.0
166.50	92.0
169.70	100.0
170.40	176.0
171.00	685.0
171.90	2069.0
173.00	1256.0
174.00	107472.0
175.00	8450.0
176.00	103256.0
177.00	6849.0
178.00	417.0
183.80	56.0
190.50	74.0
191.00	53.0
197.60	71.0
198.00	59.0
206.80	68.0
214.90	55.0
248.90	50.0
281.00	130.0

Instrument :
MSVOA_X
ClientSampleId :
BFB402

m/z	Abundance
36.00	1734.0
37.00	7868.0
38.00	8284.0
39.00	3277.0
39.90	509.0
41.10	252.0
41.60	84.0
42.20	194.0
42.90	179.0
44.00	2150.0
45.00	1476.0
45.80	222.0
46.30	220.0
47.00	2610.0
48.00	1477.0
49.00	6931.0
50.00	33032.0
51.00	10714.0
51.90	630.0
52.30	400.0
53.00	459.0
54.10	199.0
55.10	756.0
56.00	2923.0
57.00	4881.0
58.00	215.0
59.10	172.0
60.00	2056.0
61.00	8717.0
62.00	9352.0
63.10	6895.0
64.10	1111.0
65.00	1898.0
65.80	95.0
67.00	668.0
68.00	18832.0
69.00	18664.0
70.00	1534.0
71.10	118.0
72.10	1052.0
73.00	9268.0
74.00	31720.0
75.00	96584.0
76.00	8906.0
77.20	1362.0
77.90	747.0
78.90	7357.0
79.90	1934.0
80.90	7023.0
82.00	1528.0
83.00	106.0
85.90	484.0
86.90	6078.0
87.90	6212.0
88.90	274.0
89.70	113.0
91.00	799.0
92.00	5938.0
93.00	7962.0
94.00	22904.0
95.00	176000.0
96.00	10312.0
97.00	342.0
97.90	82.0
100.30	158.0
100.70	95.0
102.40	128.0
103.00	86.0
104.00	904.0
104.90	292.0
105.90	914.0
107.00	227.0
110.00	180.0
110.80	296.0
111.90	416.0
112.80	319.0
114.90	404.0
116.00	1377.0
116.90	1711.0
117.90	687.0
119.00	1192.0
120.00	75.0
121.80	75.0
122.80	88.0
124.10	327.0
126.00	79.0
126.70	121.0
127.90	1171.0
128.90	638.0
129.80	542.0
131.00	397.0
134.10	51.0

Instrument :
MSVOA_X
ClientSampleId :
BFB402

134.90	343.0
137.00	569.0
138.80	148.0
139.70	215.0
140.20	298.0
141.10	1921.0
141.90	340.0
142.90	2979.0
145.10	817.0
146.00	321.0
147.20	118.0
147.70	419.0
149.10	150.0
149.70	172.0
150.20	84.0
151.00	71.0
152.10	264.0
152.80	124.0
154.20	98.0
154.80	493.0
155.90	101.0
156.90	444.0
157.80	108.0
158.90	367.0
161.10	464.0
167.00	58.0
167.80	57.0
170.80	421.0
172.00	1914.0
173.10	2019.0
174.00	151424.0
175.00	11835.0
176.00	144832.0
177.10	8672.0
177.80	335.0
190.40	57.0
193.70	65.0
197.50	79.0
202.60	91.0
207.20	335.0
208.40	84.0
209.00	67.0
209.30	102.0
221.30	70.0
244.80	69.0
249.70	81.0
269.90	105.0

Instrument :
MSVOA_X
ClientSampleId :
BFB402

m/z	Abundance
35.90	1026.0
37.00	5220.0
38.00	4228.0
39.00	2249.0
40.00	483.0
41.20	191.0
42.10	93.0
42.70	210.0
44.00	1557.0
44.90	1112.0
46.00	405.0
47.00	1700.0
47.80	875.0
49.00	4372.0
50.00	21328.0
51.00	6133.0
52.40	194.0
53.30	271.0
54.10	139.0
55.10	242.0
56.10	1791.0
57.00	3582.0
57.90	431.0
58.60	344.0
59.90	1186.0
61.00	5933.0
62.00	6564.0
63.00	4307.0
63.90	848.0
65.10	1443.0
65.90	334.0
67.20	357.0
68.00	11580.0
69.00	12756.0
70.10	757.0
70.90	77.0
71.80	967.0
73.00	5916.0
74.00	19872.0
75.00	66416.0
76.10	4326.0
77.10	918.0
78.10	335.0
78.80	4385.0
79.90	1383.0
80.90	4824.0
81.90	1148.0
83.00	213.0
86.20	533.0
87.00	4631.0
88.00	5070.0
89.20	76.0
89.70	106.0
91.00	851.0
92.00	4292.0
93.00	6052.0
94.00	14494.0
95.00	125400.0
96.00	7139.0
97.10	280.0
97.90	57.0
99.00	67.0
100.20	69.0
100.90	53.0
103.90	732.0
104.80	126.0
106.00	813.0
106.90	164.0
110.80	267.0
112.10	78.0
112.80	221.0
114.70	173.0
115.10	257.0
115.80	676.0
116.80	1406.0
117.90	463.0
118.90	1046.0
122.70	101.0
124.00	128.0
125.80	183.0
126.50	99.0
127.90	646.0
128.90	458.0
129.80	556.0
131.00	405.0
133.00	66.0
134.80	445.0
136.60	159.0
137.10	284.0
139.20	81.0
139.80	134.0
140.90	1902.0

Instrument :
MSVOA_X
ClientSampleId :
BFB402

142.10	196.0
143.00	1879.0
145.10	708.0
145.80	293.0
146.80	83.0
147.90	387.0
148.90	189.0
150.20	167.0
151.00	71.0
152.40	130.0
152.80	154.0
154.90	274.0
156.10	108.0
156.80	494.0
157.80	156.0
158.70	94.0
161.20	522.0
162.90	101.0
167.00	114.0
170.90	366.0
171.90	2409.0
173.10	1958.0
174.00	121832.0
175.00	8587.0
176.00	120280.0
176.90	8230.0
178.00	470.0
193.70	52.0
199.90	82.0
202.60	84.0
206.90	347.0
207.30	225.0
208.90	74.0
221.30	76.0
249.80	95.0
281.20	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB402

m/z	Abundance
35.70	164.0
36.50	129.0
37.50	164.0
38.60	225.0
39.20	135.0
40.00	254.0
41.00	167.0
41.60	185.0
42.30	201.0
43.10	110.0
44.10	860.0
45.30	293.0
46.70	89.0
47.40	166.0
48.10	137.0
48.90	161.0
49.70	106.0
50.60	119.0
51.90	137.0
53.50	184.0
55.70	105.0
56.20	106.0
56.60	135.0
57.40	172.0
57.90	119.0
58.50	86.0
59.40	147.0
60.30	121.0
60.80	64.0
63.90	216.0
64.50	102.0
65.30	207.0
66.70	63.0
69.90	147.0
70.80	92.0
71.30	103.0
72.20	97.0
72.90	261.0
78.70	52.0
82.00	79.0
82.60	95.0
85.30	98.0
88.70	72.0
92.00	115.0
92.70	82.0
94.00	129.0
95.90	74.0
103.30	119.0
109.10	59.0
109.60	93.0
110.00	81.0
115.30	59.0
122.80	77.0
127.60	73.0
129.10	82.0
132.80	61.0
133.70	64.0
140.90	57.0
141.60	53.0
147.40	120.0
148.60	64.0
161.20	81.0
172.20	129.0
176.80	91.0
188.10	51.0
190.90	51.0
209.30	122.0
224.90	137.0
258.20	58.0
266.30	50.0
269.40	85.0
271.80	50.0
280.20	79.0
280.90	128.0
282.90	129.0
286.20	72.0

Instrument :
MSVOA_X
ClientSampleId :
BFB402