

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
 Data File : VX024387.D
 Acq On : 21 Sep 2021 15:38
 Operator : JC/MD
 Sample : M3782-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP05-20210915

Quant Time: Sep 21 16:40:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 21 10:52:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	151724	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	244703	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	240156	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	111646	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	102845	47.536	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	95.080%
35) Dibromofluoromethane	5.403	113	88424	53.881	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	107.760%
50) Toluene-d8	8.653	98	333906	55.852	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	111.700%
62) 4-Bromofluorobenzene	11.085	95	127112	54.635	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	109.260%
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.172	85	839	0.575	ug/l	97
3) Chloromethane	1.294	50	511	0.336	ug/l	97
5) Bromomethane	1.618	94	557	0.617	ug/l #	69
7) Trichlorofluoromethane	1.892	101	1177	0.463	ug/l #	78
9) 1,1,2-Trichlorotrifluo...	2.331	101	58504	39.167	ug/l	98
10) Methyl Iodide	2.465	142	961	0.465	ug/l #	97
11) Tert butyl alcohol	2.971	59	50	Below Cal	#	73
12) 1,1-Dichloroethene	2.325	96	33463	23.920	ug/l	99
16) Acetone	2.392	43	2431	2.635	ug/l #	74
20) Methylene Chloride	2.800	84	696	0.393	ug/l #	82
24) 1,1-Dichloroethane	3.617	63	6821	2.328	ug/l #	92
27) cis-1,2-Dichloroethene	4.507	96	6057	3.424	ug/l	90
29) Tetrahydrofuran	5.044	42	248	0.292	ug/l #	27
30) Chloroform	5.111	83	2791	0.896	ug/l #	73
31) Cyclohexane	5.568	56	3420	1.351	ug/l #	14
32) 1,1,1-Trichloroethane	5.403	97	6239	2.237	ug/l	97
36) 1,1-Dichloropropene	5.562	75	11925	5.300	ug/l #	49
38) Carbon Tetrachloride	5.690	117	4817	1.902	ug/l	92
39) Methylcyclohexane	7.135	83	8518	3.171	ug/l #	1
42) 1,2-Dichloroethane	6.105	62	1283	0.477	ug/l #	73
44) Trichloroethene	7.135	130	680594	375.394	ug/l	100
49) 1,4-Dioxane	7.671	88	772	17.708	ug/l #	31
51) 4-Methyl-2-Pentanone	8.653	43	1570	0.590	ug/l #	1
55) 1,1,2-Trichloroethane	9.159	97	1895	1.052	ug/l #	81
60) Dibromochloromethane	9.275	129	467	1.947	ug/l #	11
64) Tetrachloroethene	9.281	164	544	0.292	ug/l	92
76) 1,2,3-Trichloropropane	11.085	75	64450	25.105	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	64450	73.835	ug/l #	12
95) Naphthalene	13.780	128	181	1.309	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024387.D
Acq On : 21 Sep 2021 15:38
Operator : JC/MD
Sample : M3782-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP05-20210915

Quant Time: Sep 21 16:40:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 21 10:52:48 2021
Response via : Initial Calibration




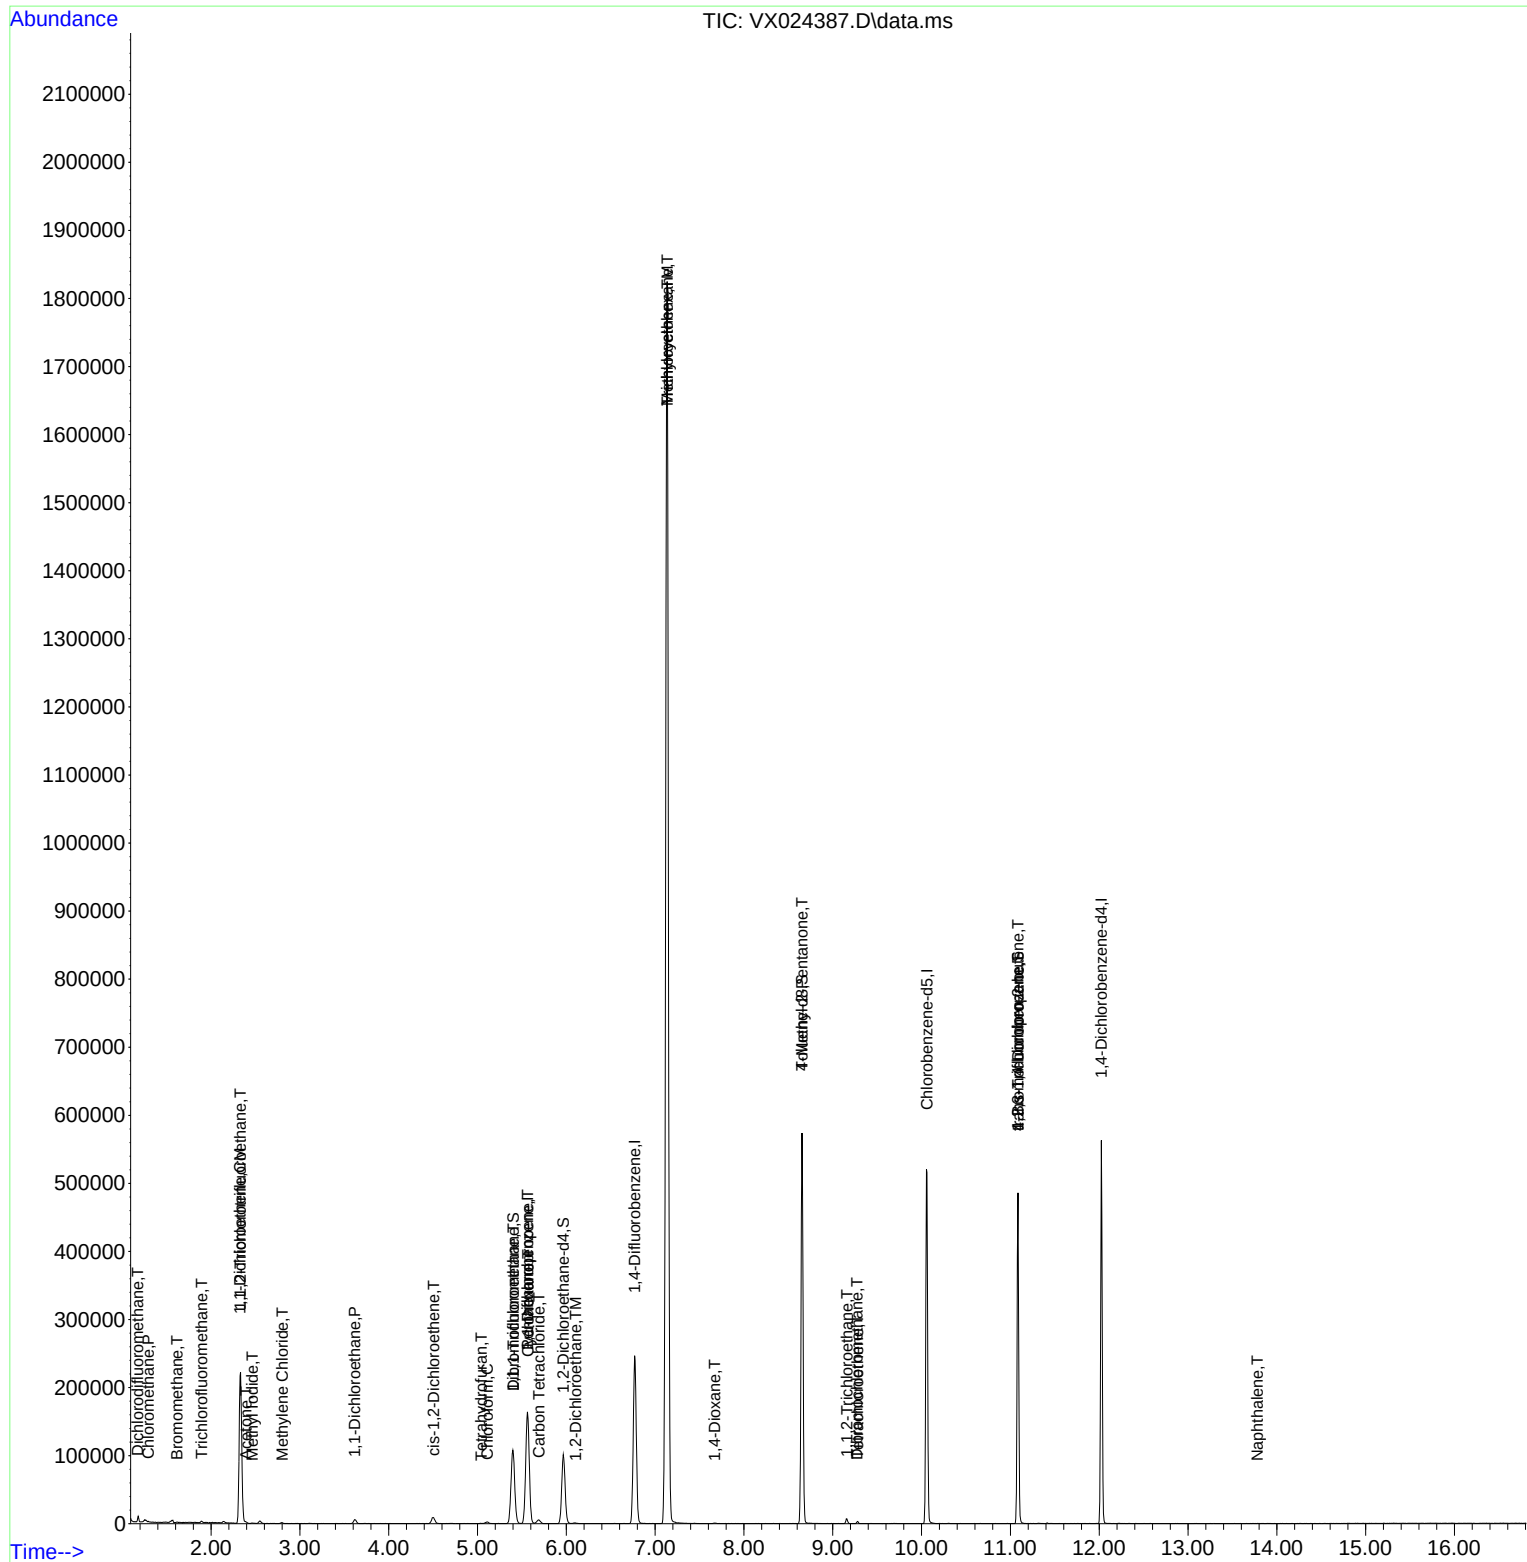


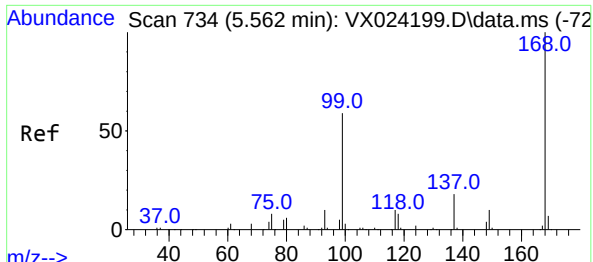

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38




Instrument :
MSVOA_X
ClientSampleId :
DUP05-20210915

Tgt Ion:168 Resp: 151724
Ion Ratio Lower Upper
168 100
99 64.3 45.8 68.6



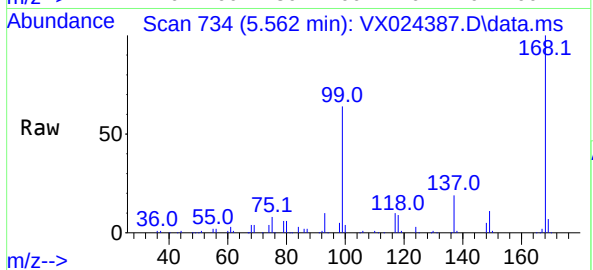


#2
Dichlorodifluoromethane
Concen: 0.575 ug/l
RT: 1.172 min Scan# 14
Delta R.T. -0.001 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38

Tgt Ion: 85 Resp: 839
Ion Ratio Lower Upper
85 100
87 31.0 16.4 49.2

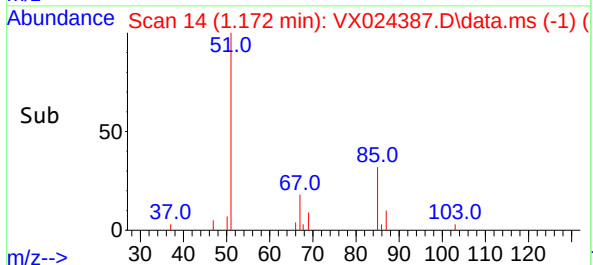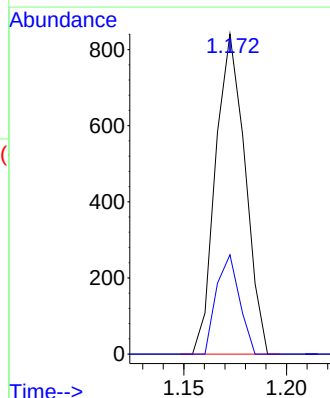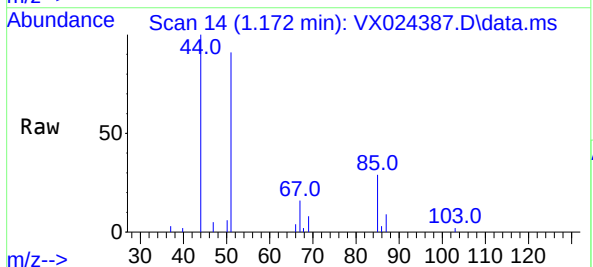

Abundance Scan 34 (1.295 min): VX024199.D\data.ms (-30)

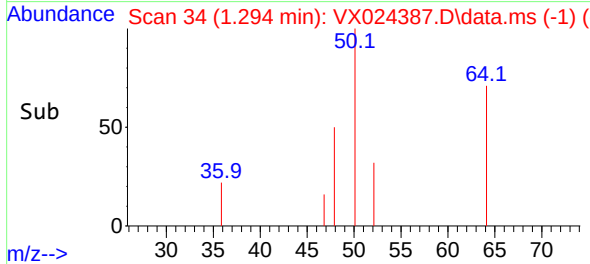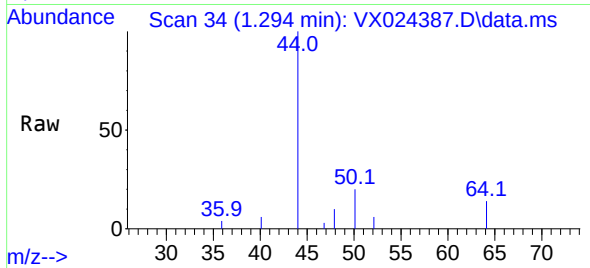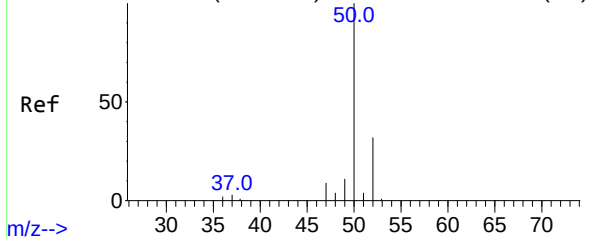

#3

Chloromethane

Concen: 0.336 ug/l

RT: 1.294 min Scan# 34


Delta R.T. -0.001 min

Lab File: VX024387.D




Acq: 21 Sep 2021 15:38

Tgt Ion: 50 Resp: 511

Ion	Ratio	Lower	Upper
50	100		
52	31.5	26.4	39.6

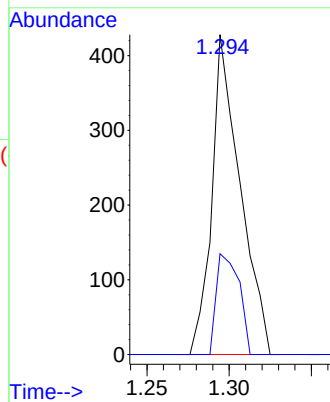

Abundance Scan 84 (1.599 min): VX024199.D\data.ms (-78)

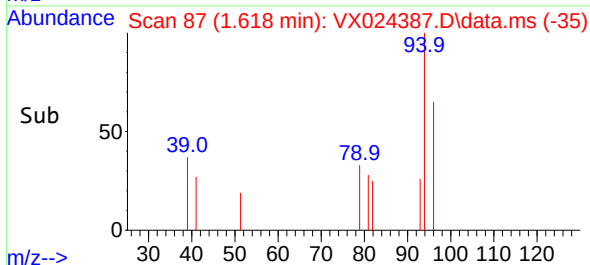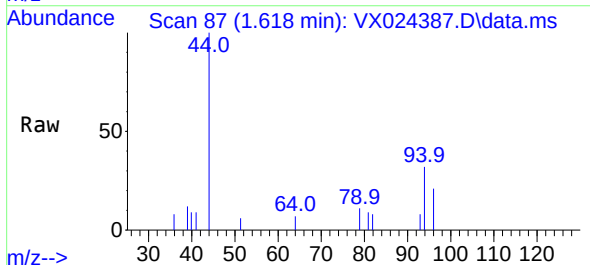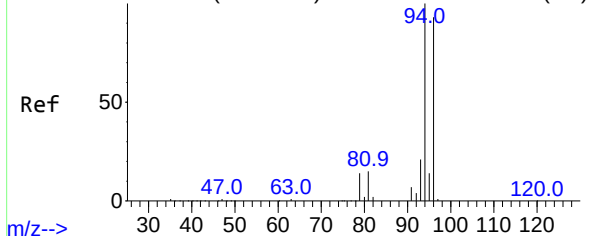

#5

Bromomethane

Concen: 0.617 ug/l

RT: 1.618 min Scan# 87


Delta R.T. 0.019 min


Lab File: VX024387.D

Acq: 21 Sep 2021 15:38

Tgt Ion: 94 Resp: 557

Ion	Ratio	Lower	Upper
94	100		
96	65.2	76.4	114.6




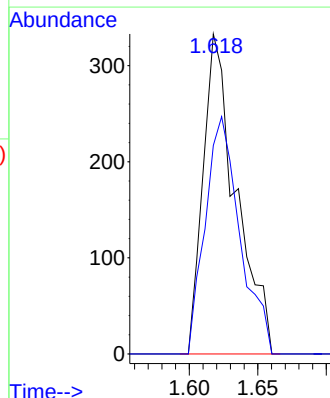




#7
Trichlorofluoromethane
Concen: 0.463 ug/l
RT: 1.892 min Scan# 132
Delta R.T. 0.006 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38




Instrument :
MSVOA_X
ClientSampleId :
DUP05-20210915


Tgt Ion:101 Resp: 1177
Ion Ratio Lower Upper
101 100
103 49.2 53.2 79.8#

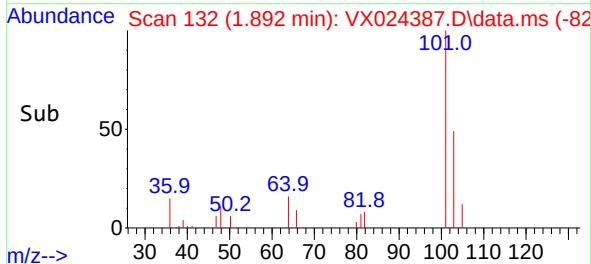

#9
1,1,2-Trichlorotrifluoroethane
Concen: 39.167 ug/l
RT: 2.331 min Scan# 204
Delta R.T. -0.000 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38

Tgt Ion:101 Resp: 58504
Ion Ratio Lower Upper
101 100
85 44.7 34.9 52.3
151 79.0 61.4 92.2


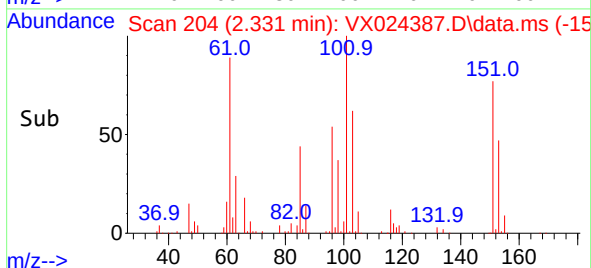
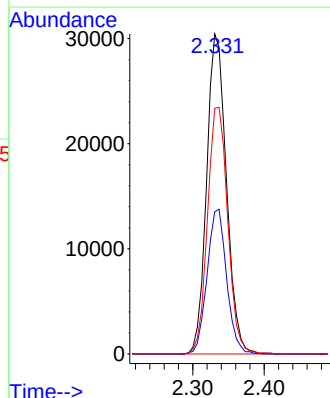
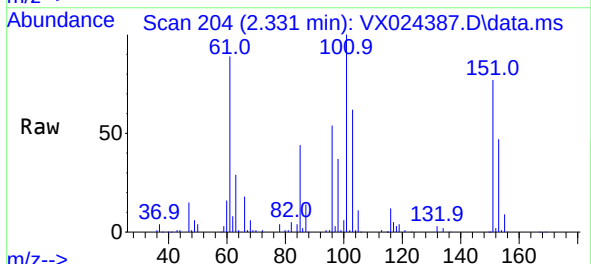




#10
Methyl Iodide
Concen: 0.465 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.012 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38




Instrument :
MSVOA_X
ClientSampleId :
DUP05-20210915


Tgt Ion:	142	Resp:	961
Ion	Ratio	Lower	Upper
142	100		
127	41.2	33.3	49.9
141	10.7	11.4	17.0#



#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.971 min Scan# 309
Delta R.T. -0.012 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38

Tgt Ion:	59	Resp:	50
Ion	Ratio	Lower	Upper
59	100		
57	0.0	7.8	11.8#

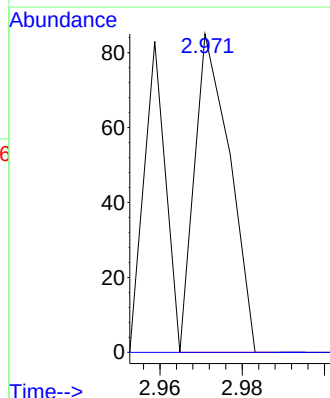



#12

1,1-Dichloroethene

Concen: 23.920 ug/l

RT: 2.325 min Scan# 203

Delta R.T. 0.006 min

Lab File: VX024387.D

Acq: 21 Sep 2021 15:38





Tgt Ion: 96 Resp: 33463

Ion Ratio Lower Upper

96 100

61 155.9 124.6 187.0

98 64.5 50.6 76.0

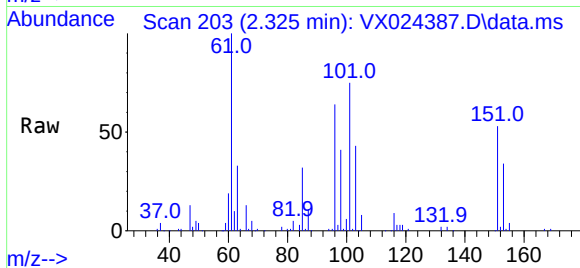

#16

Acetone

Concen: 2.635 ug/l

RT: 2.392 min Scan# 214

Delta R.T. -0.000 min

Lab File: VX024387.D




Acq: 21 Sep 2021 15:38


Tgt Ion: 43 Resp: 2431

Ion Ratio Lower Upper

43 100

58 20.0 27.8 41.8#

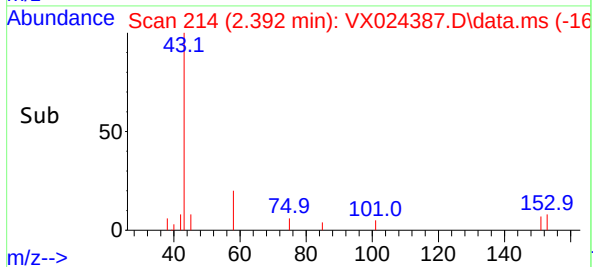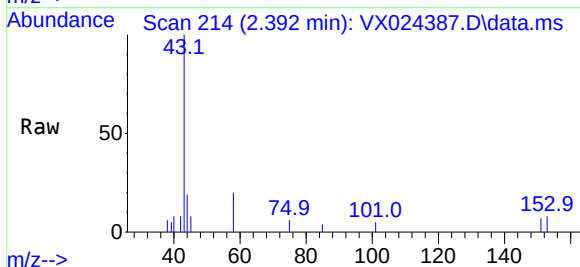



#20

Methylene Chloride

Concen: 0.393 ug/l

RT: 2.800 min Scan# 281

Delta R.T. 0.006 min

Lab File: VX024387.D

Acq: 21 Sep 2021 15:38

Instrument :

MSVOA_X

ClientSampleId :

DUP05-20210915

Tgt Ion: 84 Resp: 696





Ion Ratio Lower Upper

84 100

49 133.5 88.6 132.8#

51 43.8 27.0 40.6#

86 52.9 50.3 75.5

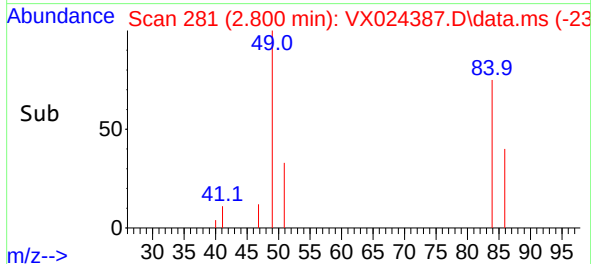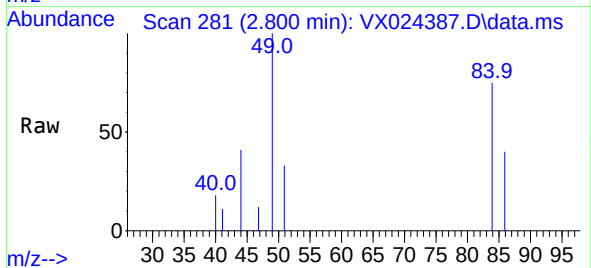

#24

1,1-Dichloroethane

Concen: 2.328 ug/l

RT: 3.617 min Scan# 415

Delta R.T. 0.000 min

Lab File: VX024387.D

Acq: 21 Sep 2021 15:38




Tgt Ion: 63 Resp: 6821


Ion Ratio Lower Upper

63 100

98 6.1 3.8 11.2

100 0.0 2.5 7.5#

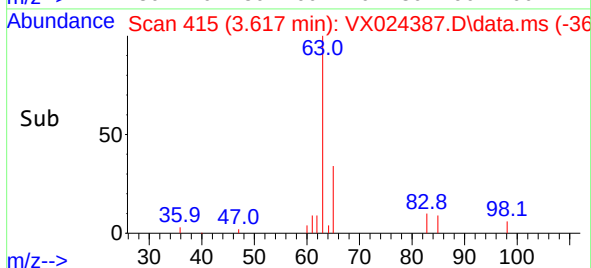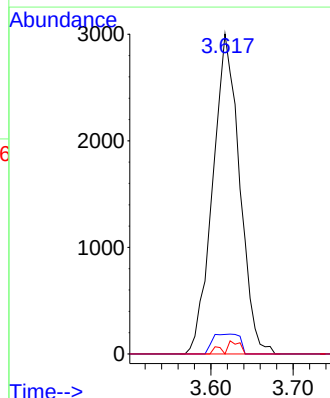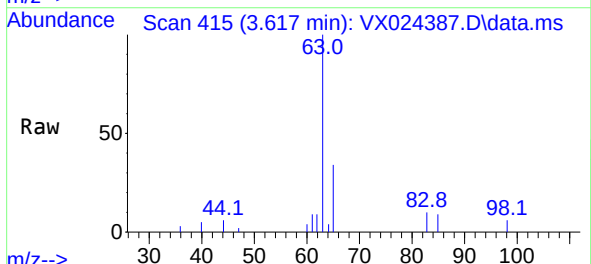







#27
cis-1,2-Dichloroethene
Concen: 3.424 ug/l
RT: 4.507 min Scan# 561
Delta R.T. 0.012 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38

Instrument :
MSVOA_X
ClientSampleId :
DUP05-20210915

Tgt Ion: 96 Resp: 6057




Ion	Ratio	Lower	Upper
96	100		
61	126.4	0.0	285.6
98	62.1	0.0	129.6

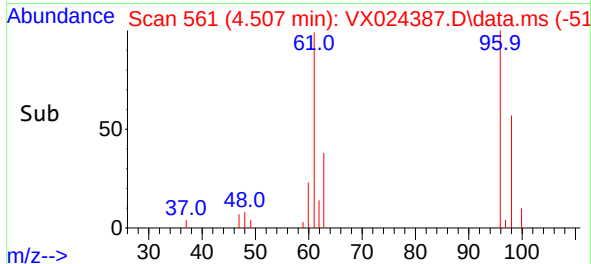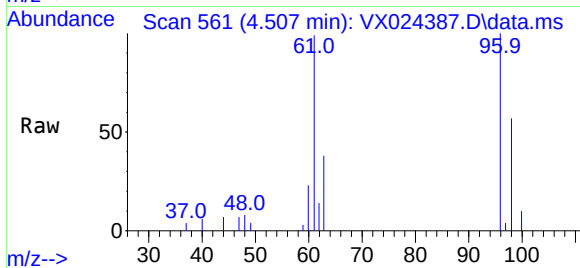


#29
Tetrahydrofuran
Concen: 0.292 ug/l
RT: 5.044 min Scan# 649
Delta R.T. 0.025 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38

Tgt Ion: 42 Resp: 248

Ion	Ratio	Lower	Upper
42	100		
72	0.0	41.7	62.5#
71	0.0	38.4	57.6#

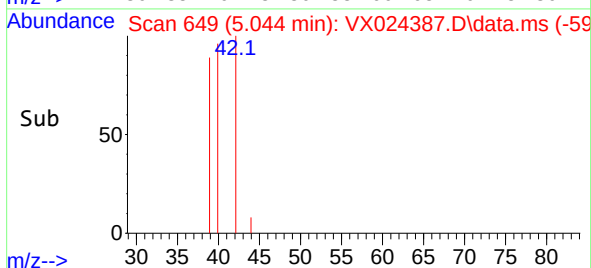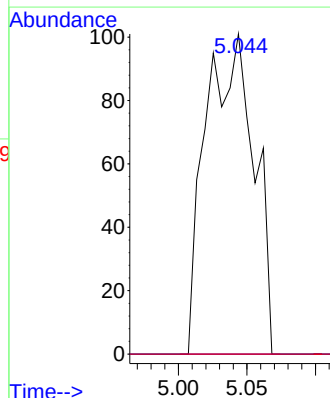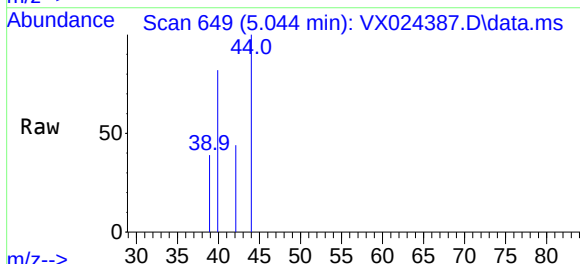



#30

Chloroform

Concen: 0.896 ug/l

RT: 5.111 min Scan# 660

Delta R.T. 0.006 min

Lab File: VX024387.D





Acq: 21 Sep 2021 15:38

Tgt Ion: 83 Resp: 2791

Ion Ratio Lower Upper

83 100

85 86.6 52.0 78.0#

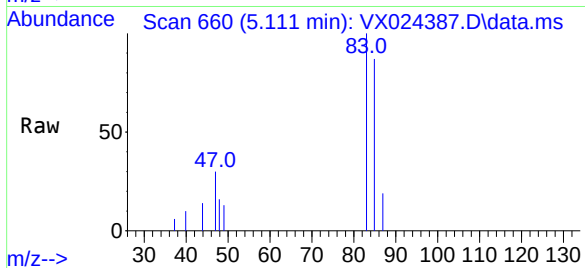

#31

Cyclohexane

Concen: 1.351 ug/l

RT: 5.568 min Scan# 735

Delta R.T. 0.091 min

Lab File: VX024387.D

Acq: 21 Sep 2021 15:38




Tgt Ion: 56 Resp: 3420


Ion Ratio Lower Upper

56 100

69 161.7 25.3 37.9#

84 120.5 71.4 107.0#


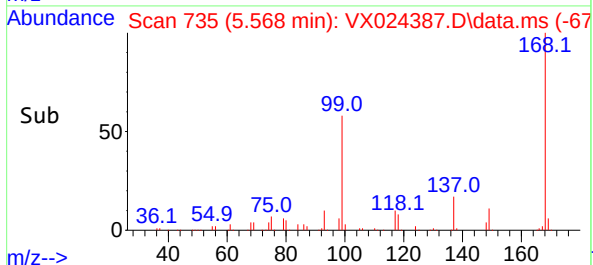
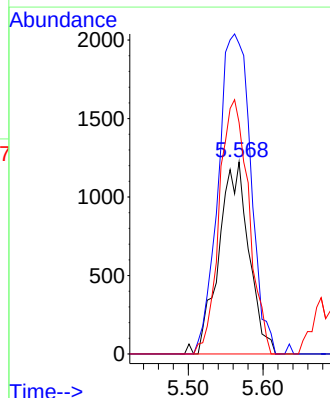
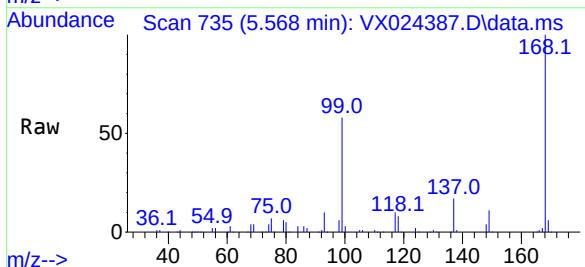




#32
1,1,1-Trichloroethane
Concen: 2.237 ug/l
RT: 5.403 min Scan# 708
Delta R.T. 0.006 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38




Instrument :
MSVOA_X
ClientSampleId :
DUP05-20210915


Tgt Ion: 97 Resp: 6239
Ion Ratio Lower Upper
97 100
99 63.2 51.5 77.3
61 46.0 34.2 51.4

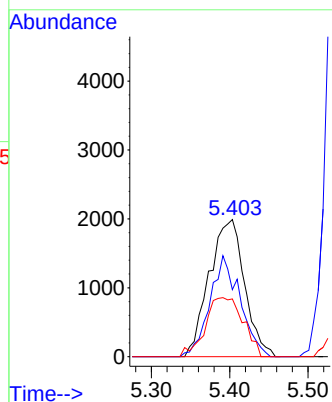

#33
1,2-Dichloroethane-d4
Concen: 47.536 ug/l
RT: 5.964 min Scan# 800
Delta R.T. -0.007 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38

Tgt Ion: 65 Resp: 102845
Ion Ratio Lower Upper
65 100
67 50.7 0.0 105.4


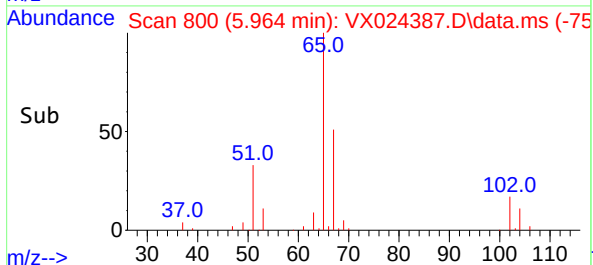
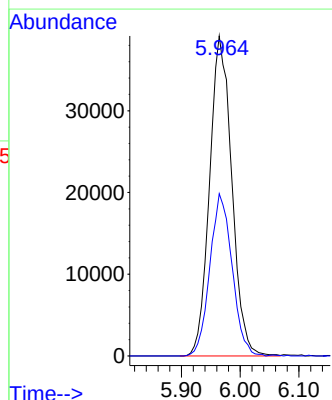
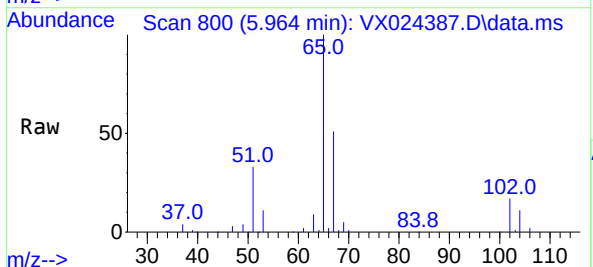


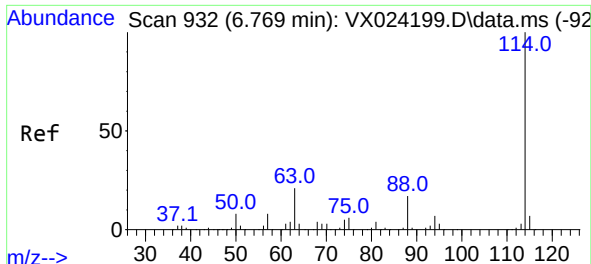

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38




Instrument :
MSVOA_X
ClientSampleId :
DUP05-20210915


Tgt Ion:114 Resp: 244703
Ion Ratio Lower Upper
114 100
63 20.5 0.0 40.8
88 16.3 0.0 32.8

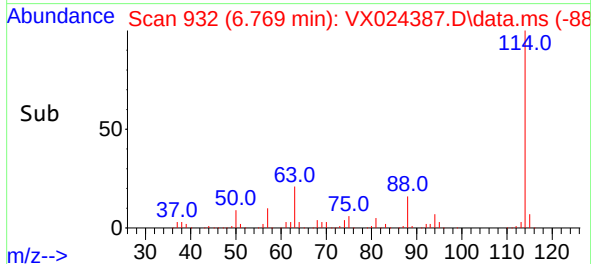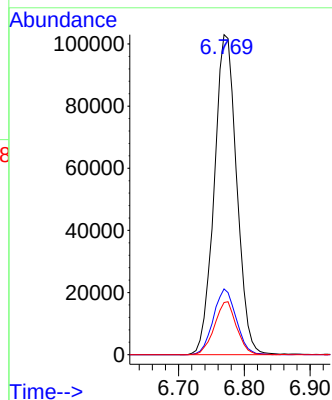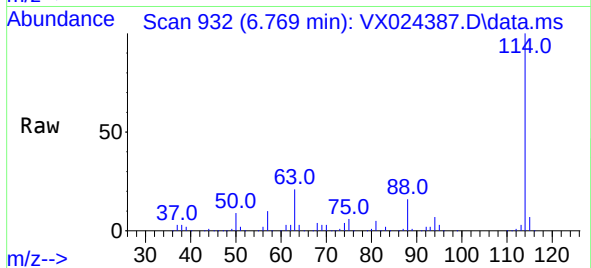

#35
Dibromofluoromethane
Concen: 53.881 ug/l
RT: 5.403 min Scan# 708
Delta R.T. 0.006 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38

Tgt Ion:113 Resp: 88424
Ion Ratio Lower Upper
113 100
111 103.5 81.9 122.9
192 20.0 16.7 25.1


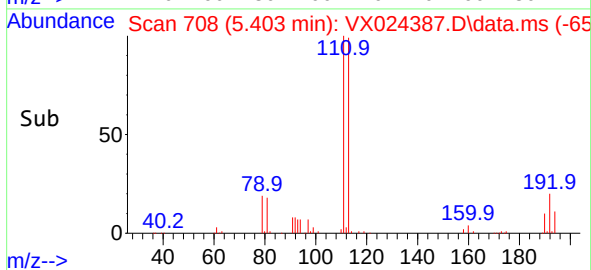
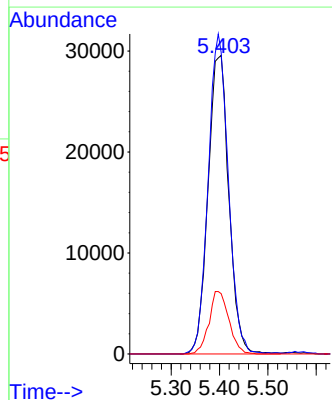
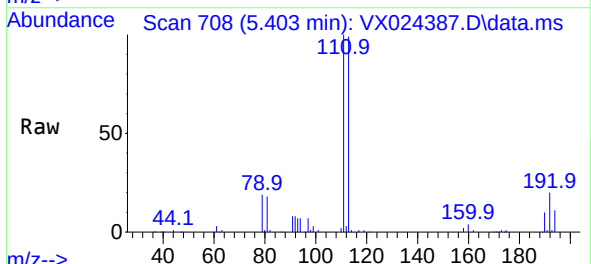




#36
1,1-Dichloropropene
Concen: 5.300 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.140 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38




Instrument :
MSVOA_X
ClientSampleId :
DUP05-20210915


Tgt Ion:	75	Resp:	11925
Ion	Ratio	Lower	Upper
75	100		
110	9.8	18.1	54.4#
77	0.0	25.3	37.9#

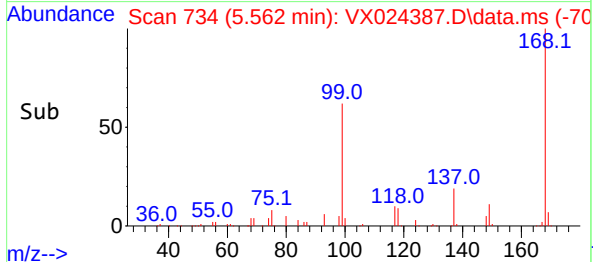

#38
Carbon Tetrachloride
Concen: 1.902 ug/l
RT: 5.690 min Scan# 755
Delta R.T. 0.006 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38

Tgt Ion:	117	Resp:	4817
Ion	Ratio	Lower	Upper
117	100		
119	86.8	76.2	114.2
121	34.2	24.8	37.2

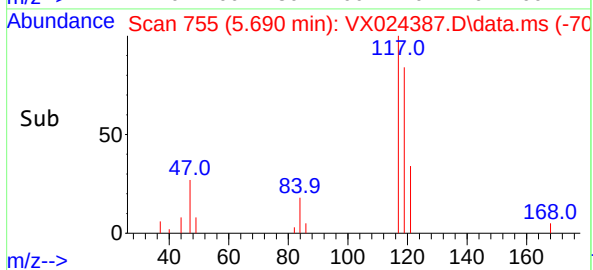



#39

Methylcyclohexane

Concen: 3.171 ug/l

RT: 7.135 min Scan# 992

Delta R.T. -0.250 min

Lab File: VX024387.D

Acq: 21 Sep 2021 15:38

Tgt Ion: 83 Resp: 8518

Ion Ratio Lower Upper

83 100

55 0.0 58.9 88.3#





98 219.8 38.1 57.1#

Instrument :

MSVOA_X

ClientSampleId :

DUP05-20210915

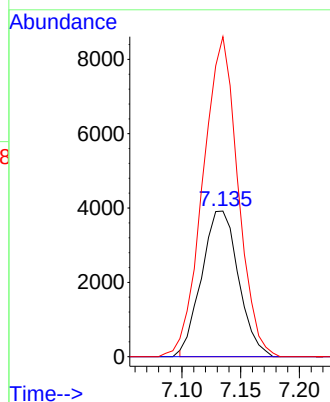

#42

1,2-Dichloroethane

Concen: 0.477 ug/l

RT: 6.105 min Scan# 823

Delta R.T. 0.006 min

Lab File: VX024387.D




Acq: 21 Sep 2021 15:38


Tgt Ion: 62 Resp: 1283

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.2


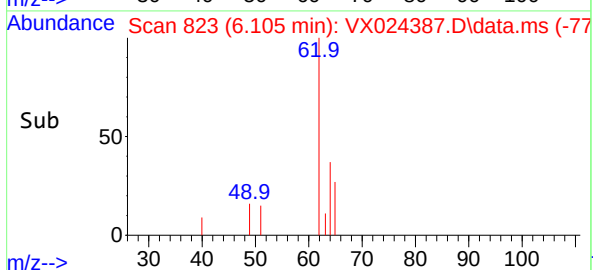






#44
Trichloroethene
Concen: 375.394 ug/l
RT: 7.135 min Scan# 992
Delta R.T. -0.000 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38




Instrument :
MSVOA_X
ClientSampleId :
DUP05-20210915


Tgt Ion:130 Resp: 680594
Ion Ratio Lower Upper
130 100
95 99.2 0.0 198.0

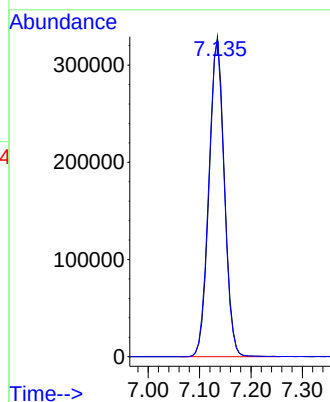

#49
1,4-Dioxane
Concen: 17.708 ug/l
RT: 7.671 min Scan# 1080
Delta R.T. 0.006 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38

Tgt Ion: 88 Resp: 772
Ion Ratio Lower Upper
88 100
43 11.3 23.2 34.8#
58 0.0 55.0 82.4#


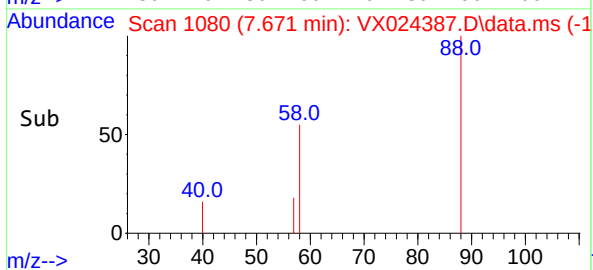






#50
Toluene-d8
Concen: 55.852 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38




Instrument :
MSVOA_X
ClientSampleId :
DUP05-20210915


Tgt Ion: 98 Resp: 333906
Ion Ratio Lower Upper
98 100
100 64.3 51.9 77.9

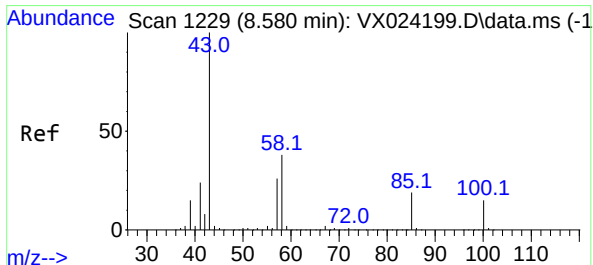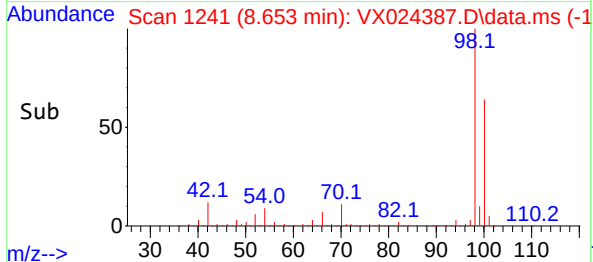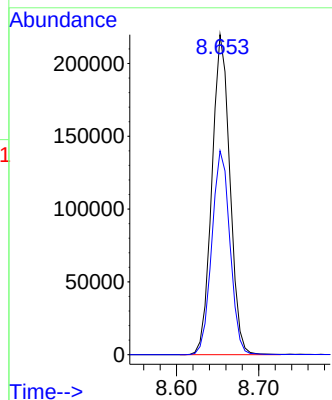

#51
4-Methyl-2-Pentanone
Concen: 0.590 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.073 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38

Tgt Ion: 43 Resp: 1570
Ion Ratio Lower Upper
43 100
58 171.0 35.4 53.0#


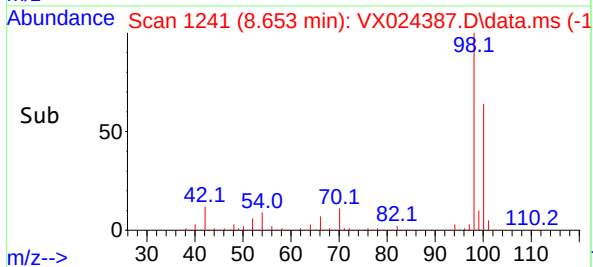
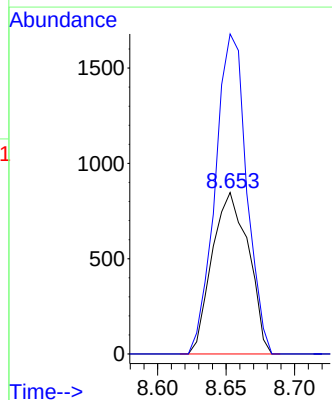
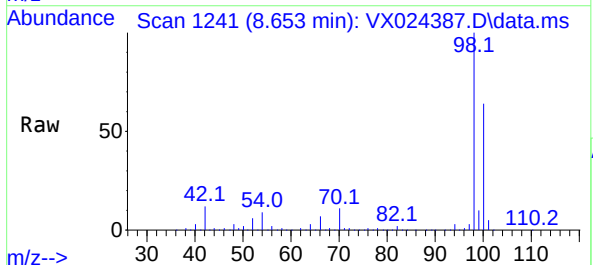




#55
1,1,2-Trichloroethane
Concen: 1.052 ug/l
RT: 9.159 min Scan# 1324
Delta R.T. -0.000 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38




Instrument :
MSVOA_X
ClientSampleId :
DUP05-20210915


Tgt Ion: 97	Resp: 1895
Ion Ratio	Lower Upper
97 100	
83 64.9	69.3 103.9#
85 46.3	44.3 66.5
99 48.3	50.3 75.5#

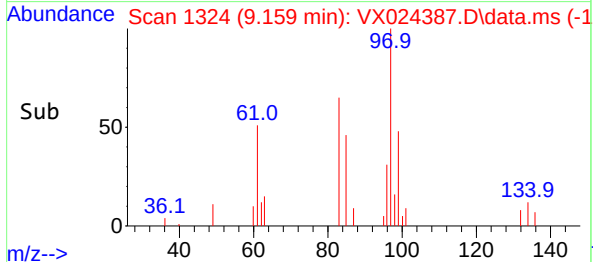

#60
Dibromochloromethane
Concen: 1.947 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.250 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38

Tgt Ion:129	Resp:	467	
Ion	Ratio	Lower	Upper
129	100		
127	0.0	38.4	115.2#



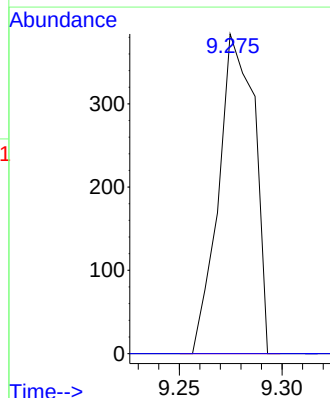





#62
4-Bromofluorobenzene
Concen: 54.635 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38




Instrument :
MSVOA_X
ClientSampleId :
DUP05-20210915


Tgt Ion: 95 Resp: 127112
Ion Ratio Lower Upper
95 100
174 78.1 0.0 154.6
176 74.1 0.0 155.8

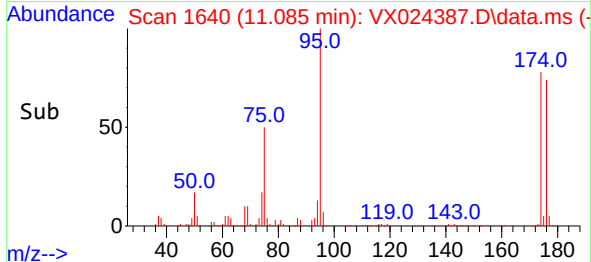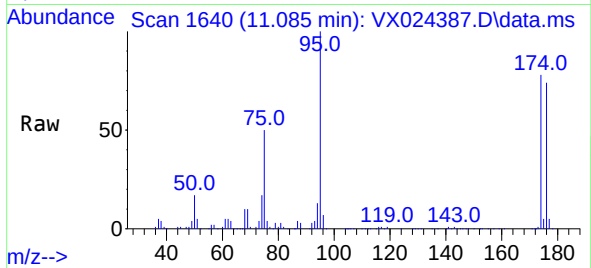

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.000 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38


Tgt Ion: 117 Resp: 240156
Ion Ratio Lower Upper
117 100
82 54.7 47.4 71.2
119 32.5 26.6 39.8

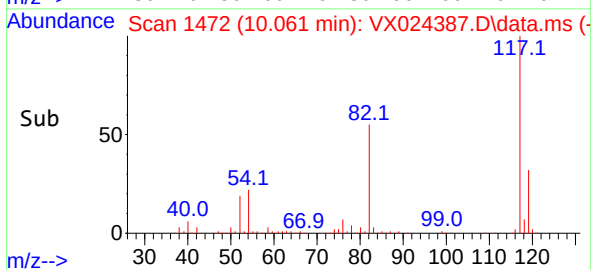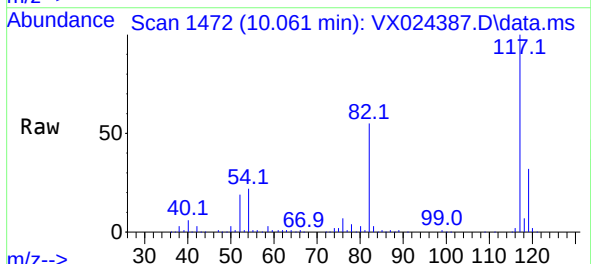






#64
Tetrachloroethene
Concen: 0.292 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. -0.000 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38

Instrument :
MSVOA_X
ClientSampleId :
DUP05-20210915




Tgt Ion:164 Resp: 544

Ion	Ratio	Lower	Upper
164	100		
166	117.0	103.4	155.2
129	84.0	70.8	106.2
131	85.0	72.5	108.7






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38



Tgt Ion:152 Resp: 111646

Ion	Ratio	Lower	Upper
152	100		
115	61.2	41.1	123.3
150	160.8	0.0	349.0









#76
1,2,3-Trichloropropane
Concen: 25.105 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38




Instrument :
MSVOA_X
ClientSampleId :
DUP05-20210915


Tgt Ion: 75 Resp: 64450
Ion Ratio Lower Upper
75 100
77 1.1 19.1 57.5#

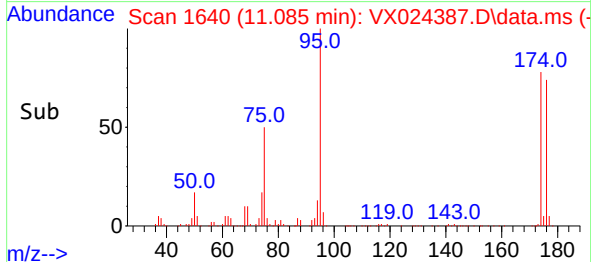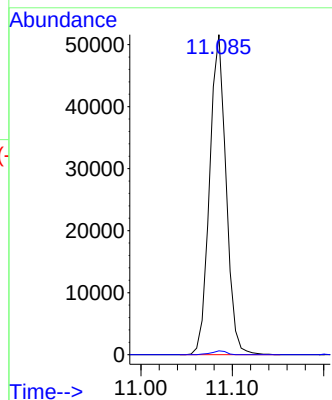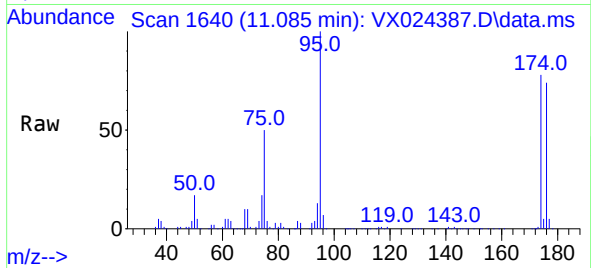

#81
trans-1,4-Dichloro-2-butene
Concen: 73.835 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.060 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38


Tgt Ion: 75 Resp: 64450
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

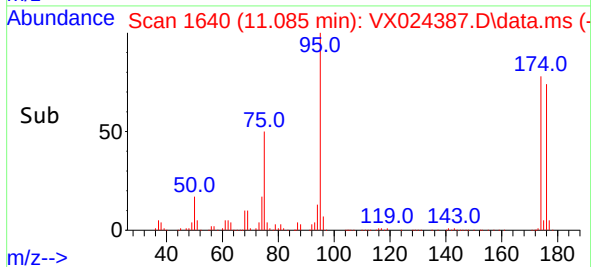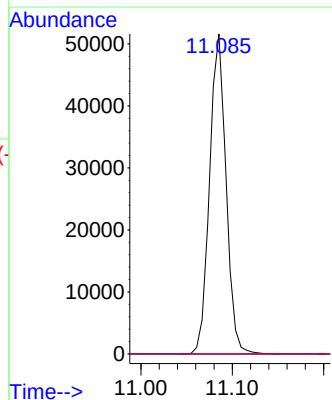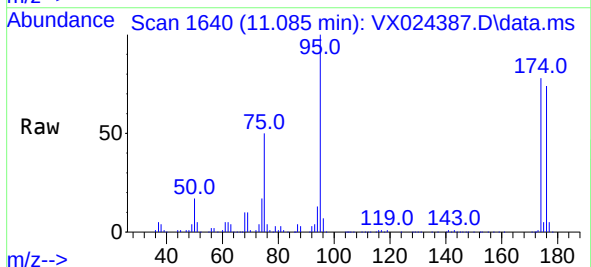



#95
Naphthalene
Concen: 1.309 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX024387.D
Acq: 21 Sep 2021 15:38

Instrument :
MSVOA_X
ClientSampleId :
DUP05-20210915

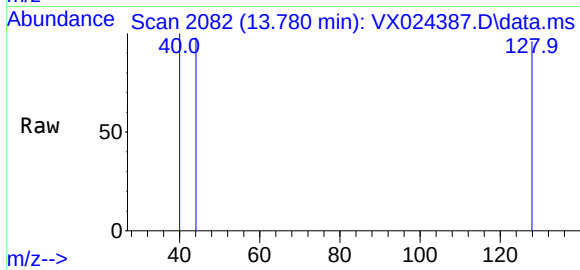

Tgt Ion:	128	Resp:	181
Ion	Ratio	Lower	Upper
128	100		
127	0.0	10.3	15.5#
129	0.0	8.8	13.2#

