

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
 Data File : VX024390.D
 Acq On : 21 Sep 2021 16:49
 Operator : JC/MD
 Sample : M3835-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SW-CB-03-(1.0)

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M

Title : SW846 8260

Signal : TIC: VX024390.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.397	693	707	722	rBV	107374	310790	31.20%	6.305%
2	5.562	722	734	749	rVV	162802	465119	46.70%	9.436%
3	5.964	790	800	807	rBV	107960	288553	28.97%	5.854%
4	6.050	807	814	827	rVB	92719	244672	24.57%	4.964%
5	6.769	923	932	950	rBV	244382	581618	58.40%	11.799%
6	8.653	1233	1241	1249	rBV	542985	846140	84.96%	17.166%
7	10.055	1465	1471	1488	rBV2	547651	995974	100.00%	20.205%
8	11.085	1634	1640	1654	rBV	452689	563313	56.56%	11.428%
9	12.024	1789	1794	1804	rVB	496204	616320	61.88%	12.503%
10	12.341	1839	1846	1851	rVB	12450	16736	1.68%	0.340%




Sum of corrected areas: 4929235

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024390.D
Acq On : 21 Sep 2021 16:49
Operator : JC/MD
Sample : M3835-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-CB-03-(1.0)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

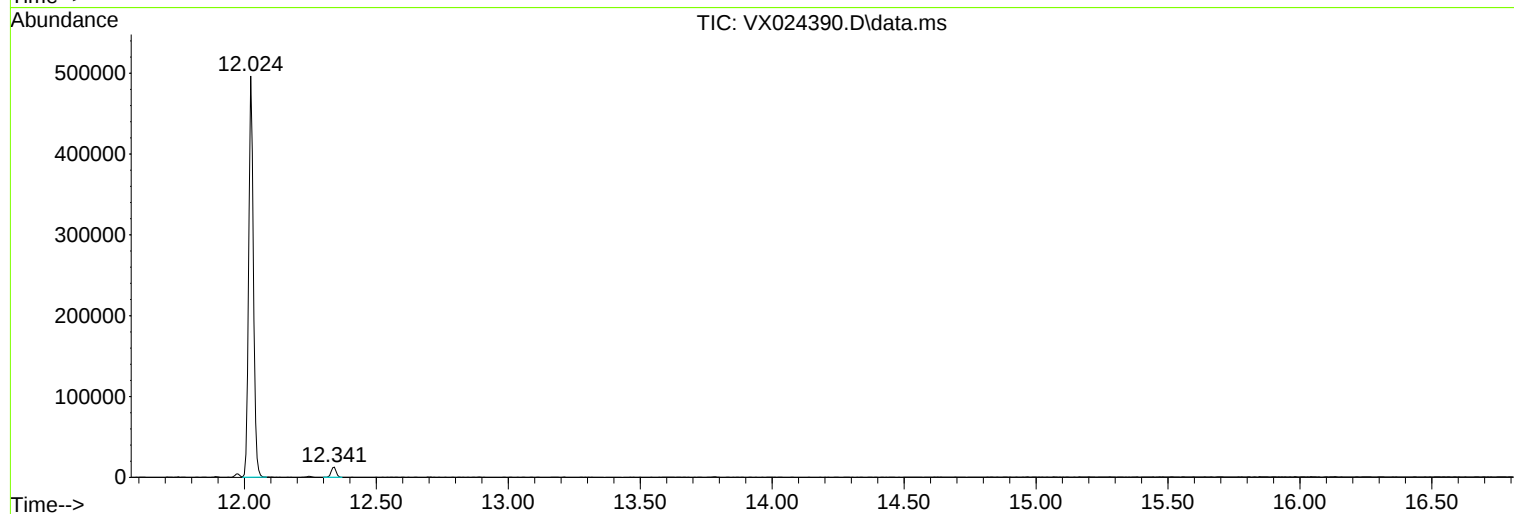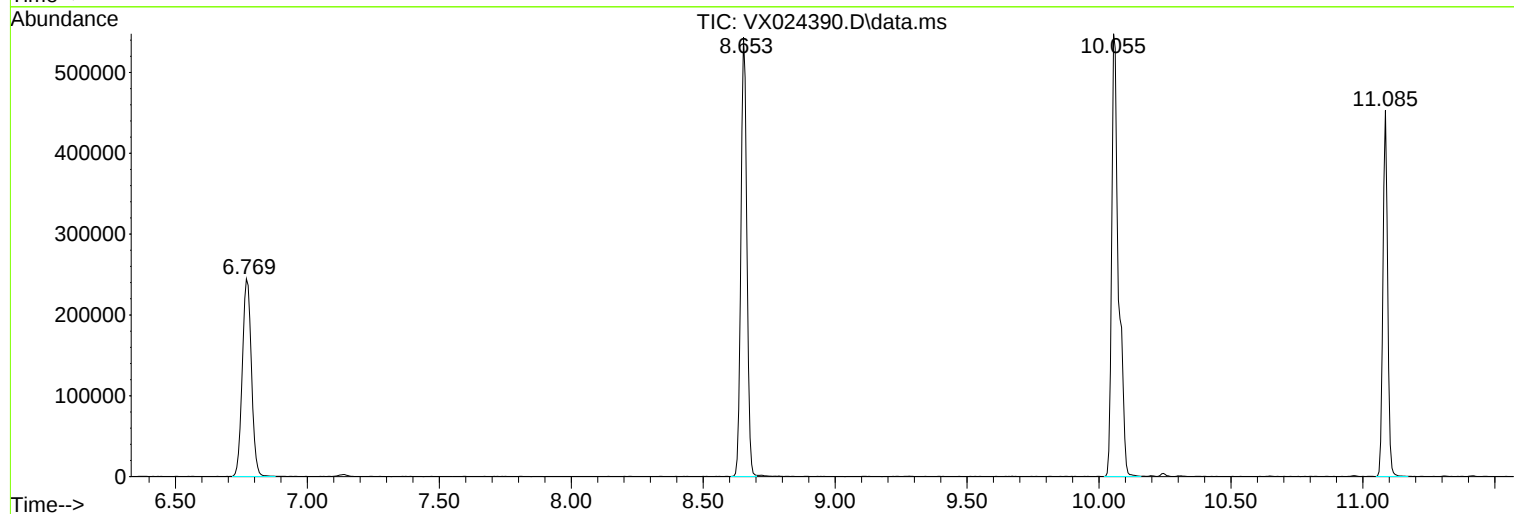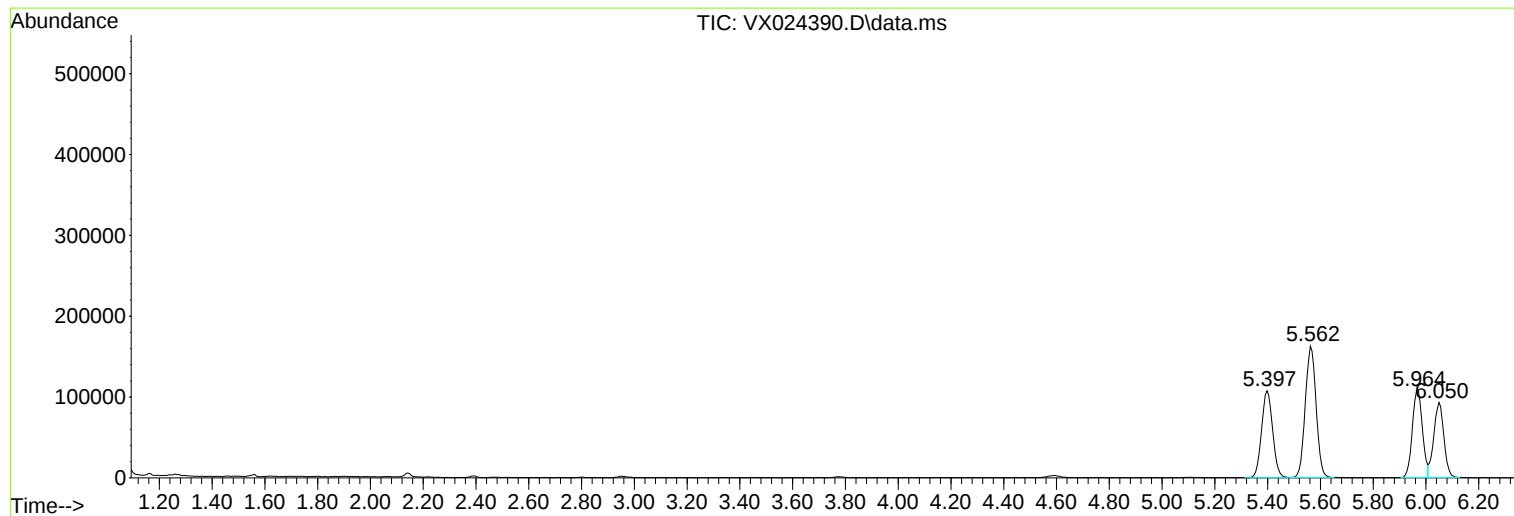

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024390.D
Acq On : 21 Sep 2021 16:49
Operator : JC/MD
Sample : M3835-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-CB-03-(1.0)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024390.D
Acq On : 21 Sep 2021 16:49
Operator : JC/MD
Sample : M3835-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-CB-03-(1.0)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------