

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
 Data File : VX024407.D
 Acq On : 22 Sep 2021 00:40
 Operator : JC/MD
 Sample : M3833-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB03-20210919

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M

Title : SW846 8260

Signal : TIC: VX024407.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	33	rVB2	11595	14269	1.96%	0.369%
2	2.550	234	240	250	rVB	6962	12280	1.69%	0.318%
3	2.959	298	307	313	rBV	3667	8963	1.23%	0.232%
4	4.593	562	575	587	rBV2	3423	11989	1.65%	0.310%
5	5.397	696	707	722	rBV2	87946	255142	35.12%	6.600%
6	5.562	723	734	747	rVB2	137884	384316	52.91%	9.942%
7	5.970	789	801	814	rBV	94614	250500	34.48%	6.480%
8	6.769	922	932	947	rBV	220033	521975	71.86%	13.503%
9	8.653	1234	1241	1255	rBV	464151	726404	100.00%	18.791%
10	10.055	1466	1471	1486	rBV	463365	646742	89.03%	16.730%
11	11.085	1634	1640	1652	rVB	391967	486922	67.03%	12.596%
12	12.024	1789	1794	1803	rBV	442013	546236	75.20%	14.130%




Sum of corrected areas: 3865738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024407.D
Acq On : 22 Sep 2021 00:40
Operator : JC/MD
Sample : M3833-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB03-20210919

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

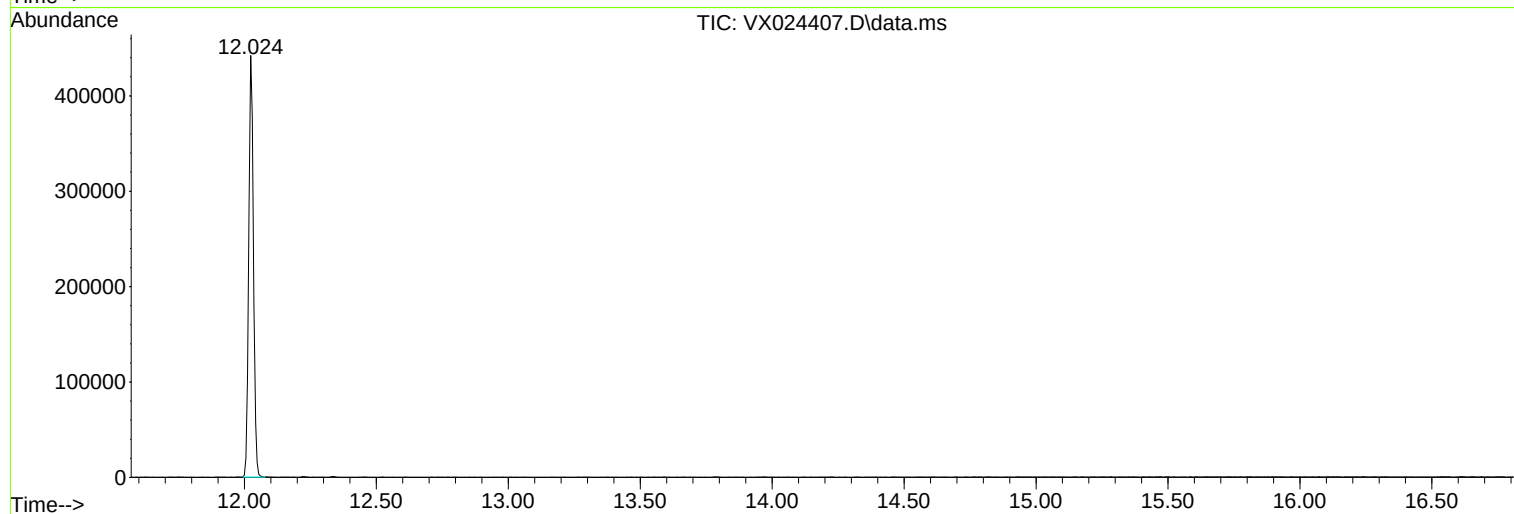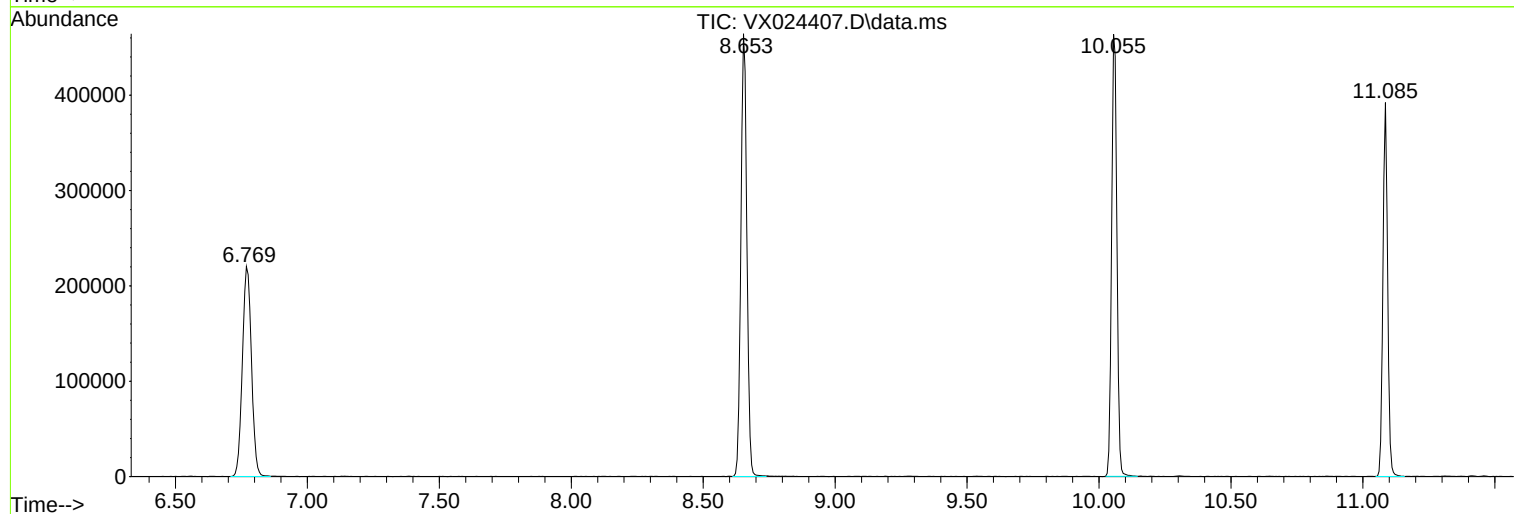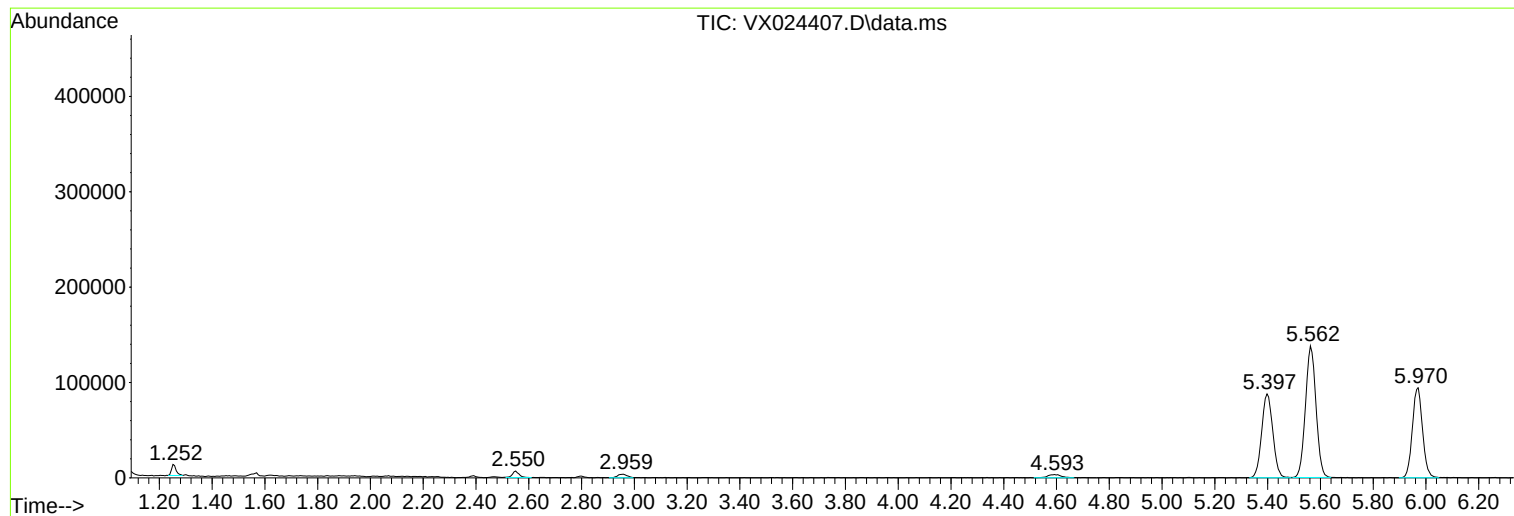

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024407.D
Acq On : 22 Sep 2021 00:40
Operator : JC/MD
Sample : M3833-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB03-20210919

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024407.D
Acq On : 22 Sep 2021 00:40
Operator : JC/MD
Sample : M3833-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB03-20210919

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------