

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
 Data File : VX024410.D
 Acq On : 22 Sep 2021 01:50
 Operator : JC/MD
 Sample : M3833-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE123D1-20210918

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M

Title : SW846 8260

Signal : TIC: VX024410.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	38	rVB4	3253	8002	1.15%	0.210%
2	2.544	232	239	249	rBV	9956	18676	2.68%	0.491%
3	5.397	693	707	722	rBV2	85628	245842	35.25%	6.467%
4	5.562	722	734	748	rVV	132444	370041	53.06%	9.734%
5	5.964	789	800	813	rBV	91643	241504	34.63%	6.353%
6	6.769	922	932	945	rBV	212255	502348	72.03%	13.214%
7	7.135	981	992	1004	rBV2	59517	130714	18.74%	3.438%
8	8.653	1234	1241	1252	rBV	456483	697399	100.00%	18.345%
9	10.055	1466	1471	1484	rBV	459960	616386	88.38%	16.214%
10	11.085	1634	1640	1651	rBV	368308	461651	66.20%	12.144%
11	12.024	1789	1794	1803	rBV	413111	508954	72.98%	13.388%




Sum of corrected areas: 3801517

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024410.D
Acq On : 22 Sep 2021 01:50
Operator : JC/MD
Sample : M3833-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE123D1-20210918

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

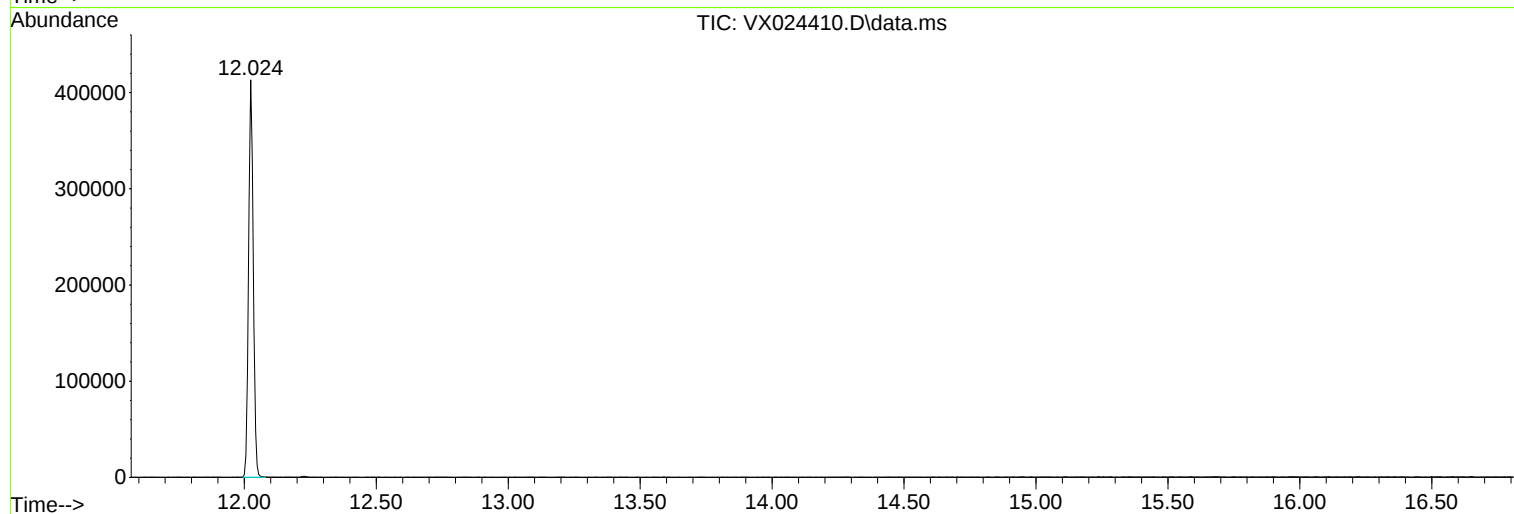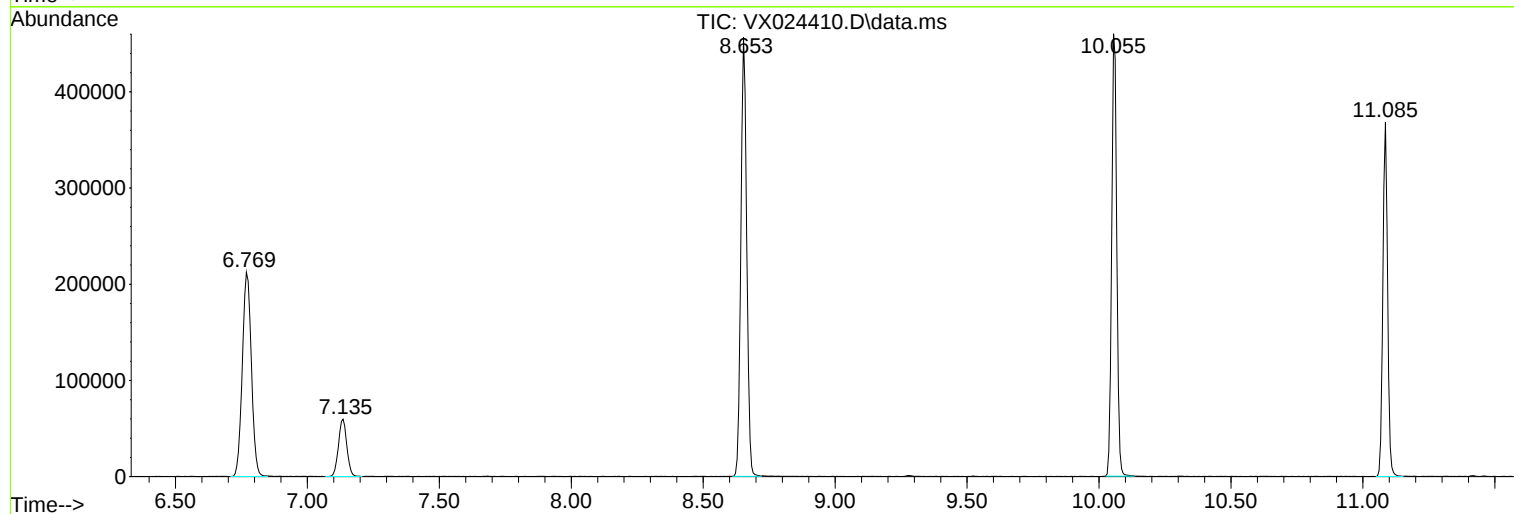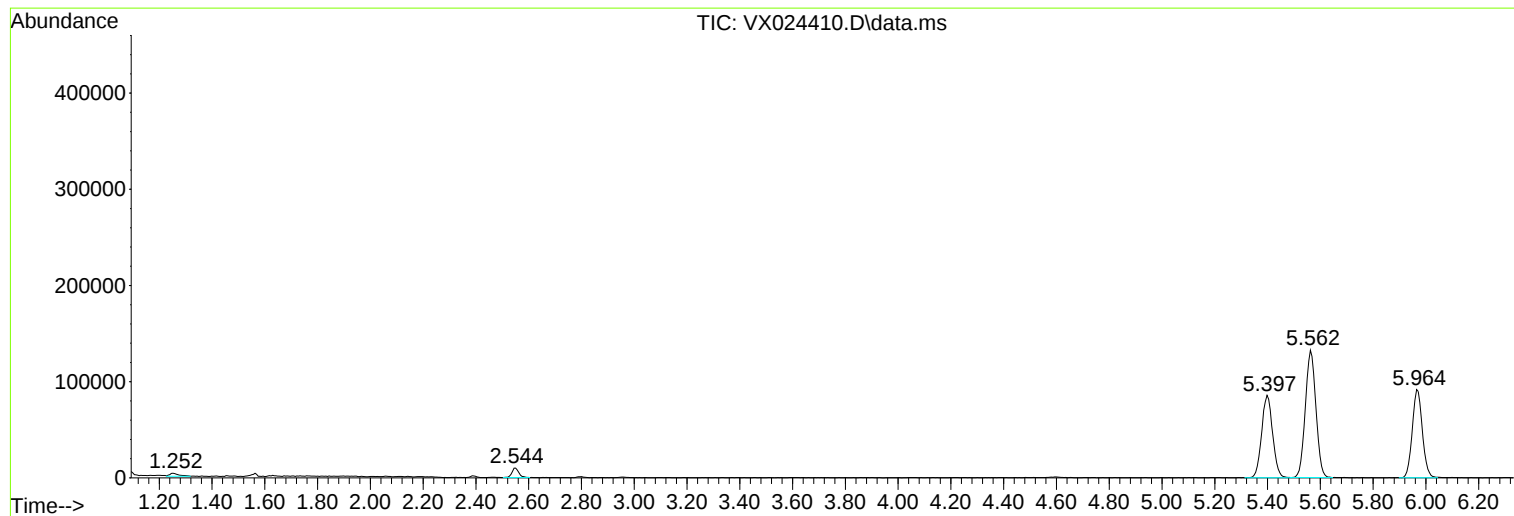

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024410.D
Acq On : 22 Sep 2021 01:50
Operator : JC/MD
Sample : M3833-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE123D1-20210918

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024410.D
Acq On : 22 Sep 2021 01:50
Operator : JC/MD
Sample : M3833-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE123D1-20210918

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
