

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
 Data File : VX024414.D
 Acq On : 22 Sep 2021 03:25
 Operator : JC/MD
 Sample : M3833-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D3-20210920

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M

Title : SW846 8260

Signal : TIC: VX024414.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.251	23	27	34	rBV3	4560	8368	1.12%	0.210%
2	2.550	231	240	249	rBV	5845	10728	1.44%	0.270%
3	5.397	695	707	721	rBV2	86834	255227	34.20%	6.415%
4	5.562	724	734	751	rVB	139777	390610	52.34%	9.817%
5	5.964	790	800	815	rBV2	94396	253601	33.98%	6.374%
6	6.769	922	932	950	rBV	222431	532520	71.35%	13.384%
7	7.135	986	992	999	rVB4	7115	15123	2.03%	0.380%
8	8.653	1234	1241	1256	rBV	489973	746344	100.00%	18.758%
9	10.055	1466	1471	1484	rBV	508723	704312	94.37%	17.702%
10	11.085	1634	1640	1652	rBV	415163	515589	69.08%	12.959%
11	12.024	1789	1794	1807	rBV	441575	546347	73.20%	13.732%




Sum of corrected areas: 3978769

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024414.D
Acq On : 22 Sep 2021 03:25
Operator : JC/MD
Sample : M3833-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20210920

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

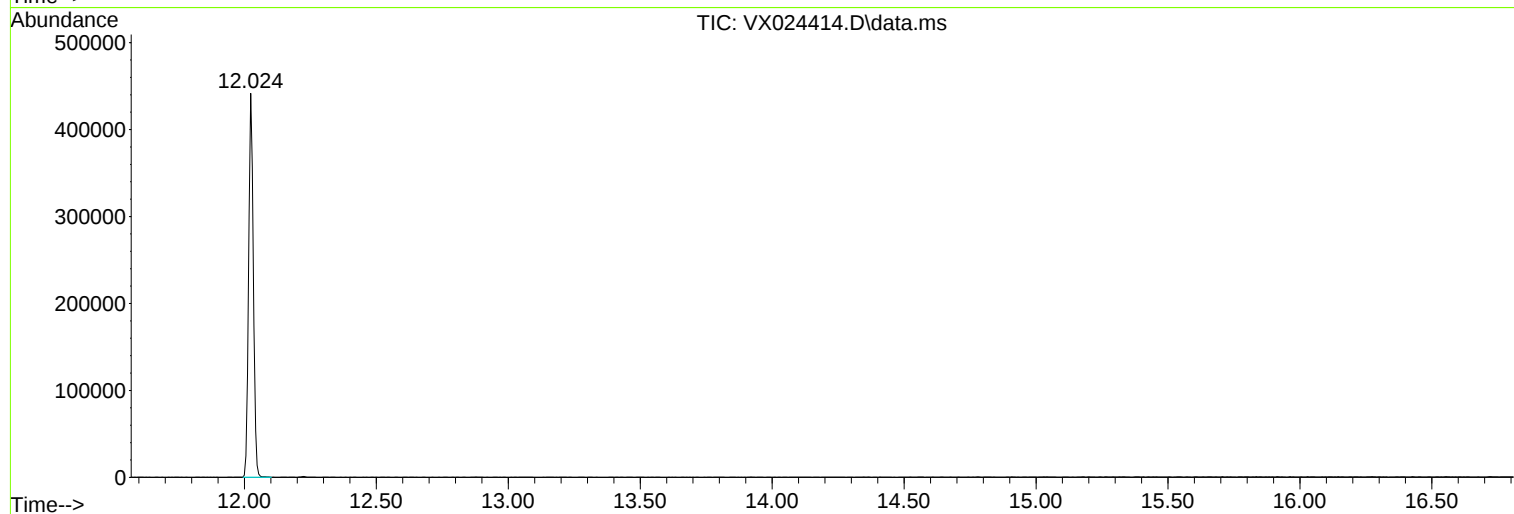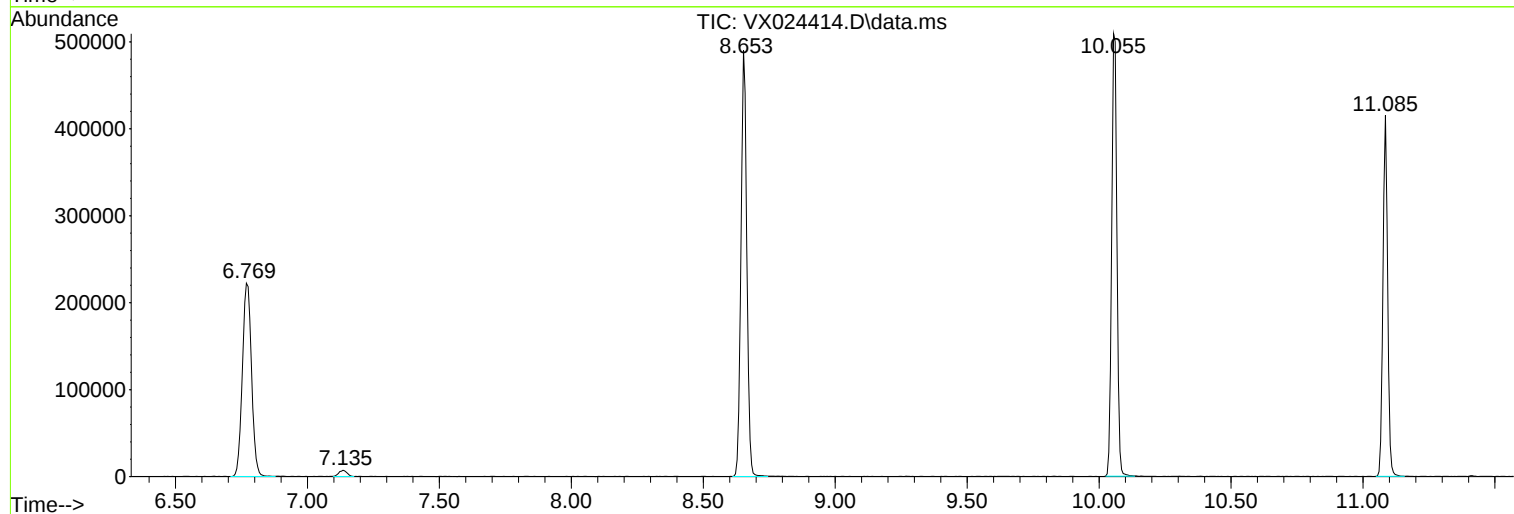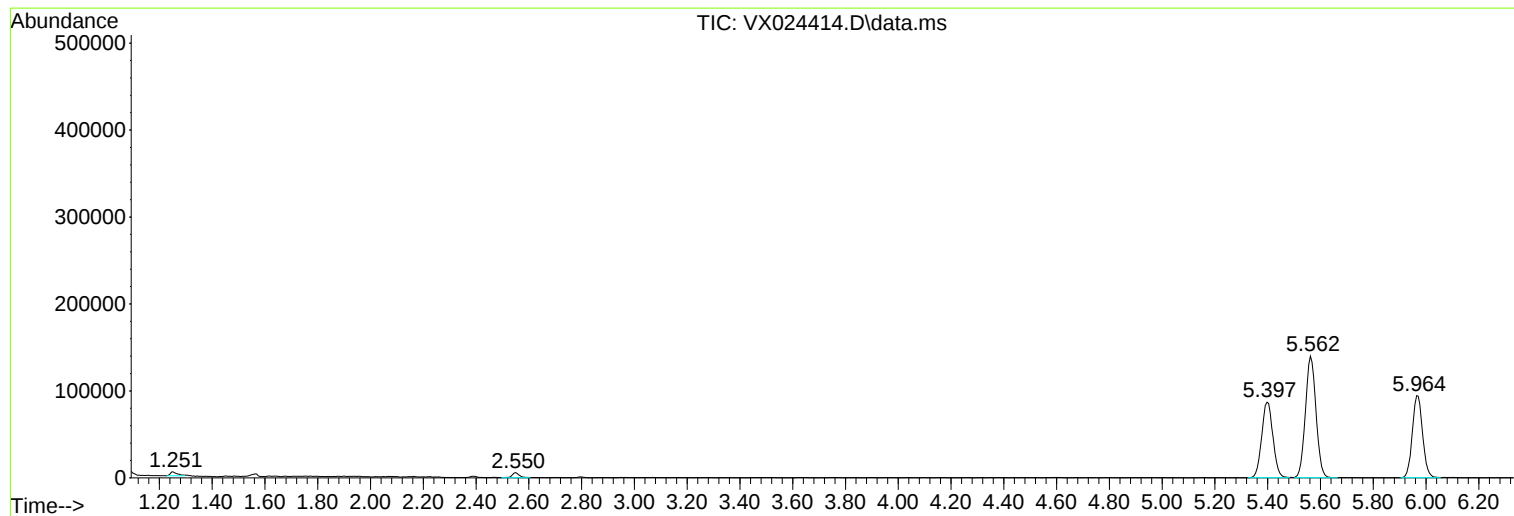

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024414.D
Acq On : 22 Sep 2021 03:25
Operator : JC/MD
Sample : M3833-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20210920

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024414.D
Acq On : 22 Sep 2021 03:25
Operator : JC/MD
Sample : M3833-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20210920

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
