

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024424.D
Acq On : 22 Sep 2021 07:20
Operator : JC/MD
Sample : M3833-06 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP08-20210919

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M

Title : SW846 8260

Signal : TIC: VX024424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.397	696	707	720	rBV2	86143	251776	32.55%	6.006%
2	5.562	723	734	749	rVB	135139	384246	49.68%	9.167%
3	5.971	790	801	819	rBV	95934	253695	32.80%	6.052%
4	6.769	922	932	952	rBV	221588	531035	68.66%	12.669%
5	8.653	1234	1241	1254	rBV	490913	753174	97.39%	17.968%
6	10.055	1465	1471	1488	rBV	555096	773395	100.00%	18.450%
7	11.085	1634	1640	1651	rBV	472057	579245	74.90%	13.819%
8	12.024	1789	1794	1806	rBV	536983	665172	86.01%	15.869%




Sum of corrected areas: 4191738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024424.D
Acq On : 22 Sep 2021 07:20
Operator : JC/MD
Sample : M3833-06 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP08-20210919

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

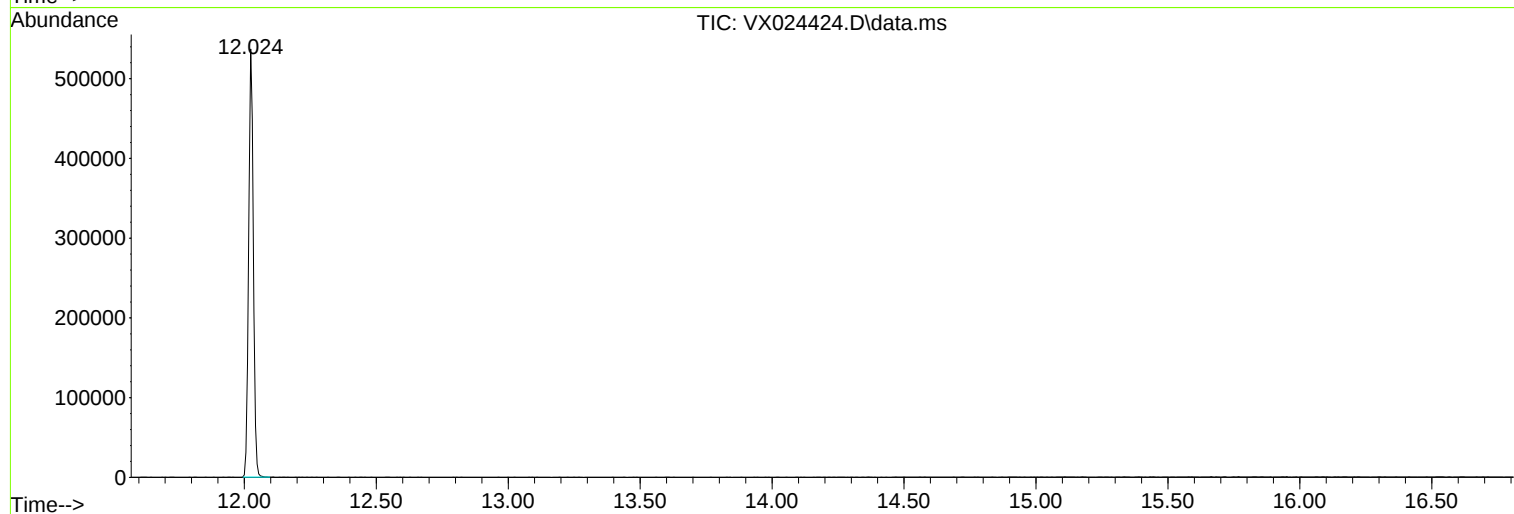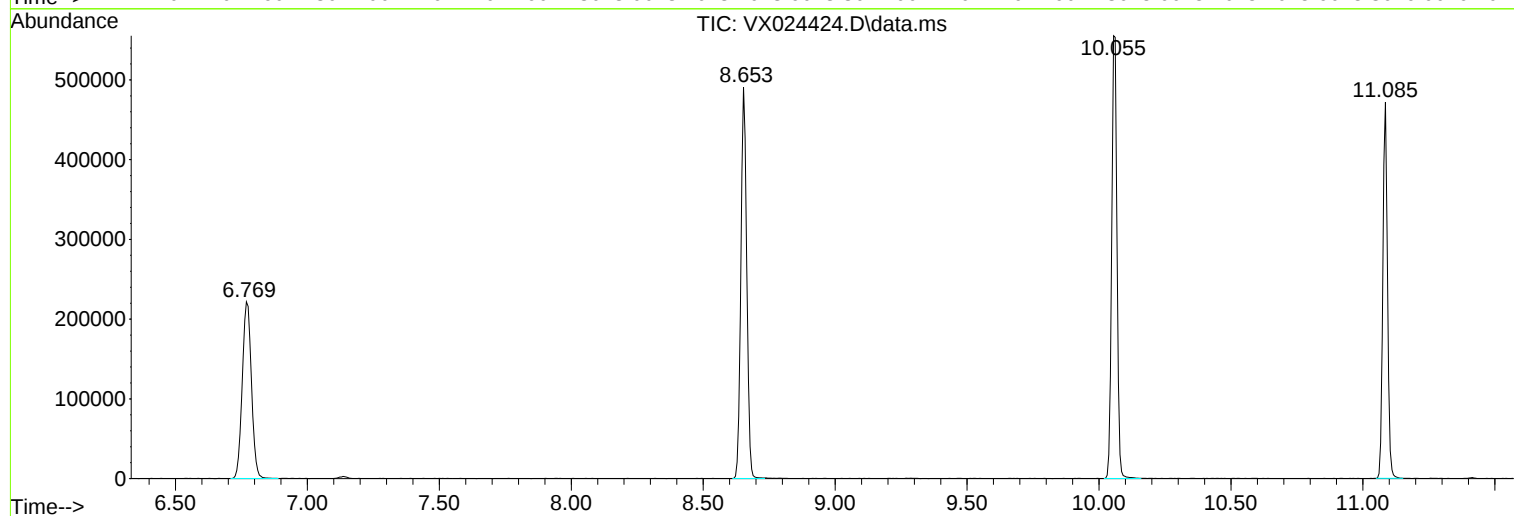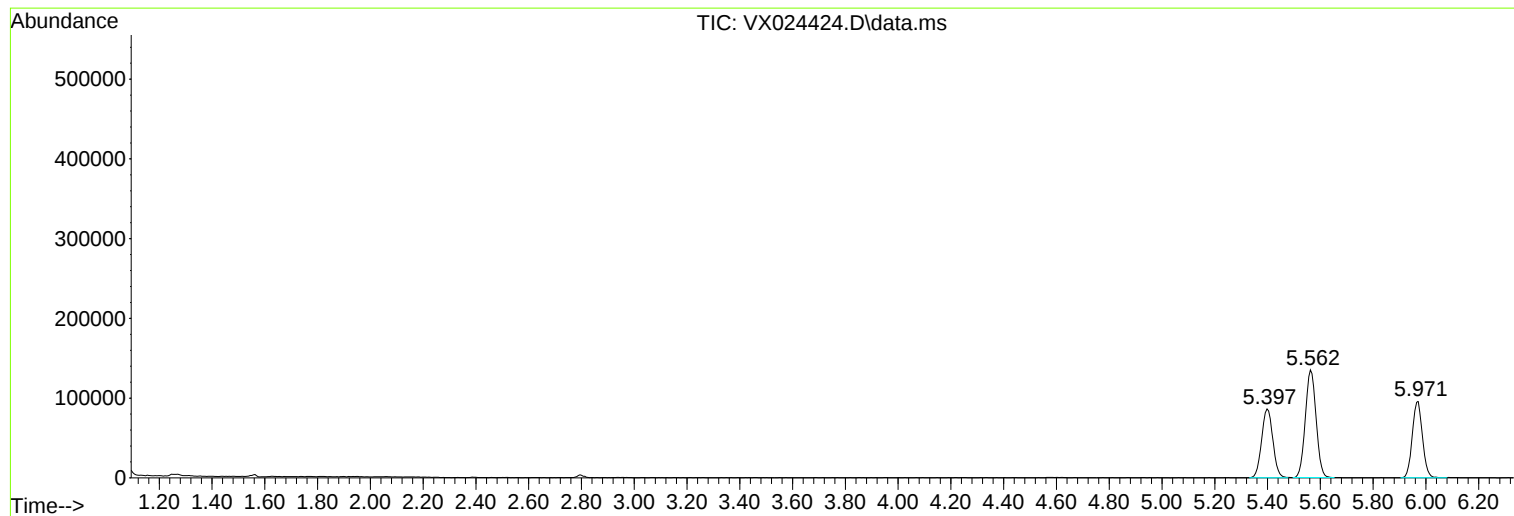

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024424.D
Acq On : 22 Sep 2021 07:20
Operator : JC/MD
Sample : M3833-06 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP08-20210919

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092121\
Data File : VX024424.D
Acq On : 22 Sep 2021 07:20
Operator : JC/MD
Sample : M3833-06 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP08-20210919

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091421W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
